

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061219\
 Data File : BM020906.D
 Acq On : 12 Jun 2019 16:40
 Operator : HP/JU
 Sample : PB120443BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	7	10	16	rVB	68700	78627	0.94%	0.095%
2	3.305	50	54	61	rVB	97048	122890	1.47%	0.148%
3	4.028	173	177	183	rVB	84721	110918	1.33%	0.134%
4	6.969	670	677	689	rVB	1617386	2489354	29.74%	3.005%
5	7.145	699	707	720	rBV	1245982	1936058	23.13%	2.337%
6	7.334	732	739	748	rBV	1690126	2692934	32.18%	3.251%
7	7.804	811	819	826	rBV	1072040	1693550	20.23%	2.044%
8	8.504	927	938	951	rBV	1932408	3097652	37.01%	3.740%
9	8.969	1008	1017	1028	rBV	1481166	2481291	29.65%	2.995%
10	9.681	1129	1138	1150	rBV	1236052	2064929	24.67%	2.493%
11	10.216	1221	1229	1238	rBV	1974587	3338701	39.89%	4.031%
12	10.592	1285	1293	1304	rVB	1382358	2343118	28.00%	2.829%
13	10.733	1309	1317	1334	rBV	1774590	3151848	37.66%	3.805%
14	12.186	1558	1564	1572	rVB	30699	48920	0.58%	0.059%
15	13.416	1765	1773	1782	rBV5	5829	13437	0.16%	0.016%
16	13.851	1841	1847	1859	rVB	3178494	4498436	53.75%	5.431%
17	14.133	1888	1895	1905	rBV	3701249	5589954	66.79%	6.748%
18	14.445	1941	1948	1959	rVB2	1957920	2971563	35.50%	3.587%
19	14.645	1975	1982	1995	rBV	1271914	1934188	23.11%	2.335%
20	15.233	2078	2082	2087	rVB	15300	18409	0.22%	0.022%
21	15.439	2110	2117	2128	rBV	4739750	6793818	81.17%	8.202%
22	15.557	2130	2137	2152	rBV	791322	1112458	13.29%	1.343%
23	15.674	2152	2157	2163	rVB	56446	80799	0.97%	0.098%
24	16.980	2375	2379	2384	rVB	8504	13714	0.16%	0.017%
25	17.192	2406	2415	2421	rBV	2348686	3374111	40.31%	4.073%
26	17.286	2425	2431	2444	rBV	4918385	6963026	83.20%	8.406%
27	17.445	2453	2458	2468	rBV4	34673	67003	0.80%	0.081%
28	18.074	2561	2565	2570	rBV5	7556	9061	0.11%	0.011%
29	19.215	2755	2759	2764	rBV	52052	69970	0.84%	0.084%
30	19.468	2798	2802	2807	rBV	43099	57153	0.68%	0.069%
31	19.580	2815	2821	2828	rBV	5731683	7751995	92.62%	9.358%
32	21.368	3120	3125	3131	rBV	2873134	3621418	43.27%	4.372%
33	23.509	3482	3489	3499	rBV	4514654	8369427	100.00%	10.104%
34	23.656	3508	3514	3522	rVB2	2057645	3874073	46.29%	4.677%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061219\
Data File : BM020906.D
Acq On : 12 Jun 2019 16:40
Operator : HP/JU
Sample : PB120443BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 82834803

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061219\
Data File : BM020906.D
Acq On : 12 Jun 2019 16:40
Operator : HP/JU
Sample : PB120443BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

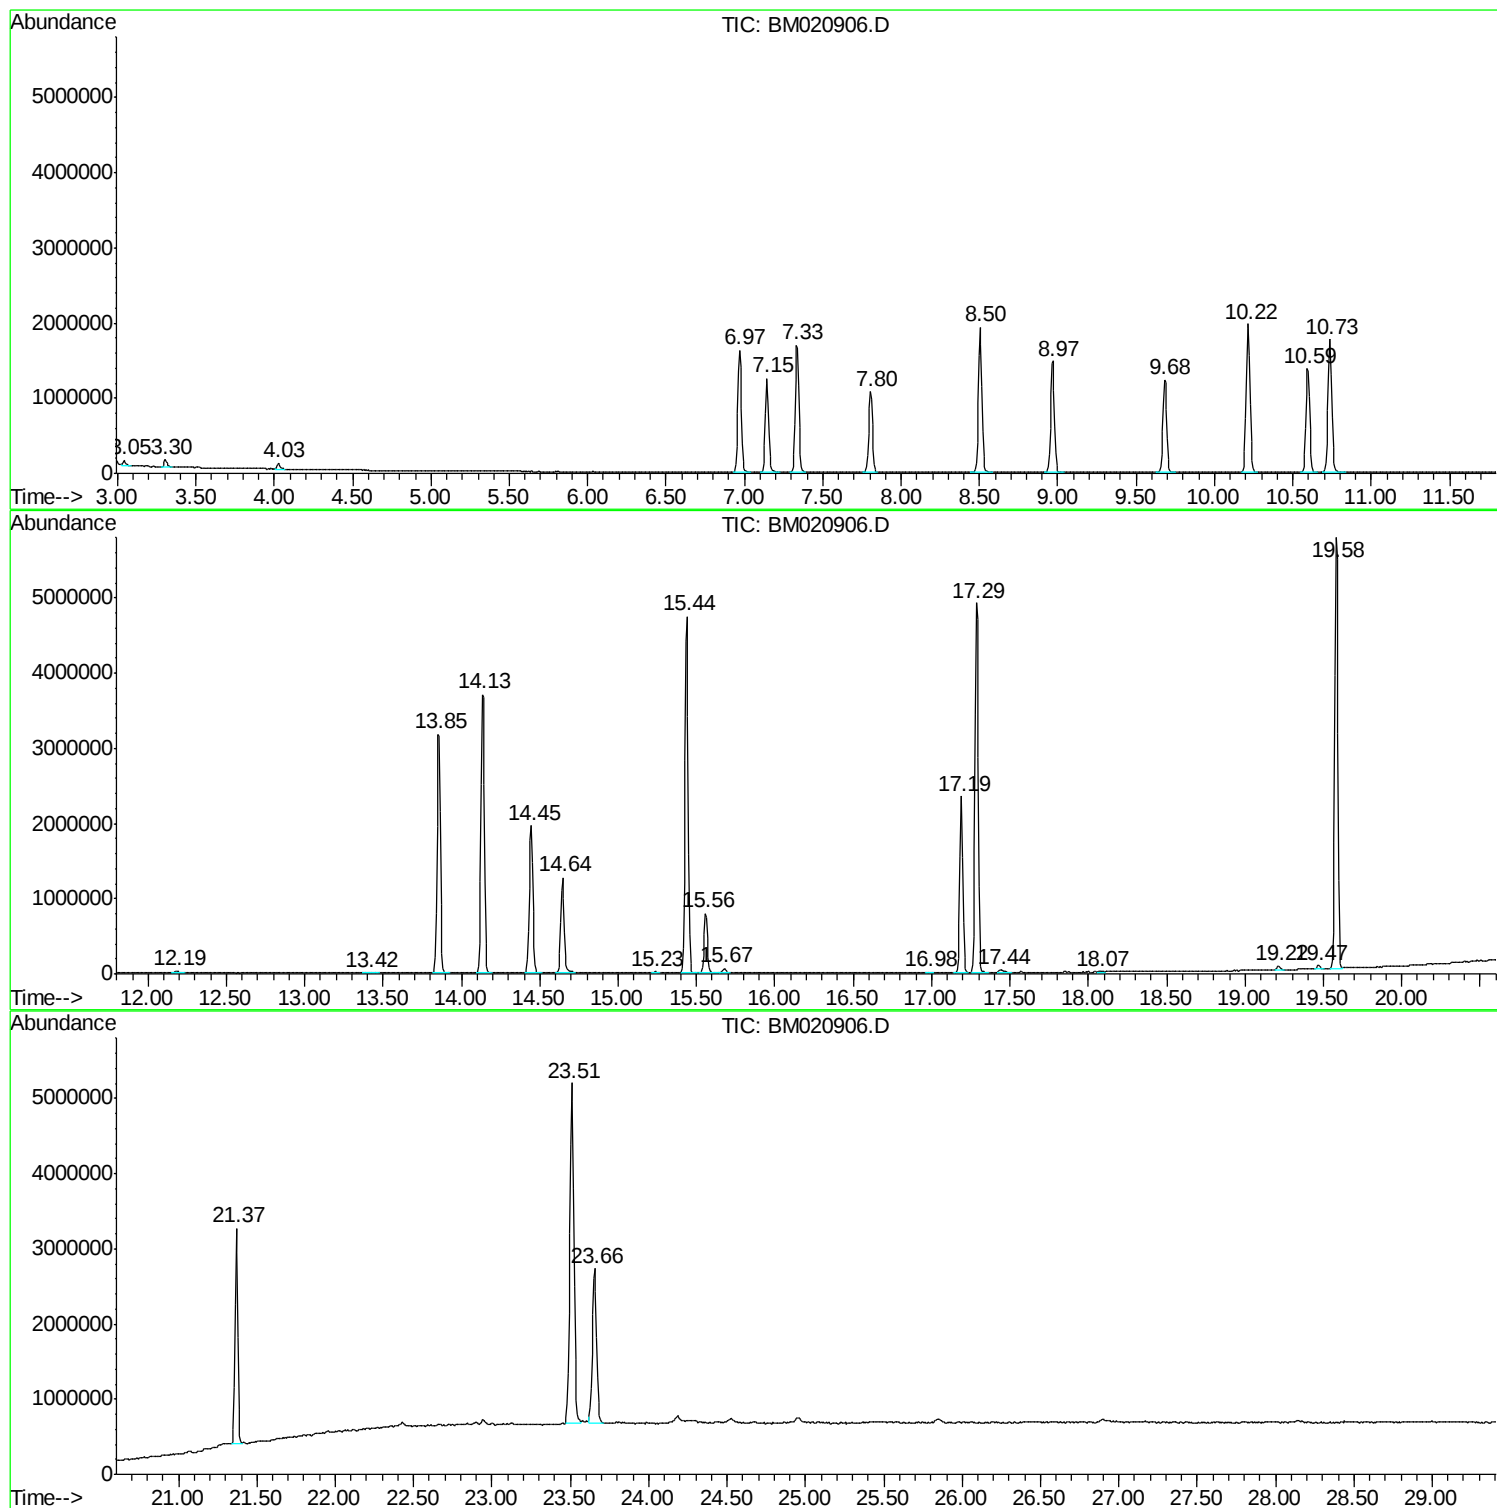

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061219\
Data File : BM020906.D
Acq On : 12 Jun 2019 16:40
Operator : HP/JU
Sample : PB120443BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061219\
Data File : BM020906.D
Acq On : 12 Jun 2019 16:40
Operator : HP/JU
Sample : PB120443BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc