
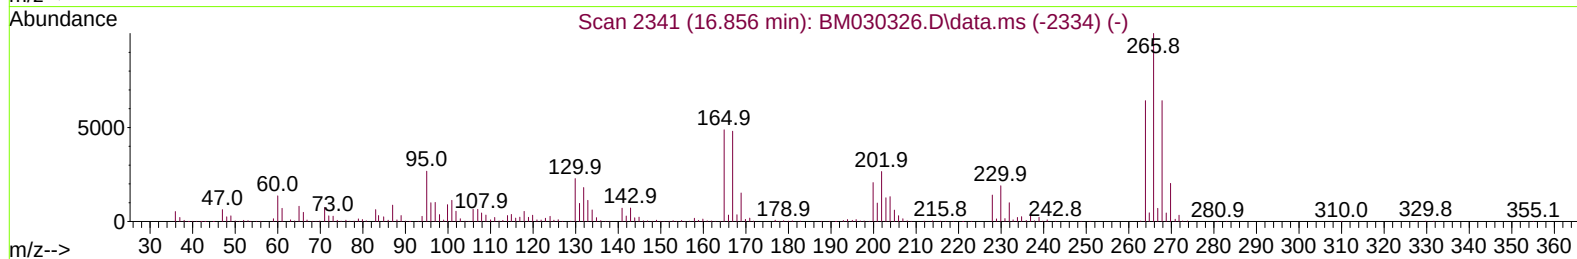
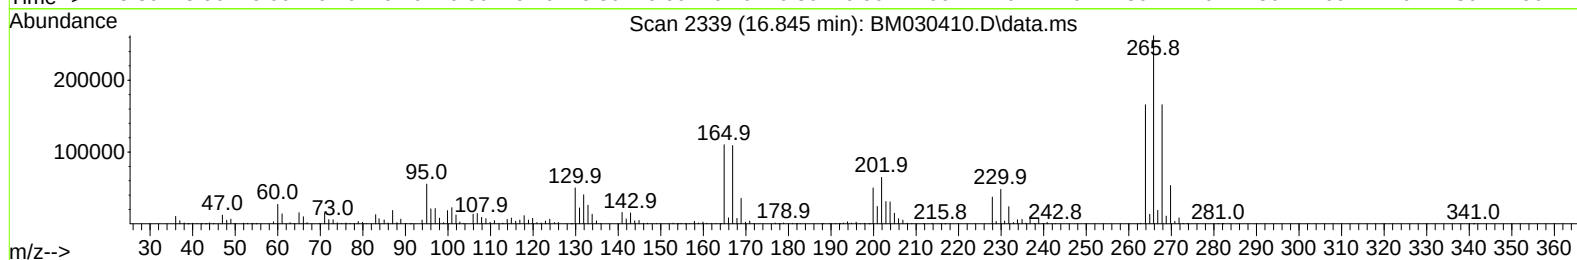


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061221\
 Data File : BM030410.D
 Acq On : 12 Jun 2021 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:59:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 14:10:50 2021
 Response via : Initial Calibration

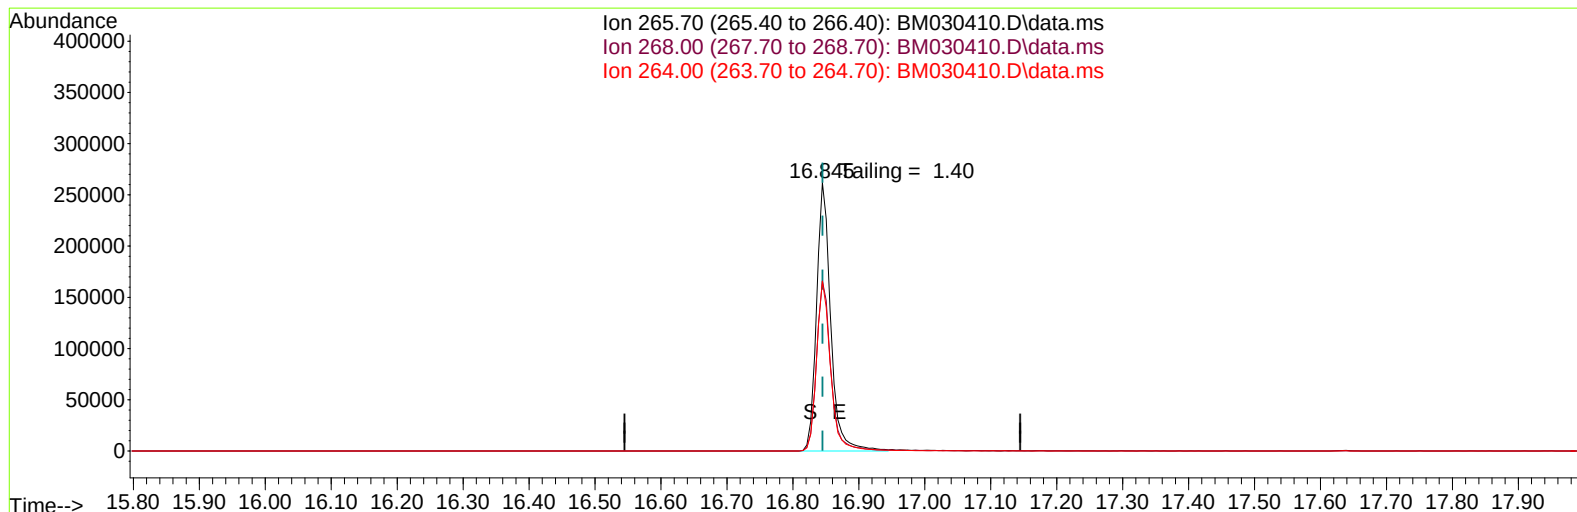

TIC: BM030410.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.000) 248205.10 ng

response 395437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.33
264.00	64.90	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061221\
Data File : BM030410.D
Acq On : 12 Jun 2021 12:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 03:59:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 14:10:50 2021
Response via : Initial Calibration

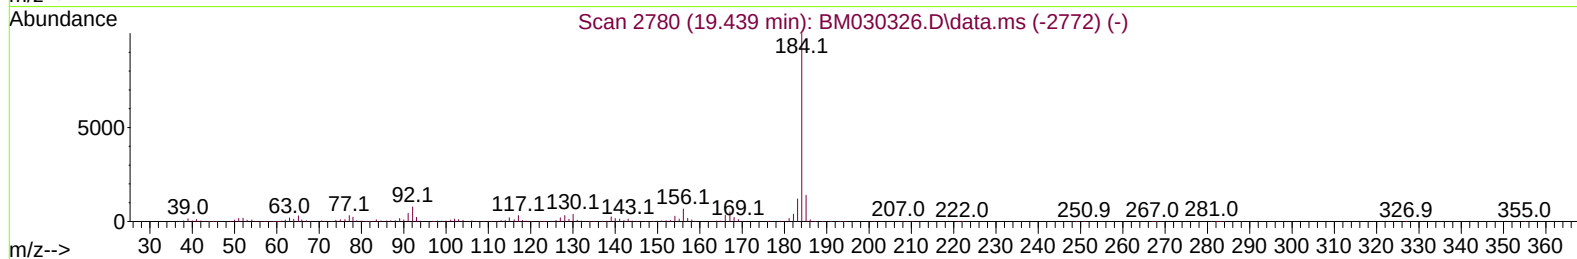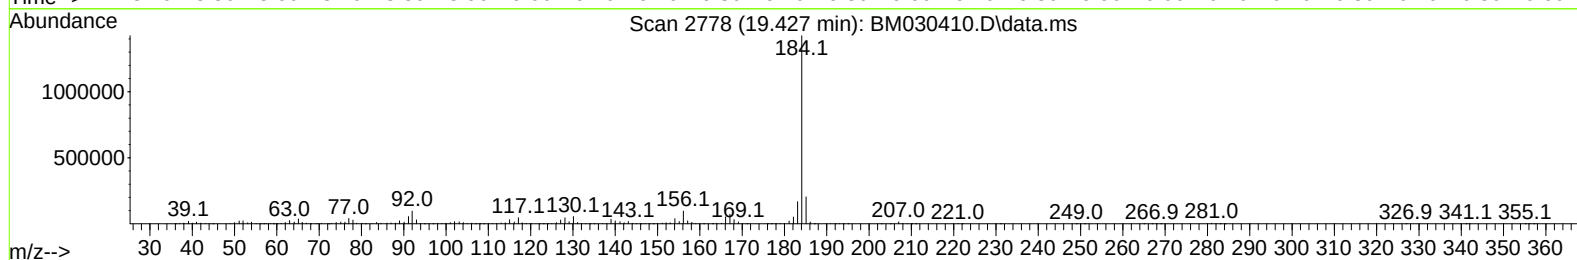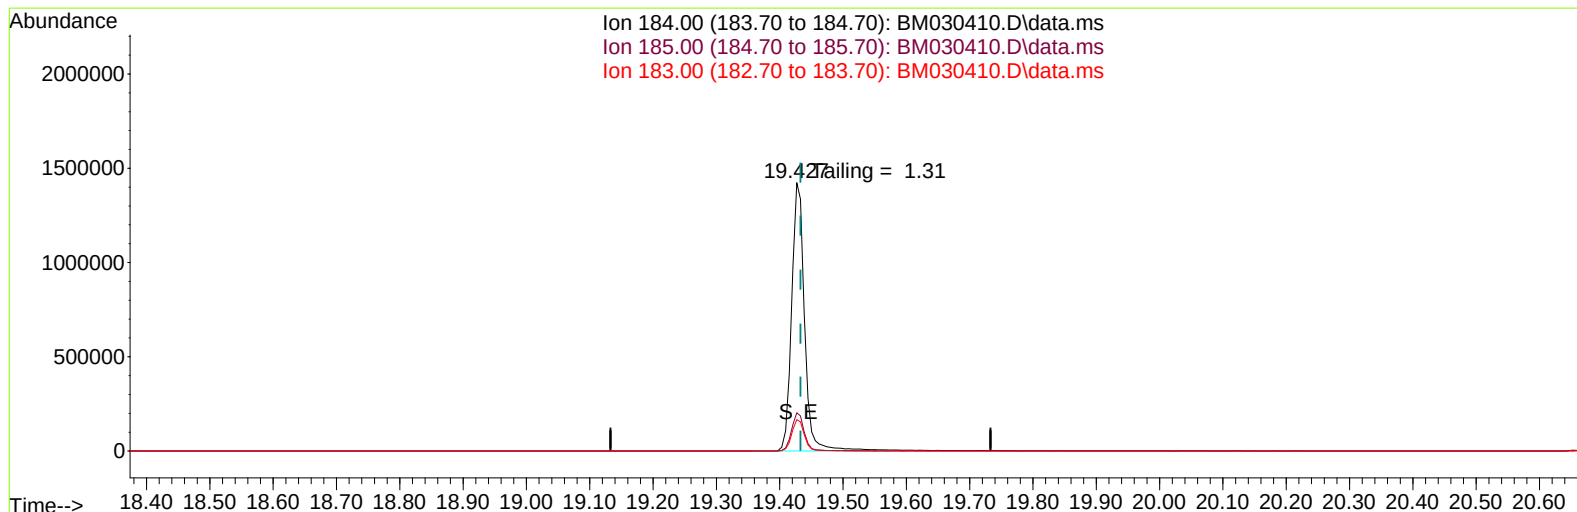

TIC: BM030410.D\data.ms

(77) Benzidine**19.427min (-0.006) 74678.94 ng****response 2038818**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.29
183.00	12.30	11.74
0.00	0.00	0.00