


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061221\
 Data File : BM030410.D
 Acq On : 12 Jun 2021 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 14:10:50 2021

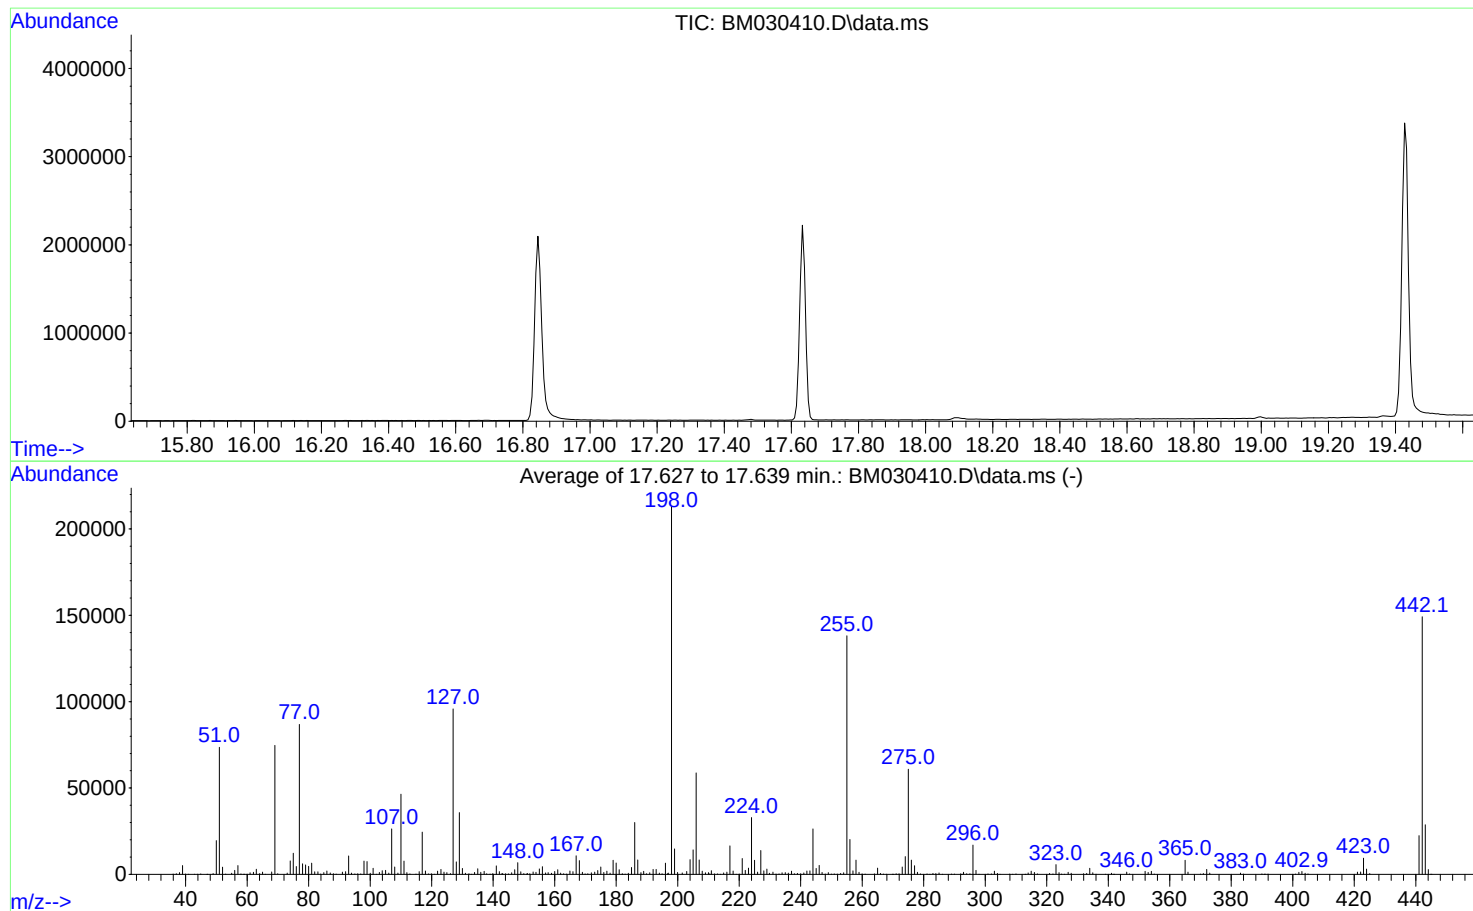




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	73583	PASS
68	69	0.00	2	1.9	1417	PASS
69	198	0.00	100	35.1	74688	PASS
70	69	0.00	2	0.5	355	PASS
127	198	10	80	45.0	95848	PASS
197	198	0.00	2	0.4	784	PASS
198	198	100	100	100.0	213013	PASS
199	198	5	9	6.9	14740	PASS
275	198	10	60	28.6	60893	PASS
365	198	1	100	3.8	8168	PASS
441	198	0.01	100	10.5	22454	PASS
442	442	50	100	100.0	149208	PASS
443	442	15	24	19.2	28712	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061221\
Data File : BM030410.D
Acq On : 12 Jun 2021 12:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 03:59:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 14:10:50 2021
Response via : Initial Calibration

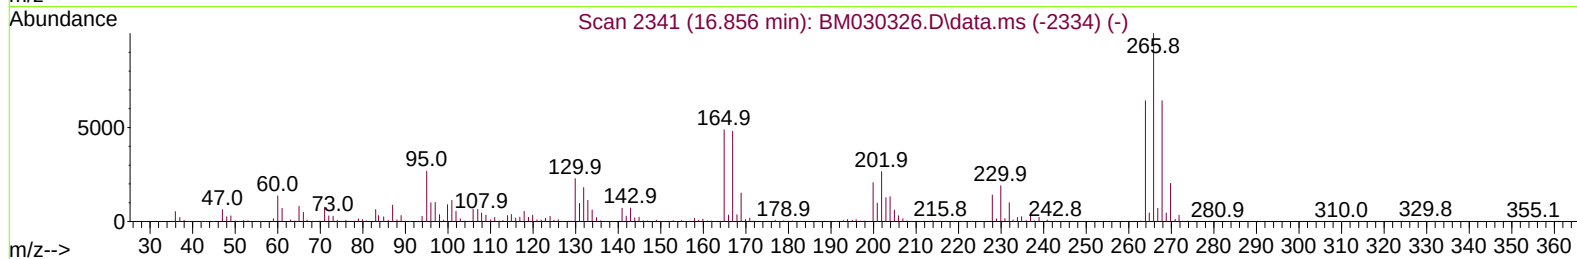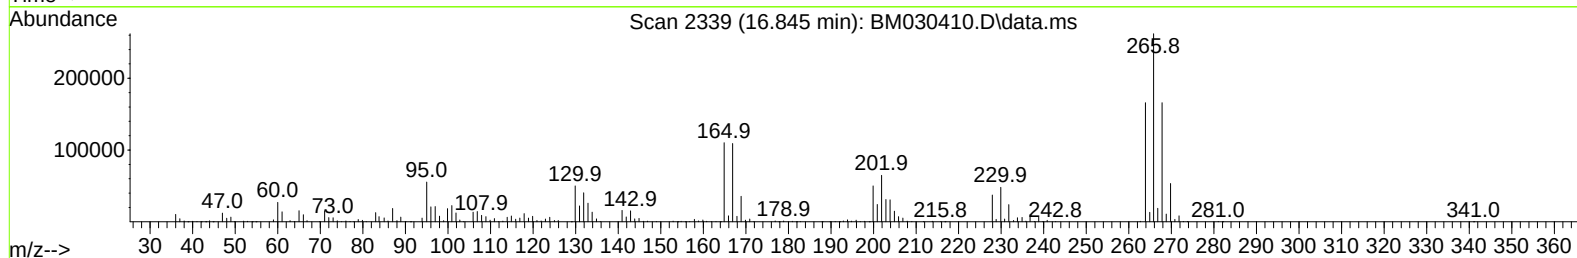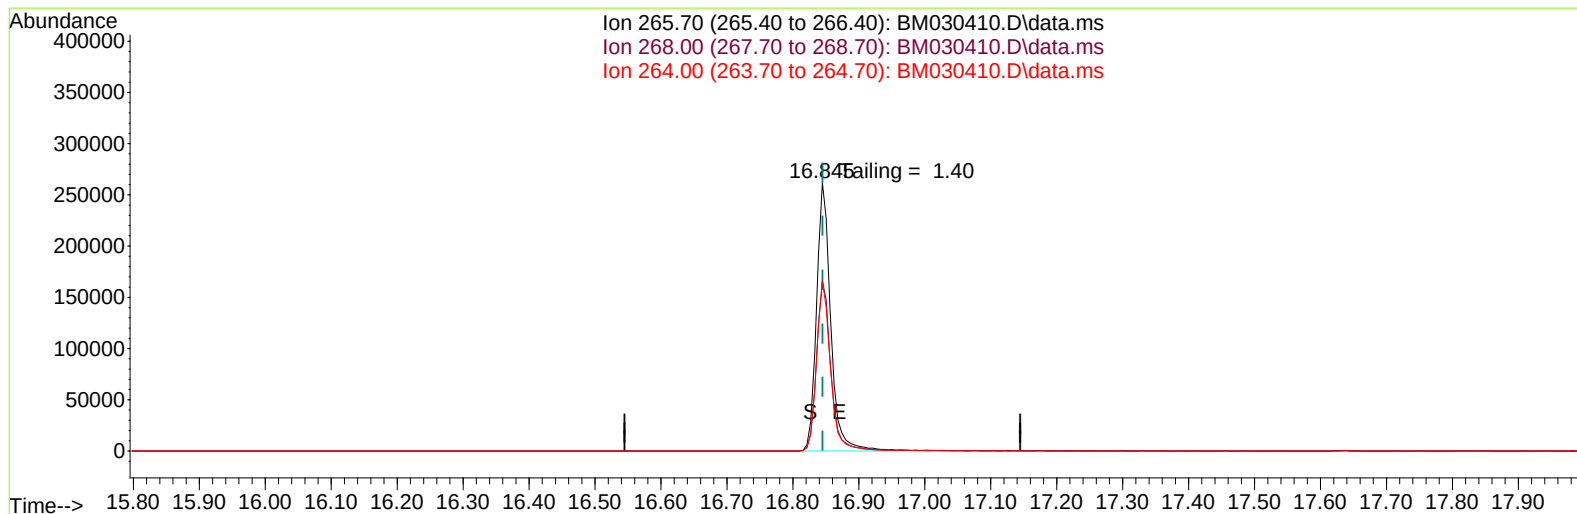

TIC: BM030410.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.000) 248205.10 ng




response 395437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	63.33
264.00	64.90	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061221\
Data File : BM030410.D
Acq On : 12 Jun 2021 12:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 03:59:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 14:10:50 2021
Response via : Initial Calibration

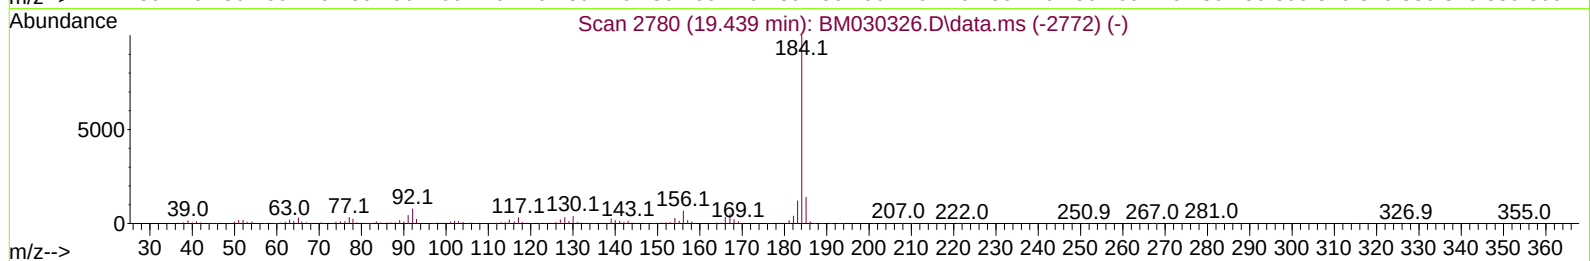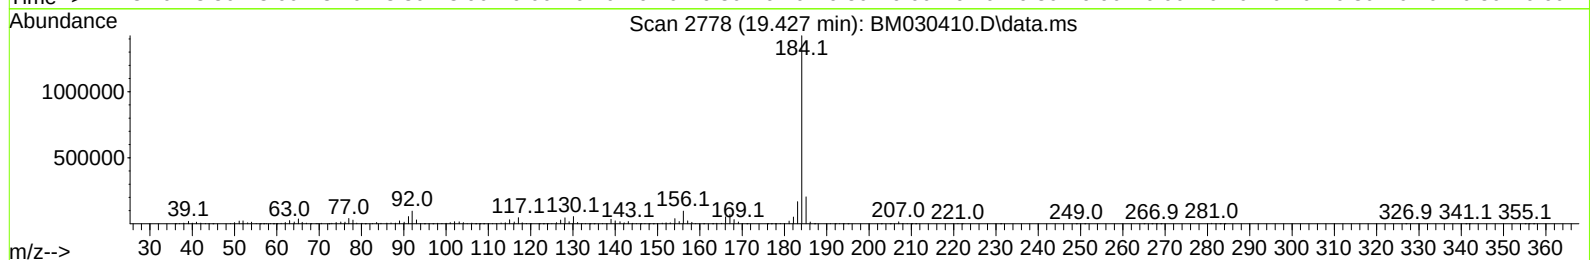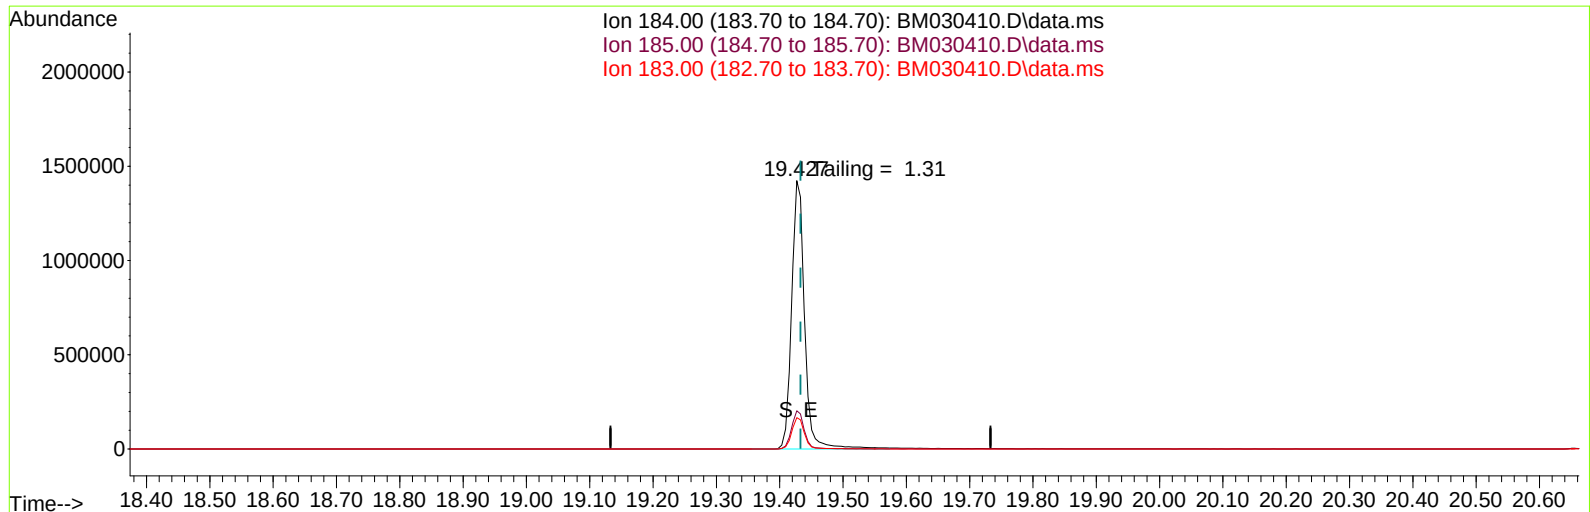

TIC: BM030410.D\data.ms

(77) Benzidine

19.427min (-0.006) 74678.94 ng

response 2038818

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.29
183.00	12.30	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/12/2021	BNA_M	<u>BM030410.D</u>
Compound Name	Response	Retention Time
DDT	985701	20.656
DDD	14009	20.221
DDE	2167	19.715
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16176	1001877	1.61

Instrument :
BNA_M
ClientSampleId :
DFTPP