
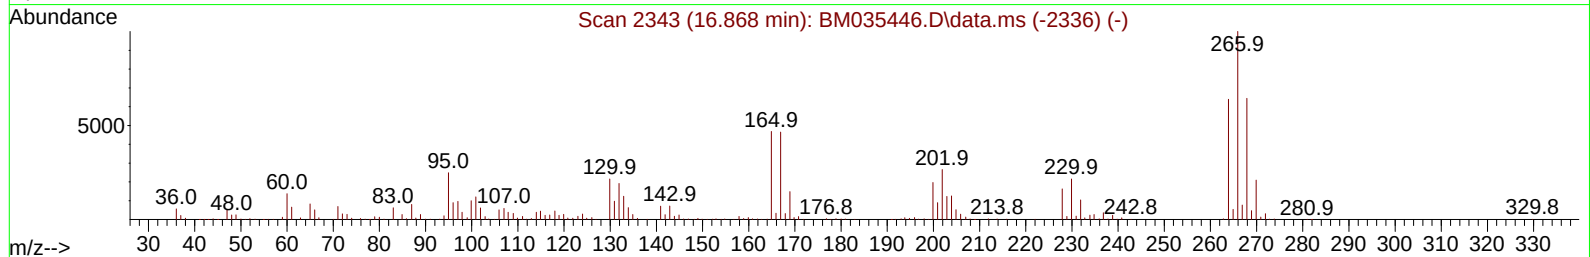
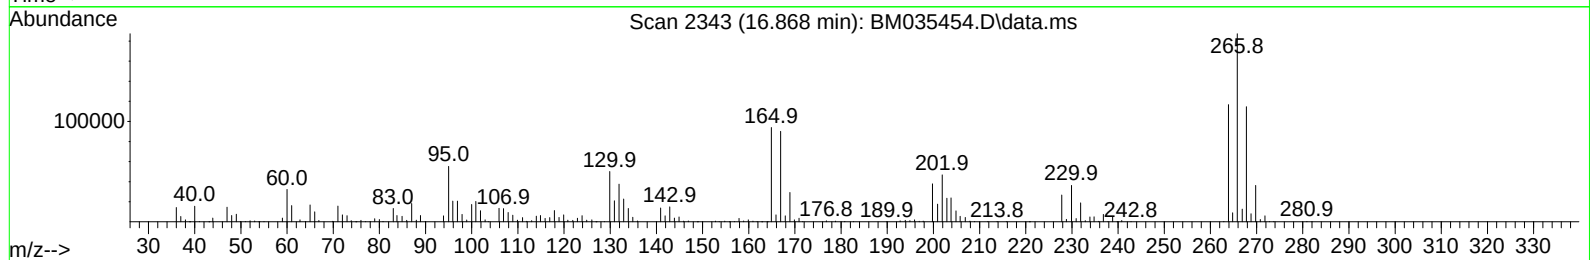


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061322\
 Data File : BM035454.D
 Acq On : 13 Jun 2022 12:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 05:10:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 16:05:33 2022
 Response via : Initial Calibration

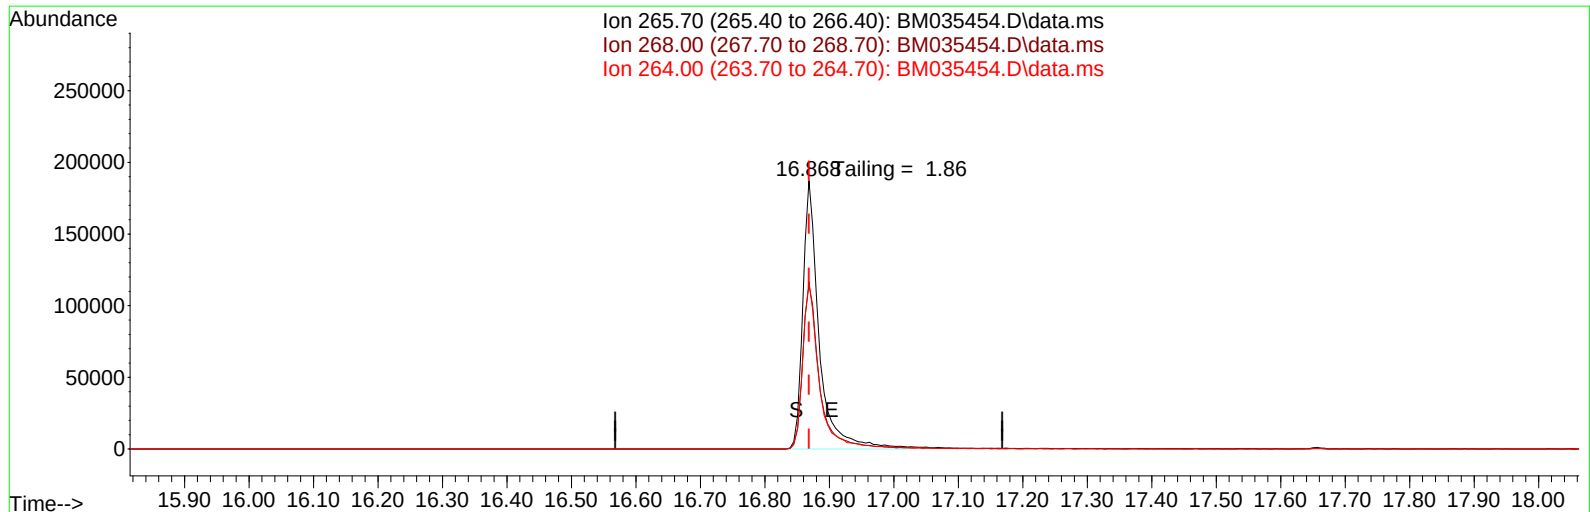

TIC: BM035454.D\data.ms

(70) Pentachlorophenol (C)

16.868min (+ 0.000) 0.00 ng

response 334983

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	61.27
264.00	63.30	62.32
0.00	0.00	0.00

