


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061322\
 Data File : BM035454.D
 Acq On : 13 Jun 2022 12:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 10 16:05:33 2022

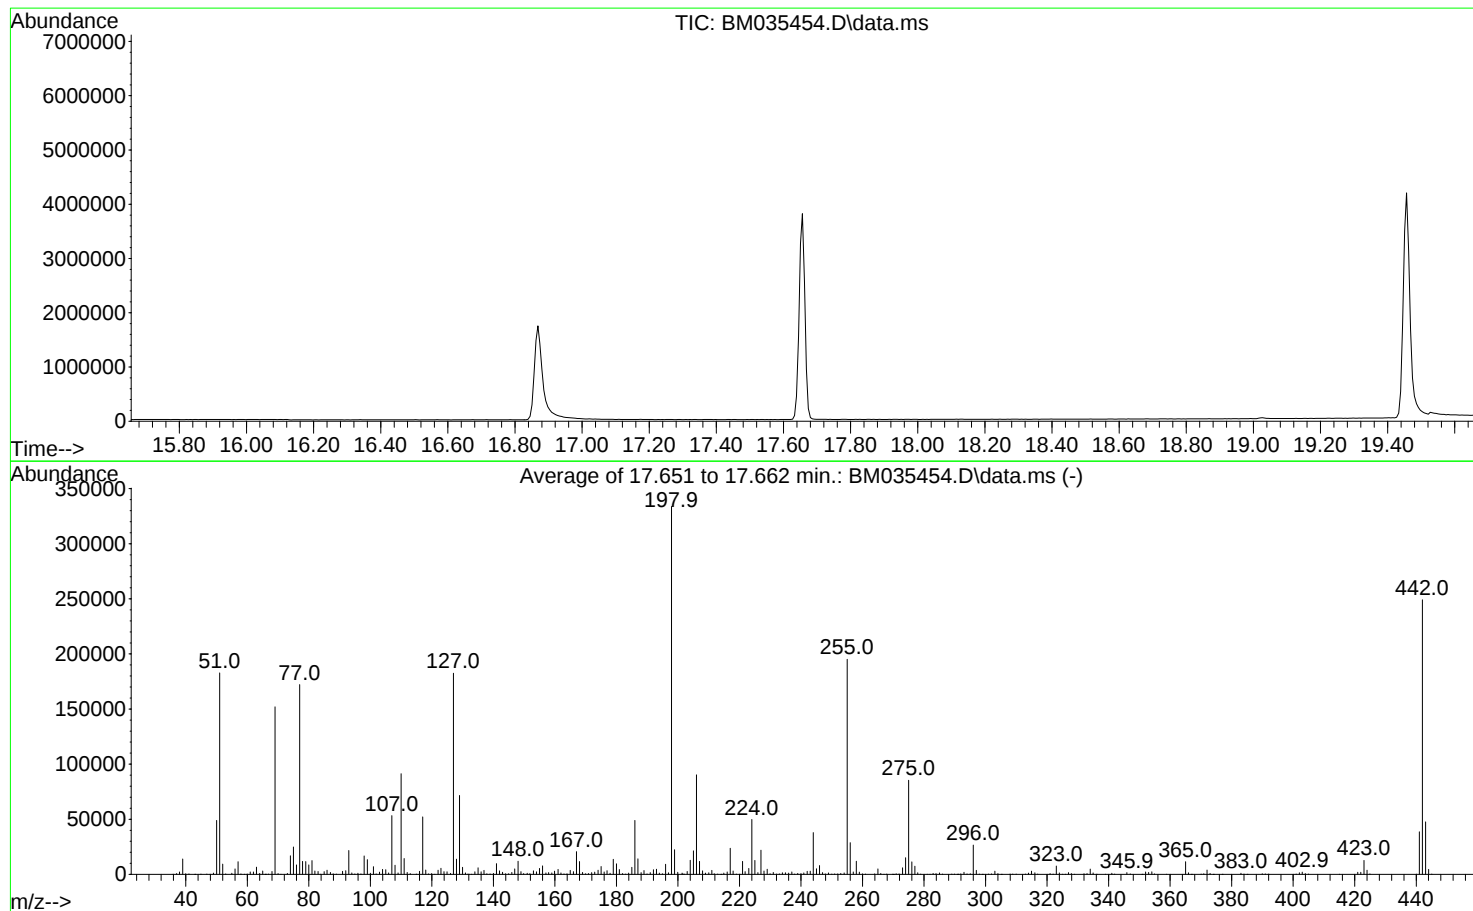




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	182797	PASS
68	69	0.00	2	1.7	2567	PASS
69	198	0.00	100	45.5	151995	PASS
70	69	0.00	2	0.5	734	PASS
127	198	10	80	54.7	182571	PASS
197	198	0.00	2	0.4	1405	PASS
198	198	100	100	100.0	333781	PASS
199	198	5	9	6.7	22400	PASS
275	198	10	60	25.6	85437	PASS
365	198	1	100	3.5	11516	PASS
441	198	0.01	100	11.6	38629	PASS
442	442	50	100	100.0	249152	PASS
443	442	15	24	19.1	47637	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061322\  
Data File : BM035454.D  
Acq On    : 13 Jun 2022  12:14  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 05:10:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 16:05:33 2022
Response via : Initial Calibration

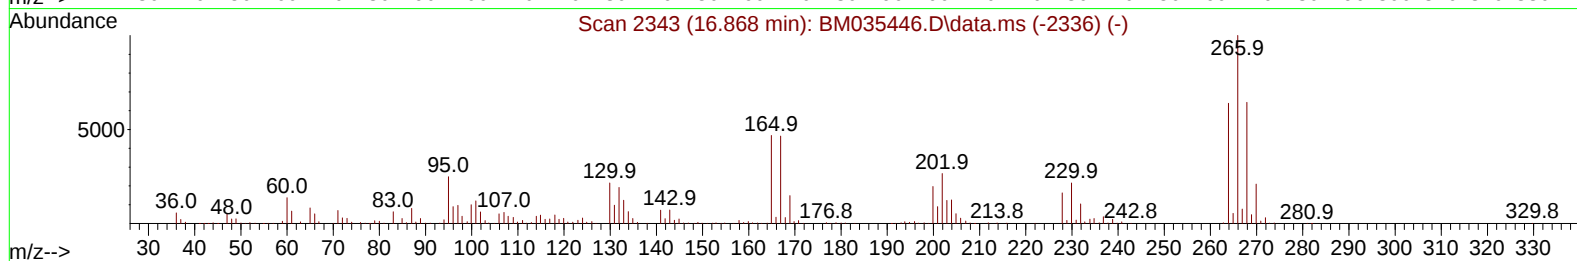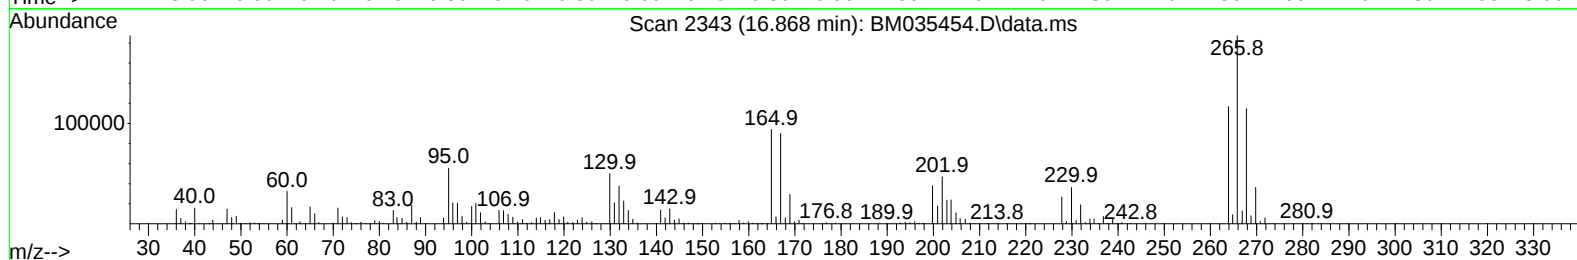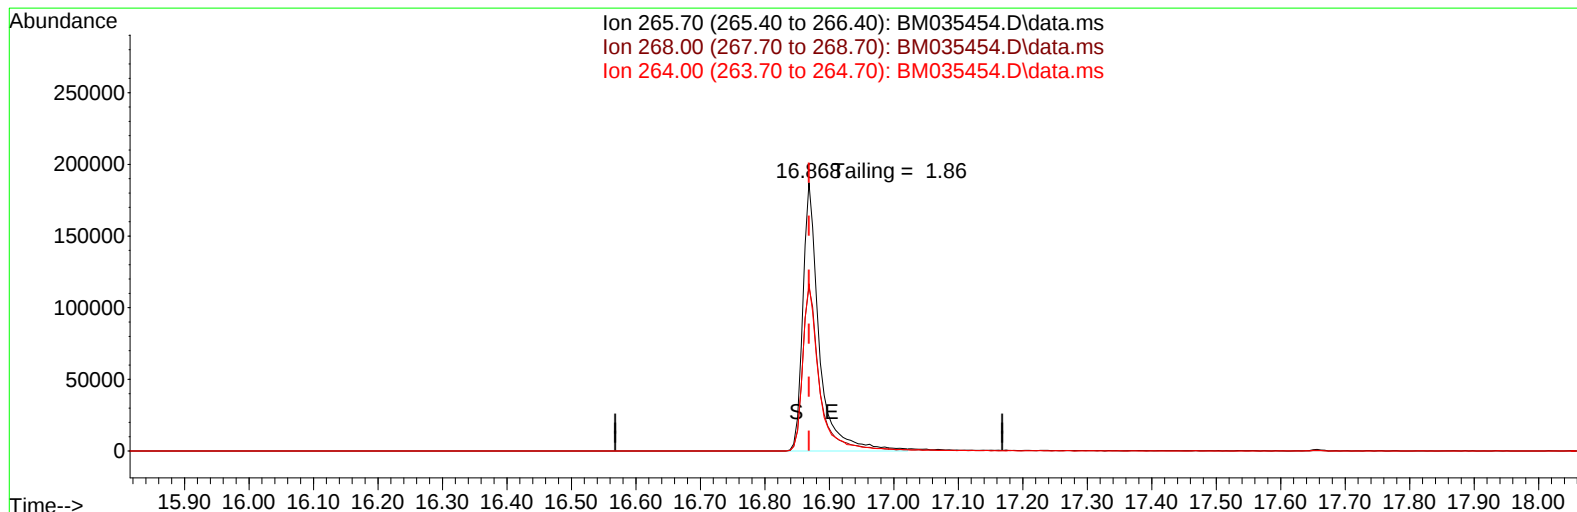

TIC: BM035454.D\data.ms

(70) Pentachlorophenol (C)

16.868min (+ 0.000) 0.00 ng




response **334983**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	61.27
264.00	63.30	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061322\
Data File : BM035454.D
Acq On : 13 Jun 2022 12:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 14 05:10:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 16:05:33 2022
Response via : Initial Calibration

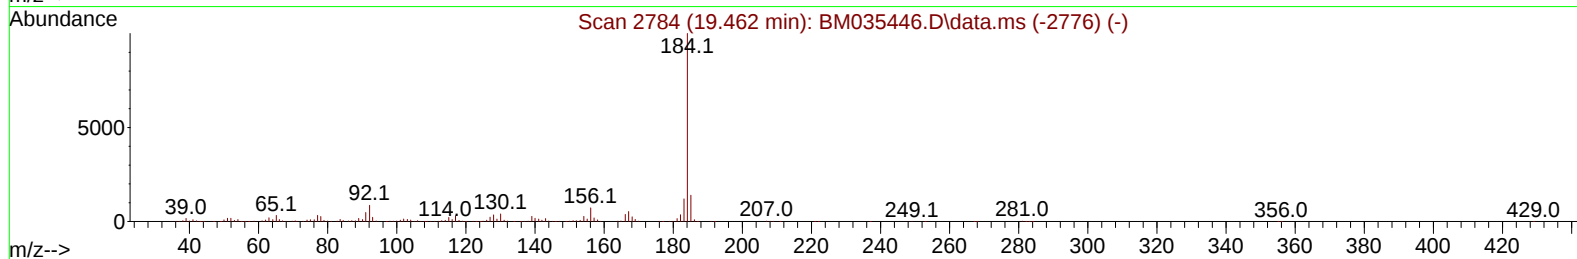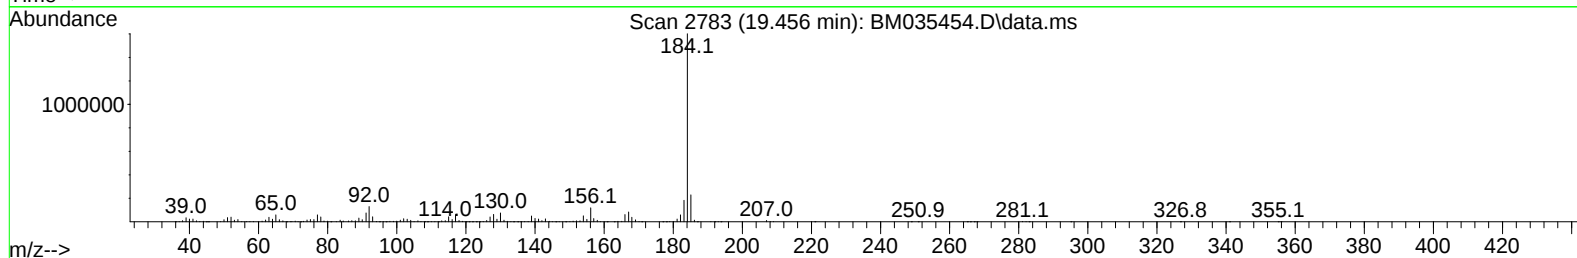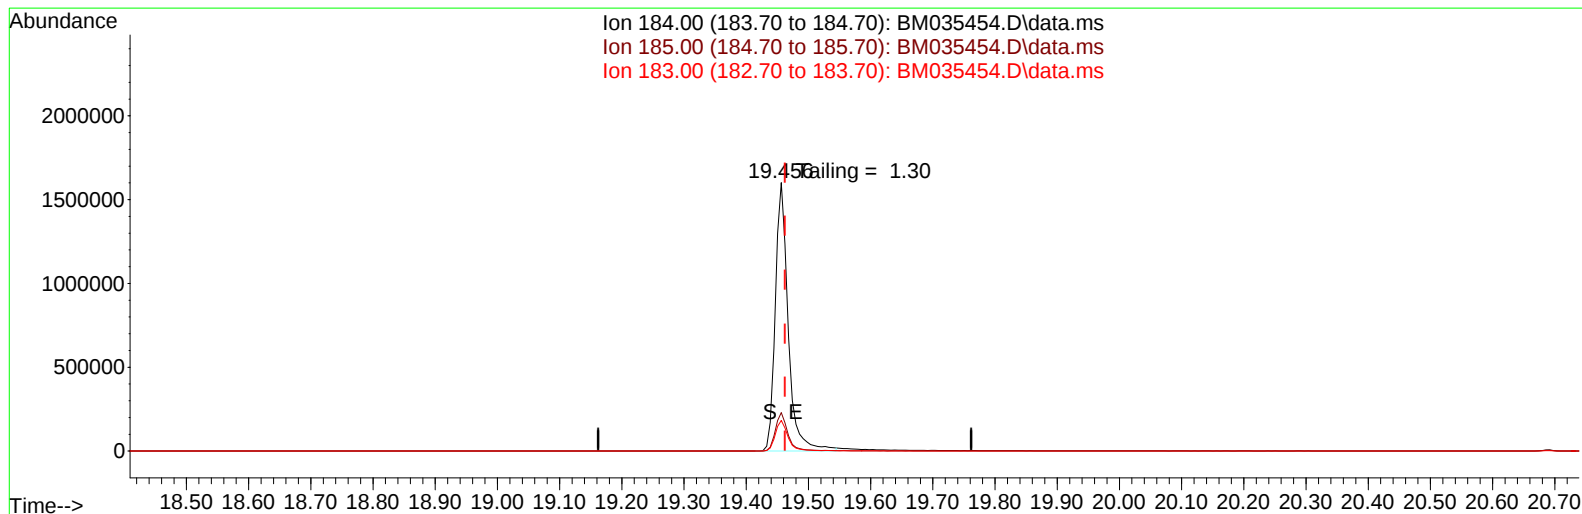

TIC: BM035454.D\data.ms

(77) Benzidine

19.456min (-0.006) 0.00 ng

response 2379658

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.35
183.00	11.90	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/13/2022	BNA_M	<u>BM035454.D</u>
Compound Name	Response	Retention Time
DDT	1529685	20.692
DDD	14945	20.256
DDE	4697	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19642	1549327	1.27

Instrument :
BNA_M
ClientSampleId :
DFTPP