
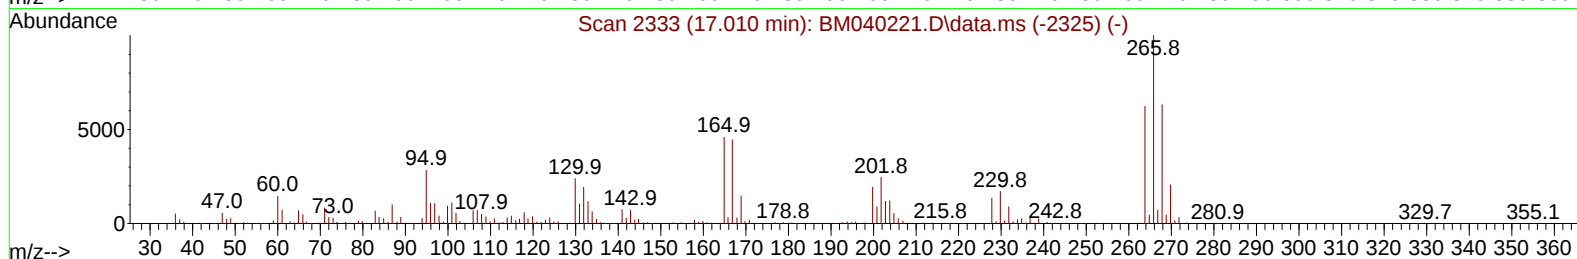
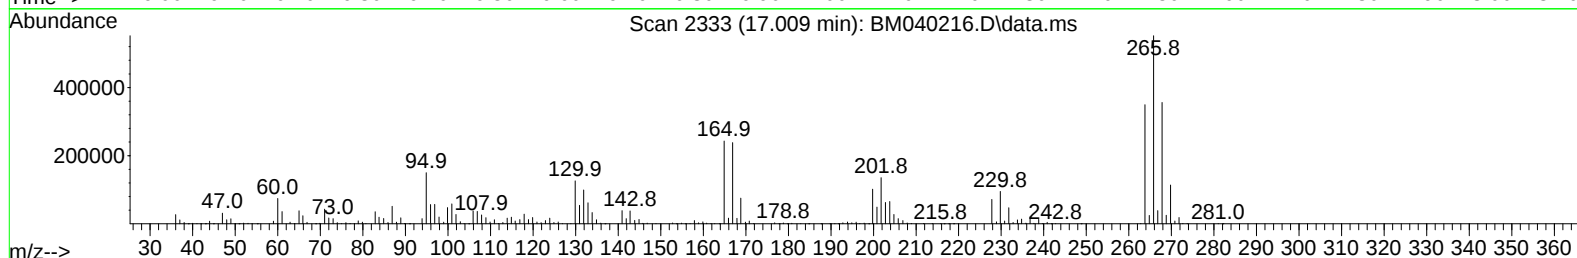


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061323\
Data File : BM040216.D
Acq On : 13 Jun 2023 09:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 14:31:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 14:16:59 2023
Response via : Initial Calibration

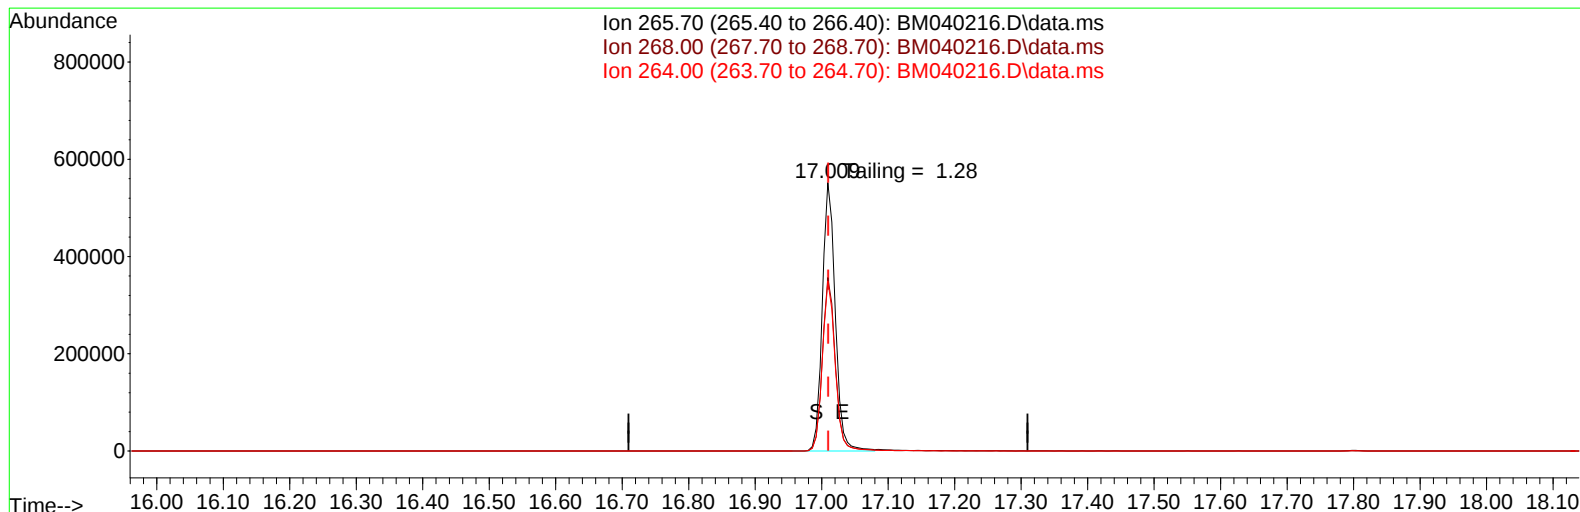

TIC: BM040216.D\data.ms

(70) Pentachlorophenol (C)




17.009min (-0.000) 0.00 ng

response 756091

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.56
264.00	62.30	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061323\
Data File : BM040216.D
Acq On : 13 Jun 2023 09:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 14:31:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 14:16:59 2023
Response via : Initial Calibration

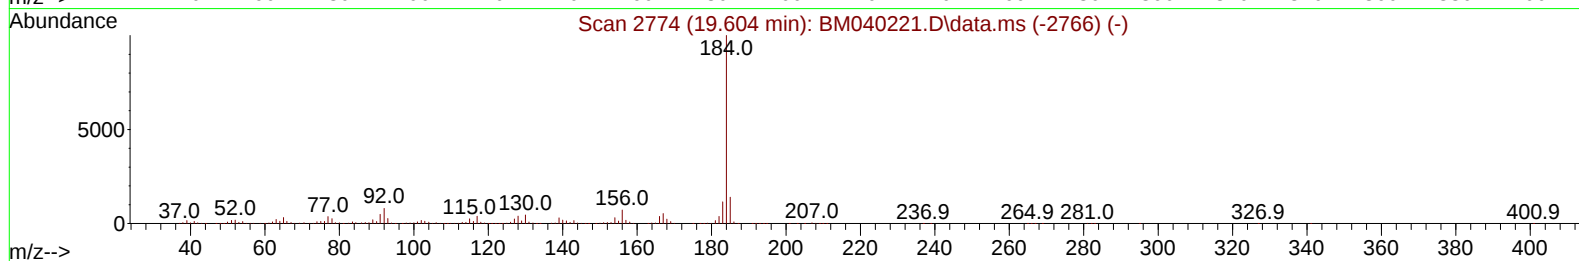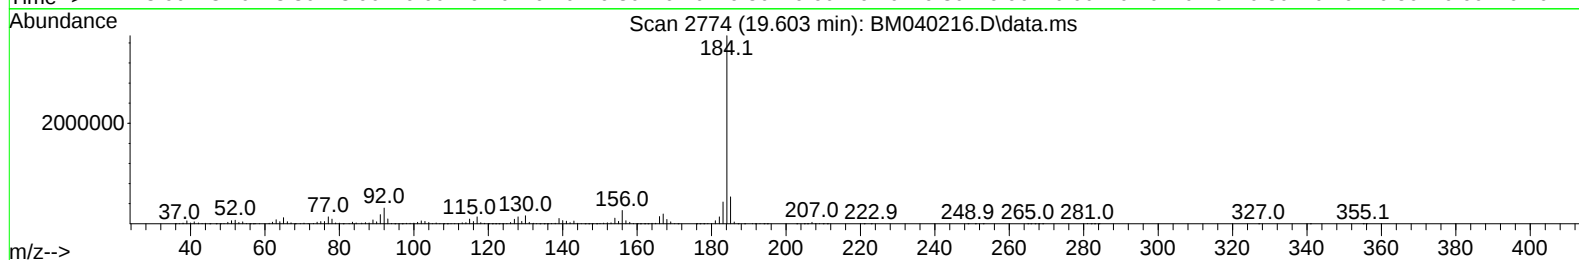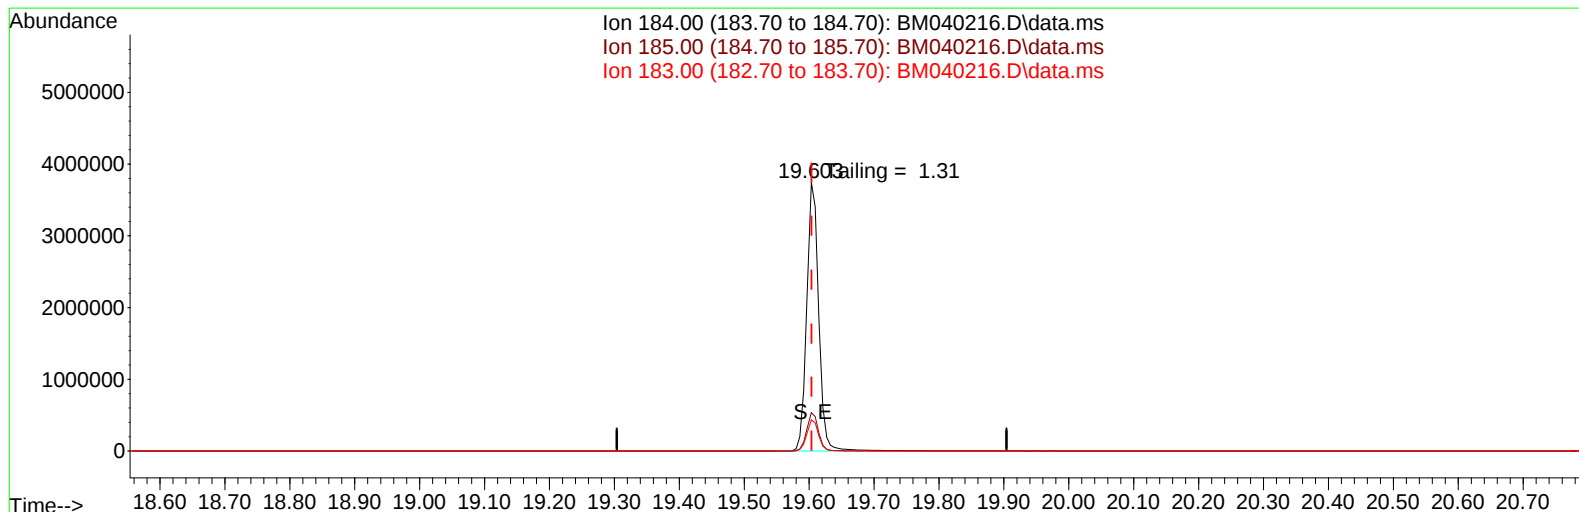

TIC: BM040216.D\data.ms

(77) Benzidine**19.603min (-0.000) 395987.96 ng****response 4789301**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.33
183.00	11.50	11.62
0.00	0.00	0.00