
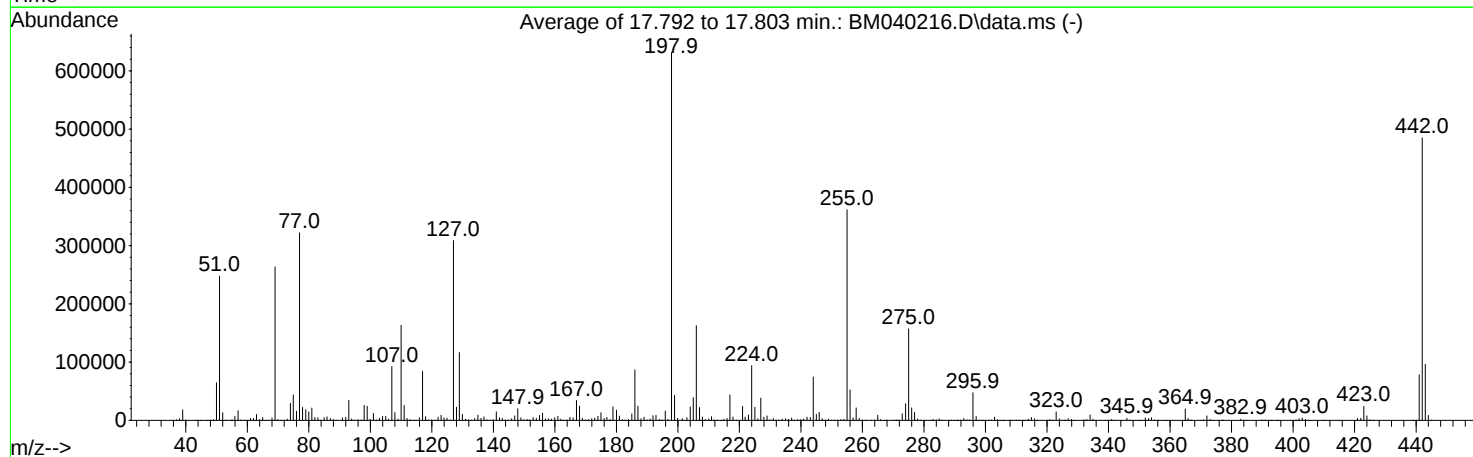


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061323\
 Data File : BM040216.D
 Acq On : 13 Jun 2023 09:21
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 13 22:36:11 2023

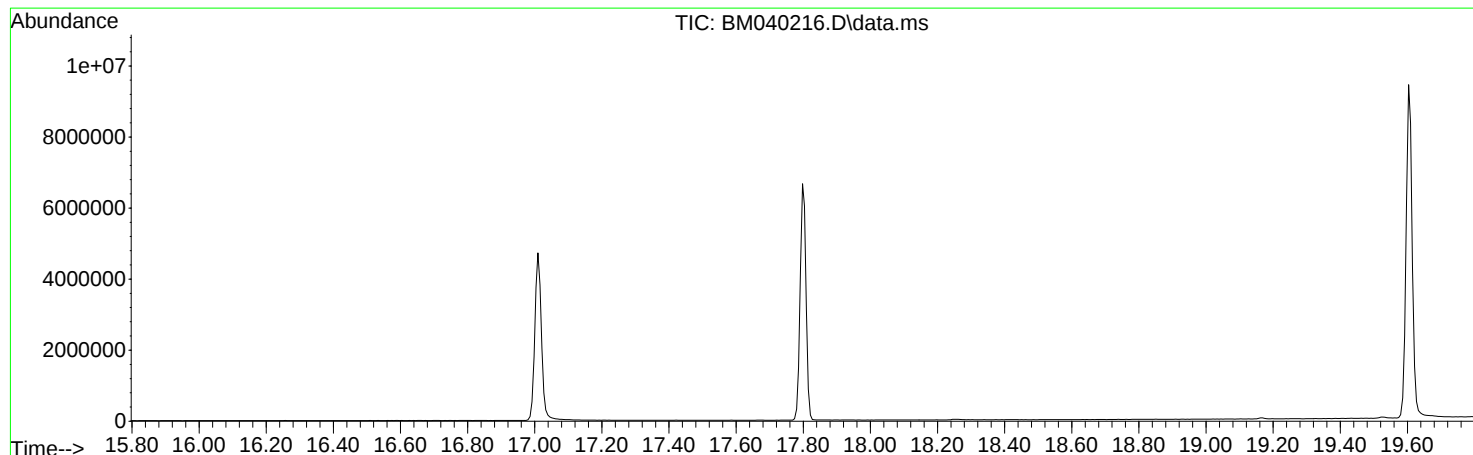

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	247949	PASS
68	69	0.00	2	1.6	4201	PASS
69	198	0.00	100	41.7	263488	PASS
70	69	0.00	2	0.5	1325	PASS
127	198	10	80	48.9	308907	PASS
197	198	0.00	2	0.3	1792	PASS
198	198	100	100	100.0	631595	PASS
199	198	5	9	6.8	42939	PASS
275	198	10	60	24.9	157189	PASS
365	198	1	100	3.1	19679	PASS
441	198	0.01	100	12.4	78227	PASS
442	442	50	100	100.0	484885	PASS
443	442	15	24	19.9	96448	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2023	BNA_M	<u>BM040216.D</u>
Compound Name	Response	Retention Time
DDT	2239416	20.839
DDD	22679	20.45
DDE	931	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23610	2263026	1.04

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061323\
Data File : BM040216.D
Acq On : 13 Jun 2023 09:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 13 14:31:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 14:16:59 2023
Response via : Initial Calibration

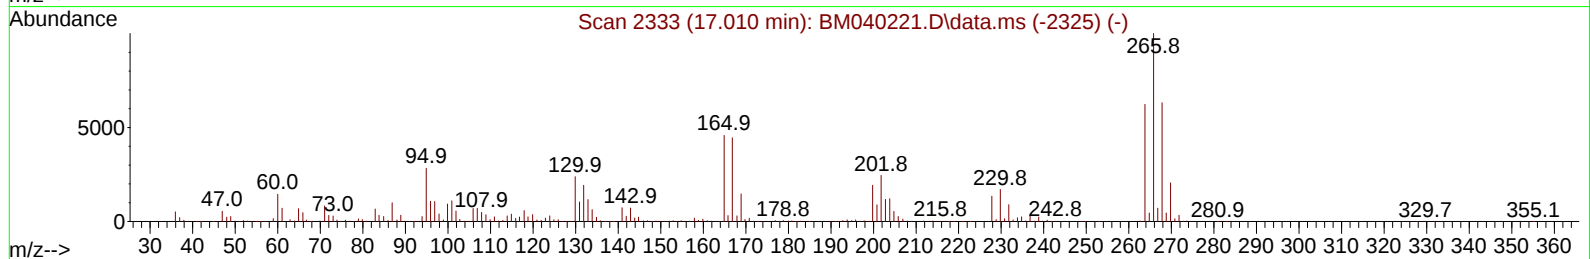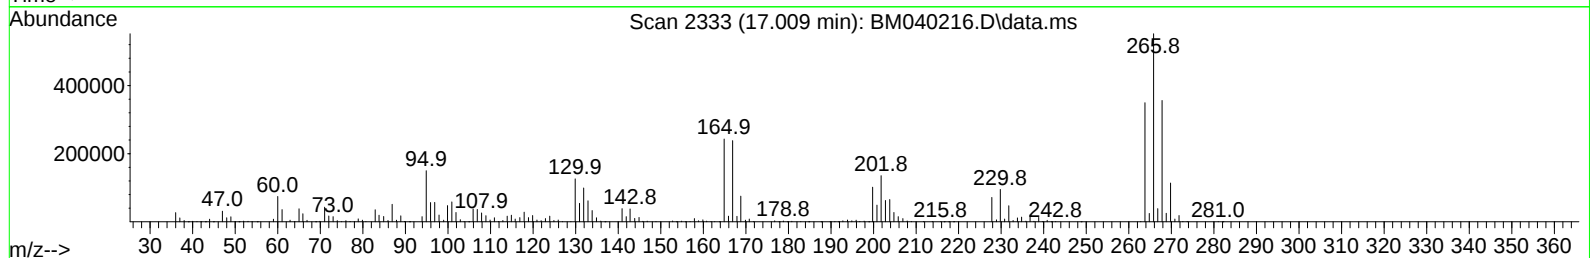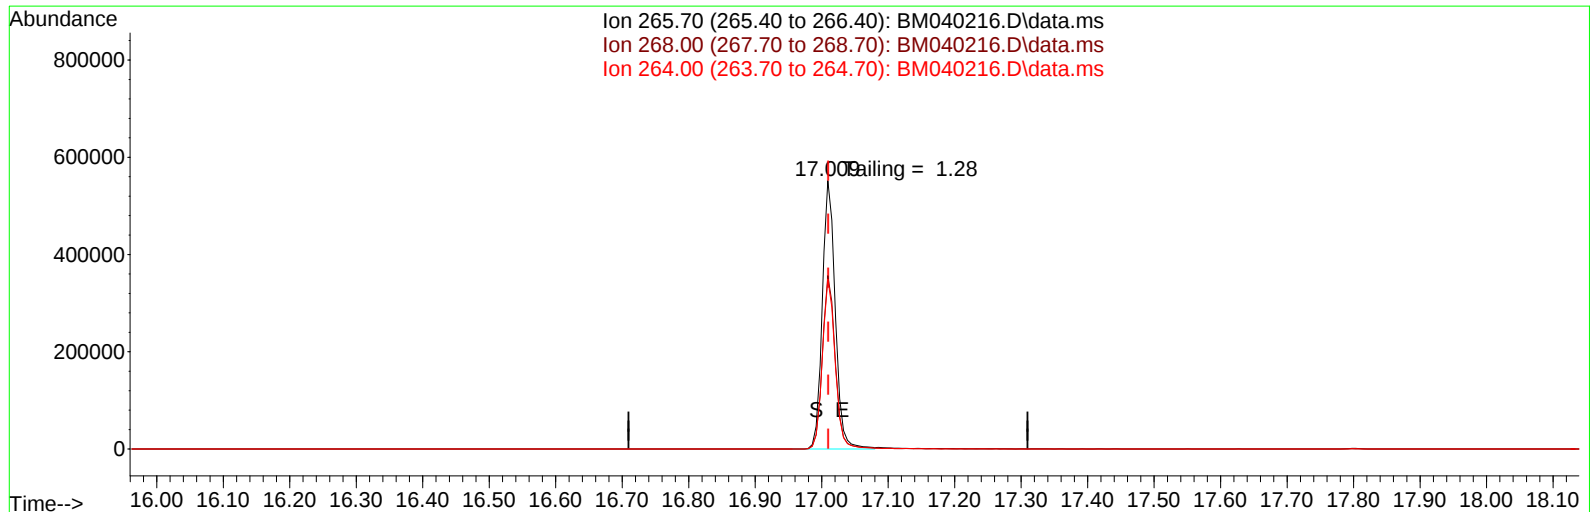

TIC: BM040216.D\data.ms

(70) Pentachlorophenol (C)

17.009min (-0.000) 0.00 ng




response 756091

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.56
264.00	62.30	63.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061323\
 Data File : BM040216.D
 Acq On : 13 Jun 2023 09:21
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 13 14:31:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 13 14:16:59 2023
 Response via : Initial Calibration

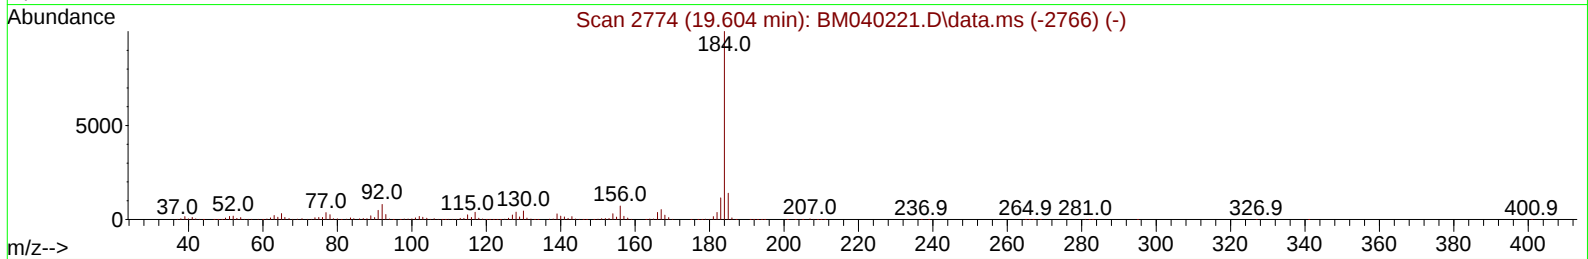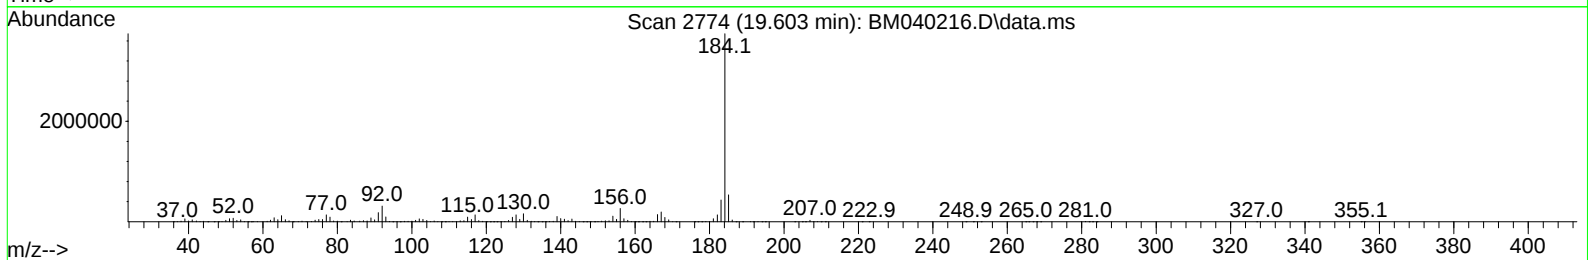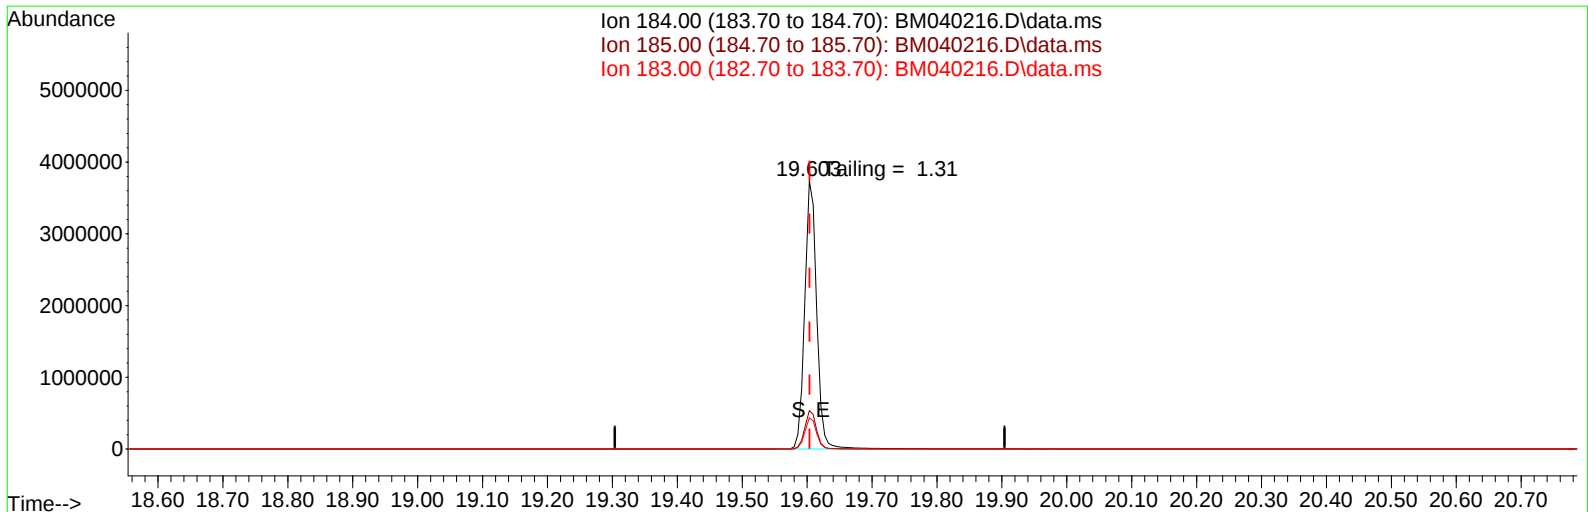

TIC: BM040216.D\data.ms

(77) Benzidine**19.603min (-0.000) 395987.96 ng****response 4789301**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.33
183.00	11.50	11.62
0.00	0.00	0.00