

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061423\
 Data File : BM040242.D
 Acq On : 14 Jun 2023 18:13
 Operator : MA/JU
 Sample : PB153389BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK389

Quant Time: Jun 15 00:51:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 15 00:31:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.974	152	11268	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	40357	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.610	164	21997	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	39940	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	26066	0.400	ng/ul	0.00
23) Perylene-d12	23.956	264	27407	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.350	96	93292	6.705	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.373	152	18700	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.380	212	29043	0.447	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.604	166	6043	0.082	ng/ul#	14
20) Pyrene	19.742	202	5448	0.059	ng/ul#	1
26) Benzo(a)pyrene	23.801	252	9964	0.120	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061423\
Data File : BM040242.D
Acq On : 14 Jun 2023 18:13
Operator : MA/JU
Sample : PB153389BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Quant Time: Jun 15 00:51:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 00:31:16 2023
Response via : Initial Calibration




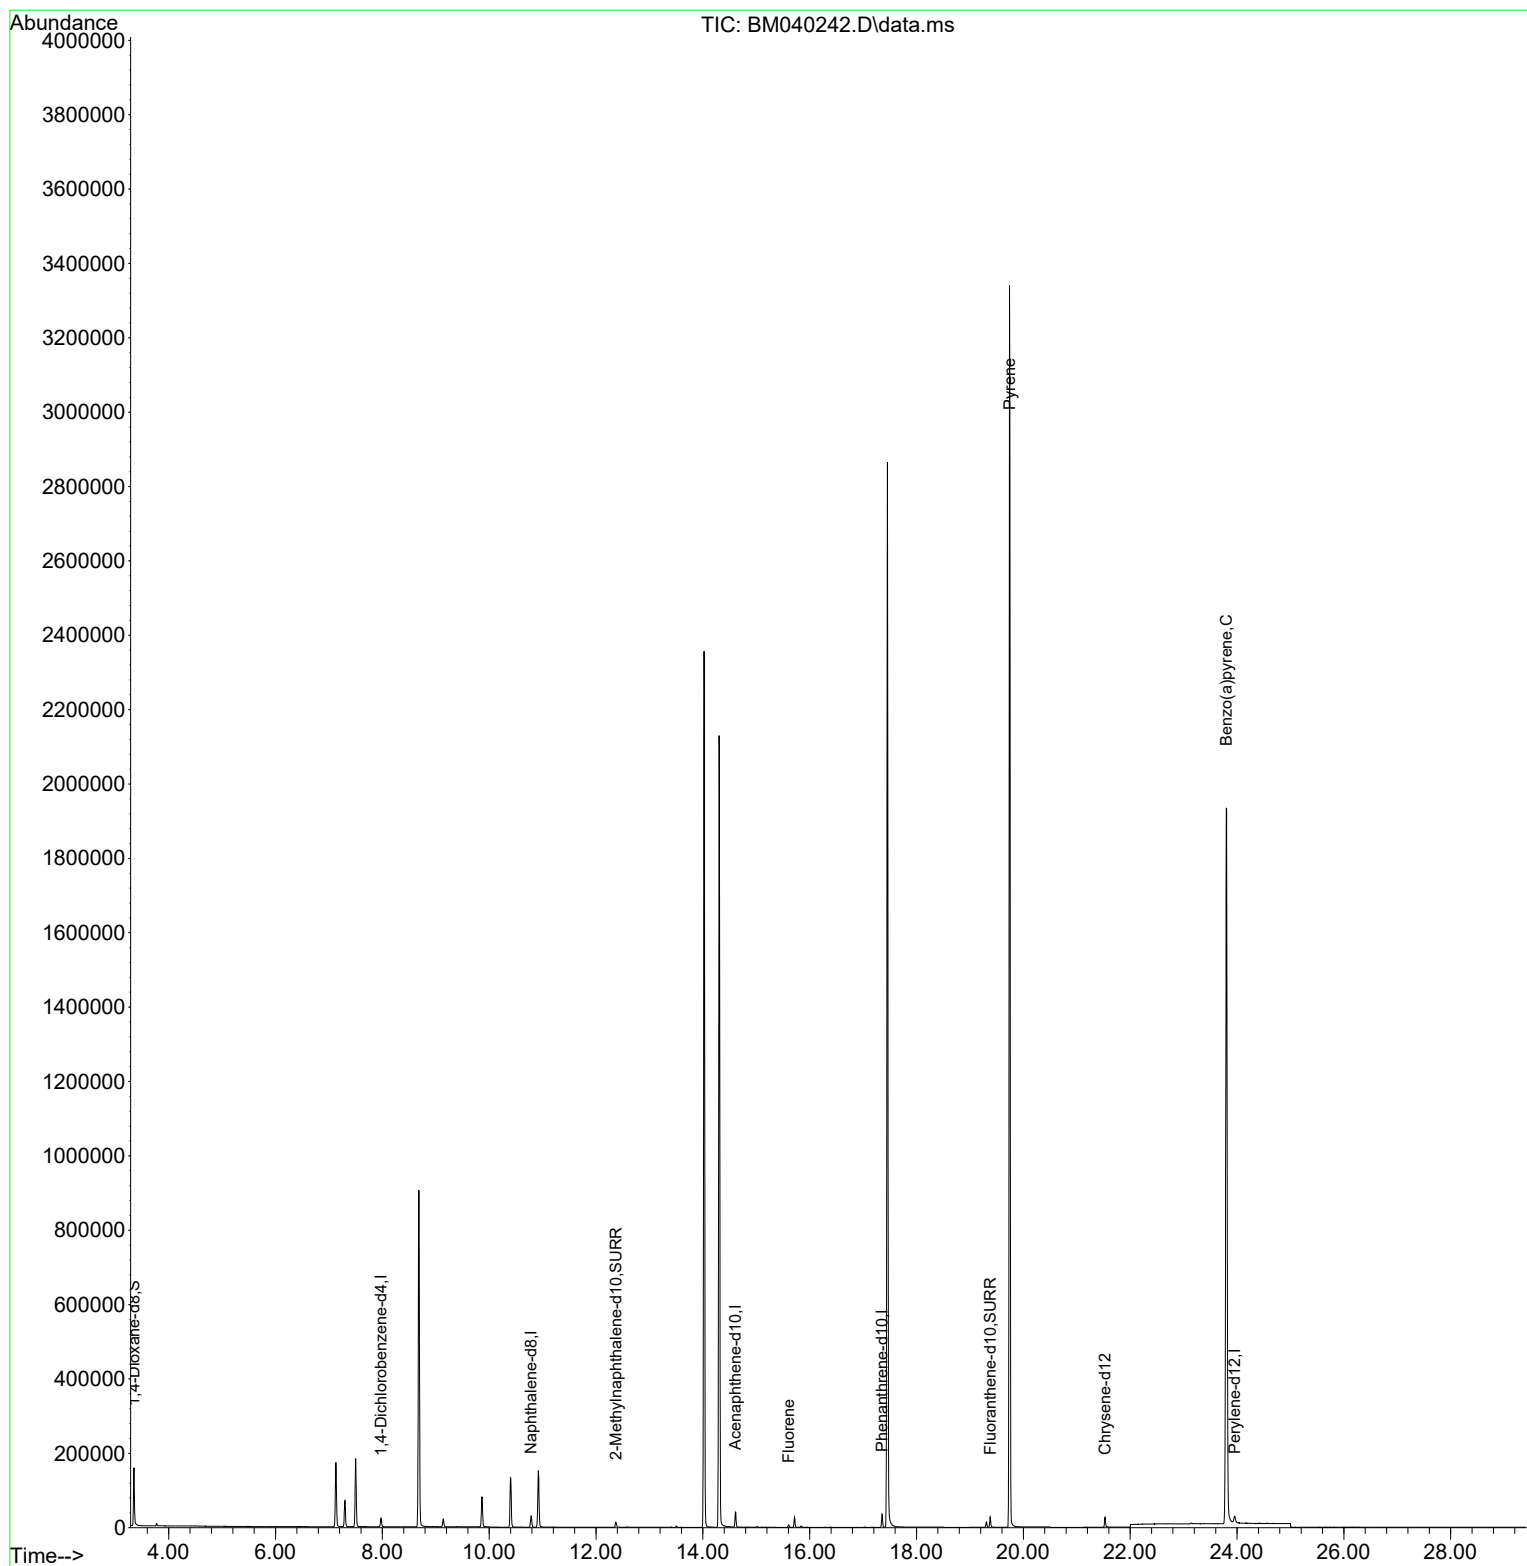


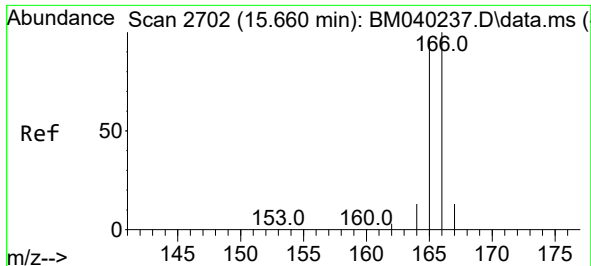

#12
Fluorene
Concen: 0.082 ng/ul
RT: 15.604 min Scan# 2
Delta R.T. -0.055 min
Lab File: BM040242.D
Acq: 14 Jun 2023 18:13




Instrument :
BNA_M
ClientSampleId :
SBLK389


Tgt Ion:166 Resp: 6043
Ion Ratio Lower Upper
166 100
165 6.9 78.2 117.4#
167 31.6 11.0 16.4#

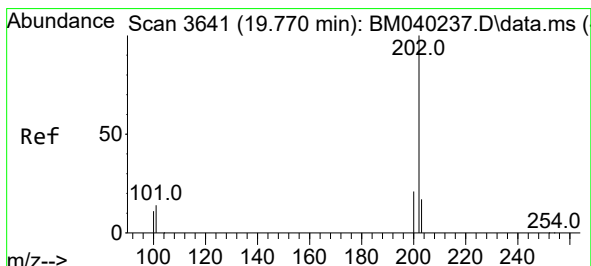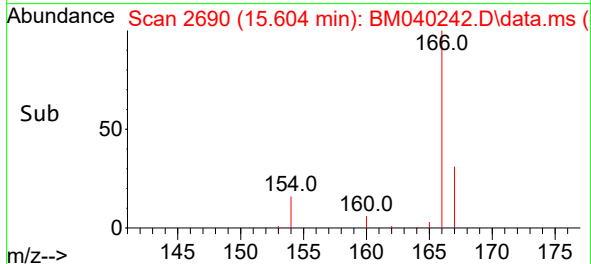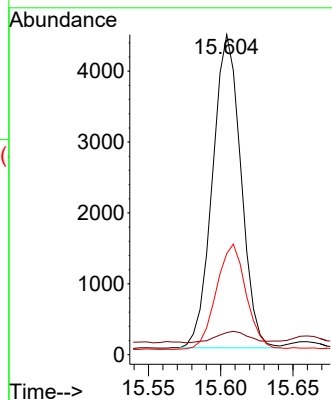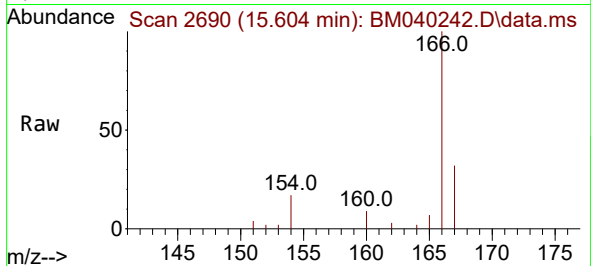

#20
Pyrene
Concen: 0.059 ng/ul
RT: 19.742 min Scan# 3635
Delta R.T. -0.028 min
Lab File: BM040242.D
Acq: 14 Jun 2023 18:13


Tgt Ion:202 Resp: 5448
Ion Ratio Lower Upper
202 100
101 158.8 11.8 17.8#
100 1218.4 9.3 13.9#

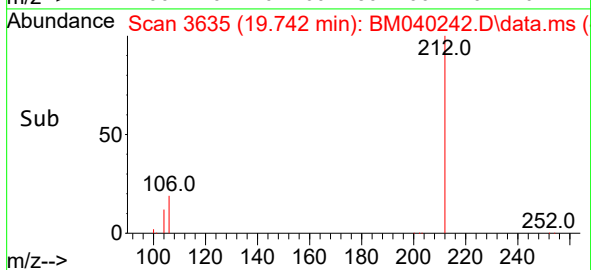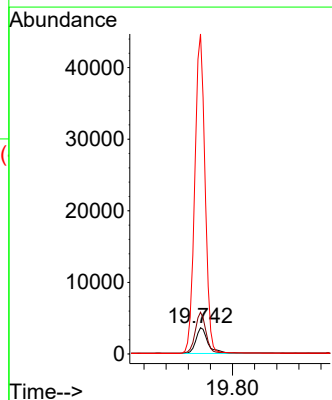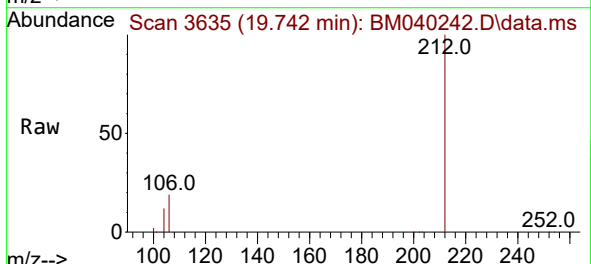

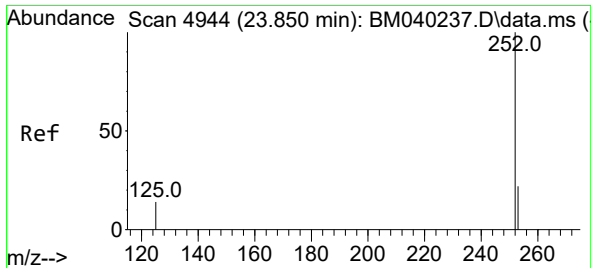

#26
Benzo(a)pyrene
Concen: 0.120 ng/ul
RT: 23.801 min Scan# 4927
Delta R.T. -0.050 min
Lab File: BM040242.D
Acq: 14 Jun 2023 18:13

Instrument :
BNA_M
ClientSampleId :
SBLK389

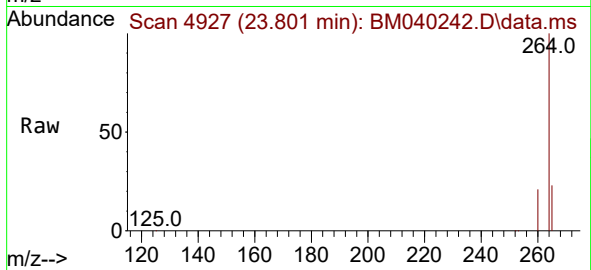

Tgt Ion:252 Resp: 9964
Ion Ratio Lower Upper
252 100
253 48.1 23.4 35.0#
125 44.7 19.7 29.5#

