

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061523\
 Data File : BM040253.D
 Acq On : 15 Jun 2023 09:20
 Operator : MA/JU
 Sample : PB153389BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK389

Quant Time: Jun 15 23:41:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 15 00:31:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.970	152	10341	0.400	ng/ul	0.00
4) Naphthalene-d8	10.784	136	37855	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.610	164	20412	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	37337	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	22052	0.400	ng/ul	0.00
23) Perylene-d12	23.956	264	22174	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	84666	6.630	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.367	152	17533	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	26829	0.488	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.742	202	4957	0.064	ng/ul#	1
26) Benzo(a)pyrene	23.801	252	8240	0.123	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061523\
Data File : BM040253.D
Acq On : 15 Jun 2023 09:20
Operator : MA/JU
Sample : PB153389BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Quant Time: Jun 15 23:41:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 00:31:16 2023
Response via : Initial Calibration

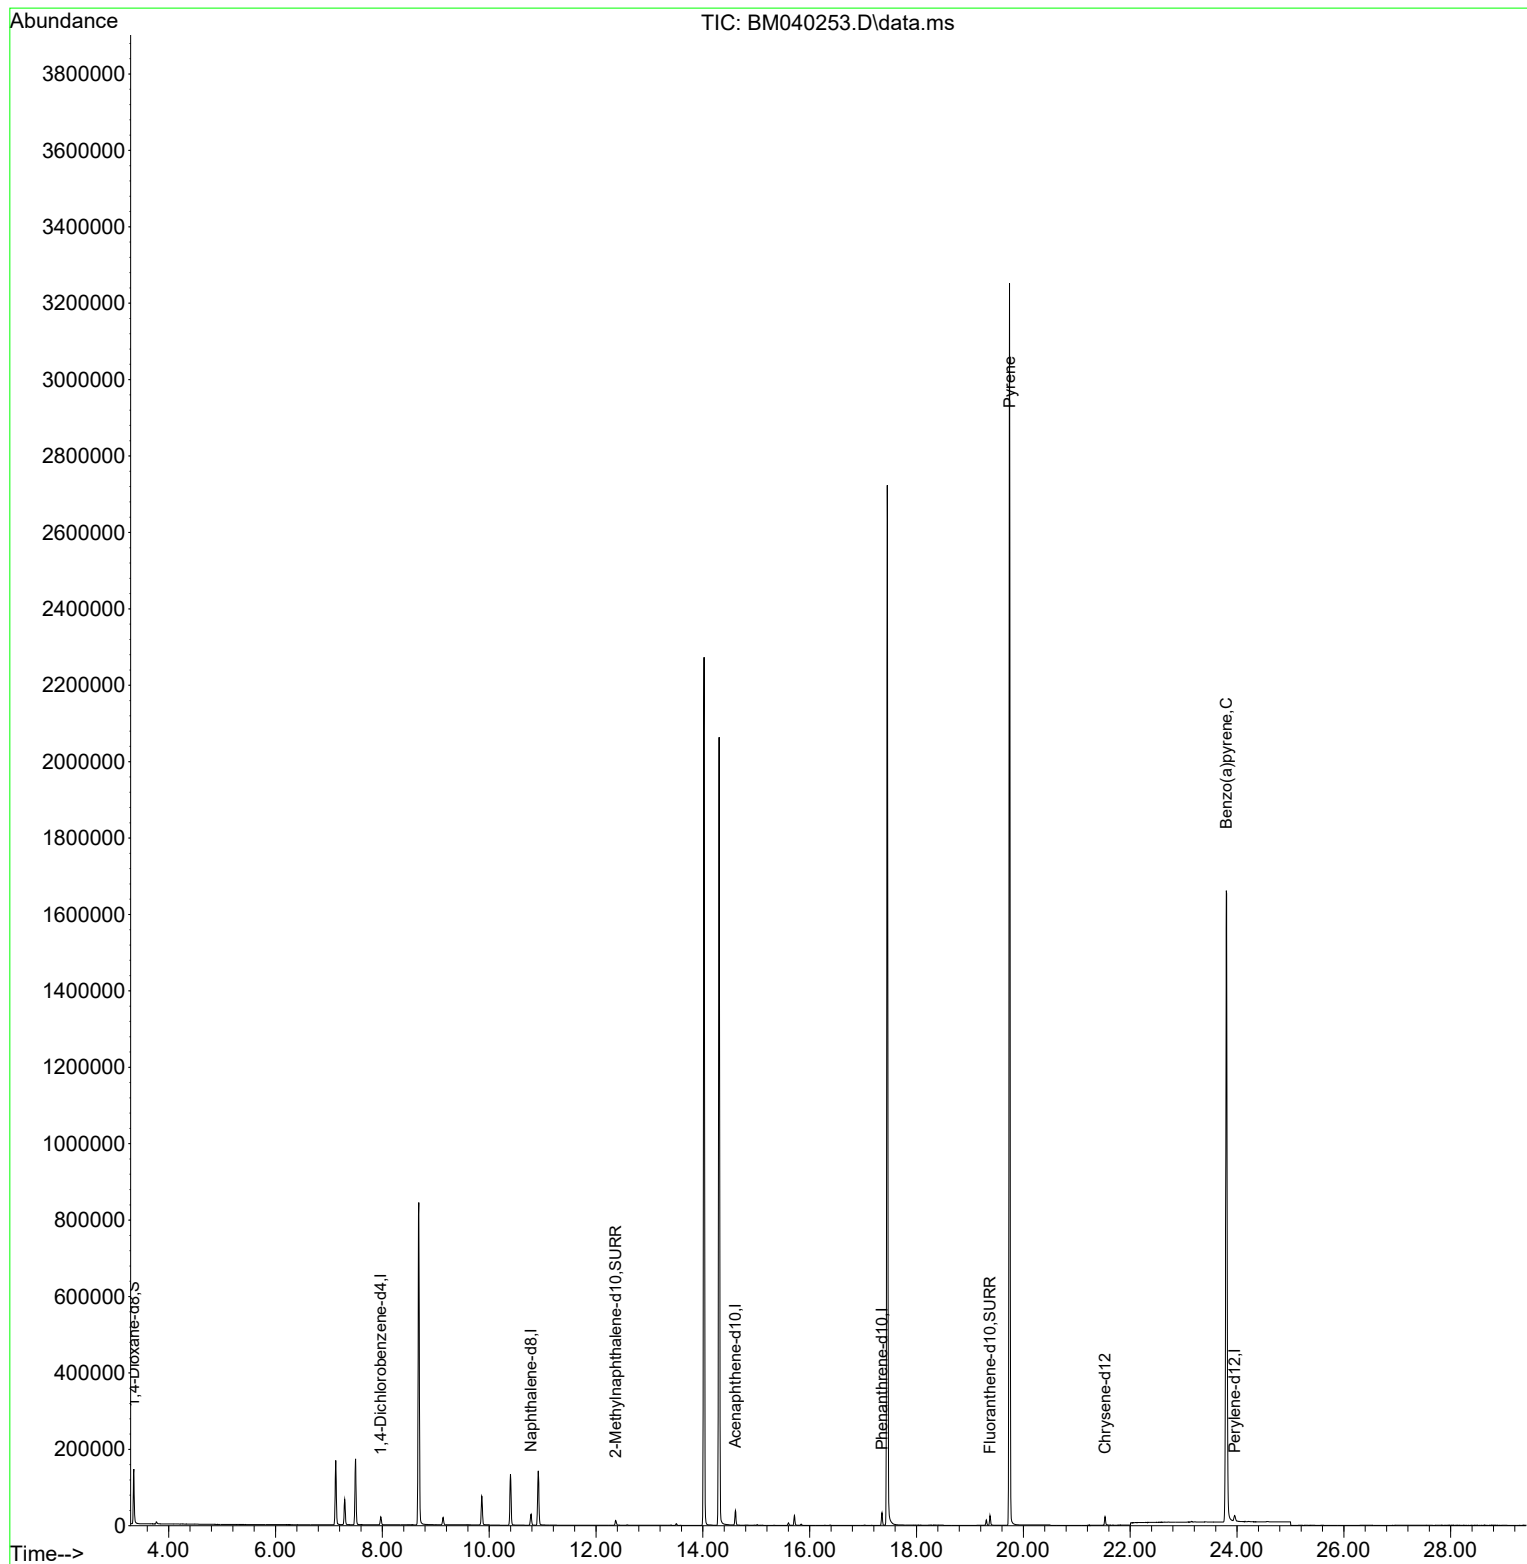

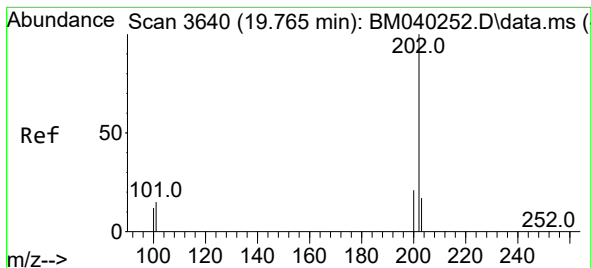

#20

Pyrene

Concen: 0.064 ng/ul

RT: 19.742 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM040253.D

Acq: 15 Jun 2023 09:20

Instrument :

BNA_M

ClientSampleId :

SBLK389





Tgt Ion:202 Resp: 4957

Ion Ratio Lower Upper

202 100

101 156.1 11.8 17.8#

100 1161.1 9.3 13.9#

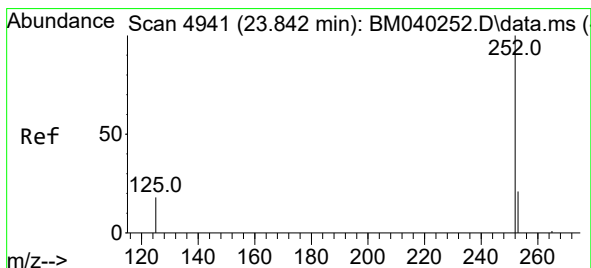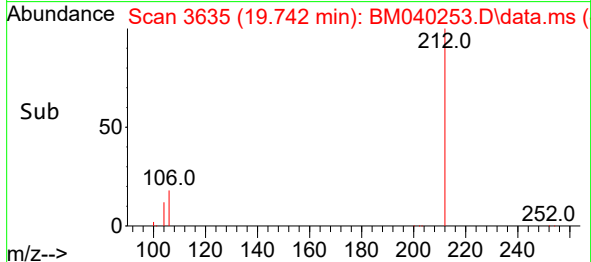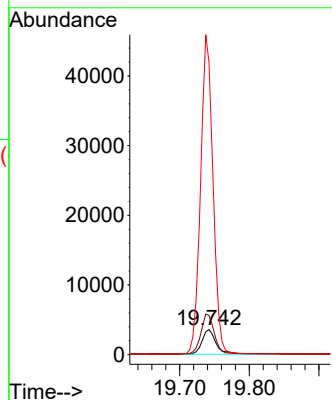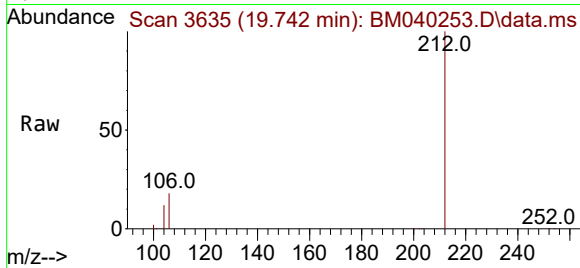

#26

Benzo(a)pyrene

Concen: 0.123 ng/ul

RT: 23.801 min Scan# 4927

Delta R.T. -0.050 min

Lab File: BM040253.D

Acq: 15 Jun 2023 09:20

Tgt Ion:252 Resp: 8240

Ion Ratio Lower Upper

252 100

253 48.9 23.4 35.0#

125 50.2 19.7 29.5#

