

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061523\
 Data File : BM040264.D
 Acq On : 15 Jun 2023 18:02
 Operator : MA/JU
 Sample : PB153389BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK389

Quant Time: Jun 15 23:43:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 15 00:31:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.974	152	11851	0.400	ng/ul	0.00
4) Naphthalene-d8	10.783	136	43728	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.609	164	22281	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.353	188	38471	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	21014	0.400	ng/ul	0.00
23) Perylene-d12	23.955	264	22213	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	99021	6.766	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.367	152	19878	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	26496	0.506	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.604	166	6241	0.084	ng/ul#	13
20) Pyrene	19.742	202	4676	0.063	ng/ul#	1
26) Benzo(a)pyrene	23.800	252	8013	0.119	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061523\
Data File : BM040264.D
Acq On : 15 Jun 2023 18:02
Operator : MA/JU
Sample : PB153389BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK389

Quant Time: Jun 15 23:43:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 00:31:16 2023
Response via : Initial Calibration




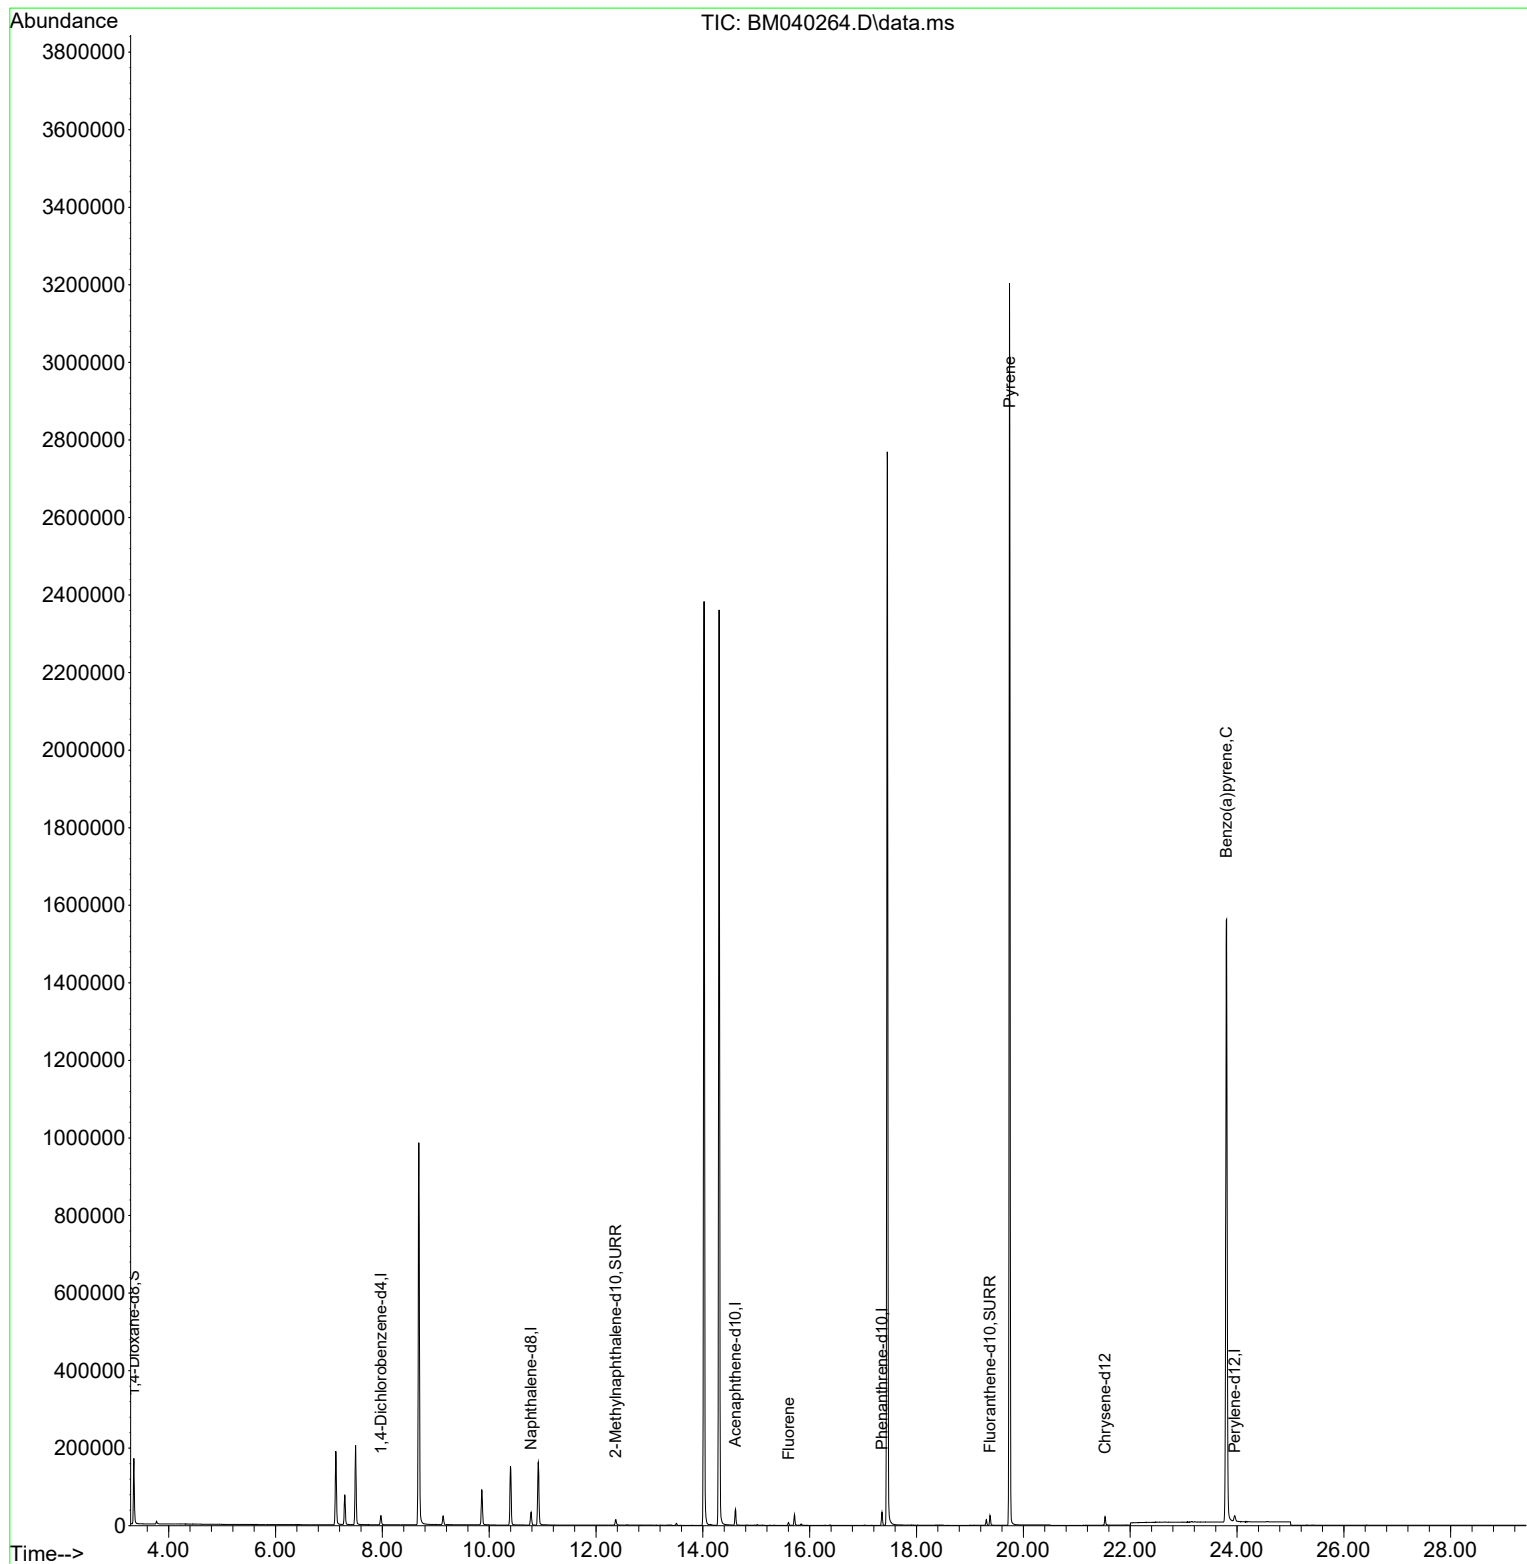


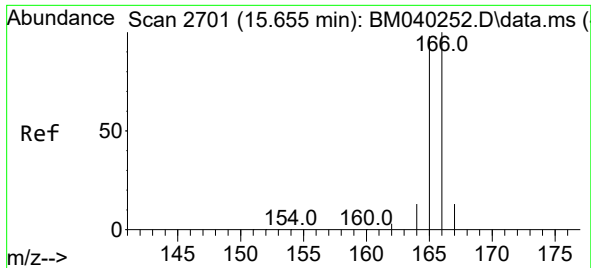

#12
Fluorene
Concen: 0.084 ng/ul
RT: 15.604 min Scan# 2
Delta R.T. -0.056 min
Lab File: BM040264.D
Acq: 15 Jun 2023 18:02




Instrument :
BNA_M
ClientSampleId :
SBLK389


Tgt Ion:166 Resp: 6241
Ion Ratio Lower Upper
166 100
165 7.5 78.2 117.4#
167 34.6 11.0 16.4#

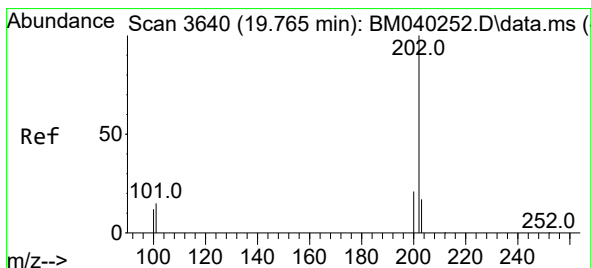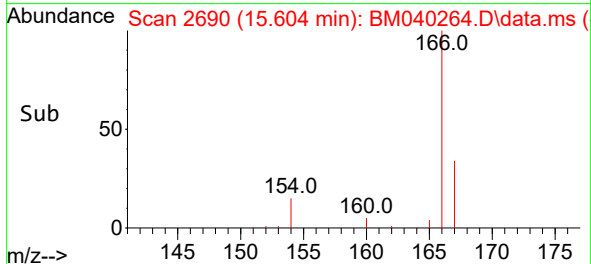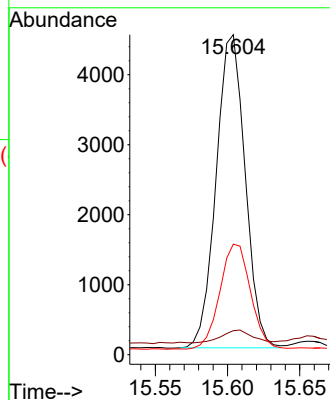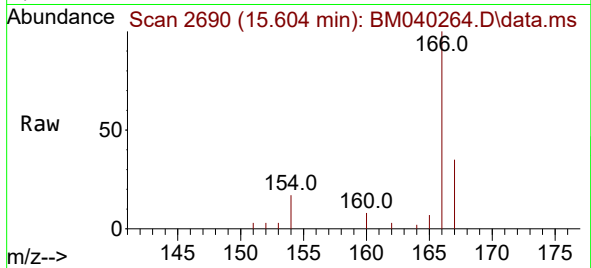

#20
Pyrene
Concen: 0.063 ng/ul
RT: 19.742 min Scan# 3635
Delta R.T. -0.028 min
Lab File: BM040264.D
Acq: 15 Jun 2023 18:02


Tgt Ion:202 Resp: 4676
Ion Ratio Lower Upper
202 100
101 163.8 11.8 17.8#
100 1233.4 9.3 13.9#

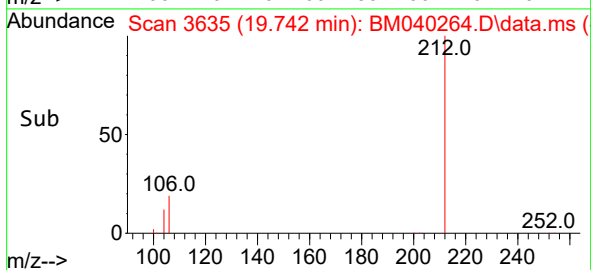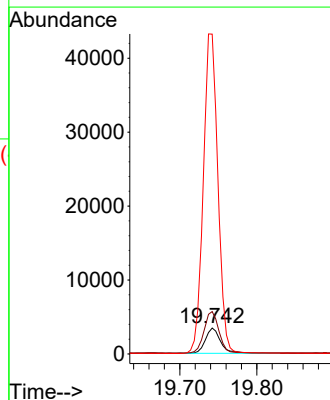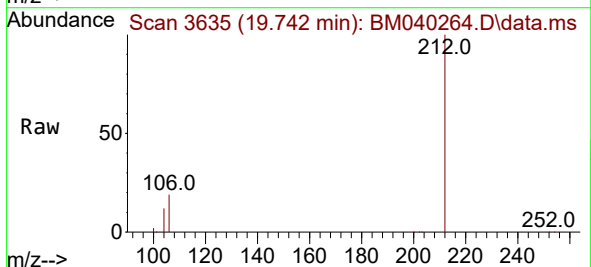

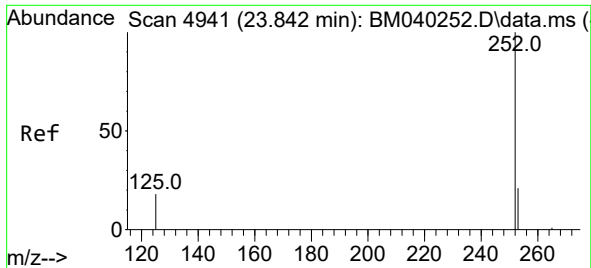

#26
Benzo(a)pyrene
Concen: 0.119 ng/ul
RT: 23.800 min Scan# 4941
Delta R.T. -0.050 min
Lab File: BM040264.D
Acq: 15 Jun 2023 18:02

Instrument :
BNA_M
ClientSampleId :
SBLK389

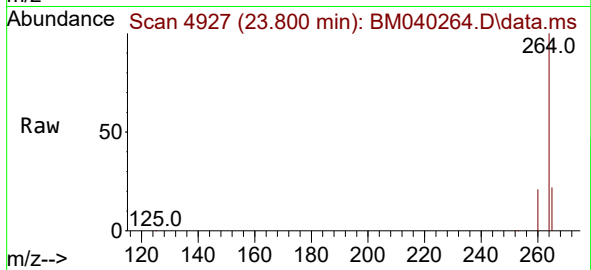

Tgt Ion:252 Resp: 8013
Ion Ratio Lower Upper
252 100
253 51.9 23.4 35.0#
125 52.3 19.7 29.5#

