
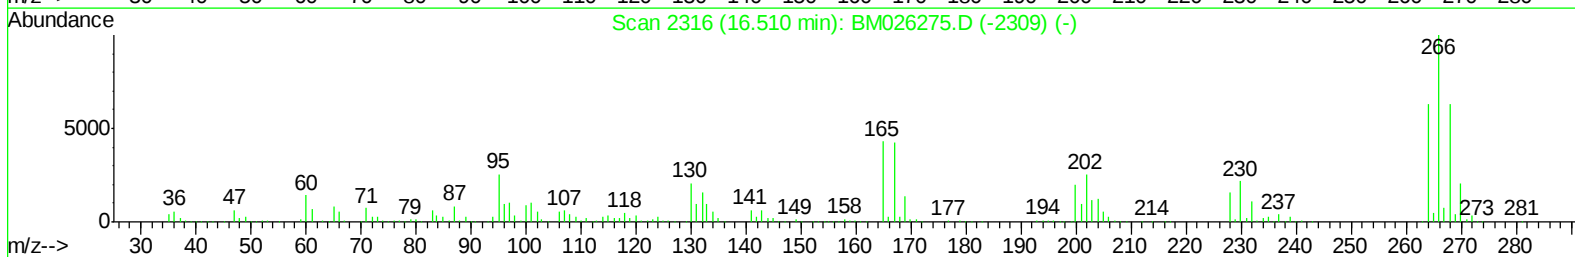
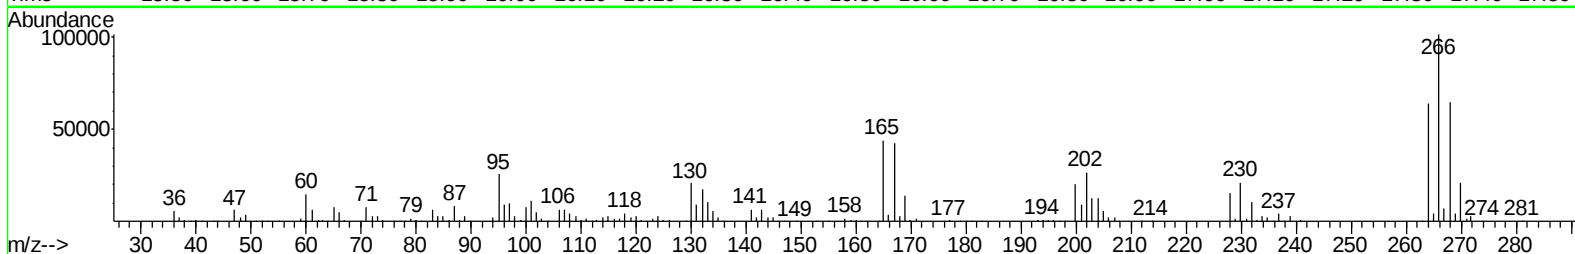


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061620\
Data File : BM026406.D
Acq On : 16 Jun 2020 08:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 02:08:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 16 10:23:36 2020
Response via : Initial Calibration

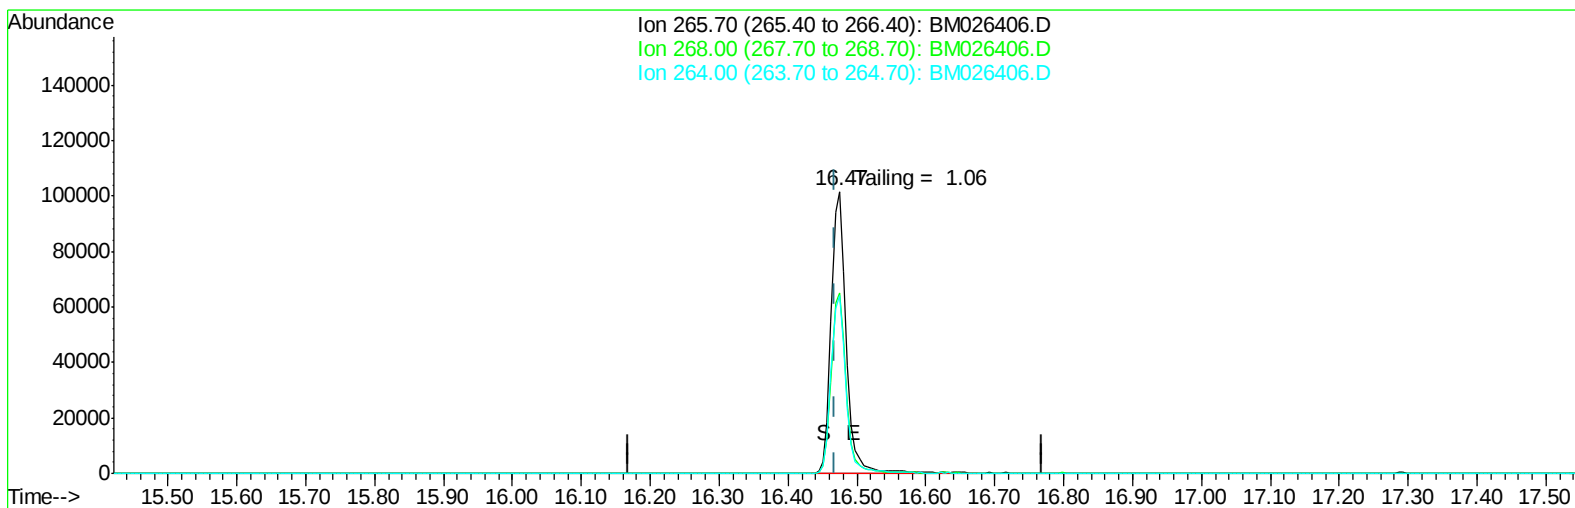

TIC: BM026406.D

(70) Pentachlorophenol (C)




16.474min (+0.006) 33595.11ng

response 150823

Ion	Exp%	Act%
265.70	100	100
268.00	62.80	63.93
264.00	63.20	63.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061620\
Data File : BM026406.D
Acq On : 16 Jun 2020 08:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 02:08:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 16 10:23:36 2020
Response via : Initial Calibration

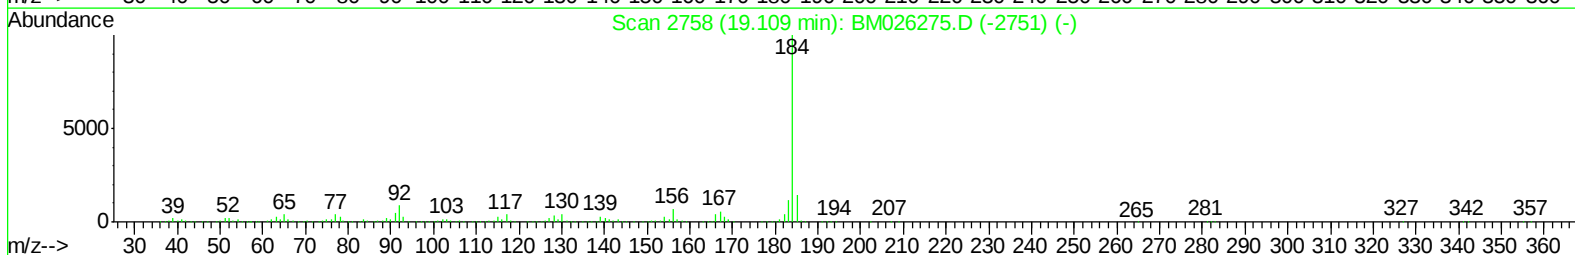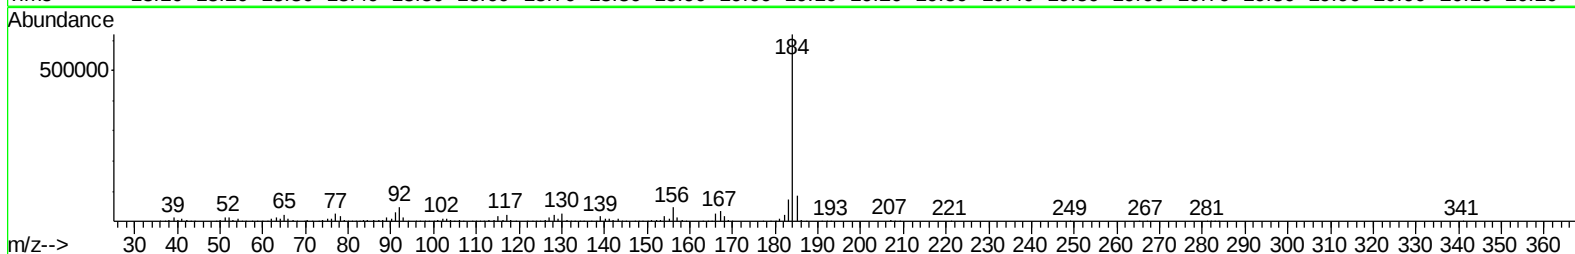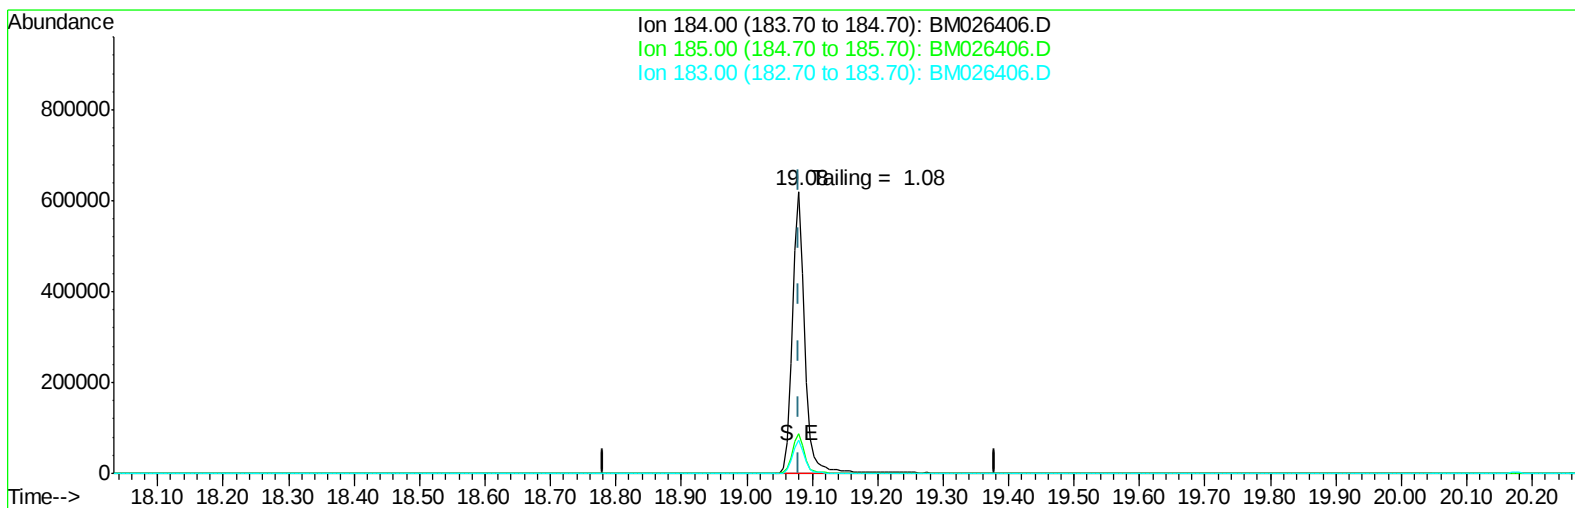

TIC: BM026406.D

(77) Benzidine

19.080min (-0.000) 9207.36ng

response 820659

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.02
183.00	11.80	11.78
0.00	0.00	0.00