
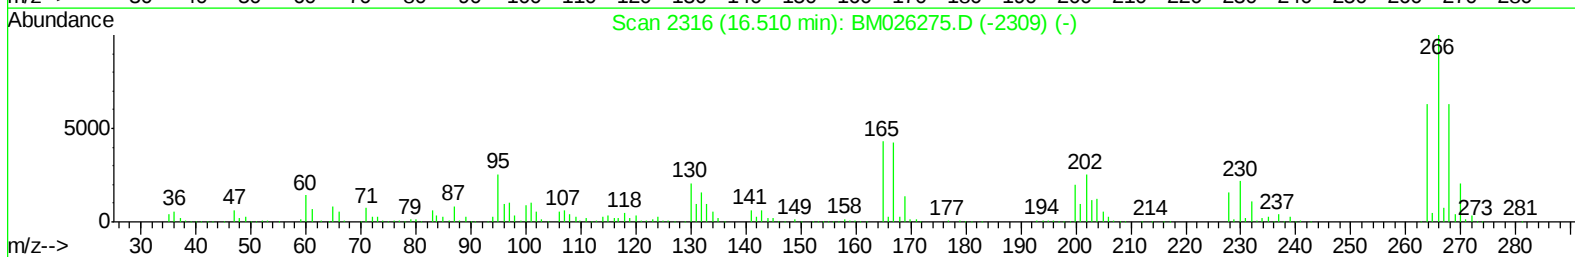
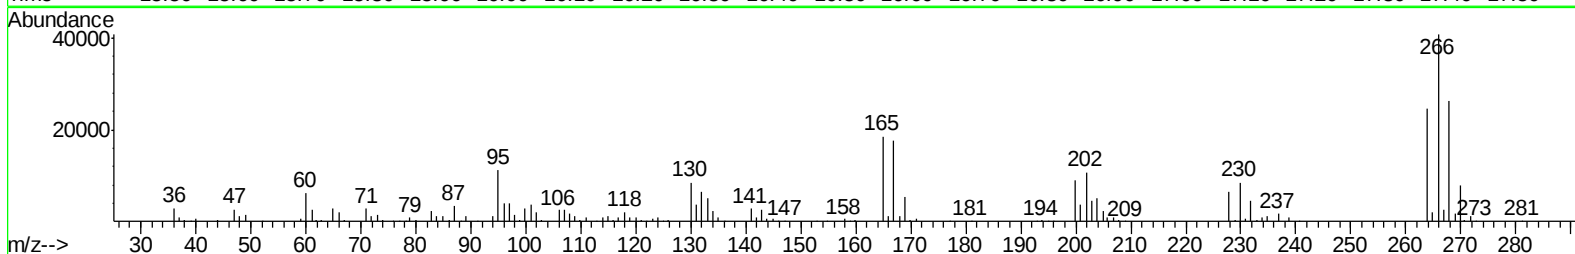


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061620\
Data File : BM026410.D
Acq On : 16 Jun 2020 12:14
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 02:11:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 16 10:23:36 2020
Response via : Initial Calibration

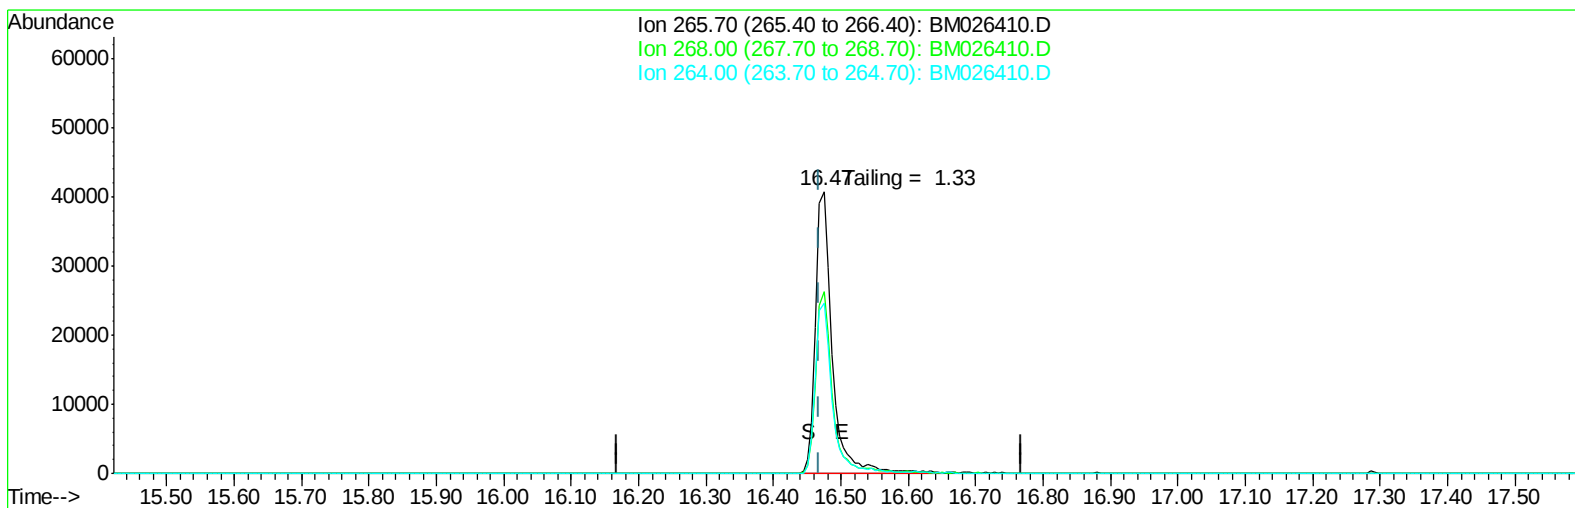

TIC: BM026410.D

(70) Pentachlorophenol (C)

16.474min (+0.005) 22118.26ng

response 67780

Ion	Exp%	Act%
265.70	100	100
268.00	62.80	64.73
264.00	63.20	60.57
0.00	0.00	0.00

