


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061620\  
 Data File : BM026406.D  
 Acq On : 16 Jun 2020 08:18  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM060520.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jun 16 10:23:36 2020

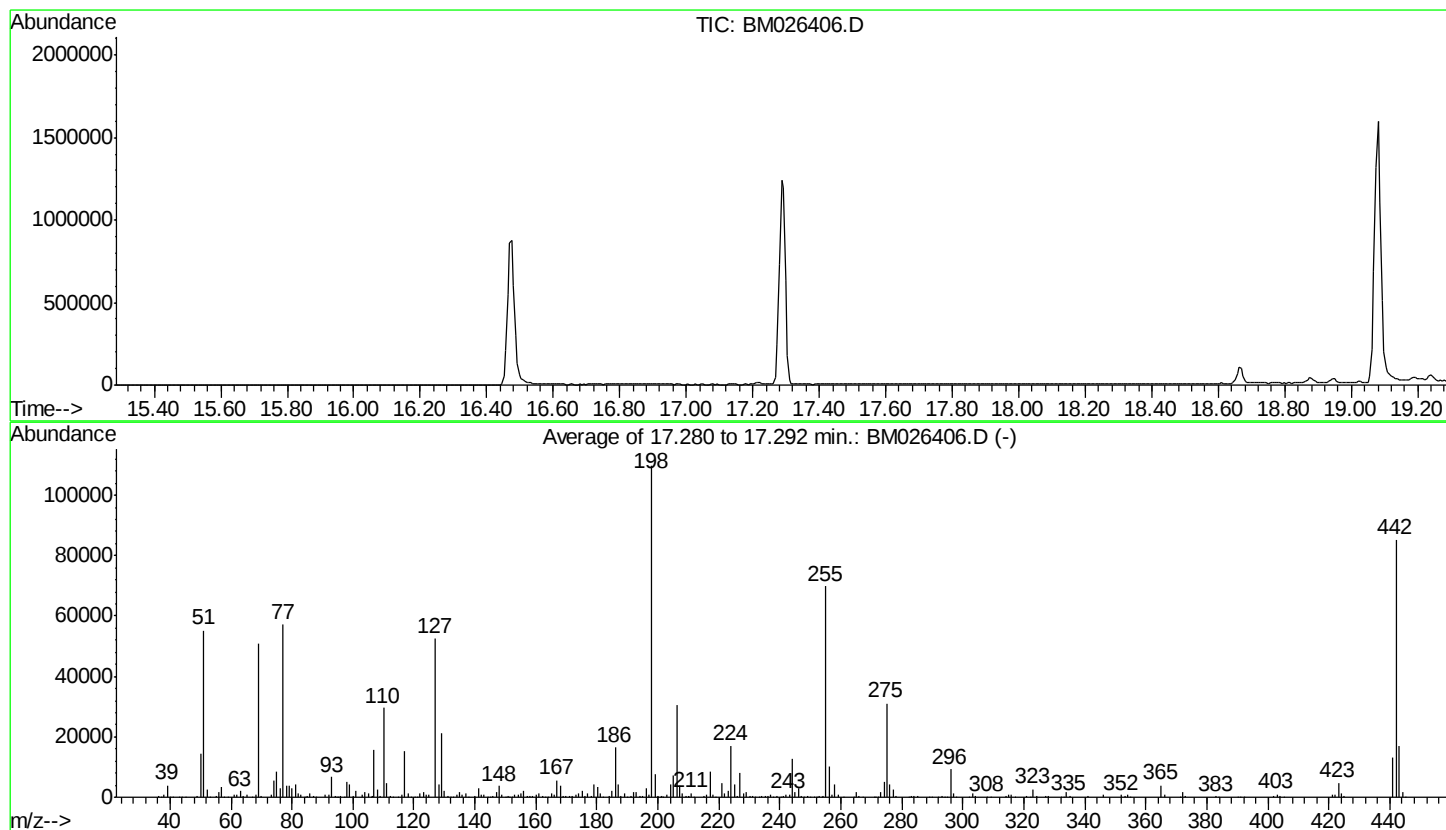

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 50.3      | 55205   | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 1017    | PASS             |
| 69          | 198          | 0.00         | 100          | 46.4      | 50912   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 308     | PASS             |
| 127         | 198          | 10           | 80           | 47.7      | 52405   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 653     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 109797  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 7462    | PASS             |
| 275         | 198          | 10           | 60           | 28.3      | 31018   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 3943    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.0      | 13191   | PASS             |
| 442         | 198          | 50           | 100          | 77.7      | 85317   | PASS             |
| 443         | 442          | 15           | 24           | 20.1      | 17161   | PASS             |