


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061620\
 Data File : BM026410.D
 Acq On : 16 Jun 2020 12:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 16 10:23:36 2020

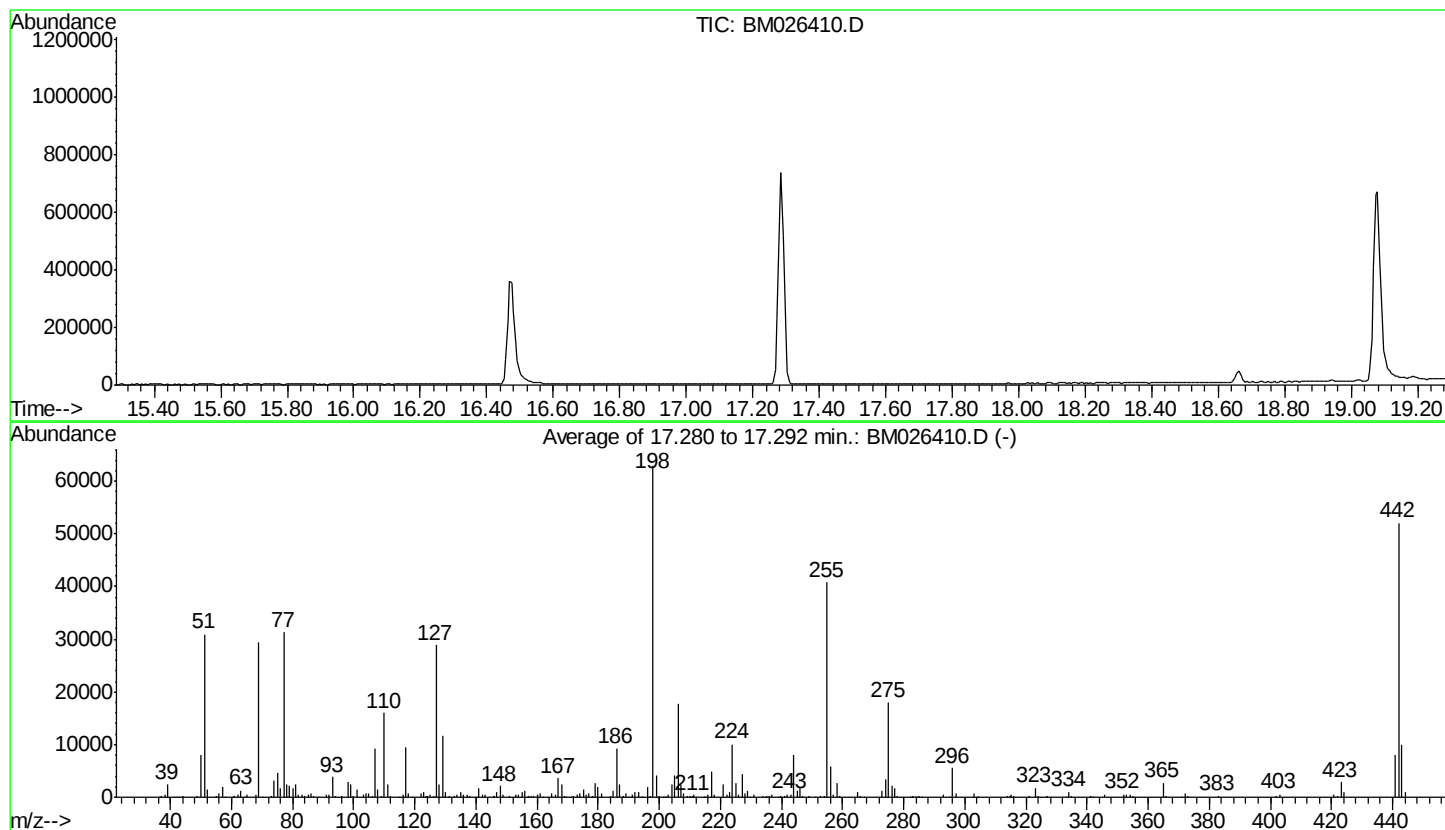

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	30882	PASS
68	69	0.00	2	1.9	571	PASS
69	198	0.00	100	46.5	29309	PASS
70	69	0.00	2	0.4	107	PASS
127	198	10	80	45.9	28925	PASS
197	198	0.00	2	0.6	371	PASS
198	198	100	100	100.0	62968	PASS
199	198	5	9	6.5	4095	PASS
275	198	10	60	28.4	17911	PASS
365	198	1	100	4.3	2690	PASS
441	198	0.01	100	12.9	8125	PASS
442	198	50	100	82.8	52128	PASS
443	442	15	24	19.1	9957	PASS