

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061622\
 Data File : BM035479.D
 Acq On : 16 Jun 2022 14:03
 Operator : CG/JU
 Sample : SSTD01048
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048

Quant Time: Jun 17 01:04:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 00:59:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	225257	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	927537	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	548923	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	1108522	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	1156002	20.000	ng/u1	0.00
88) Perylene-d12	23.733	264	1247951	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	21614	3.965	ng/uL	0.00
4) Pyridine-d5	3.693	84	108380	7.707	ng/u1	0.00
7) Phenol-d5	7.004	99	147879	8.908	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.151	67	95214	9.090	ng/u1	0.00
11) 2-Chlorophenol-d4	7.351	132	136441	9.271	ng/u1	0.00
15) 4-Methylphenol-d8	8.545	113	121986	8.747	ng/u1	0.00
21) Nitrobenzene-d5	8.981	128	62422	8.584	ng/u1	0.00
24) 2-Nitrophenol-d4	9.704	143	64555	7.928	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	110159	7.606	ng/u1	0.00
31) 4-Chloroaniline-d4	10.763	131	175656	8.796	ng/u1	0.00
46) Dimethylphthalate-d6	13.869	166	351041	8.778	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	432479	9.048	ng/u1	0.00
54) 4-Nitrophenol-d4	14.721	143	28373	4.002	ng/u1	0.02
60) Fluorene-d10	15.451	176	311934	9.220	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	47783	6.675	ng/u1	0.00
73) Anthracene-d10	17.304	188	472419	9.156	ng/u1	0.00
81) Pyrene-d10	19.598	212	534171	8.676	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.586	264	564148	8.920	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.305	88	20806	3.673	ng/uL	92
5) Pyridine	3.710	79	123201	8.452	ng/u1	92
6) Benzaldehyde	6.963	77	86820	10.540	ng/u1	91
8) Phenol	7.034	94	156960	8.990	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.240	93	129901	9.599	ng/u1	98
12) 2-Chlorophenol	7.387	128	140176	9.323	ng/u1	99
13) 2-Methylphenol	8.275	108	118874	9.071	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.351	45	200995	10.455	ng/u1	99
16) Acetophenone	8.645	105	196467	9.095	ng/u1	94
17) N-Nitroso-di-n-propyla...	8.628	70	92115	8.995	ng/u1	98
18) 4-Methylphenol	8.610	108	125995	8.997	ng/u1	96
19) Hexachloroethane	8.887	117	57900	8.859	ng/u1	91
22) Nitrobenzene	9.022	77	132868	7.641	ng/u1	97
23) Isophorone	9.545	82	249249	8.121	ng/u1	100
25) 2-Nitrophenol	9.734	139	71961	8.255	ng/u1	98
26) 2,4-Dimethylphenol	9.804	107	140641	8.186	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.028	93	164911	8.927	ng/u1	99
29) 2,4-Dichlorophenol	10.286	162	118696	8.128	ng/u1	98
30) Naphthalene	10.657	128	449613	9.372	ng/u1	99
32) 4-Chloroaniline	10.786	127	173265	8.676	ng/u1	98
33) Hexachlorobutadiene	10.945	225	77298	7.279	ng/u1	98
34) Caprolactam	11.580	113	29730	7.066	ng/u1	93
35) 4-Chloro-3-methylphenol	11.933	107	118799	8.103	ng/u1	99
36) 2-Methylnaphthalene	12.280	142	291501	9.070	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061622\
 Data File : BM035479.D
 Acq On : 16 Jun 2022 14:03
 Operator : CG/JU
 Sample : SST01048
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST010048

Quant Time: Jun 17 01:04:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 00:59:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.498	142	296490	9.204	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.651	216	143470	8.128	ng/ul	99
40) Hexachlorocyclopentadiene	12.627	237	26664	2.118	ng/ul	92
41) 2,4,6-Trichlorophenol	12.910	196	84897	7.531	ng/ul	97
42) 2,4,5-Trichlorophenol	12.998	196	88023	7.357	ng/ul	97
43) 1,1'-Biphenyl	13.292	154	384638	9.051	ng/ul	100
44) 2-Chloronaphthalene	13.333	162	297392	9.024	ng/ul	99
45) 2-Nitroaniline	13.557	65	67094	7.246	ng/ul	96
47) Dimethylphthalate	13.921	163	359822	8.986	ng/ul	100
48) 2,6-Dinitrotoluene	14.045	165	64724	8.115	ng/ul	95
50) Acenaphthylene	14.174	152	484437	9.431	ng/ul	98
51) 3-Nitroaniline	14.386	138	60115	7.860	ng/ul	97
52) Acenaphthene	14.521	153	317407	9.278	ng/ul	99
53) 2,4-Dinitrophenol	14.627	184	21751	4.163	ng/ul	97
55) 4-Nitrophenol	14.745	109	15055	2.264	ng/ul	93
56) Dibenzofuran	14.857	168	447647	9.356	ng/ul	99
57) 2,4-Dinitrotoluene	14.845	165	97034	8.664	ng/ul#	87
58) 2,3,4,6-Tetrachlorophenol	15.098	232	76672	7.910	ng/ul#	97
59) Diethylphthalate	15.280	149	364858	8.998	ng/ul	99
61) Fluorene	15.504	166	366187	9.407	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.498	204	172481	8.728	ng/ul	99
63) 4-Nitroaniline	15.551	138	46625	6.729	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.610	198	48832	6.806	ng/ul#	98
67) N-Nitrosodiphenylamine	15.715	169	309095	9.217	ng/ul	99
68) 4-Bromophenyl-phenylether	16.392	248	99006	8.433	ng/ul	99
69) Hexachlorobenzene	16.515	284	117655	8.776	ng/ul	98
70) Atrazine	16.674	200	102713	7.850	ng/ul	97
71) Pentachlorophenol	16.880	266	48019	5.360	ng/ul	95
72) Phenanthrene	17.245	178	575108	9.581	ng/ul	99
74) Anthracene	17.339	178	582912	9.530	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.257	216	158329	8.199	ng/ul	98
76) Pentachlorobenzene	14.780	250	143006	8.621	ng/ul	97
77) Carbazole	17.615	167	515449	9.522	ng/ul	99
78) Di-n-butylphthalate	18.174	149	658688	8.503	ng/ul	99
80) Fluoranthene	19.268	202	648571	8.770	ng/ul	99
82) Pyrene	19.627	202	680630	8.941	ng/ul	99
83) Butylbenzylphthalate	20.527	149	279178	8.562	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.315	252	208613	8.778	ng/ul	98
85) Benzo(a)anthracene	21.380	228	660270	8.940	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.309	149	421418	8.595	ng/ul	99
87) Chrysene	21.433	228	668849	9.289	ng/ul	100
89) Di-n-octyl phthalate	22.209	149	739499	8.265	ng/ul	100
90) Benzo(b)fluoranthene	23.027	252	728451	8.975	ng/ul	99
91) Benzo(k)fluoranthene	23.074	252	661648	8.581	ng/ul	98
93) Benzo(a)pyrene	23.633	252	699419	8.845	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.156	276	823050	9.058	ng/ul	99
95) Dibenzo(a,h)anthracene	26.162	278	704715	9.029	ng/ul	99
96) Benzo(g,h,i)perylene	26.897	276	697215	9.224	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

BNA M

ClientSampleId :

SSTD010048





[illegible]



#2
1,4-Dioxane
Concen: 3.673 ng/uL
RT: 3.305 min Scan# 31
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion: 88 Resp: 20806
Ion Ratio Lower Upper
88 100
43 40.8 27.8 41.8
58 83.5 61.8 92.8



#5
Pyridine
Concen: 8.452 ng/uL
RT: 3.710 min Scan# 106
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion: 79 Resp: 123201
Ion Ratio Lower Upper
79 100
52 91.0 67.8 101.6
51 46.1 31.4 47.0









#6
Benzaldehyde
Concen: 10.540 ng/ul
RT: 6.963 min Scan# 659
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion: 77 Resp: 86820
Ion Ratio Lower Upper
77 100
105 93.6 84.6 127.0
106 93.7 80.3 120.5

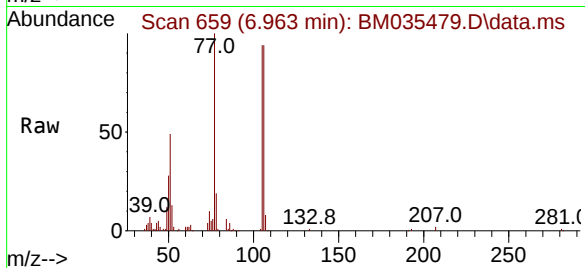

#8
Phenol
Concen: 8.990 ng/ul
RT: 7.034 min Scan# 671
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion: 94 Resp: 156960
Ion Ratio Lower Upper
94 100
65 28.8 21.3 31.9
66 35.1 27.4 41.0

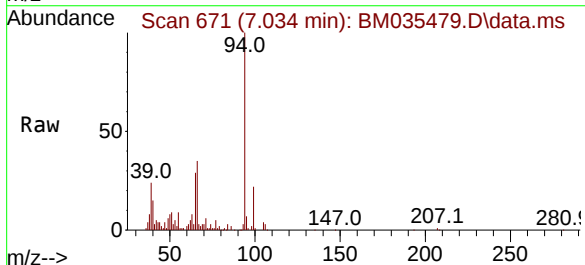







#10
Bis(2-Chloroethyl)ether
Concen: 9.599 ng/ul
RT: 7.240 min Scan# 706
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Instrument :
BNA_M
ClientSampleId :
SSTD010048

Tgt Ion: 93 Resp: 129901




Ion	Ratio	Lower	Upper
93	100		
63	77.7	64.0	96.0
95	32.8	25.8	38.6

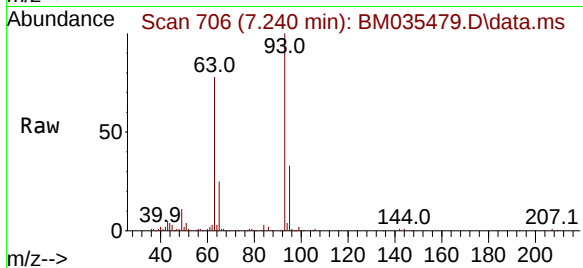


#12
2-Chlorophenol
Concen: 9.323 ng/ul
RT: 7.387 min Scan# 731
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion: 128 Resp: 140176

Ion	Ratio	Lower	Upper
128	100		
64	45.0	36.9	55.3
130	32.5	25.6	38.4

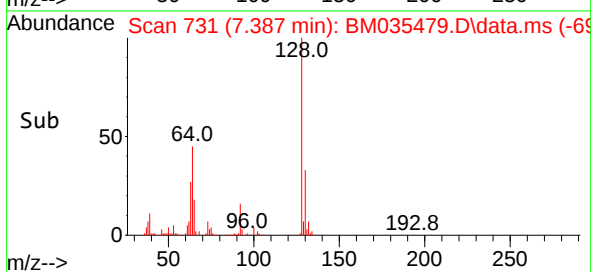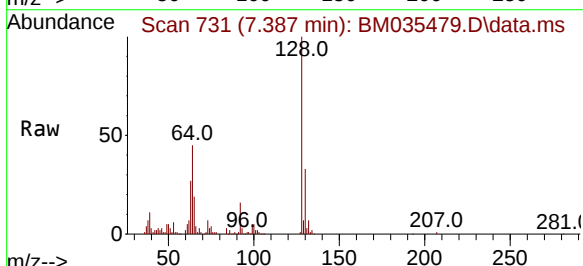



#13

2-Methylphenol

Concen: 9.071 ng/ul

RT: 8.275 min Scan# 882

Delta R.T. 0.000 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03

Instrument :

BNA_M

ClientSampleId :





SSTD010048

Tgt Ion:108 Resp: 118874

Ion Ratio Lower Upper

108 100

107 92.8 75.0 112.4

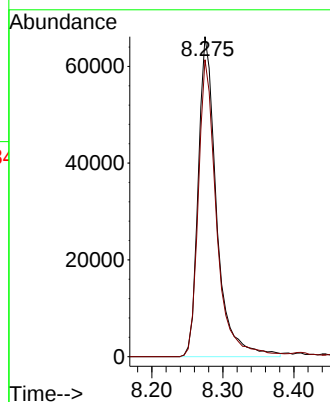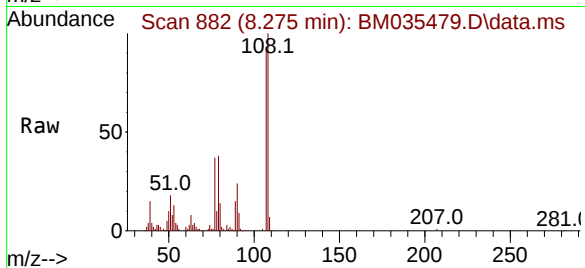

#14

2,2'-oxybis(1-Chloropropane)

Concen: 10.455 ng/ul

RT: 8.351 min Scan# 895

Delta R.T. 0.006 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03




Tgt Ion: 45 Resp: 200995


Ion Ratio Lower Upper

45 100

77 13.3 10.6 15.8

79 11.0 8.3 12.5




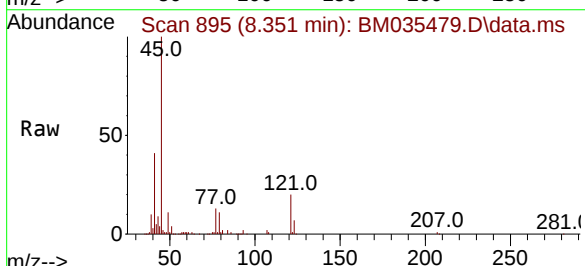




#16
Acetophenone
Concen: 9.095 ng/ul
RT: 8.645 min Scan# 945
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:105 Resp: 196467
Ion Ratio Lower Upper
105 100
77 80.1 59.8 89.6
51 31.0 22.1 33.1



#17
N-Nitroso-di-n-propylamine
Concen: 8.995 ng/ul
RT: 8.628 min Scan# 942
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion: 70 Resp: 92115
Ion Ratio Lower Upper
70 100
42 61.2 49.6 74.4
101 10.0 8.1 12.1
130 25.0 18.4 27.6









#18
4-Methylphenol
Concen: 8.997 ng/ul
RT: 8.610 min Scan# 911
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:108 Resp: 125995
Ion Ratio Lower Upper
108 100
107 117.2 90.3 135.5

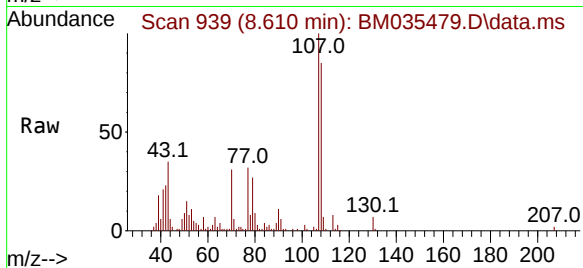

#19
Hexachloroethane
Concen: 8.859 ng/ul
RT: 8.887 min Scan# 986
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:117 Resp: 57900
Ion Ratio Lower Upper
117 100
201 94.4 81.8 122.6
199 54.9 51.6 77.4




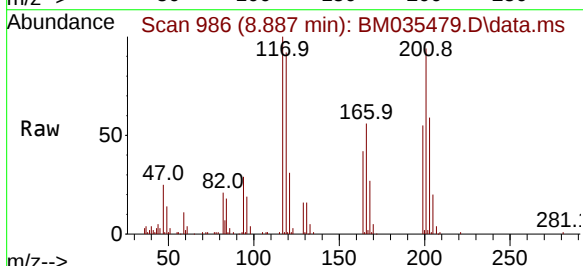




#22
Nitrobenzene
Concen: 7.641 ng/ul
RT: 9.022 min Scan# 1009
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion: 77 Resp: 132868
Ion Ratio Lower Upper
77 100
123 49.0 37.4 56.0
65 12.5 10.8 16.2



#23
Isophorone
Concen: 8.121 ng/ul
RT: 9.545 min Scan# 1098
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion: 82 Resp: 249249
Ion Ratio Lower Upper
82 100
95 6.9 5.5 8.3
138 19.0 15.3 22.9









#25
2-Nitrophenol
Concen: 8.255 ng/ul
RT: 9.734 min Scan# 1130
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:139 Resp: 71961
Ion Ratio Lower Upper
139 100
65 50.4 39.8 59.6
109 26.5 22.2 33.4

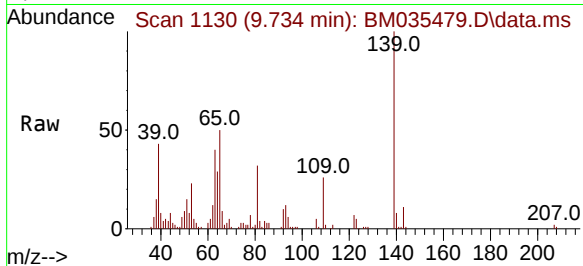

#26
2,4-Dimethylphenol
Concen: 8.186 ng/ul
RT: 9.804 min Scan# 1142
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:107 Resp: 140641
Ion Ratio Lower Upper
107 100
121 54.2 42.7 64.1
122 87.9 71.5 107.3

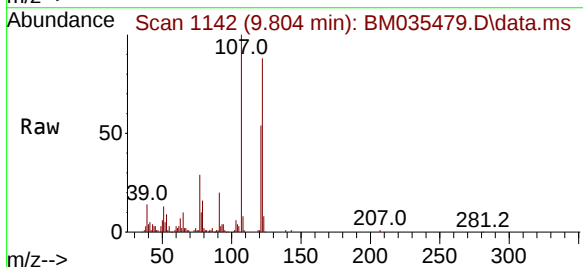



#27

Bis(2-Chloroethoxy)methane

Concen: 8.927 ng/ul

RT: 10.028 min Scan# 1180

Delta R.T. 0.000 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion: 93 Resp: 164911

Ion Ratio Lower Upper

93 100

95 32.8 26.1 39.1

123 12.5 9.4 14.0

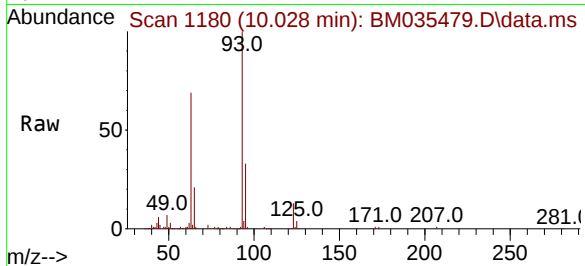

#29

2,4-Dichlorophenol

Concen: 8.128 ng/ul

RT: 10.286 min Scan# 1224

Delta R.T. 0.012 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03




Tgt Ion:162 Resp: 118696


Ion Ratio Lower Upper

162 100

164 64.3 51.8 77.6

98 34.0 29.5 44.3




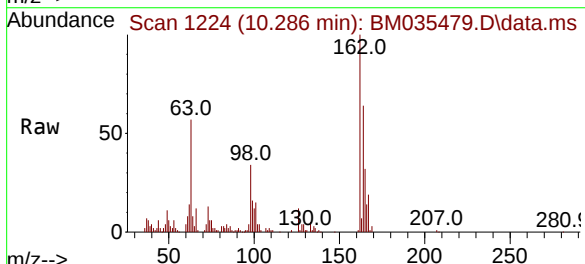




#30
Naphthalene
Concen: 9.372 ng/ul
RT: 10.657 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:128 Resp: 449613
Ion Ratio Lower Upper
128 100
129 10.7 8.8 13.2
127 13.1 10.6 16.0



#32
4-Chloroaniline
Concen: 8.676 ng/ul
RT: 10.786 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:127 Resp: 173265
Ion Ratio Lower Upper
127 100
129 30.7 25.3 37.9





#33

Hexachlorobutadiene

Concen: 7.279 ng/ul

RT: 10.945 min Scan# 11

Delta R.T. 0.000 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion:225 Resp: 77298

Ion Ratio Lower Upper

225 100

223 64.6 50.0 75.0

227 63.9 49.9 74.9

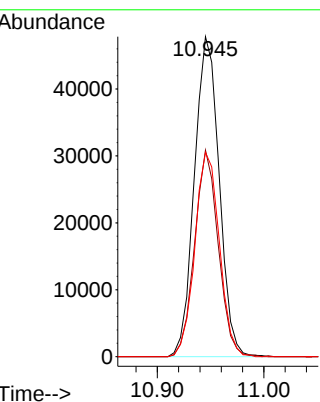

#34

Caprolactam

Concen: 7.066 ng/ul

RT: 11.580 min Scan# 1444

Delta R.T. 0.006 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03




Tgt Ion:113 Resp: 29730


Ion Ratio Lower Upper

113 100

55 172.3 150.2 225.4

56 130.5 102.1 153.1



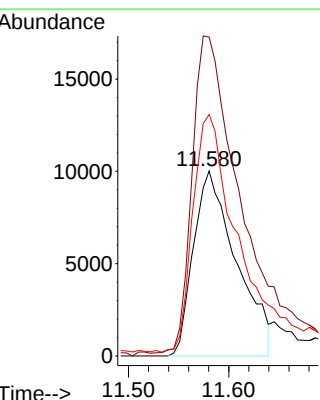





#35
4-Chloro-3-methylphenol
Concen: 8.103 ng/ul
RT: 11.933 min Scan# 11
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:107 Resp: 118799
Ion Ratio Lower Upper
107 100
144 24.9 20.3 30.5
142 81.6 64.4 96.6

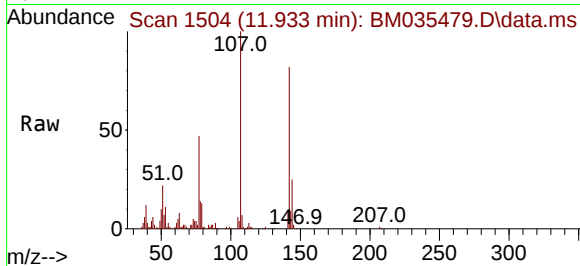

#36
2-Methylnaphthalene
Concen: 9.070 ng/ul
RT: 12.280 min Scan# 1563
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:142 Resp: 291501
Ion Ratio Lower Upper
142 100
141 86.9 70.7 106.1




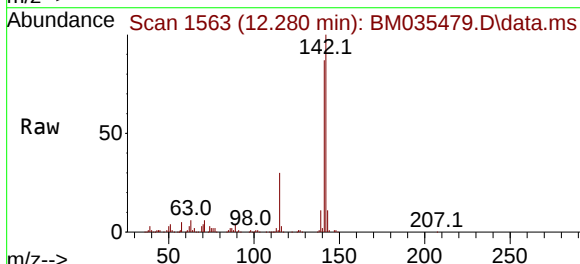




#37
1-Methylnaphthalene
Concen: 9.204 ng/ul
RT: 12.498 min Scan# 1600
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:142 Resp: 296490
Ion Ratio Lower Upper
142 100
141 92.6 75.2 112.8
116 3.5 2.6 3.8

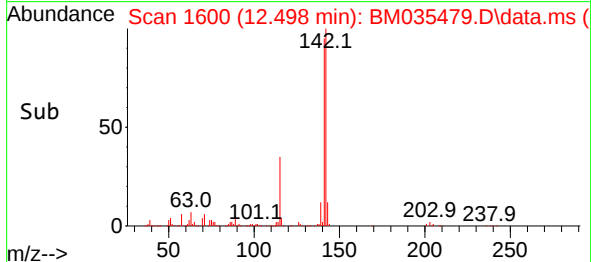

#39
1,2,4,5-Tetrachlorobenzene
Concen: 8.128 ng/ul
RT: 12.651 min Scan# 1626
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:216 Resp: 143470
Ion Ratio Lower Upper
216 100
214 78.8 62.4 93.6
179 20.9 17.3 25.9
108 17.4 14.0 21.0


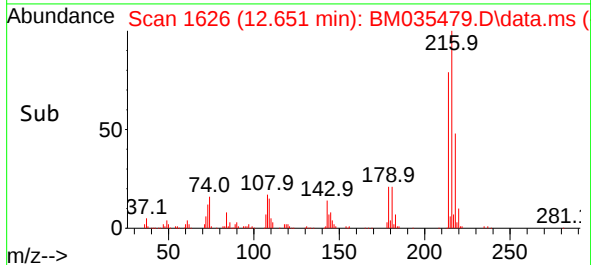






#40
Hexachlorocyclopentadiene
Concen: 2.118 ng/ul
RT: 12.627 min Scan# 1
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:237 Resp: 26664
Ion Ratio Lower Upper
237 100
235 53.5 48.4 72.6
272 12.4 11.6 17.4

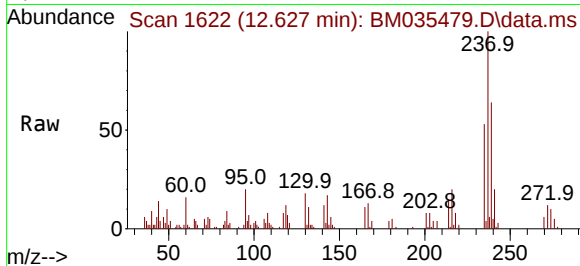

#41
2,4,6-Trichlorophenol
Concen: 7.531 ng/ul
RT: 12.910 min Scan# 1670
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:196 Resp: 84897
Ion Ratio Lower Upper
196 100
198 93.8 77.8 116.6
200 30.6 25.0 37.6

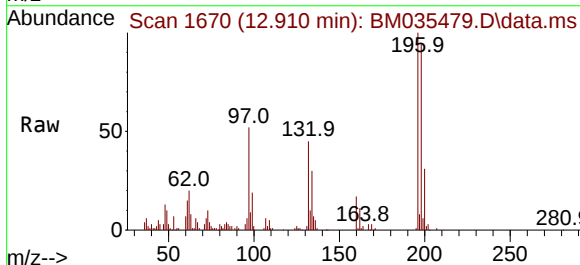



#42

2,4,5-Trichlorophenol

Concen: 7.357 ng/ul

RT: 12.998 min Scan# 1

Delta R.T. 0.006 min

Lab File: BM035479.D


Acq: 16 Jun 2022 14:03

Instrument :

BNA_M

ClientSampleId :

SSTD010048

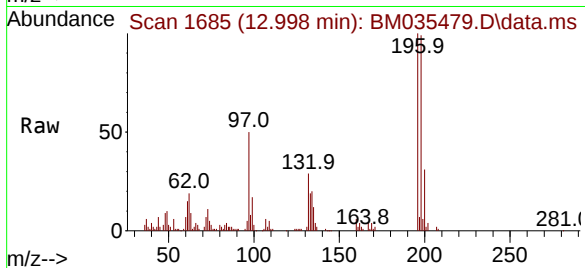




Tgt Ion:196 Resp: 88023

Ion Ratio Lower Upper

196 100

198 99.3 76.8 115.2

200 30.9 24.9 37.3



#43

1,1'-Biphenyl

Concen: 9.051 ng/ul

RT: 13.292 min Scan# 1735

Delta R.T. 0.000 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03




Tgt Ion:154 Resp: 384638


Ion Ratio Lower Upper

154 100

153 40.5 32.4 48.6

76 13.3 10.1 15.1




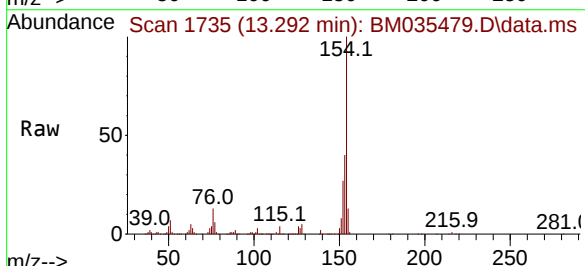


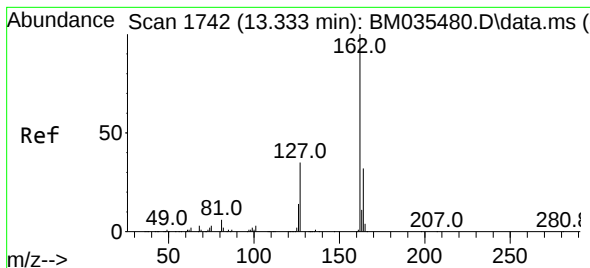

#44
2-Chloronaphthalene
Concen: 9.024 ng/ul
RT: 13.333 min Scan# 1742
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:162 Resp: 297392
Ion Ratio Lower Upper
162 100
164 33.3 25.4 38.0
127 39.3 31.6 47.4

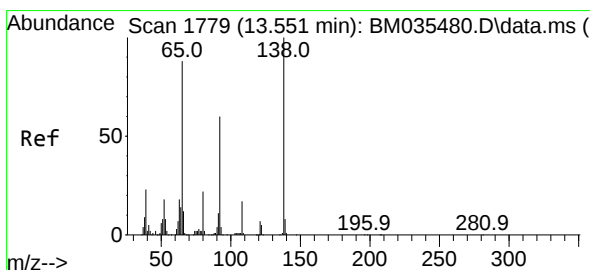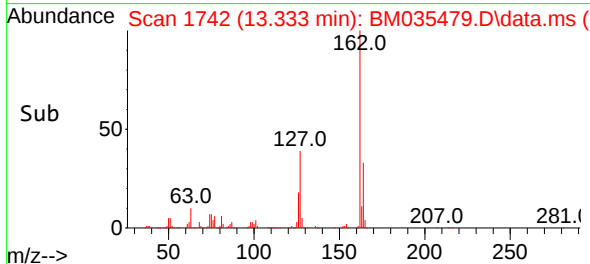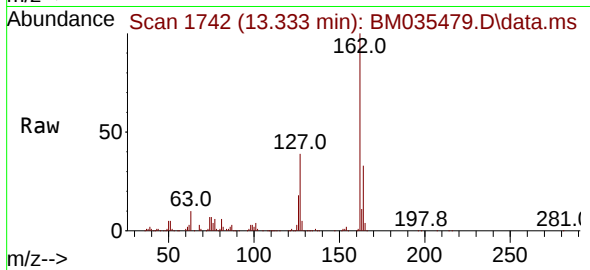

#45
2-Nitroaniline
Concen: 7.246 ng/ul
RT: 13.557 min Scan# 1780
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion: 65 Resp: 67094
Ion Ratio Lower Upper
65 100
92 66.3 54.5 81.7
138 108.4 91.2 136.8


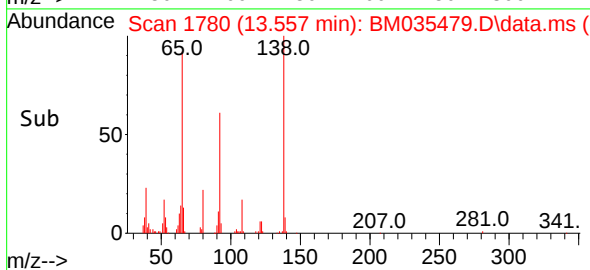

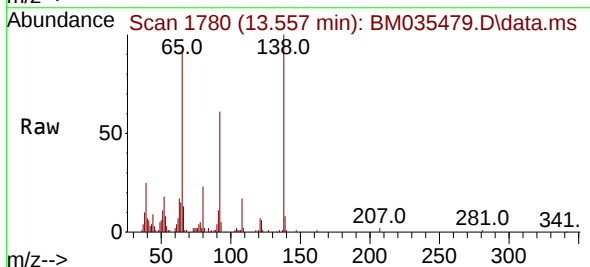




#47
Dimethylphthalate
Concen: 8.986 ng/ul
RT: 13.921 min Scan# 1842
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:163 Resp: 359822
Ion Ratio Lower Upper
163 100
194 3.7 3.2 4.8
164 10.0 7.9 11.9

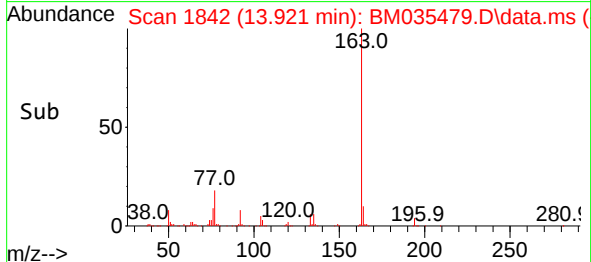

#48
2,6-Dinitrotoluene
Concen: 8.115 ng/ul
RT: 14.045 min Scan# 1863
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:165 Resp: 64724
Ion Ratio Lower Upper
165 100
89 58.2 42.5 63.7
121 21.1 17.2 25.8









#50
Acenaphthylene
Concen: 9.431 ng/ul
RT: 14.174 min Scan# 1885
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:152 Resp: 484437
Ion Ratio Lower Upper
152 100
151 19.1 16.1 24.1
153 12.5 10.6 15.8

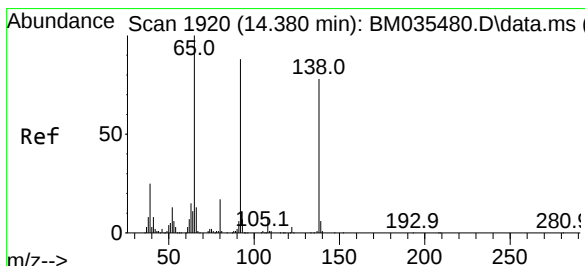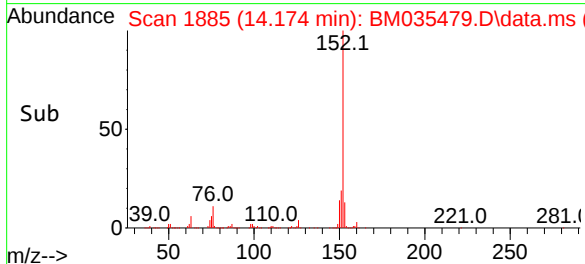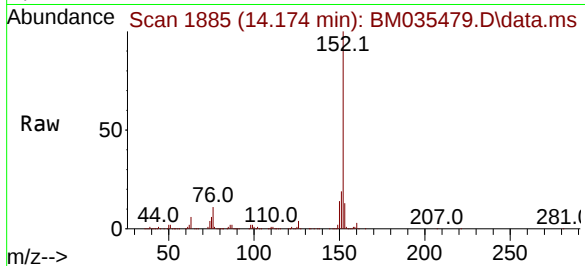

#51
3-Nitroaniline
Concen: 7.860 ng/ul
RT: 14.386 min Scan# 1921
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:138 Resp: 60115
Ion Ratio Lower Upper
138 100
108 11.5 8.1 12.1
92 110.0 90.4 135.6


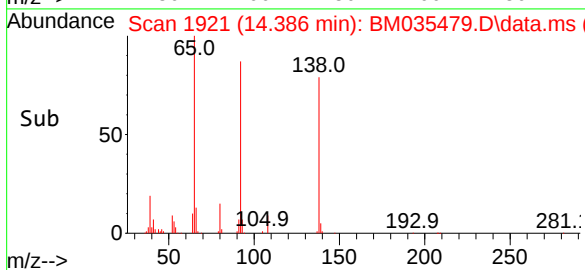

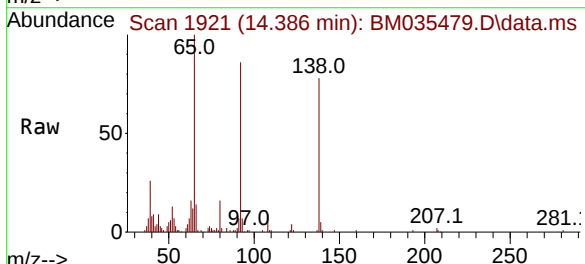




#52
Acenaphthene
Concen: 9.278 ng/ul
RT: 14.521 min Scan# 1944
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:153 Resp: 317407
Ion Ratio Lower Upper
153 100
152 48.2 37.1 55.7
154 88.6 71.3 106.9

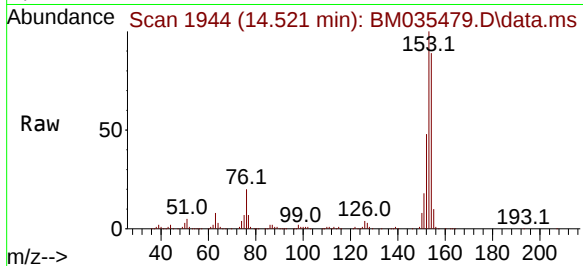

#53
2,4-Dinitrophenol
Concen: 4.163 ng/ul
RT: 14.627 min Scan# 1962
Delta R.T. 0.018 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:184 Resp: 21751
Ion Ratio Lower Upper
184 100
63 67.0 54.2 81.4
154 57.1 49.3 73.9




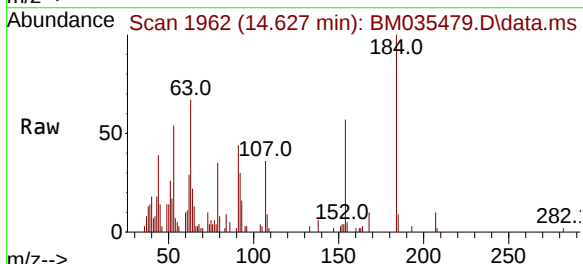




#55
4-Nitrophenol
Concen: 2.264 ng/ul
RT: 14.745 min Scan# 1977
Delta R.T. 0.029 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:109 Resp: 15055
Ion Ratio Lower Upper
109 100
139 150.5 124.9 187.3
65 140.5 122.2 183.4

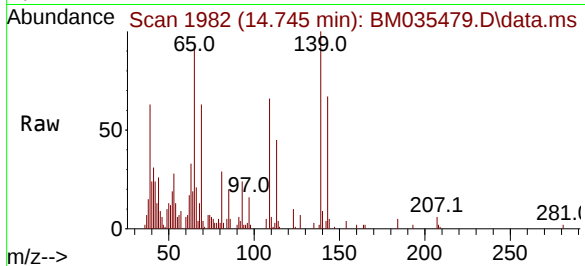

#56
Dibenzofuran
Concen: 9.356 ng/ul
RT: 14.857 min Scan# 2001
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:168 Resp: 447647
Ion Ratio Lower Upper
168 100
139 36.7 30.1 45.1




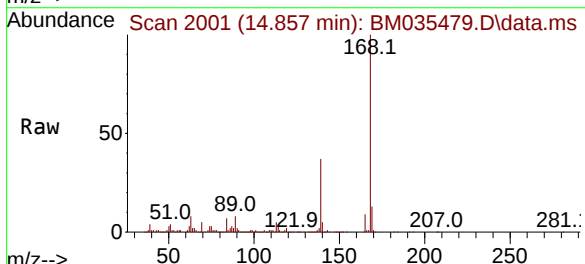




#57
2,4-Dinitrotoluene
Concen: 8.664 ng/ul
RT: 14.845 min Scan# 1999
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:165 Resp: 97034
Ion Ratio Lower Upper
165 100
63 53.9 35.9 53.9
182 2.4 2.5 3.7#

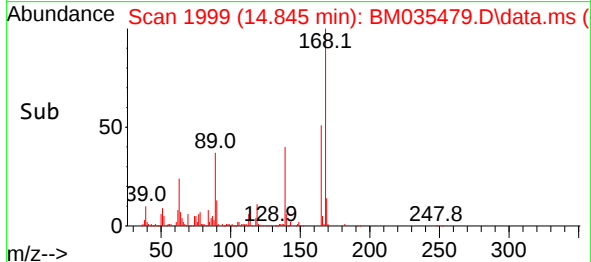

#58
2,3,4,6-Tetrachlorophenol
Concen: 7.910 ng/ul
RT: 15.098 min Scan# 2042
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:232 Resp: 76672
Ion Ratio Lower Upper
232 100
131 47.9 36.7 55.1
130 2.6 1.7 2.5#
166 32.5 24.4 36.6









#59
Diethylphthalate
Concen: 8.998 ng/ul
RT: 15.280 min Scan# 2073
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:149 Resp: 364858
Ion Ratio Lower Upper
149 100
177 20.8 16.8 25.2
150 12.5 10.2 15.4



#61
Fluorene
Concen: 9.407 ng/ul
RT: 15.504 min Scan# 2111
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:166 Resp: 366187
Ion Ratio Lower Upper
166 100
165 98.9 77.2 115.8
167 13.3 11.0 16.4









#62
4-Chlorophenyl-phenylether
Concen: 8.728 ng/ul
RT: 15.498 min Scan# 2110
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:204 Resp: 172481
Ion Ratio Lower Upper
204 100
206 32.9 25.9 38.9
141 64.5 50.6 75.8



#63
4-Nitroaniline
Concen: 6.729 ng/ul
RT: 15.551 min Scan# 2119
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:138 Resp: 46625
Ion Ratio Lower Upper
138 100
92 50.7 39.2 58.8
108 67.6 51.6 77.4









#66
4,6-Dinitro-2-methylphenol
Concen: 6.806 ng/ul
RT: 15.610 min Scan# 2129
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:198 Resp: 48832
Ion Ratio Lower Upper
198 100
182 7.3 4.2 6.4#
77 25.8 19.9 29.9

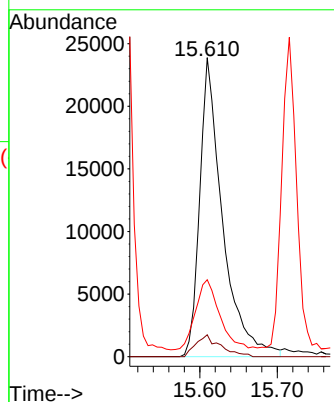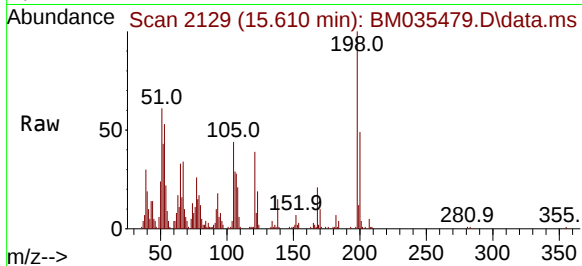

#67
N-Nitrosodiphenylamine
Concen: 9.217 ng/ul
RT: 15.715 min Scan# 2147
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:169 Resp: 309095
Ion Ratio Lower Upper
169 100
168 66.1 53.8 80.6
167 35.2 28.7 43.1



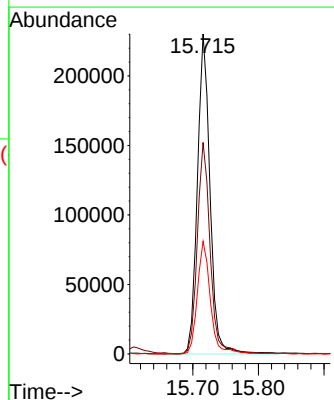
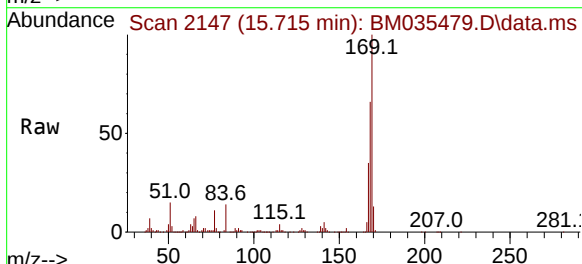




#68
4-Bromophenyl-phenylether
Concen: 8.433 ng/ul
RT: 16.392 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:248 Resp: 99006
Ion Ratio Lower Upper
248 100
250 95.4 77.3 115.9
141 74.8 59.8 89.8



#69
Hexachlorobenzene
Concen: 8.776 ng/ul
RT: 16.515 min Scan# 2283
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:284 Resp: 117655
Ion Ratio Lower Upper
284 100
142 34.3 28.6 42.8
249 30.0 24.6 37.0





#70

Atrazine

Concen: 7.850 ng/ul

RT: 16.674 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion:200 Resp: 102713

Ion Ratio Lower Upper

200 100

173 27.7 21.3 31.9

215 46.8 39.0 58.6



#71

Pentachlorophenol

Concen: 5.360 ng/ul

RT: 16.880 min Scan# 2345

Delta R.T. 0.006 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03




Tgt Ion:266 Resp: 48019


Ion Ratio Lower Upper

266 100

264 65.9 49.5 74.3

268 60.2 51.0 76.4









#72
Phenanthrene
Concen: 9.581 ng/u1
RT: 17.245 min Scan# 2407
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:178 Resp: 575108
Ion Ratio Lower Upper
178 100
179 14.7 12.2 18.2
176 18.5 14.9 22.3

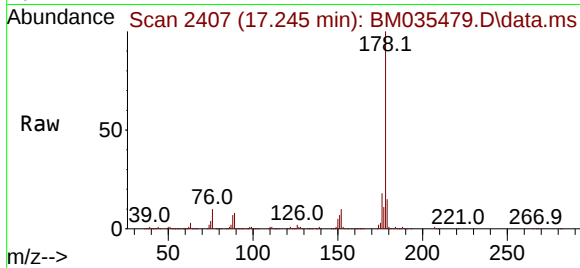

#74
Anthracene
Concen: 9.530 ng/u1
RT: 17.339 min Scan# 2423
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:178 Resp: 582912
Ion Ratio Lower Upper
178 100
179 14.8 12.2 18.2
176 17.0 14.4 21.6


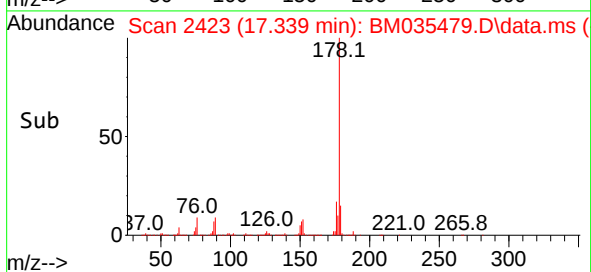

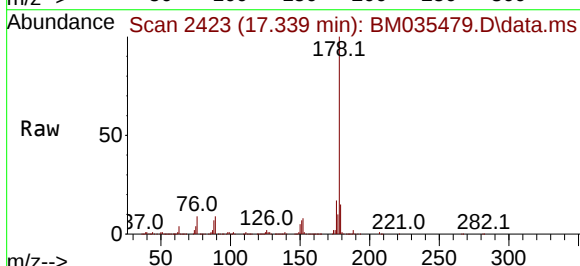




#75
1,2,3,4-Tetrachlorobenzene
Concen: 8.199 ng/uL
RT: 13.257 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:216 Resp: 158329
Ion Ratio Lower Upper
216 100
214 77.2 60.9 91.3
218 48.6 37.5 56.3



#76
Pentachlorobenzene
Concen: 8.621 ng/uL
RT: 14.780 min Scan# 1988
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:250 Resp: 143006
Ion Ratio Lower Upper
250 100
248 62.0 50.4 75.6
252 60.1 51.1 76.7









#77
 Carbazole
 Concen: 9.522 ng/ul
 RT: 17.615 min Scan# 2470
 Delta R.T. 0.000 min
 Lab File: BM035479.D
 Acq: 16 Jun 2022 14:03




Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048


Tgt Ion:167 Resp: 515449
 Ion Ratio Lower Upper
 167 100
 166 20.8 17.4 26.0
 139 12.9 10.1 15.1

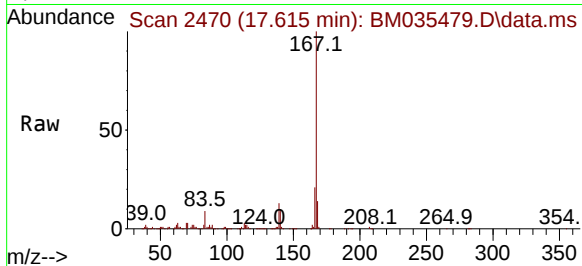

#78
 Di-n-butylphthalate
 Concen: 8.503 ng/ul
 RT: 18.174 min Scan# 2565
 Delta R.T. 0.000 min
 Lab File: BM035479.D
 Acq: 16 Jun 2022 14:03

Tgt Ion:149 Resp: 658688
 Ion Ratio Lower Upper
 149 100
 150 9.4 7.3 10.9
 104 4.5 3.7 5.5




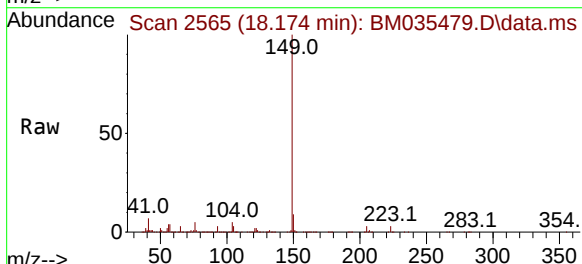




#80
Fluoranthene
Concen: 8.770 ng/ul
RT: 19.268 min Scan# 2751
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:202 Resp: 648571
Ion Ratio Lower Upper
202 100
101 12.1 10.1 15.1
100 9.9 7.8 11.6

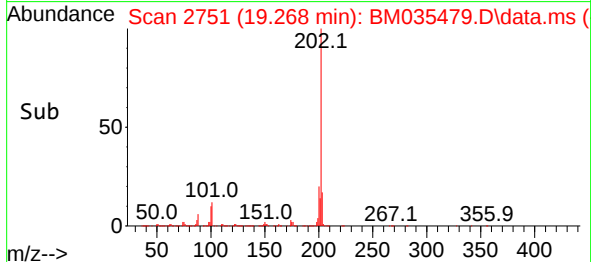

#82
Pyrene
Concen: 8.941 ng/ul
RT: 19.627 min Scan# 2812
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:202 Resp: 680630
Ion Ratio Lower Upper
202 100
101 15.3 11.9 17.9
100 13.3 10.2 15.4









#83
Butylbenzylphthalate
Concen: 8.562 ng/ul
RT: 20.527 min Scan# 2965
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:149 Resp: 279178
Ion Ratio Lower Upper
149 100
91 69.6 53.2 79.8
206 18.8 16.0 24.0



#84
3,3'-Dichlorobenzidine
Concen: 8.778 ng/ul
RT: 21.315 min Scan# 3099
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:252 Resp: 208613
Ion Ratio Lower Upper
252 100
254 63.6 52.4 78.6
126 13.6 10.8 16.2









#85
Benzo(a)anthracene
Concen: 8.940 ng/ul
RT: 21.380 min Scan# 3110
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:228 Resp: 660270
Ion Ratio Lower Upper
228 100
229 19.6 15.6 23.4
226 25.8 21.7 32.5



#86
Bis(2-ethylhexyl)phthalate
Concen: 8.595 ng/ul
RT: 21.309 min Scan# 3098
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:149 Resp: 421418
Ion Ratio Lower Upper
149 100
167 26.7 21.5 32.3
279 4.0 3.4 5.2









#87
Chrysene
Concen: 9.289 ng/ul
RT: 21.433 min Scan# 3118
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:228 Resp: 668849
Ion Ratio Lower Upper
228 100
226 29.5 23.7 35.5
229 19.4 15.5 23.3

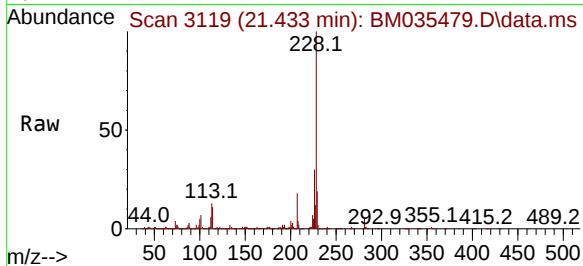

#89
Di-n-octyl phthalate
Concen: 8.265 ng/ul
RT: 22.209 min Scan# 3251
Delta R.T. 0.000 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:149 Resp: 739499



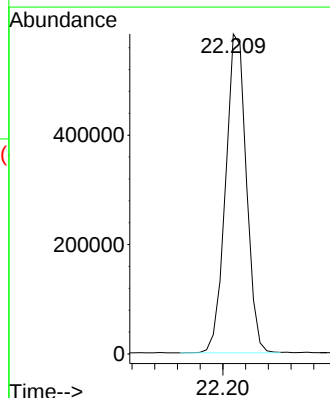
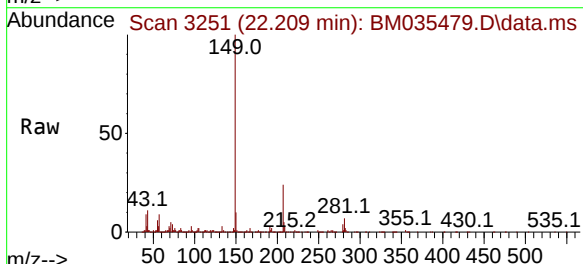




#90
Benzo(b)fluoranthene
Concen: 8.975 ng/ul
RT: 23.027 min Scan# 3389
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03




Instrument :
BNA_M
ClientSampleId :
SSTD010048


Tgt Ion:252 Resp: 728451
Ion Ratio Lower Upper
252 100
253 21.8 17.5 26.3
125 12.8 10.7 16.1



#91
Benzo(k)fluoranthene
Concen: 8.581 ng/ul
RT: 23.074 min Scan# 3398
Delta R.T. 0.006 min
Lab File: BM035479.D
Acq: 16 Jun 2022 14:03

Tgt Ion:252 Resp: 661648
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.0
125 12.0 10.6 15.8

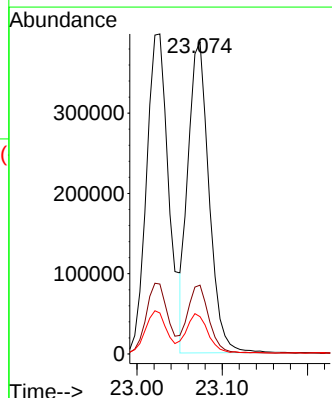



#93

Benzo(a)pyrene

Concen: 8.845 ng/ul

RT: 23.633 min Scan# 34

Delta R.T. 0.006 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03

Instrument :

BNA_M

ClientSampleId :

SSTD010048





Tgt Ion:252 Resp: 699419

Ion Ratio Lower Upper

252 100

253 22.0 17.3 25.9

125 14.3 11.8 17.8

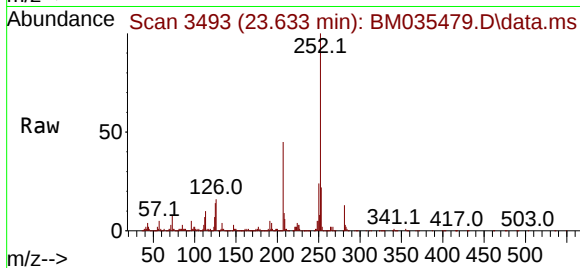

#94

Indeno(1,2,3-cd)pyrene

Concen: 9.058 ng/ul

RT: 26.156 min Scan# 3922

Delta R.T. 0.006 min

Lab File: BM035479.D

Acq: 16 Jun 2022 14:03




Tgt Ion:276 Resp: 823050


Ion Ratio Lower Upper

276 100

138 31.1 25.6 38.4

277 25.4 20.1 30.1




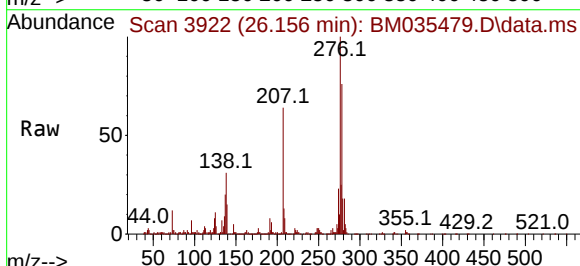




#95
 Dibenzo(a,h)anthracene
 Concen: 9.029 ng/ul
 RT: 26.162 min Scan# 3923
 Delta R.T. 0.000 min
 Lab File: BM035479.D
 Acq: 16 Jun 2022 14:03

Instrument :
 BNA_M
 ClientSampleId :
 SSTD010048

Tgt Ion:278 Resp: 704715
 Ion Ratio Lower Upper
 278 100
 139 21.0 16.2 24.2
 279 23.1 18.7 28.1



#96
 Benzo(g,h,i)perylene
 Concen: 9.224 ng/ul
 RT: 26.897 min Scan# 4048
 Delta R.T. 0.000 min
 Lab File: BM035479.D
 Acq: 16 Jun 2022 14:03

Tgt Ion:276 Resp: 697215
 Ion Ratio Lower Upper
 276 100
 138 26.5 21.3 31.9
 277 23.4 18.6 28.0

