

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061623\
 Data File : BM040277.D
 Acq On : 16 Jun 2023 12:51
 Operator : MA/JU
 Sample : PB153382BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK382

Quant Time: Jun 16 23:38:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 15 00:31:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.970	152	9060	0.400	ng/ul	0.00
4) Naphthalene-d8	10.778	136	32939	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.610	164	16635	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.349	188	27844	0.400	ng/ul	0.00
17) Chrysene-d12	21.526	240	13697	0.400	ng/ul	# 0.00
23) Perylene-d12	23.950	264	15585	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	73146	6.538	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.367	152	13557	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	15995	0.468	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.737	202	3181	0.066	ng/ul#	1
26) Benzo(a)pyrene	23.795	252	5760	0.122	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061623\
Data File : BM040277.D
Acq On : 16 Jun 2023 12:51
Operator : MA/JU
Sample : PB153382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK382

Quant Time: Jun 16 23:38:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 00:31:16 2023
Response via : Initial Calibration

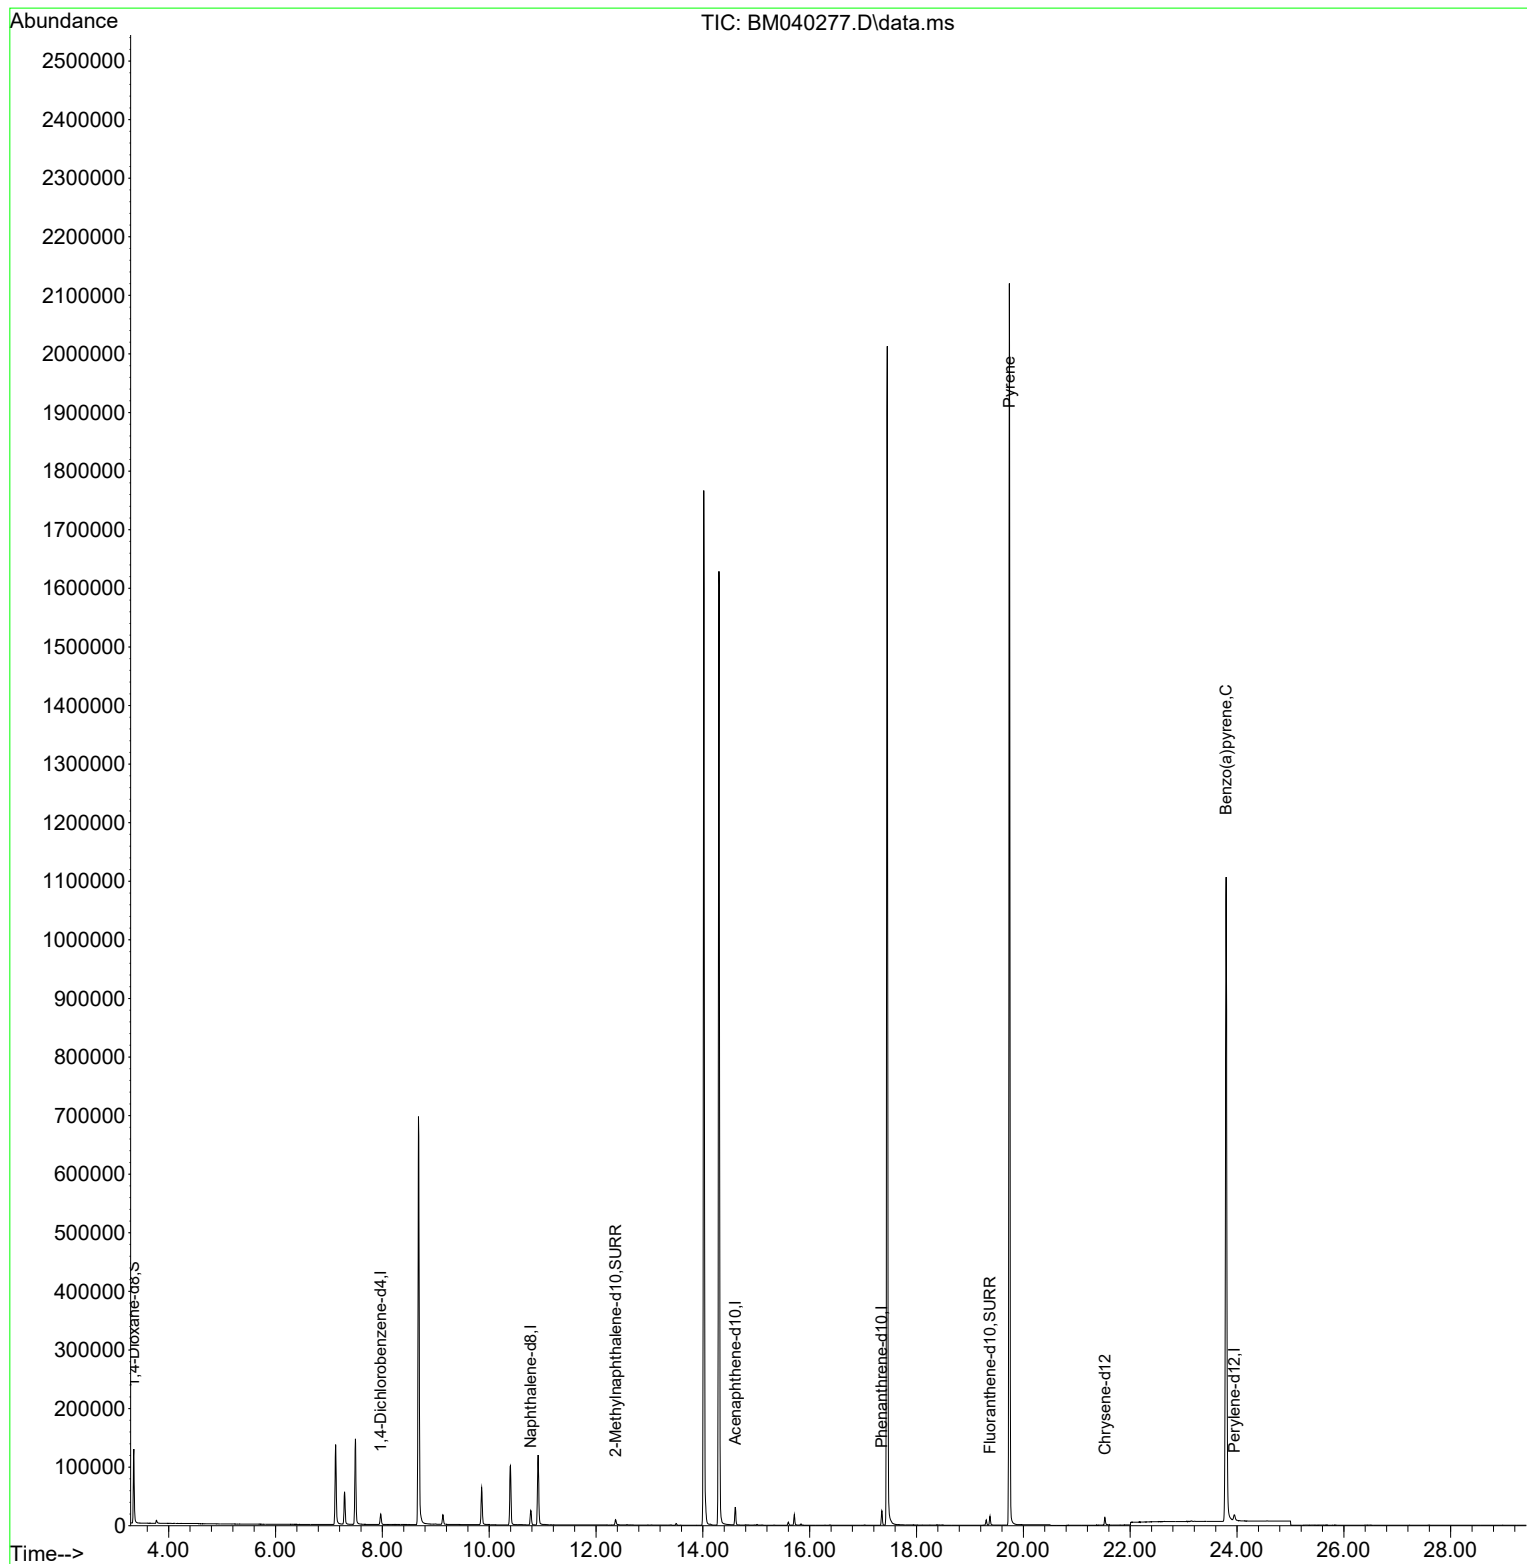

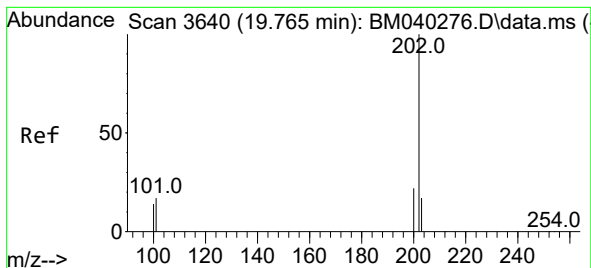

#20

Pyrene

Concen: 0.066 ng/ul

RT: 19.737 min Scan# 3

Delta R.T. -0.033 min

Lab File: BM040277.D

Acq: 16 Jun 2023 12:51

Instrument :

BNA_M

ClientSampleId :

SBLK382





Tgt Ion:202 Resp: 3181

Ion Ratio Lower Upper

202 100

101 176.5 11.8 17.8#

100 1339.9 9.3 13.9#

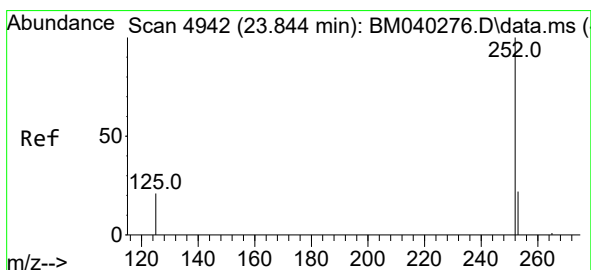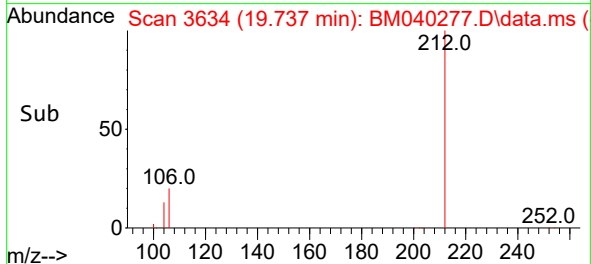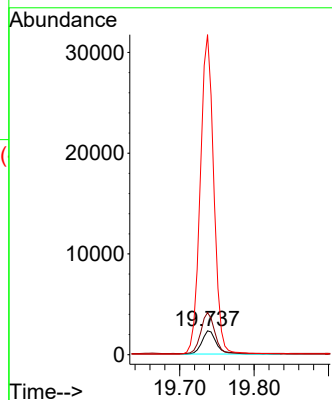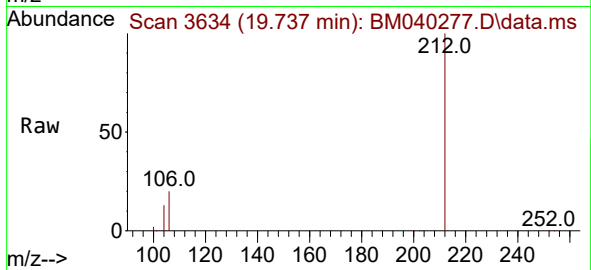

#26

Benzo(a)pyrene

Concen: 0.122 ng/ul

RT: 23.795 min Scan# 4925

Delta R.T. -0.056 min

Lab File: BM040277.D

Acq: 16 Jun 2023 12:51

Tgt Ion:252 Resp: 5760

Ion Ratio Lower Upper

252 100

253 51.2 23.4 35.0#

125 57.2 19.7 29.5#

