

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061719\
 Data File : BM020988.D
 Acq On : 17 Jun 2019 20:37
 Operator : HP/JU
 Sample : K3332-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A41W7

Quant Time: Jun 18 01:36:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 17 09:33:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	254125	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	1148259	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	779859	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1967458	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	2058714	20.00	ng/ul	0.00
85) Perylene-d12	23.64	264	2147431	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	25428	4.75	ng/uL	0.00
5) Phenol-d5	6.96	99	499192	22.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	332756	25.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	441666	24.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	423667	22.95	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	231393	24.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	266785	25.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	511749	24.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	653922	29.79	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1863956	26.45	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	2186571	25.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	242742	21.18	ng/ul	0.00
57) Fluorene-d10	15.43	176	1602265	26.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	230743	19.08	ng/ul	-0.01
70) Anthracene-d10	17.27	188	2633473	25.76	ng/ul	0.00
78) Pyrene-d10	19.57	212	3037899	24.59	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.49	264	3347938	26.42	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.89	163	304624	4.749	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061719\
Data File : BM020988.D
Acq On : 17 Jun 2019 20:37
Operator : HP/JU
Sample : K3332-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A41W7

Quant Time: Jun 18 01:36:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 17 09:33:39 2019
Response via : Initial Calibration

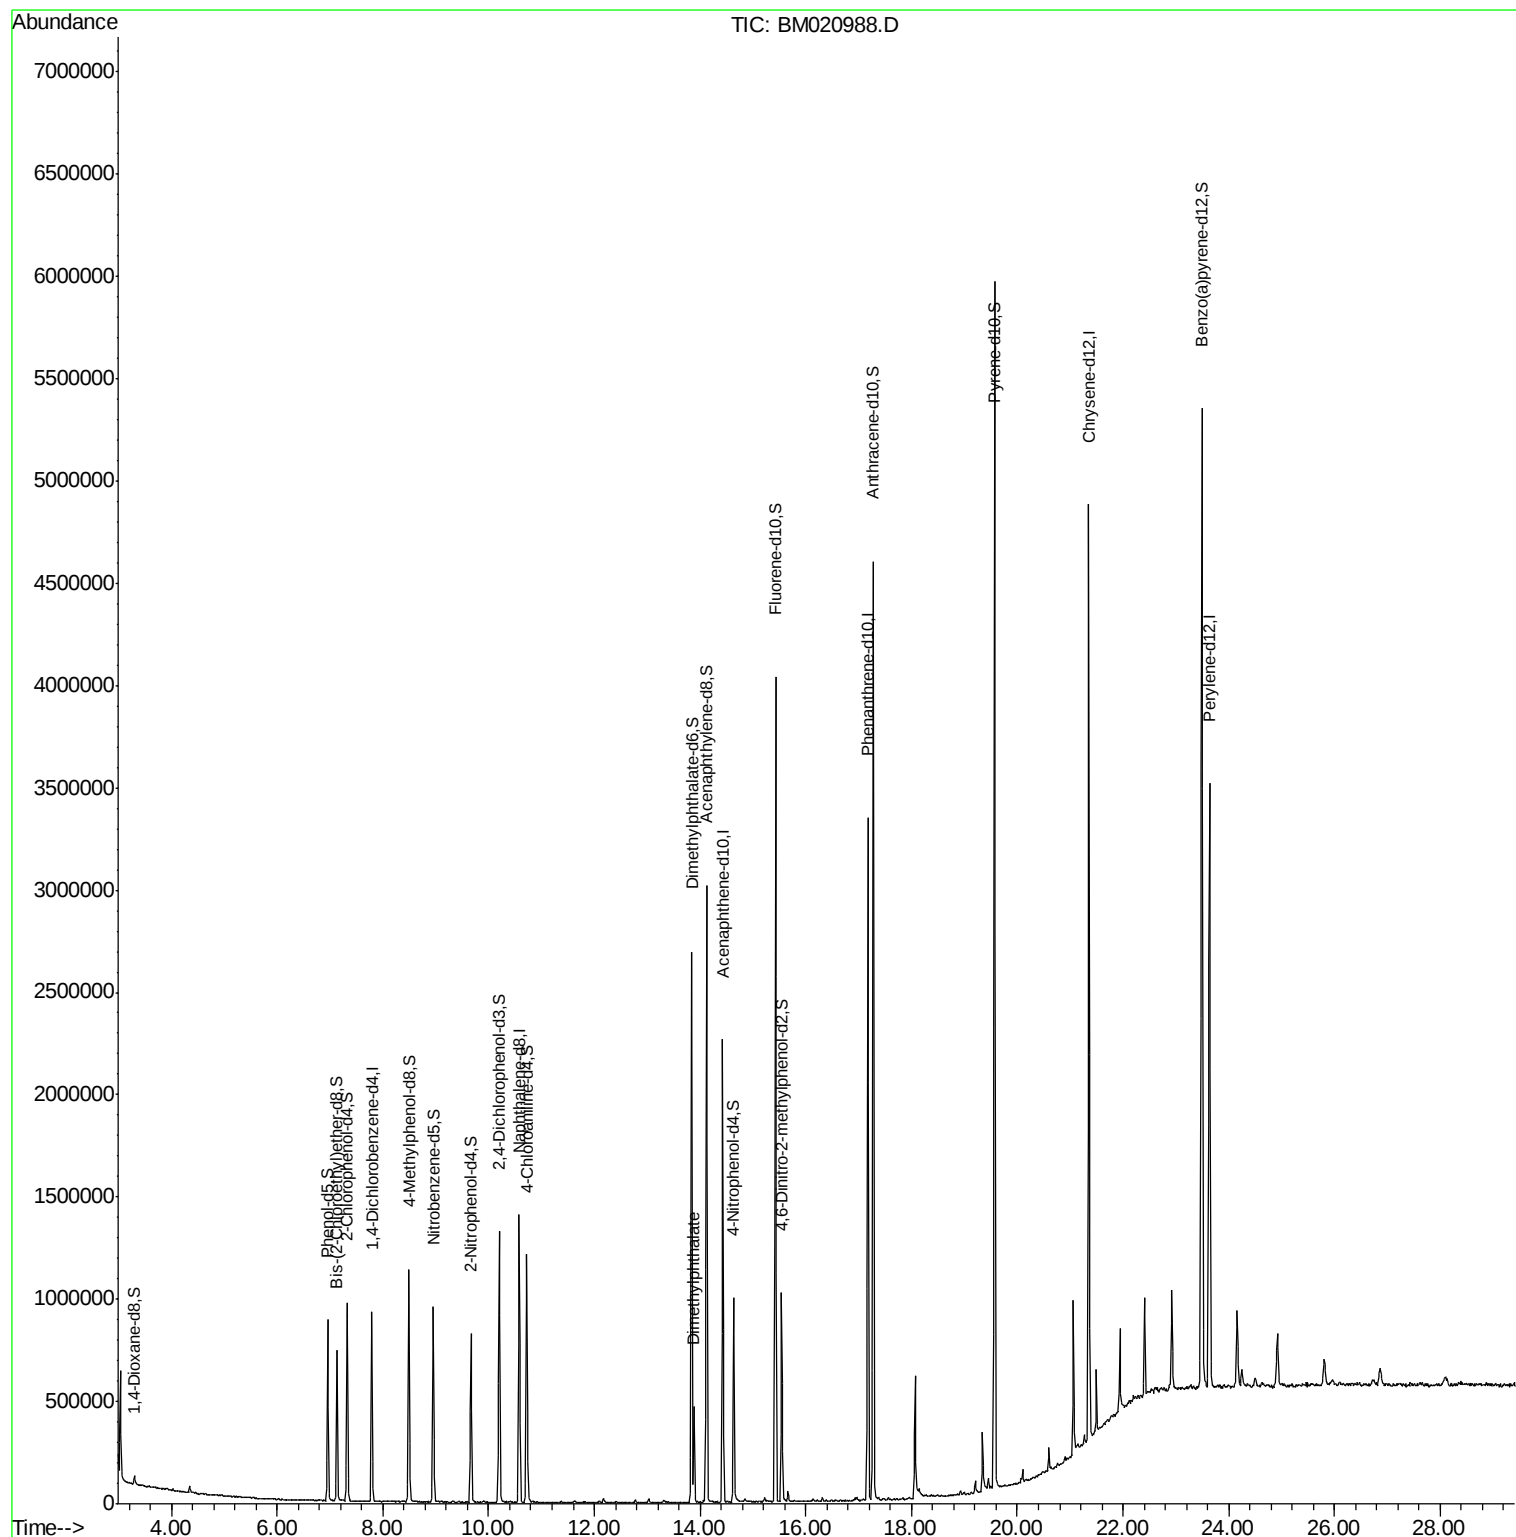

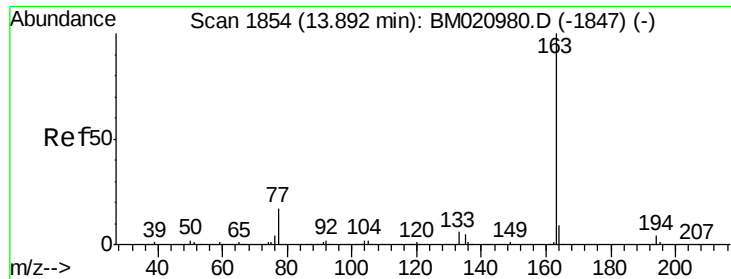

#44

Dimethylphthalate

Concen: 4.749 ng/ul

RT: 13.89 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BM020988.D

Acq: 17 Jun 2019 20:37

Instrument :

BNA_M

ClientSampleId :

A41W7


Tot Ion:163 Resp: 304624

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.2

164 10.1 7.7 11.5

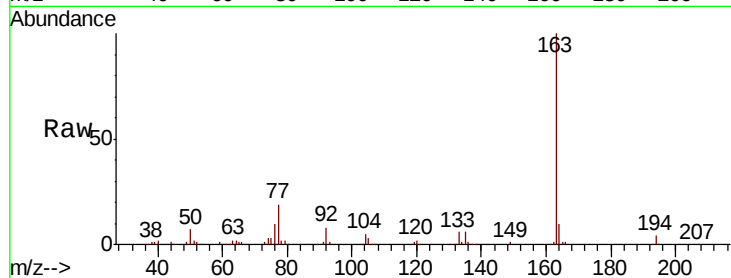

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

