

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
 Data File : BM026430.D
 Acq On : 17 Jun 2020 17:42
 Operator : JU/CG
 Sample : L2959-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG2J6

Quant Time: Jun 17 18:17:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 17 16:26:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	118632	20.00	ng/ul	0.00
18) Naphthalene-d8	10.15	136	557725	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	370022	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	827950	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	922851	20.00	ng/ul	0.00
86) Perylene-d12	23.12	264	989163	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.98	96	15846	4.68	ng/uL	0.00
5) Phenol-d5	6.60	99	273548	25.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.75	67	190066	27.49	ng/ul	0.00
9) 2-Chlorophenol-d4	6.93	132	210367	23.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.12	113	234172	27.22	ng/ul	0.00
19) Nitrobenzene-d5	8.54	128	111833	22.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.26	143	126941	23.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	219023	21.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.30	131	251752	24.05	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	731306	23.51	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	814389	21.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	101331	19.64	ng/ul	0.00
58) Fluorene-d10	15.06	176	573542	21.48	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	122650	22.63	ng/ul	0.00
71) Anthracene-d10	16.90	188	860418	20.42	ng/ul	0.00
79) Pyrene-d10	19.22	212	963558	19.04	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.98	264	980463	17.93	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.52	163	209982	6.499	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
Data File : BM026430.D
Acq On : 17 Jun 2020 17:42
Operator : JU/CG
Sample : L2959-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG2J6

Quant Time: Jun 17 18:17:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 17 16:26:10 2020
Response via : Initial Calibration

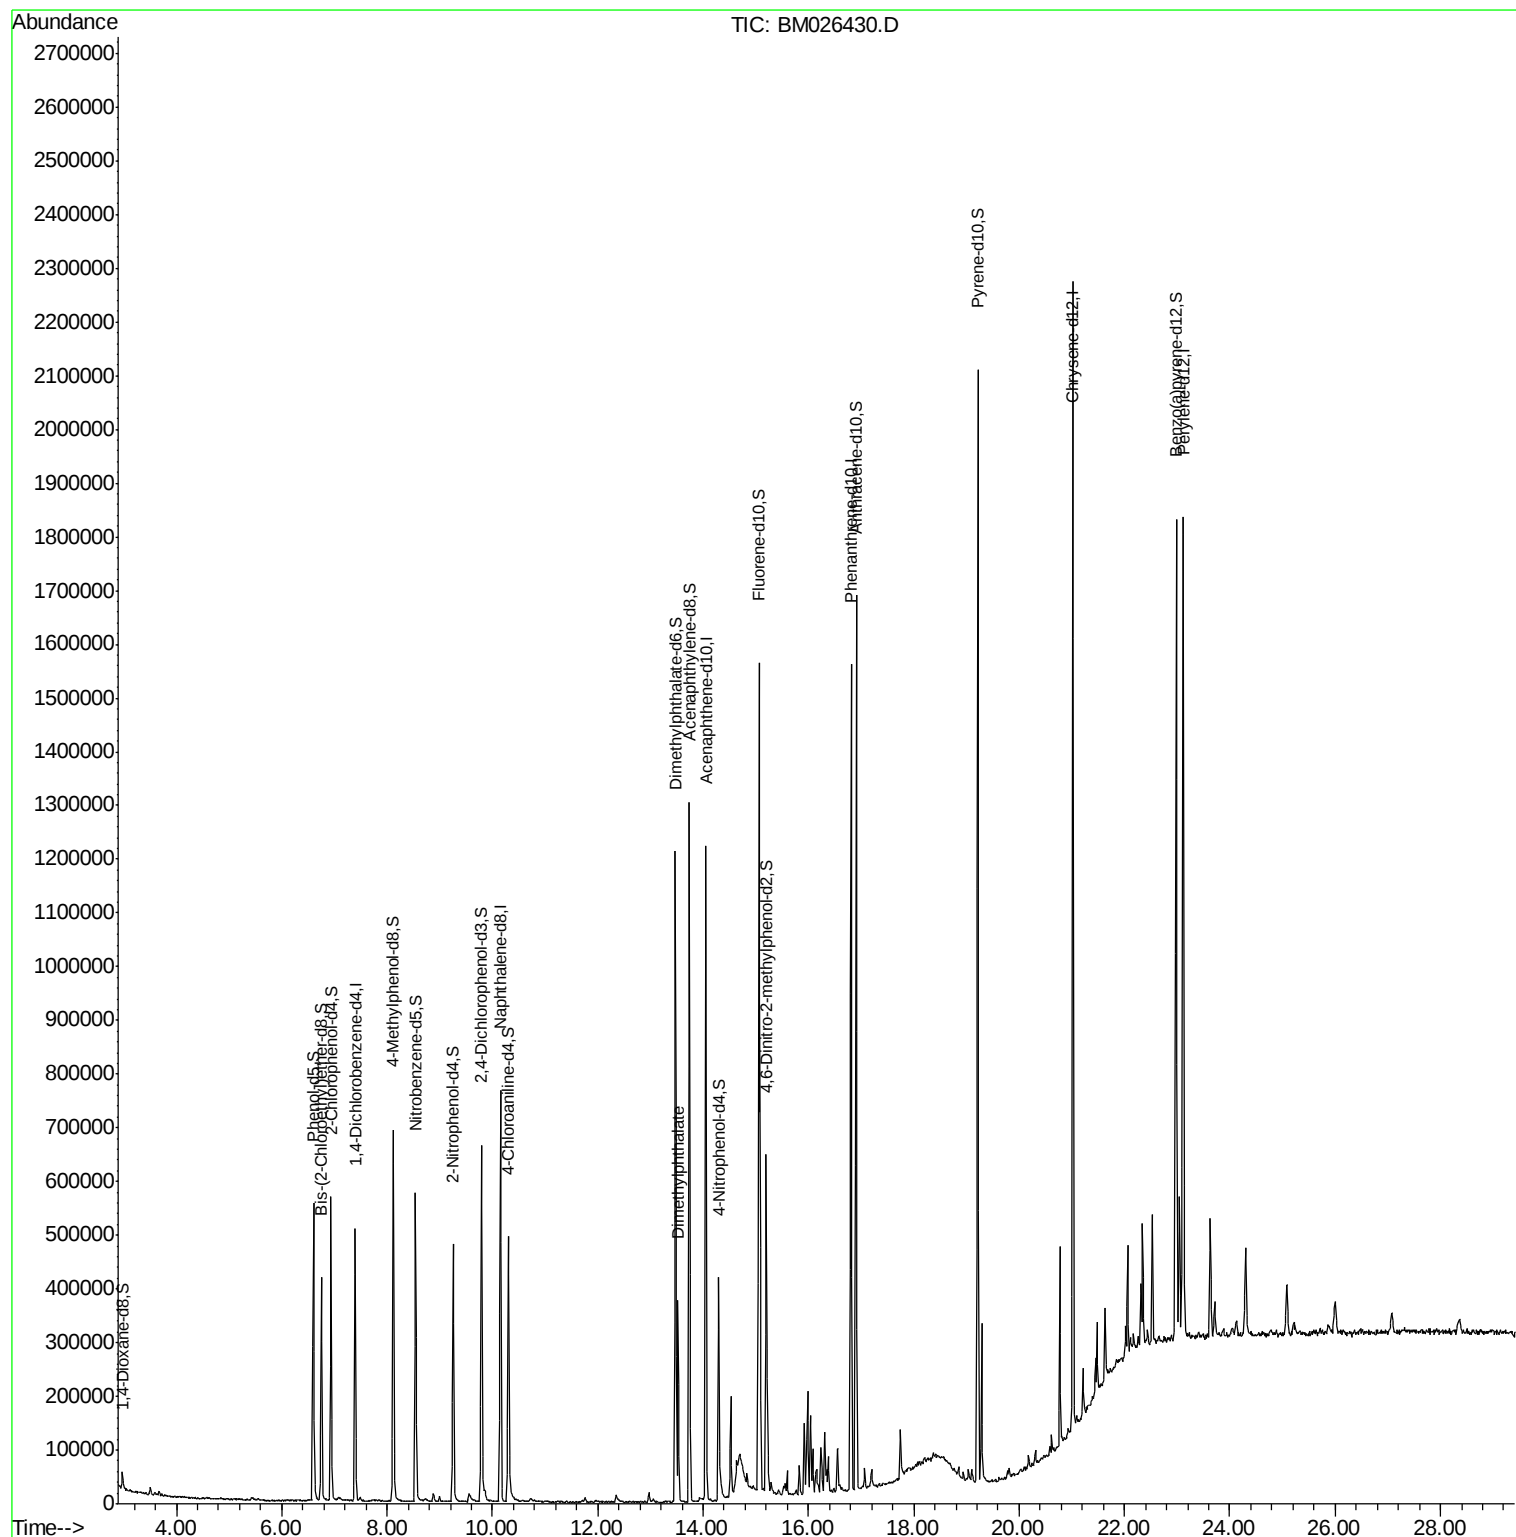

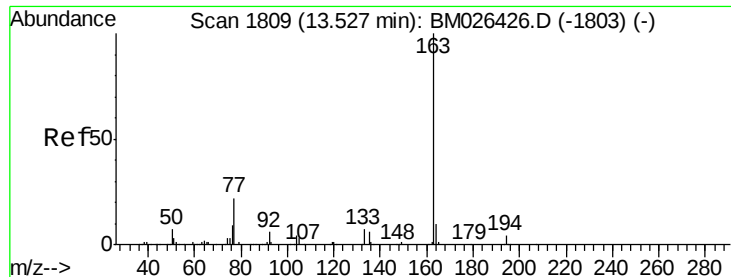

#45

Dimethylphthalate

Concen: 6.499 ng/ul

RT: 13.52 min Scan# 1808

Delta R.T. -0.01 min

Lab File: BM026430.D

Acq: 17 Jun 2020 17:42

Instrument :

BNA_M

ClientSampleId :

BG2J6

Tot Ion:163 Resp: 209982

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.4 7.8 11.6

