

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
 Data File : BM026451.D
 Acq On : 18 Jun 2020 06:56
 Operator : JU/CG
 Sample : L3006-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETXC9

Quant Time: Jun 18 08:45:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 18 04:30:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	114202	20.00	ng/ul	0.00
18) Naphthalene-d8	10.15	136	440346	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.05	164	283426	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.80	188	619947	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	511850	20.00	ng/ul	-0.01
86) Perylene-d12	23.10	264	437823	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	0.00	176	0	0.00	ng/ul	
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul	
79) Pyrene-d10	0.00	212	0	0.00	ng/ul	
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
77) Fluoranthene	18.87	202	44970	1.059	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
Data File : BM026451.D
Acq On : 18 Jun 2020 06:56
Operator : JU/CG
Sample : L3006-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETXC9

Quant Time: Jun 18 08:45:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 18 04:30:42 2020
Response via : Initial Calibration

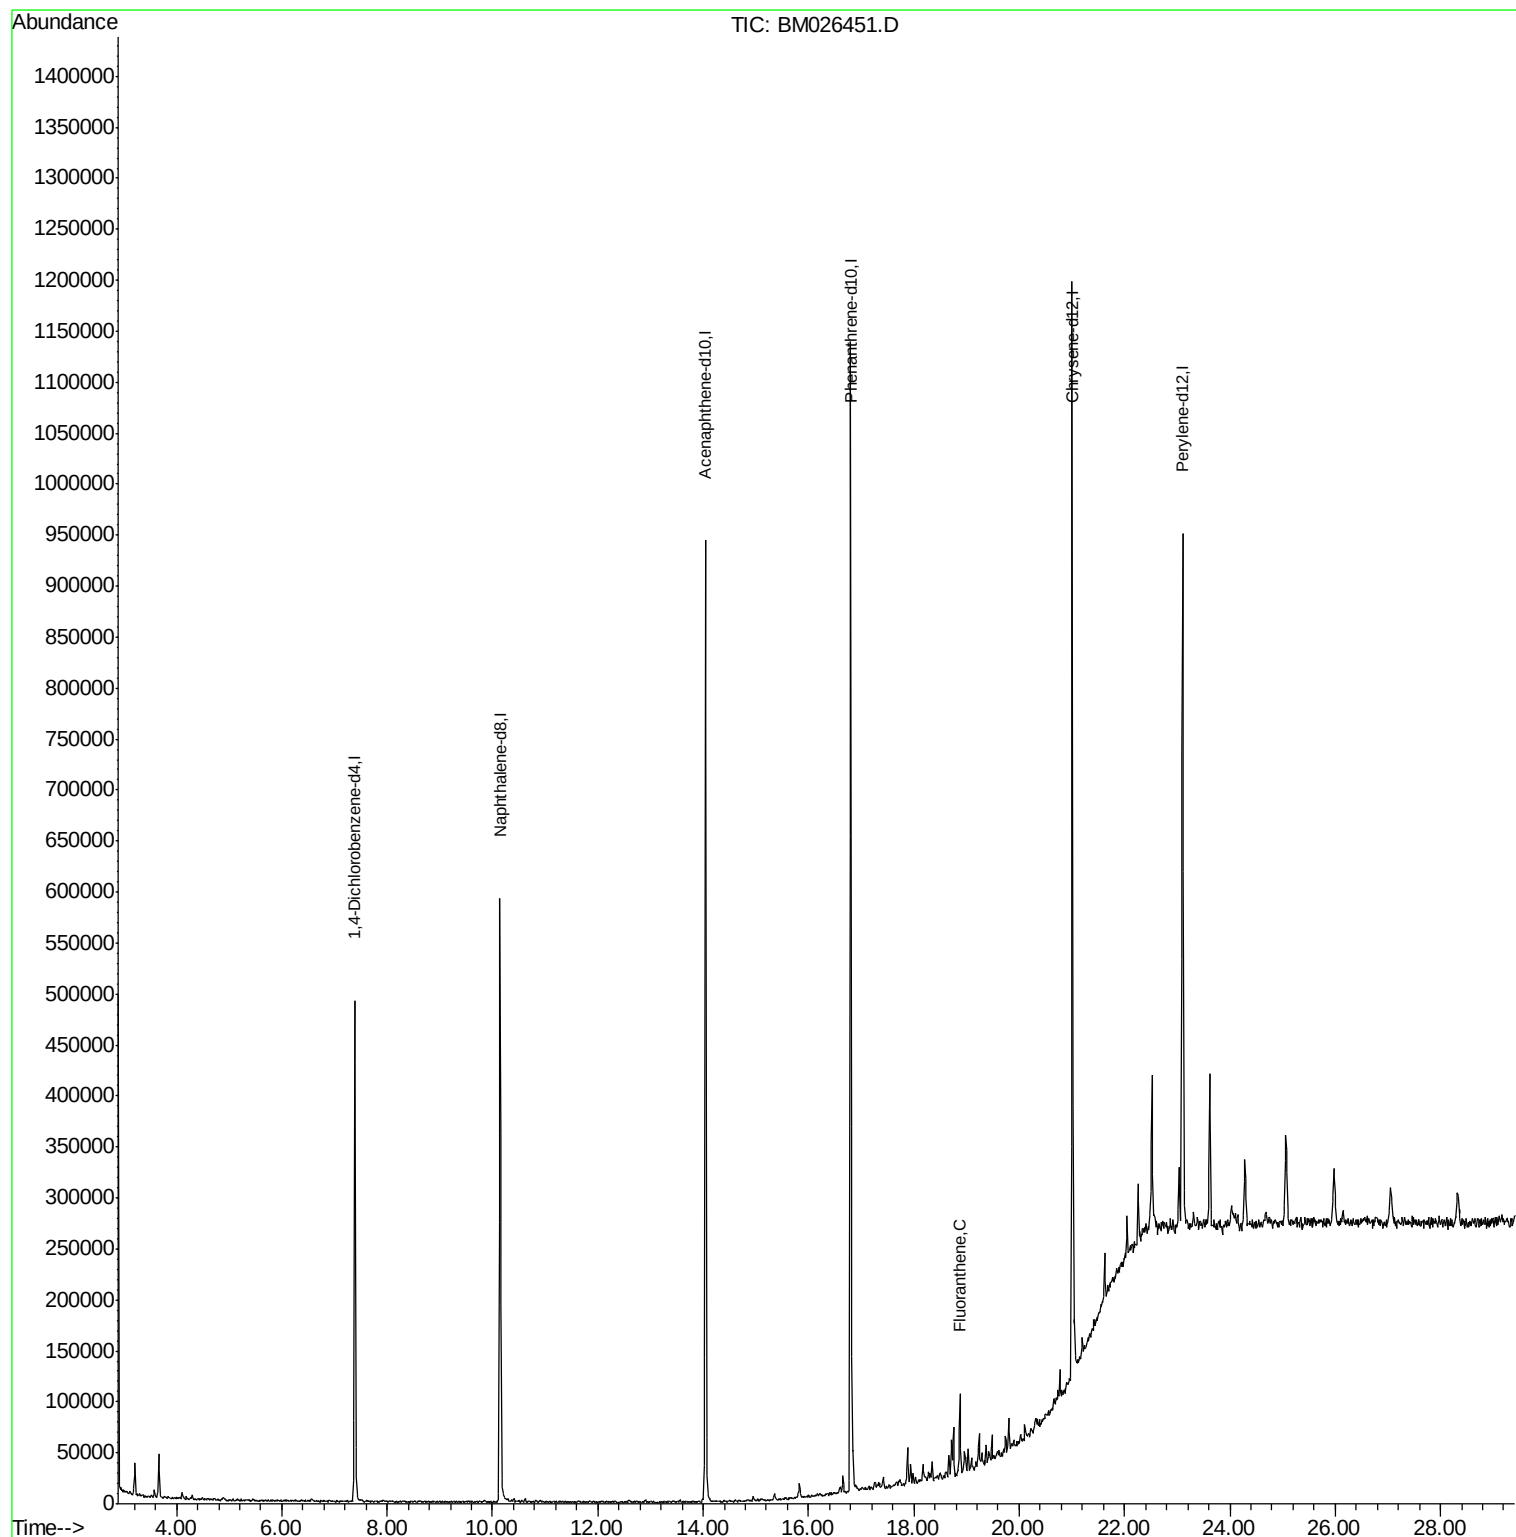

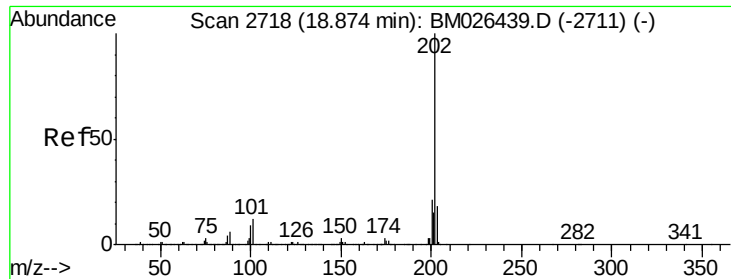

#77
 Fluoranthene
 Concen: 1.059 ng/ul
 RT: 18.87 min Scan# 2718
 Delta R.T. -0.01 min
 Lab File: BM026451.D
 Acq: 18 Jun 2020 06:56

Instrument :
 BNA_M
 ClientSampleId :
 ETXC9

Tot Ion	Ratio	Lower	Upper
202	100		
101	9.9	8.6	12.8
100	8.3	6.8	10.2

