

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
 Data File : BM026447.D
 Acq On : 18 Jun 2020 04:32
 Operator : JU/CG
 Sample : PB129466BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	51	54	57	rVB3	7304	7956	0.45%	0.106%
2	3.499	103	104	107	rBV3	2132	1920	0.11%	0.026%
3	3.663	128	132	139	rVB	5924	9478	0.53%	0.126%
4	4.134	210	212	215	rVB4	2004	2099	0.12%	0.028%
5	4.516	274	277	281	rBV4	1842	3139	0.18%	0.042%
6	4.599	286	291	294	rVV6	2111	4380	0.25%	0.058%
7	5.551	450	453	456	rVB4	1356	1872	0.11%	0.025%
8	5.746	483	486	489	rVB3	1956	2063	0.12%	0.027%
9	6.446	602	605	608	rBV5	1467	1817	0.10%	0.024%
10	6.934	684	688	691	rBV4	1348	1821	0.10%	0.024%
11	7.387	758	765	777	rBV	384942	600138	33.78%	7.999%
12	7.875	843	848	851	rBV5	1337	2274	0.13%	0.030%
13	10.145	1226	1234	1247	rBV	442954	781472	43.99%	10.415%
14	10.234	1247	1249	1251	rVV3	5111	5579	0.31%	0.074%
15	10.251	1251	1252	1256	rVV3	2624	3462	0.19%	0.046%
16	10.286	1256	1258	1263	rVB4	1597	2234	0.13%	0.030%
17	12.892	1699	1701	1706	rVB3	1191	1801	0.10%	0.024%
18	14.045	1891	1897	1913	rBV	716132	1085480	61.10%	14.467%
19	16.592	2325	2330	2336	rBV3	3162	5374	0.30%	0.072%
20	16.804	2360	2366	2380	rBV	1041129	1509235	84.95%	20.115%
21	16.910	2380	2384	2387	rVB6	3004	5799	0.33%	0.077%
22	17.280	2444	2447	2450	rBV4	1242	1899	0.11%	0.025%
23	17.368	2459	2462	2466	rBV4	2079	2708	0.15%	0.036%
24	17.404	2466	2468	2473	rVB4	1592	2206	0.12%	0.029%
25	18.204	2601	2604	2606	rBV5	2386	2664	0.15%	0.036%
26	21.015	3076	3082	3092	rBV	1336027	1776546	100.00%	23.678%
27	23.103	3431	3437	3447	rVB	997749	1677596	94.43%	22.359%


Sum of corrected areas: 7503012

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
Data File : BM026447.D
Acq On : 18 Jun 2020 04:32
Operator : JU/CG
Sample : PB129466BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

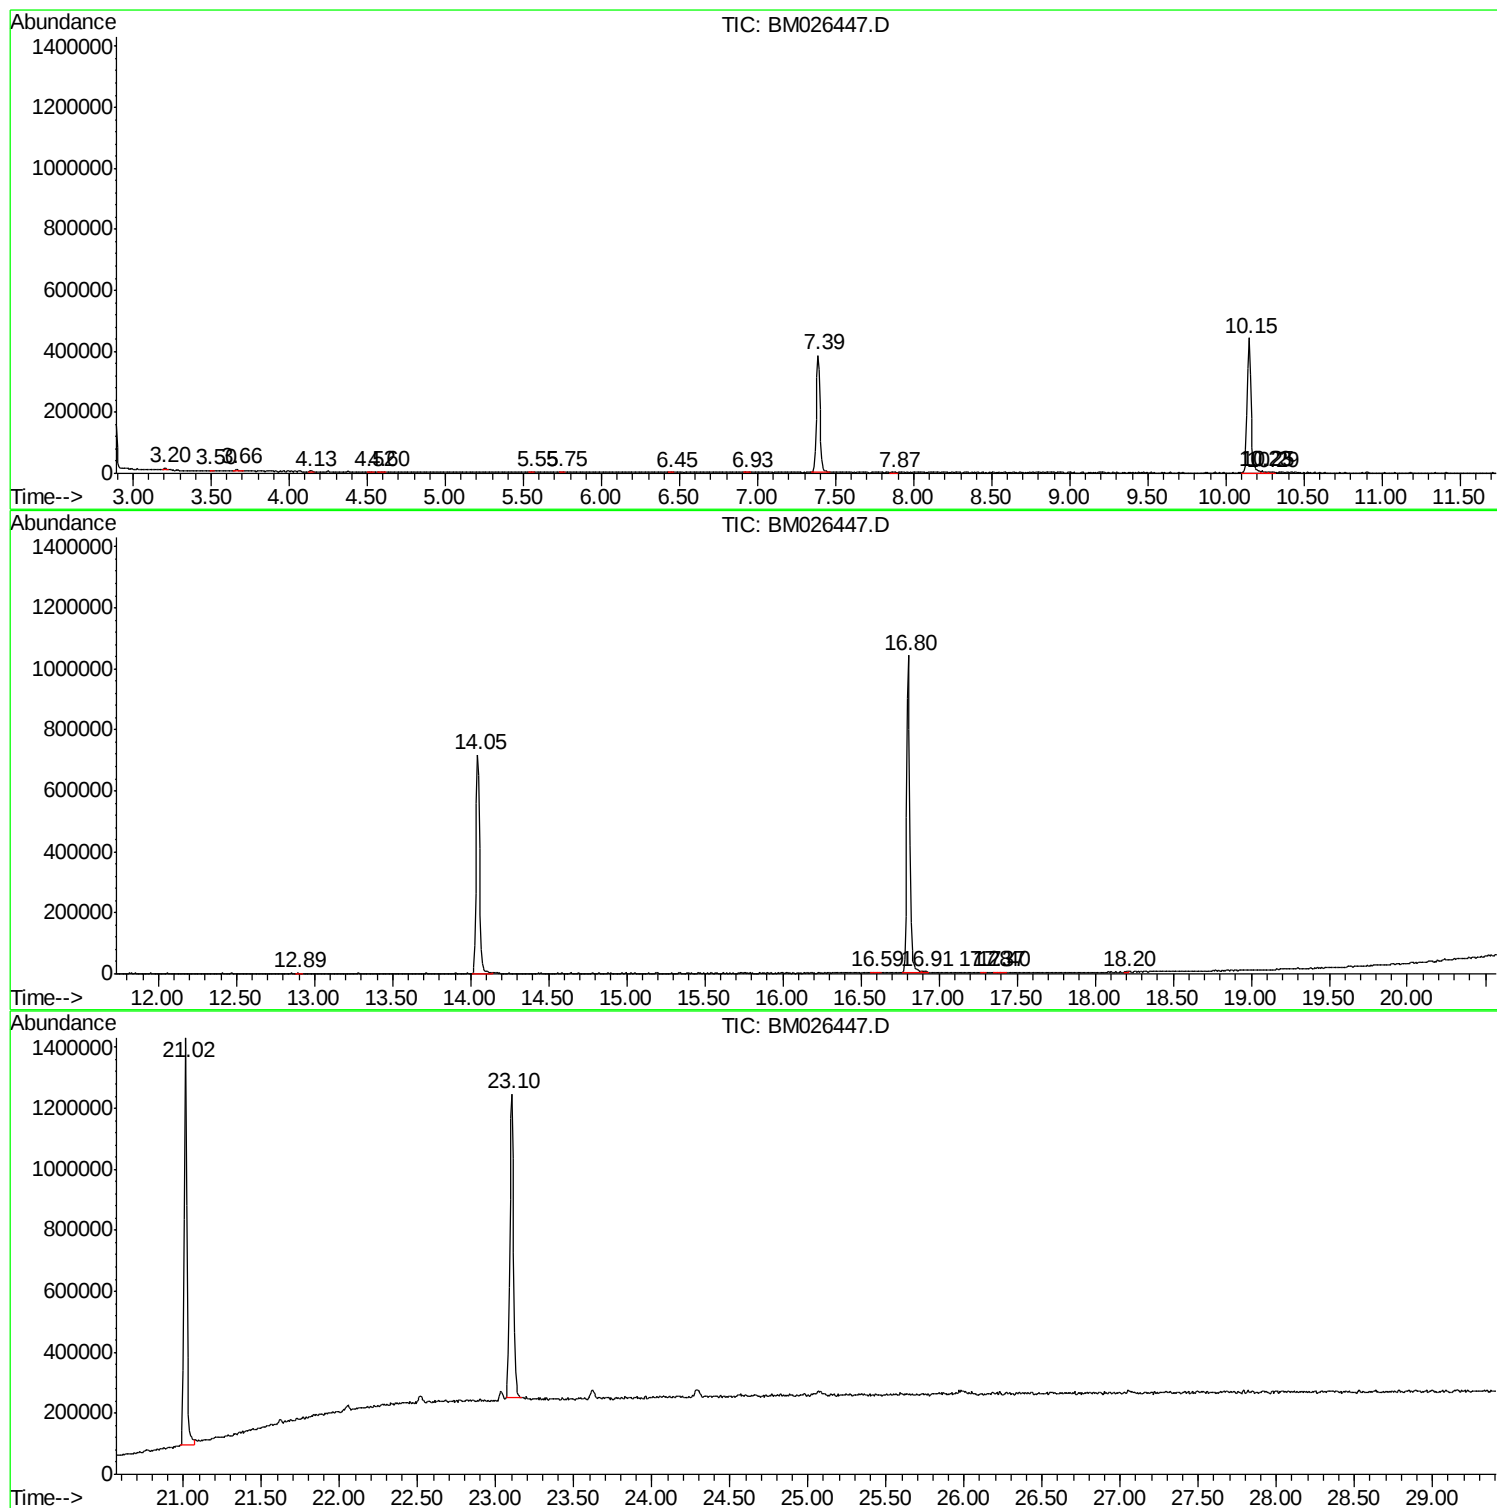

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061720\
Data File : BM026447.D
Acq On : 18 Jun 2020 04:32
Operator : JU/CG
Sample : PB129466BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061720\
Data File : BM026447.D
Acq On : 18 Jun 2020 04:32
Operator : JU/CG
Sample : PB129466BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc