

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
 Data File : BM026450.D
 Acq On : 18 Jun 2020 06:20
 Operator : JU/CG
 Sample : PB129525BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	51	54	58	rVB4	8239	9744	0.57%	0.134%
2	3.305	69	71	74	rBV3	1852	1811	0.11%	0.025%
3	3.663	128	132	135	rBV	7057	7175	0.42%	0.098%
4	3.805	155	156	158	rBV2	1829	1751	0.10%	0.024%
5	4.104	205	207	208	rBV2	2681	1853	0.11%	0.025%
6	4.163	215	217	220	rBV4	1400	1918	0.11%	0.026%
7	4.593	287	290	293	rBV5	2199	3272	0.19%	0.045%
8	5.169	386	388	391	rBV4	1594	1993	0.12%	0.027%
9	5.228	396	398	402	rBV4	1343	2068	0.12%	0.028%
10	7.387	756	765	778	rBV	409684	630775	37.04%	8.657%
11	10.145	1227	1234	1246	rBV	462673	792238	46.52%	10.873%
12	10.681	1319	1325	1326	rBV3	1226	1705	0.10%	0.023%
13	14.045	1891	1897	1917	rBV	698604	1046369	61.44%	14.361%
14	16.592	2326	2330	2333	rBV3	3214	4299	0.25%	0.059%
15	16.804	2360	2366	2385	rBV	929876	1395297	81.93%	19.149%
16	17.057	2405	2409	2412	rVB5	1149	1951	0.11%	0.027%
17	17.439	2471	2474	2477	rVB4	1424	1943	0.11%	0.027%
18	18.527	2656	2659	2660	rBV3	2093	2172	0.13%	0.030%
19	18.615	2672	2674	2677	rBV4	2069	1976	0.12%	0.027%
20	19.080	2751	2753	2756	rBV4	2412	2541	0.15%	0.035%
21	19.145	2762	2764	2766	rBV2	2415	2485	0.15%	0.034%
22	21.015	3077	3082	3093	rBV	1350206	1702950	100.00%	23.372%
23	23.103	3431	3437	3448	rVB	972333	1668114	97.95%	22.894%


Sum of corrected areas: 7286400

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061720\
Data File : BM026450.D
Acq On : 18 Jun 2020 06:20
Operator : JU/CG
Sample : PB129525BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

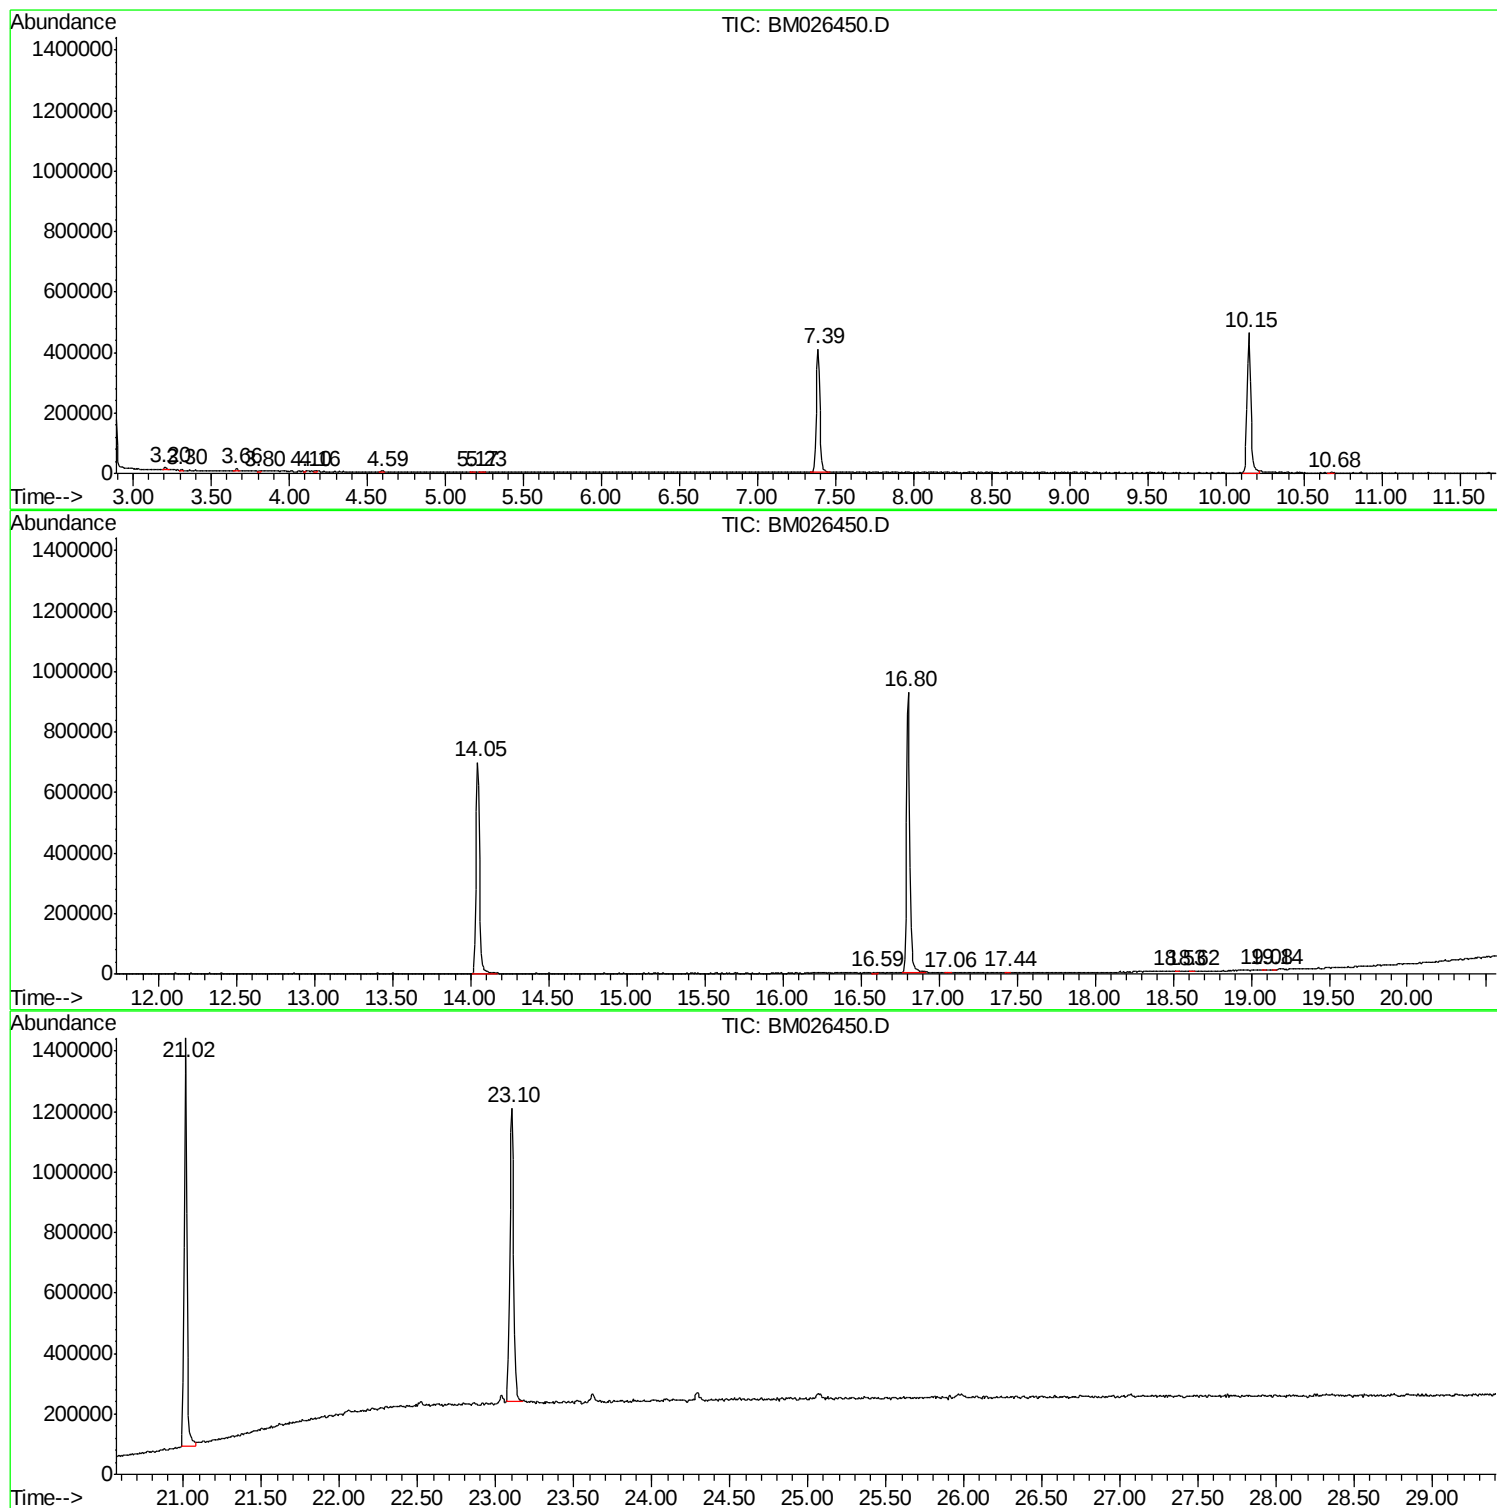

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061720\
Data_File : BM026450.D
Acq_On : 18-Jun-2020 06:200
Operator : JU/CGG
Sample : PB129525BLL
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
SBLK25

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
