

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015698.D
 Acq On : 18 Jun 2018 18:40
 Operator : SJ/JU
 Sample : PB110347BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 19 04:38:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:38:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	72915	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	326843	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	193556	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.67	188	462377	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	557241	20.00	ng/ul	0.00
85) Perylene-d12	24.19	264	611252	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	11172	7.45	ng/uL	0.00
5) Phenol-d5	7.47	99	206183	31.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.64	67	140397	35.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.85	132	179259	35.42	ng/ul	0.00
13) 4-Methylphenol-d8	9.04	113	173003	30.34	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	86260	39.25	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	93455	39.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	167628	34.25	ng/ul	0.00
29) 4-Chloroaniline-d4	11.30	131	246823	45.25	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	671404	41.90	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	723166	41.84	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	99254	32.09	ng/ul	0.00
57) Fluorene-d10	15.93	176	542537	40.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	88076	31.62	ng/ul	0.00
70) Anthracene-d10	17.77	188	905879	42.98	ng/ul	0.00
78) Pyrene-d10	20.02	212	1072180	44.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	1334432	43.55	ng/ul	0.00

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	9.03	70	4933	1.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015698.D
 Acq On : 18 Jun 2018 18:40
 Operator : SJ/JU
 Sample : PB110347BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :


Quant Time: Jun 19 04:38:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:38:16 2018
 Response via : Initial Calibration

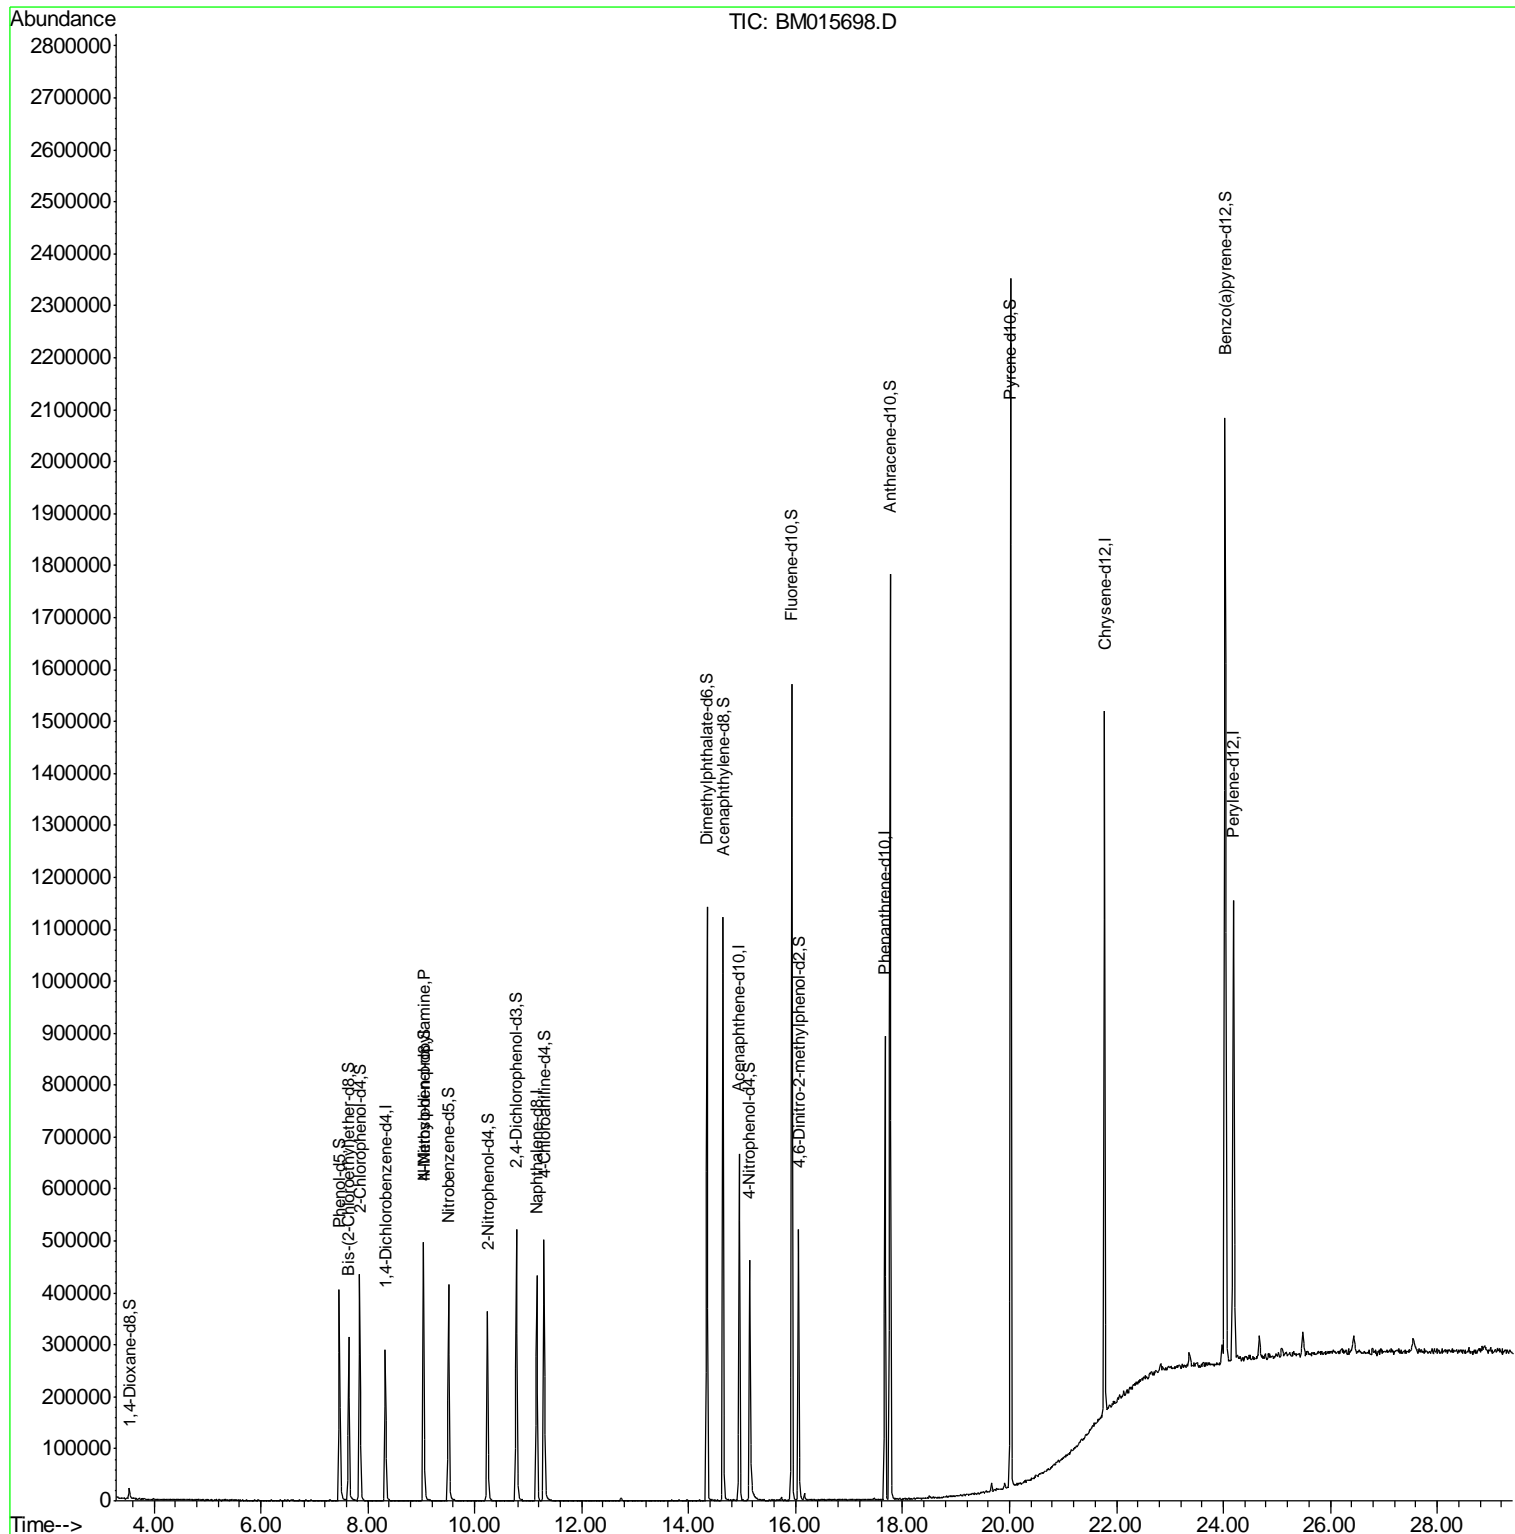

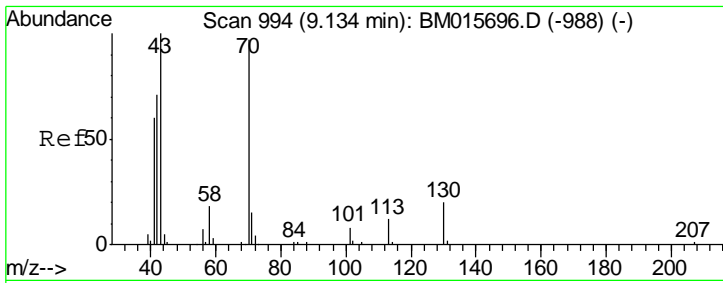

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.045 ng/ul
 RT: 9.03 min Scan# 977
 Delta R.T. -0.10 min
 Lab File: BM015698.D
 Acq: 18 Jun 2018 18:40

Instrument :
 BNA_M
ClientSampled :

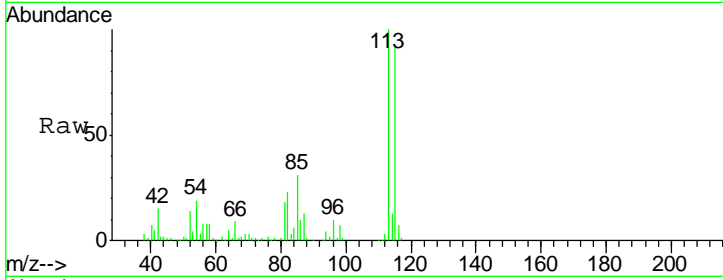

Tot Ion	Ion	Resp	Lower	Upper
4933	70	100		
	42	449.9	35.4	53.0#
	101	0.0	8.4	12.6#
	130	0.0	18.2	27.4#

