

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015694.D
 Acq On : 18 Jun 2018 11:56
 Operator : SJ/JU
 Sample : J3506-01DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C07Z8DL

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:24 PM

Quant Time: Jun 19 04:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:16:21 2018
 Response via : Initial Calibration

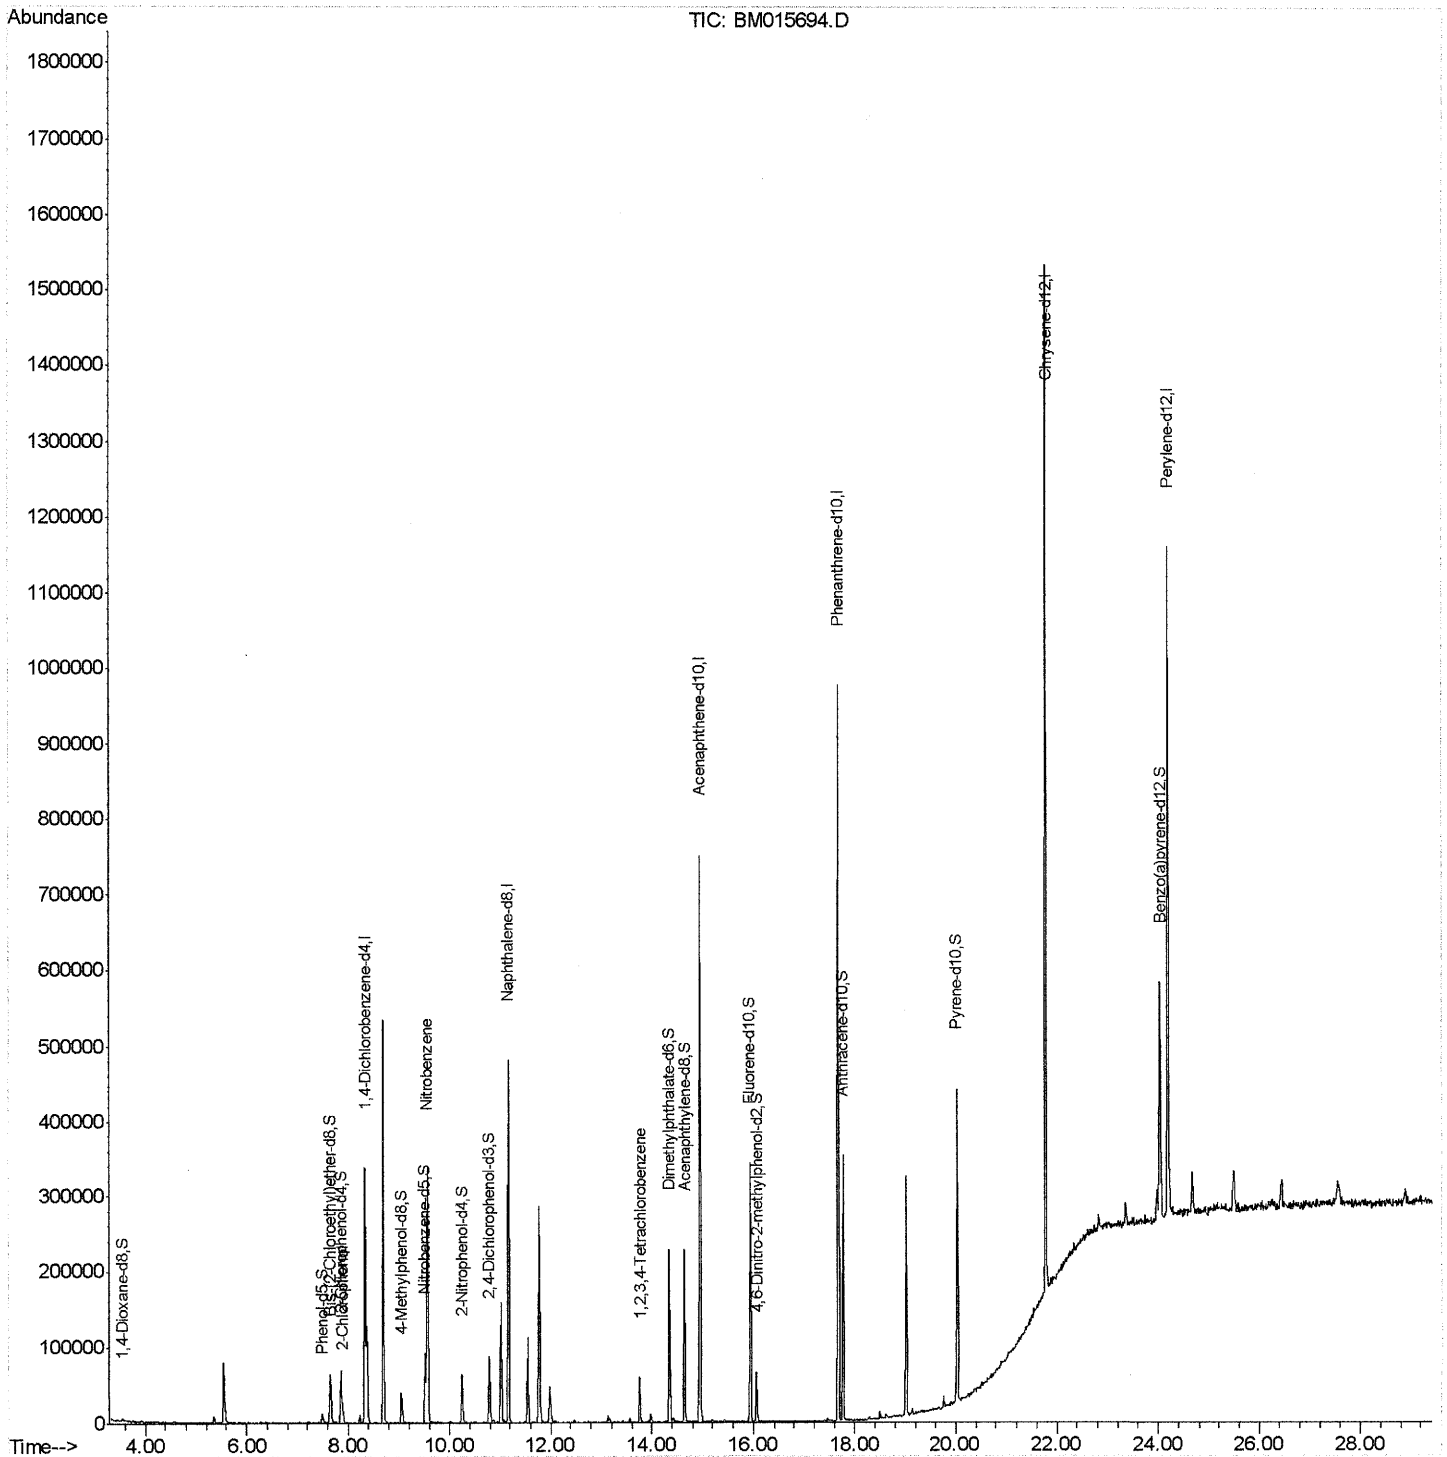

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015694.D
 Acq On : 18 Jun 2018 11:56
 Operator : SJ/JU
 Sample : J3506-01DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C07Z8DL

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:24 PM

Quant Time: Jun 19 04:16:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:16:21 2018
 Response via : Initial Calibration

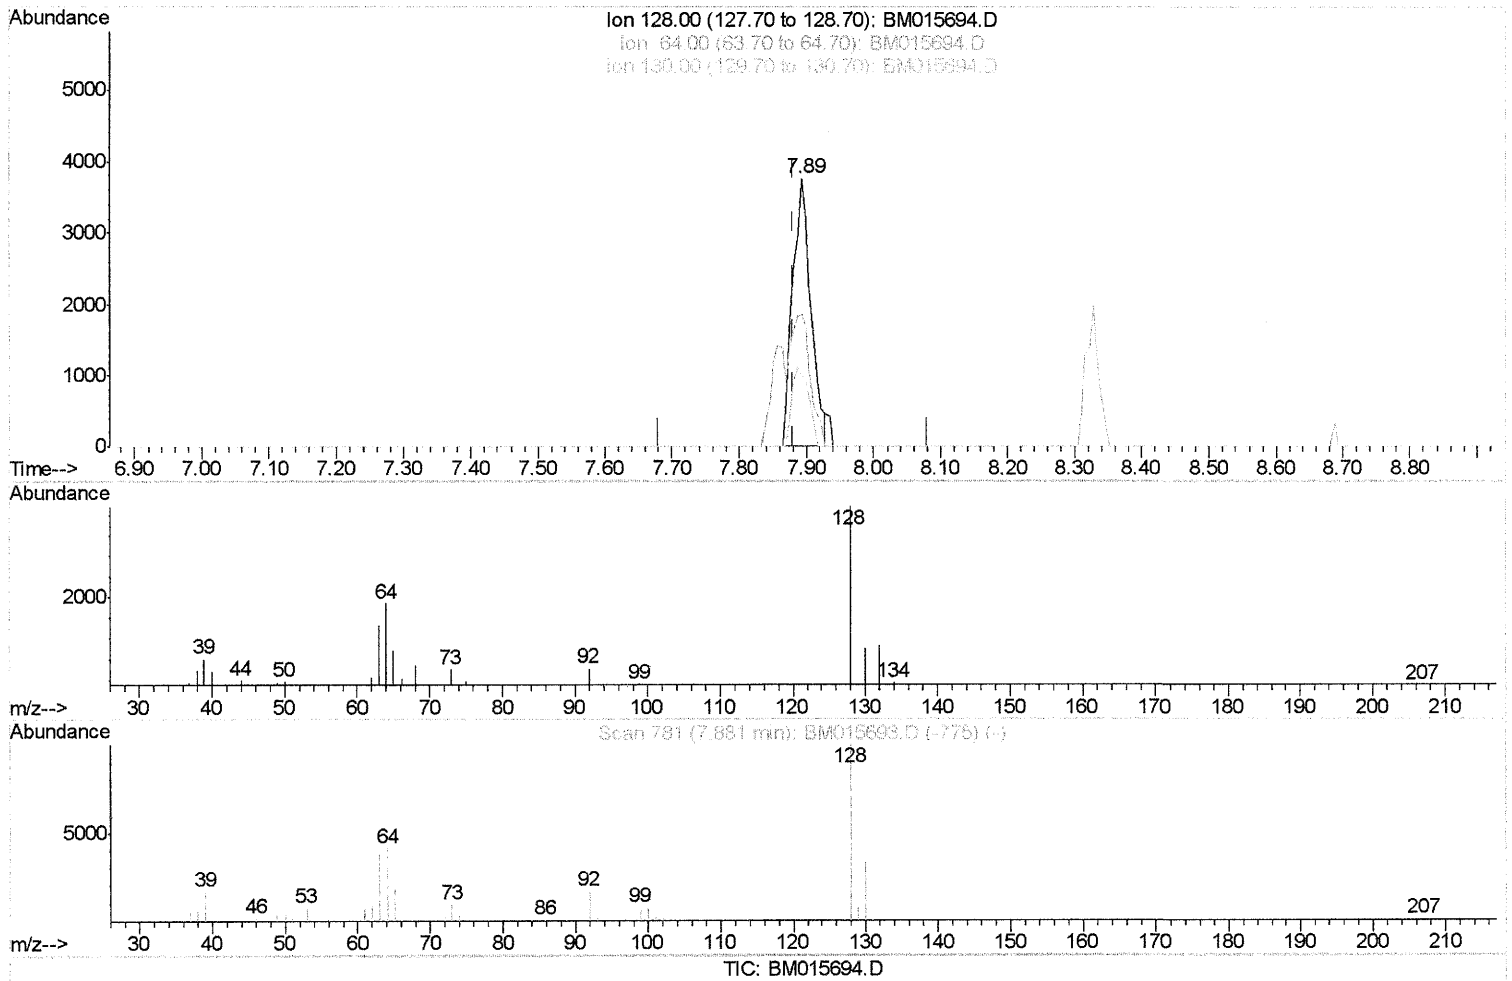

(10) 2-Chlorophenol

7.892min (+0.012) 1.22ng/ul

response 7180

Ion	Exp%	Act%
128.00	100	100
64.00	39.90	50.09#
130.00	32.00	27.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015694.D
 Acq On : 18 Jun 2018 11:56
 Operator : SJ/JU
 Sample : J3506-01DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C07Z8DL

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:24 PM

Quant Time: Jun 19 04:16:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:16:21 2018
 Response via : Initial Calibration

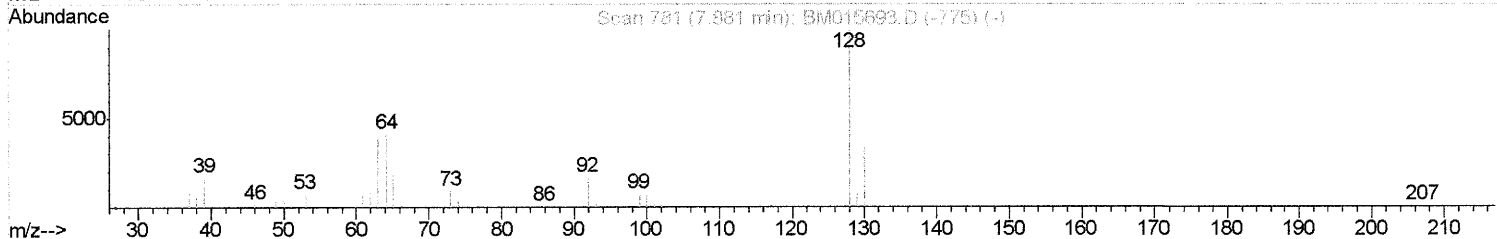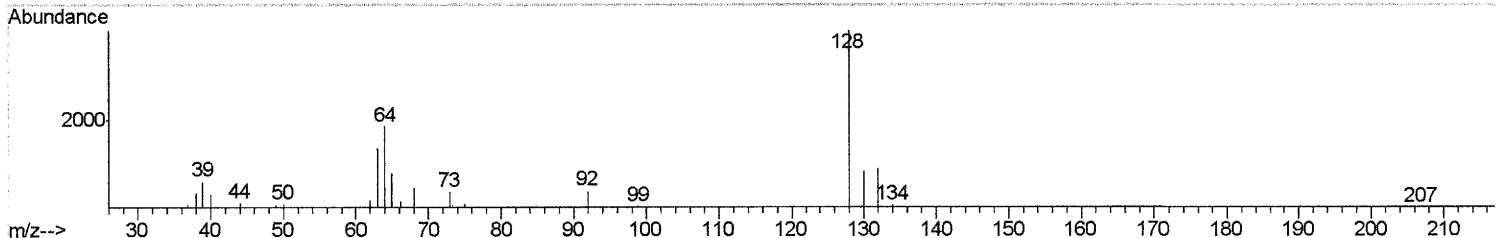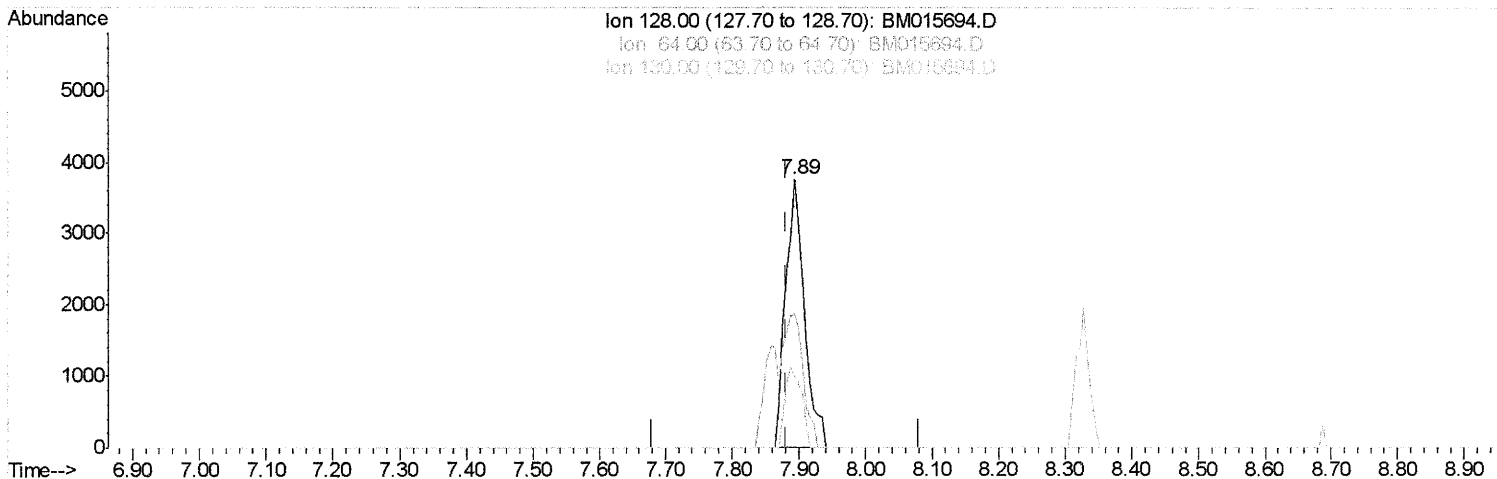

TIC: BM015694.D

(10) 2-Chlorophenol

7.892min (+0.012) 1.24ng/ul m *SJ 6/20/18*

response 7327

Ion	Exp%	Act%
128.00	100	100
64.00	39.90	50.09#
130.00	32.00	27.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_M
ClientSampled :
C07Z8DL

Manual Integrations
APPROVED

Sohil
6/19/2018 6:02:24 PM

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
Data File : BM015694.D
Acq On : 18 Jun 2018 11:56
Operator : SJ/JU
Sample : J3506-01DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 19 04:22:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 19 04:16:21 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	82279	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	371220	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	221816	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.67	188	522651	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	582109	20.00	ng/ul	0.00
85) Perylene-d12	24.19	264	608344	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	2167	1.28	ng/uL	0.00
5) Phenol-d5	7.49	99	8055	1.08	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.65	67	30822	6.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.86	132	29636	5.19	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	17335	2.69	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	17758	7.11	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	18351	6.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	31699	5.70	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	14.34	166	142432	7.76	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	151835	7.67	ng/ul	0.00
51) 4-Nitrophenol-d4	15.19	143	1292	0.36	ng/ul	0.05
57) Fluorene-d10	15.93	176	120949	7.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	12523	3.98	ng/ul	0.00
70) Anthracene-d10	17.77	188	184954	7.76	ng/ul	0.00
78) Pyrene-d10	20.02	212	208891	8.34	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	230456	7.56	ng/ul	0.00

Target Compounds

				Ovalue	
10) 2-Chlorophenol	7.89	128	7327m	1.245	ng/ul
20) Nitrobenzene	9.56	77	177006	26.254	ng/ul
72) 1,2,3,4-Tetrachlorobenzene	13.76	216	16269	2.581	ng/uL

SJ 6/20/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed