

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015699.D
 Acq On : 18 Jun 2018 19:18
 Operator : SJ/JU
 Sample : J3527-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAXP7

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:32 PM

Quant Time: Jun 19 04:48:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:38:16 2018
 Response via : Initial Calibration

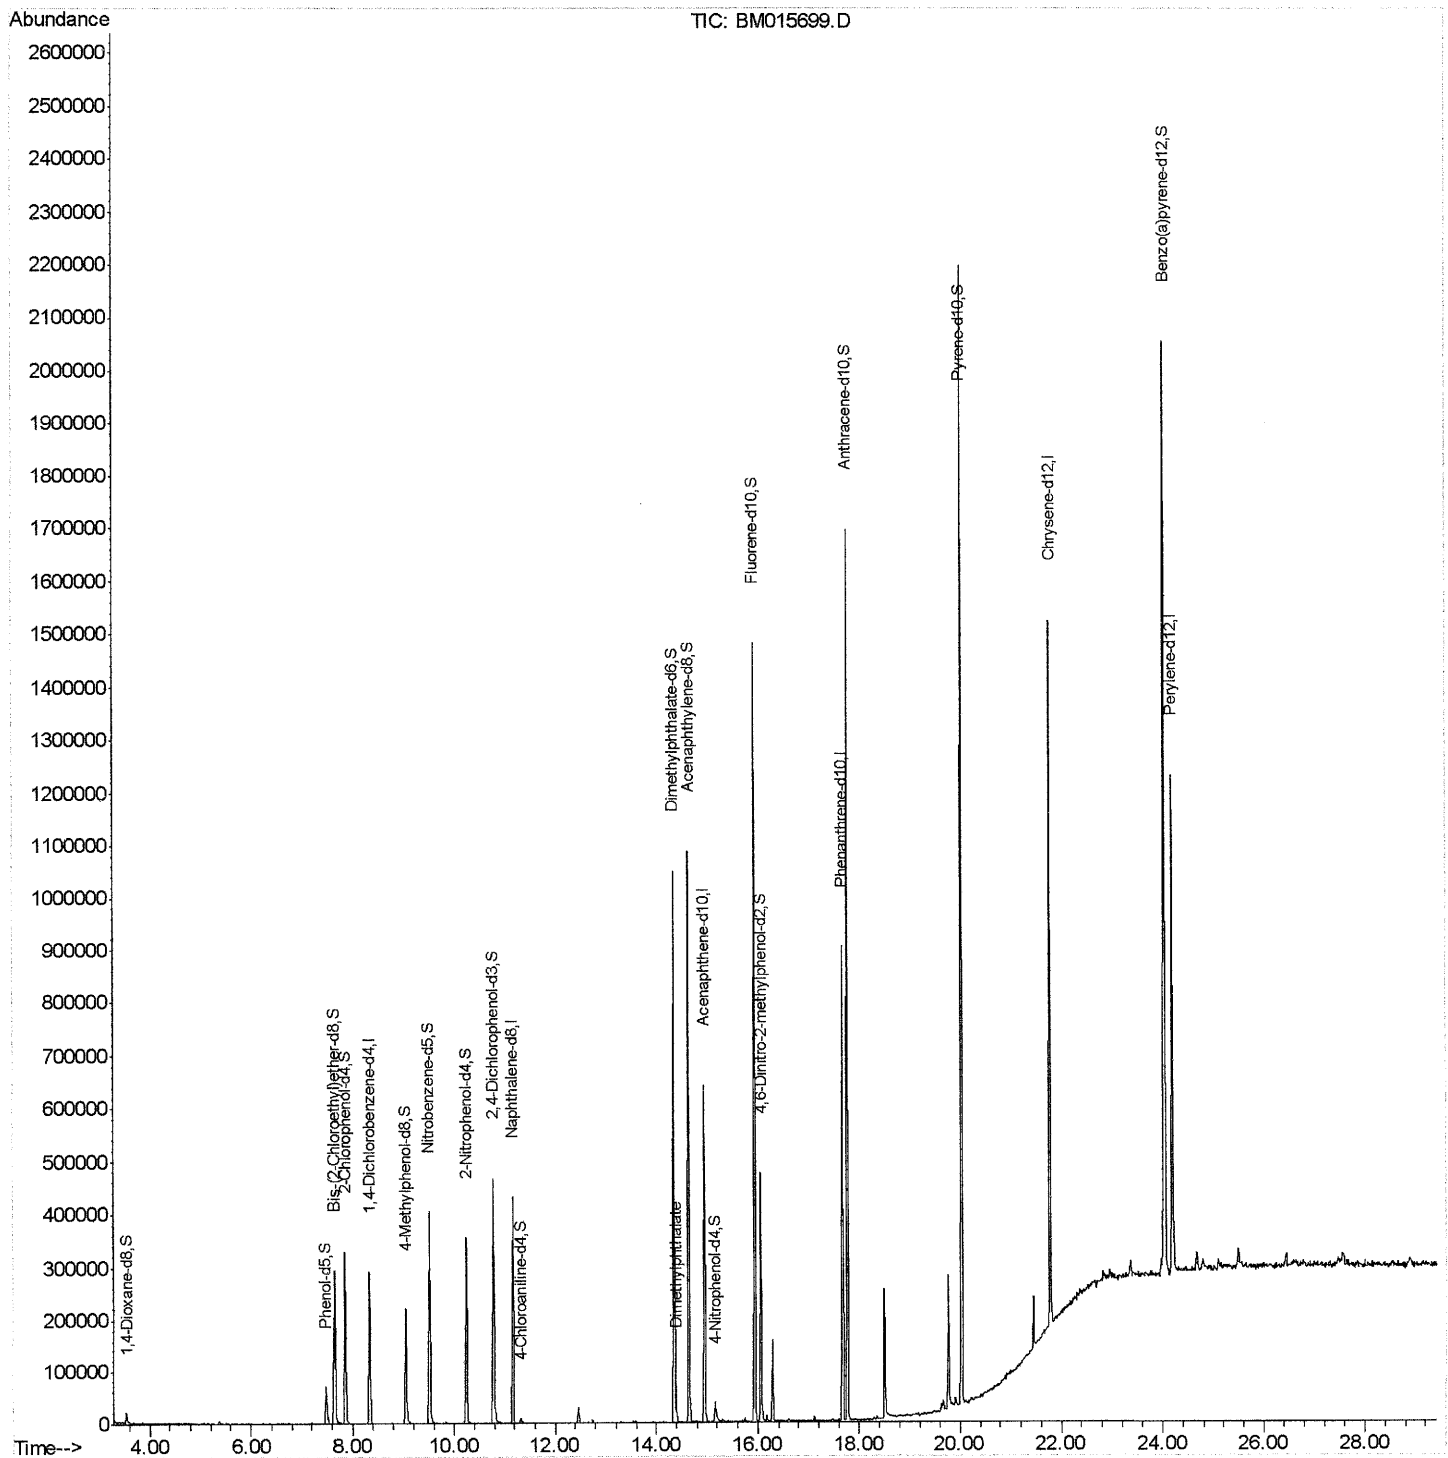

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015699.D
 Acq On : 18 Jun 2018 19:18
 Operator : SJ/JU
 Sample : J3527-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAXP7

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:32 PM

Quant Time: Jun 19 04:38:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:38:16 2018
 Response via : Initial Calibration

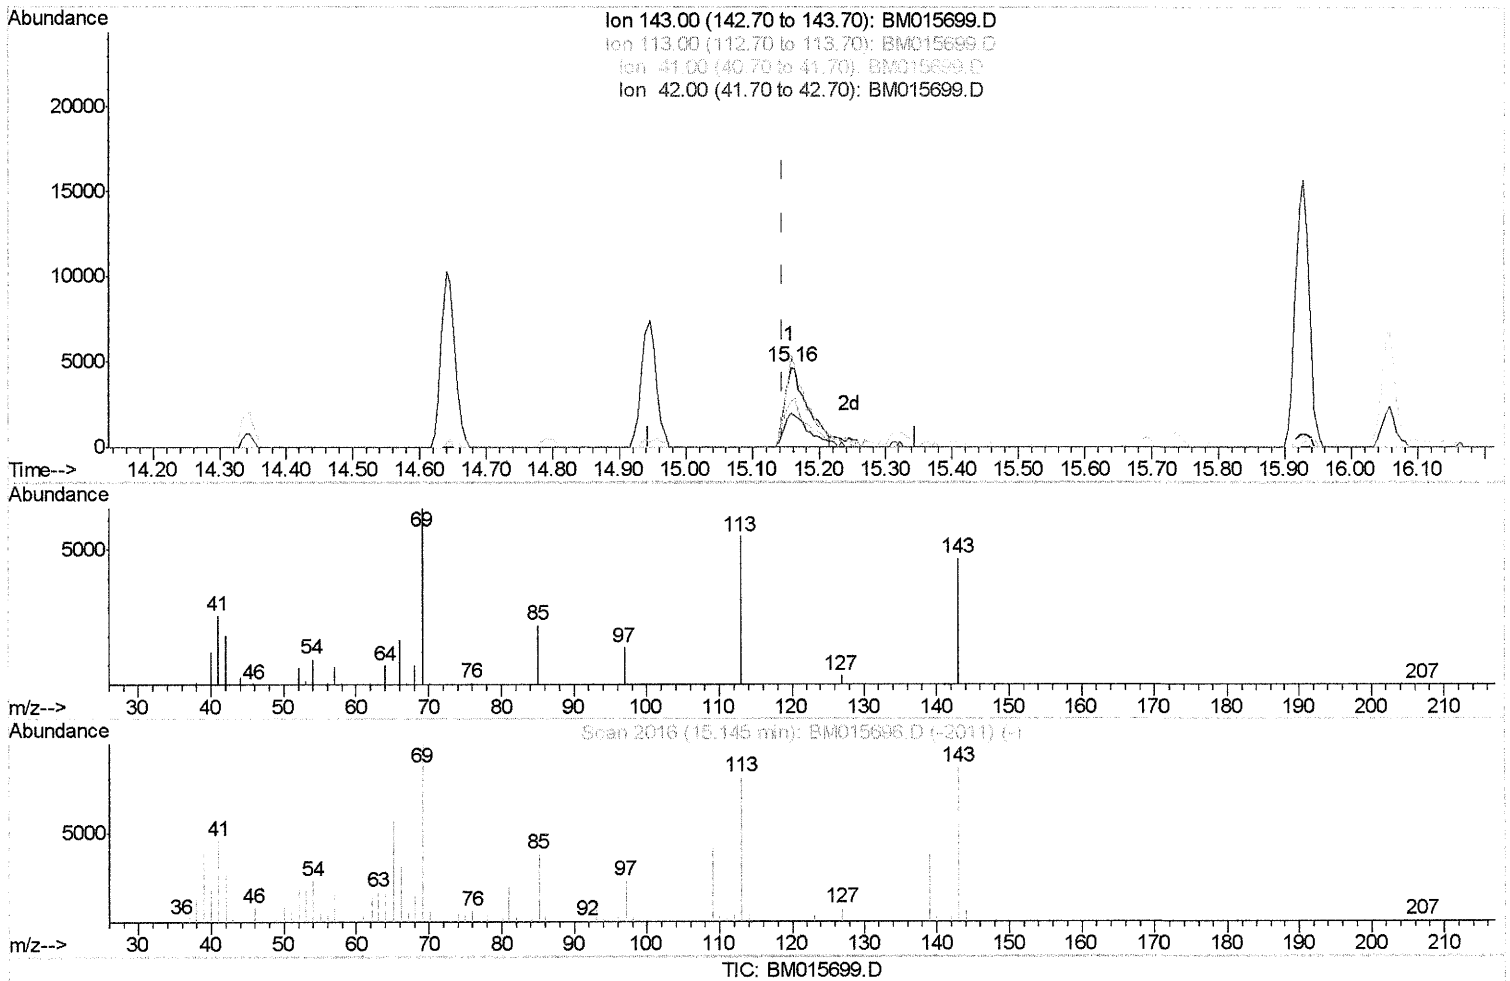

(51) 4-Nitrophenol-d4 (S)

15.157min (+0.012) 3.65ng/ul

response 11318

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	116.34#
41.00	28.80	58.02#
42.00	19.10	43.33#

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015699.D
 Acq On : 18 Jun 2018 19:18
 Operator : SJ/JU
 Sample : J3527-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DAXP7

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:32 PM

Quant Time: Jun 19 04:38:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:38:16 2018
 Response via : Initial Calibration

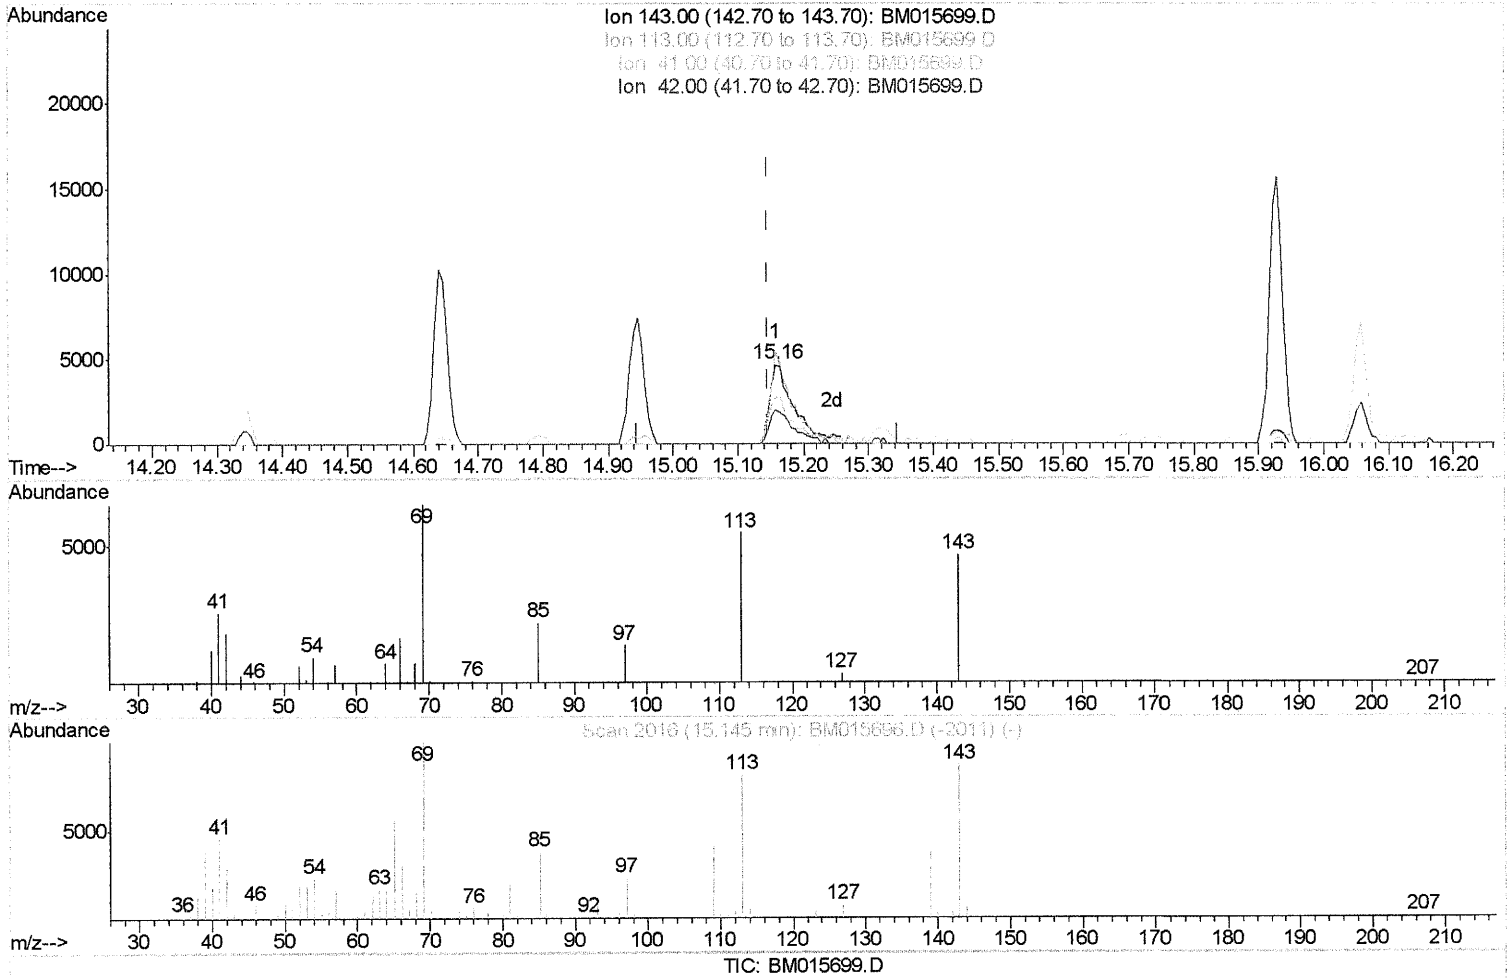

(51) 4-Nitrophenol-d4 (S)

15.157min (+0.012) 4.06ng/ul m

51 6/20/18

response 12578

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	116.34#
41.00	28.80	58.02#
42.00	19.10	43.33#

Quantitation Report (QT Reviewed)

Instrument :
BNA_M
ClientSampleId :
DAXP7

Manual Integrations
APPROVED

Sohil
6/19/2018 6:02:32 PM

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
Data File : BM015699.D
Acq On : 18 Jun 2018 19:18
Operator : SJ/JU
Sample : J3527-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 19 04:48:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 19 04:38:16 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	73335	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	327457	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	194053	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.67	188	465723	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	570730	20.00	ng/ul	0.00
85) Perylene-d12	24.19	264	635562	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	10271	6.81	ng/uL	0.00
5) Phenol-d5	7.47	99	39939	6.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.64	67	131313	32.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.85	132	138985	27.30	ng/ul	0.00
13) 4-Methylphenol-d8	9.04	113	78544	13.70	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	81697	37.10	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	91720	38.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	157846	32.19	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	7511	1.37	ng/ul	0.02
43) Dimethylphthalate-d6	14.35	166	599818	37.34	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	694248	40.07	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	12578m	4.06	ng/ul	0.01
57) Fluorene-d10	15.93	176	517892	38.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	76891	27.41	ng/ul	0.00
70) Anthracene-d10	17.77	188	815243	38.40	ng/ul	0.00
78) Pyrene-d10	20.02	212	968409	39.45	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	1233538	38.72	ng/ul	0.00

Target Compounds				Ovalue
44) Dimethylphthalate	14.39	163	39569	2.412 ng/ul 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed