

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015703.D
 Acq On : 18 Jun 2018 21:49
 Operator : SJ/JU
 Sample : J3527-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAXQ0

Quant Time: Jun 19 04:39:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:38:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	87778	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	382103	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	220376	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.67	188	513957	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	616819	20.00	ng/ul	0.00
85) Perylene-d12	24.19	264	672981	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	11834	6.55	ng/uL	0.00
5) Phenol-d5	7.47	99	45185	5.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.64	67	132806	27.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.85	132	144028	23.64	ng/ul	0.00
13) 4-Methylphenol-d8	9.04	113	88358	12.87	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	82322	32.04	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	91251	33.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	159021	27.79	ng/ul	0.00
29) 4-Chloroaniline-d4	11.32	131	7705	1.21	ng/ul	0.02
43) Dimethylphthalate-d6	14.34	166	571715	31.34	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	672410	34.17	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	11541	3.28	ng/ul	0.01
57) Fluorene-d10	15.93	176	491818	31.86	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	70774	22.86	ng/ul	0.00
70) Anthracene-d10	17.77	188	754804	32.21	ng/ul	0.00
78) Pyrene-d10	20.02	212	886431	33.41	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	1079871	32.01	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.39	163	67270	3.611	ng/ul	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
Data File : BM015703.D
Acq On : 18 Jun 2018 21:49
Operator : SJ/JU
Sample : J3527-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DAXQ0

Quant Time: Jun 19 04:39:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 19 04:38:16 2018
Response via : Initial Calibration

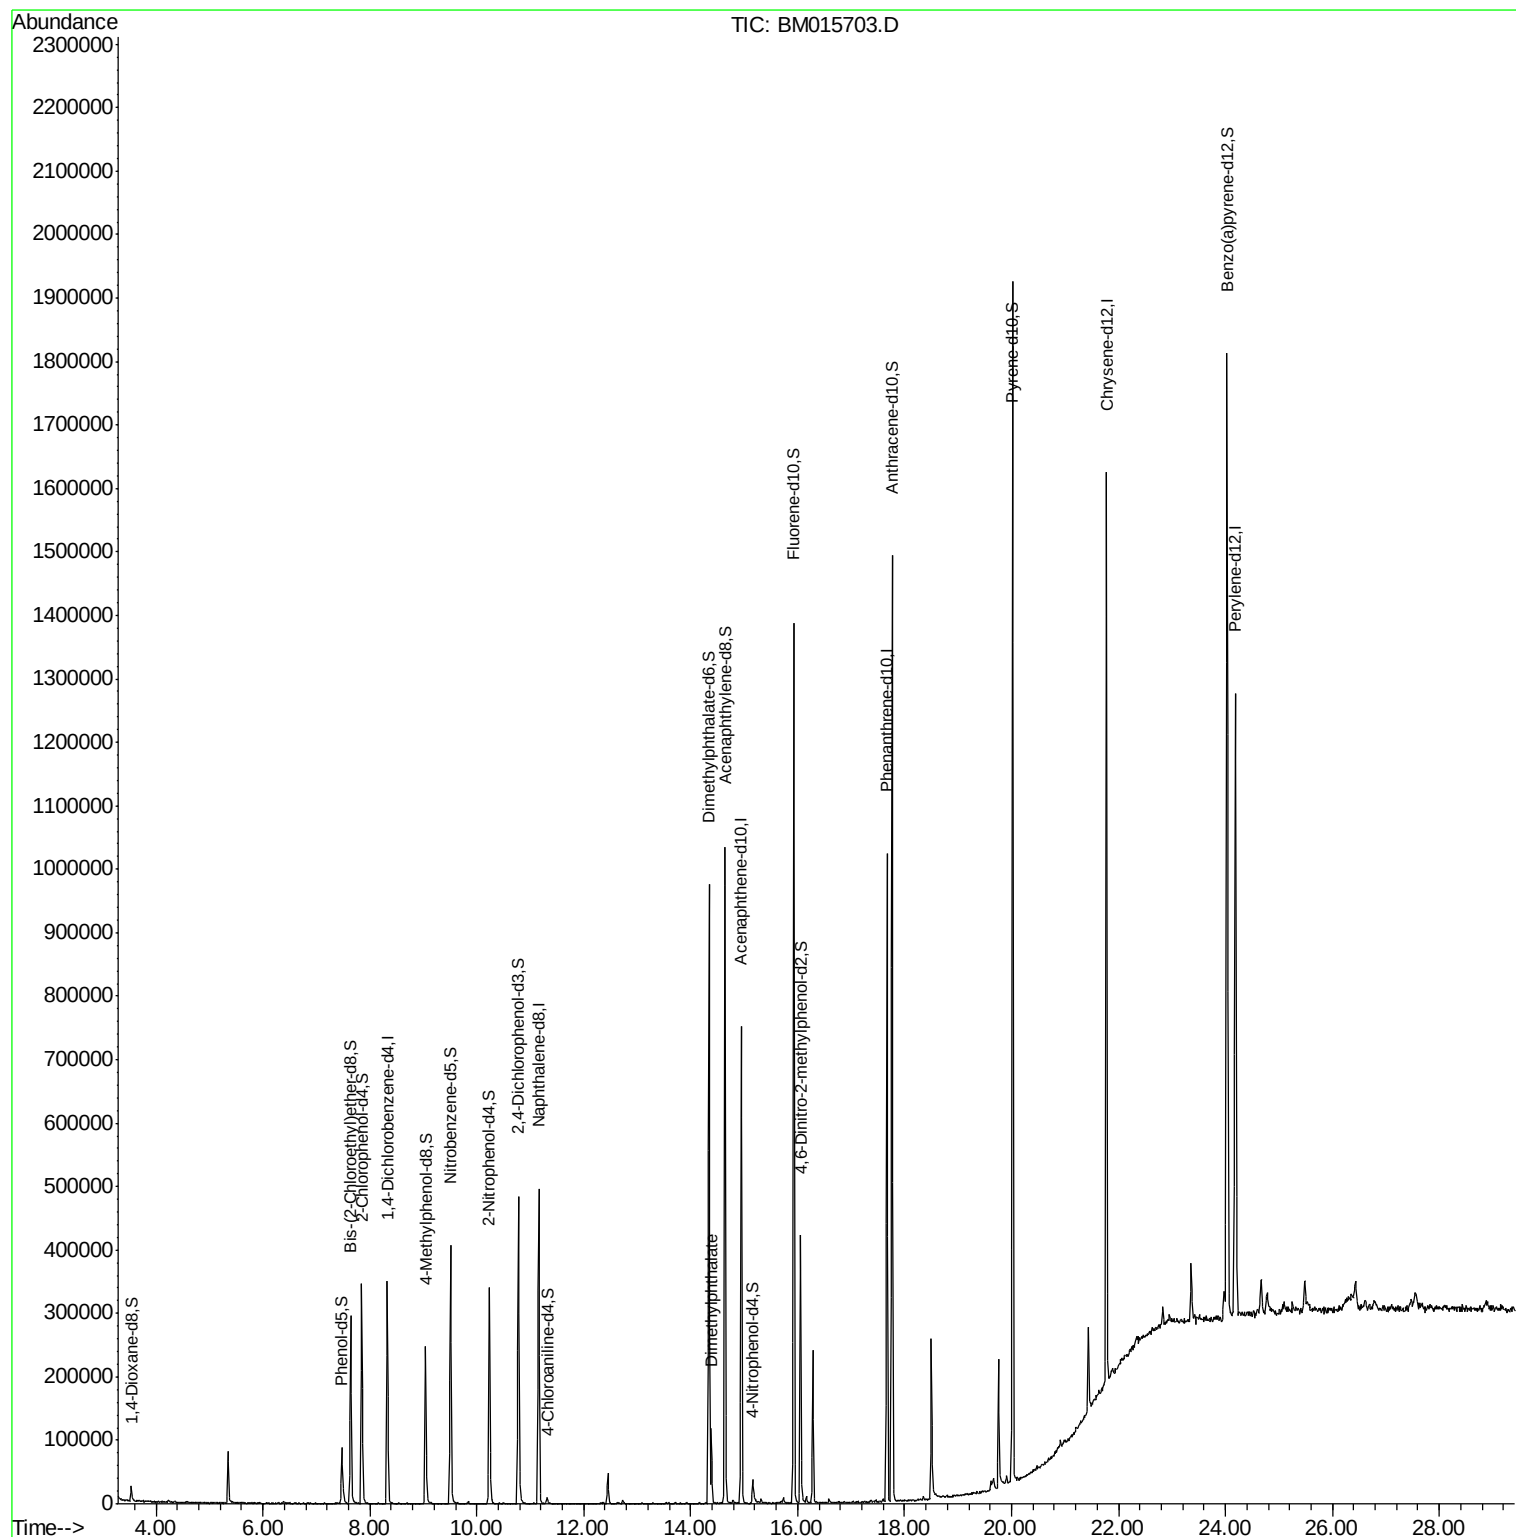

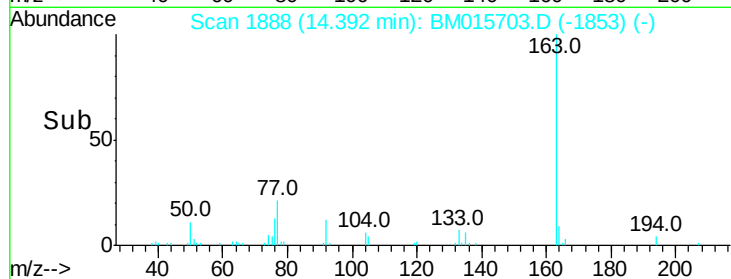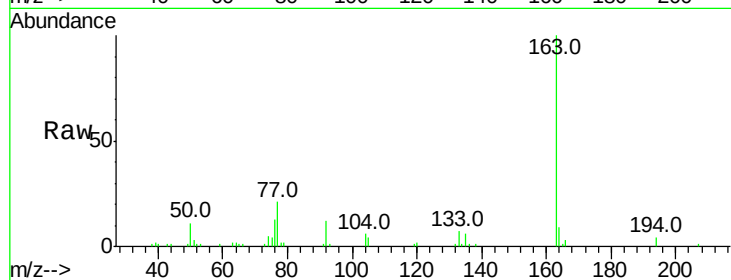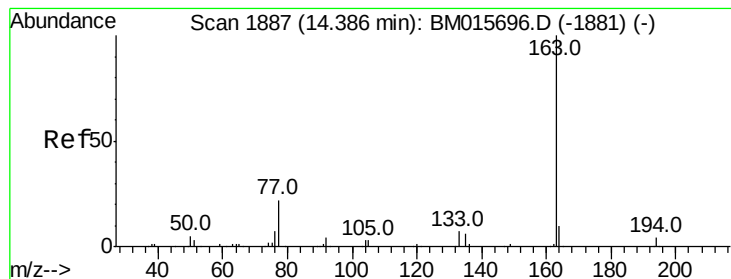

#44

Dimethylphthalate

Concen: 3.611 ng/ul

RT: 14.39 min Scan# 1888

Delta R.T. 0.01 min

Lab File: BM015703.D

Acq: 18 Jun 2018 21:49

Instrument :

BNA_M

ClientSampleId :

DAXQ0

Tot Ion:163 Resp: 67270

Ion Ratio Lower Upper

163 100

194 3.7 3.2 4.8

164 9.0 7.8 11.8

