

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015705.D
 Acq On : 18 Jun 2018 23:04
 Operator : SJ/JU
 Sample : J3527-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAXQ1

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:43 PM

Quant Time: Jun 19 05:01:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 04:38:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	91793	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	398006	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	227761	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.67	188	527708	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	611979	20.00	ng/ul	0.00
85) Perylene-d12	24.19	264	637318	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	9908	5.24	ng/uL	0.00
5) Phenol-d5	7.49	99	5457m	0.65	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.65	67	7487	1.49	ng/ul	0.01
9) 2-Chlorophenol-d4	7.86	132	9150	1.44	ng/ul	0.01
13) 4-Methylphenol-d8	9.06	113	6466	0.90	ng/ul	0.02
19) Nitrobenzene-d5	9.52	128	3387	1.27	ng/ul	0.01
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	7669	1.29	ng/ul	0.02
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	29075	1.54	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	26941	1.32	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	0.00
57) Fluorene-d10	15.93	176	24455	1.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	1659	0.52	ng/ul	0.01
70) Anthracene-d10	17.77	188	36560	1.52	ng/ul	0.00
78) Pyrene-d10	20.02	212	43631	1.66	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	49999	1.57	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.39	163	134242	6.972	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
Data File : BM015705.D
Acq On : 18 Jun 2018 23:04
Operator : SJ/JU
Sample : J3527-06
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DAXQ1

Quant Time: Jun 19 05:01:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 19 04:38:16 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
6/19/2018 6:02:43 PM

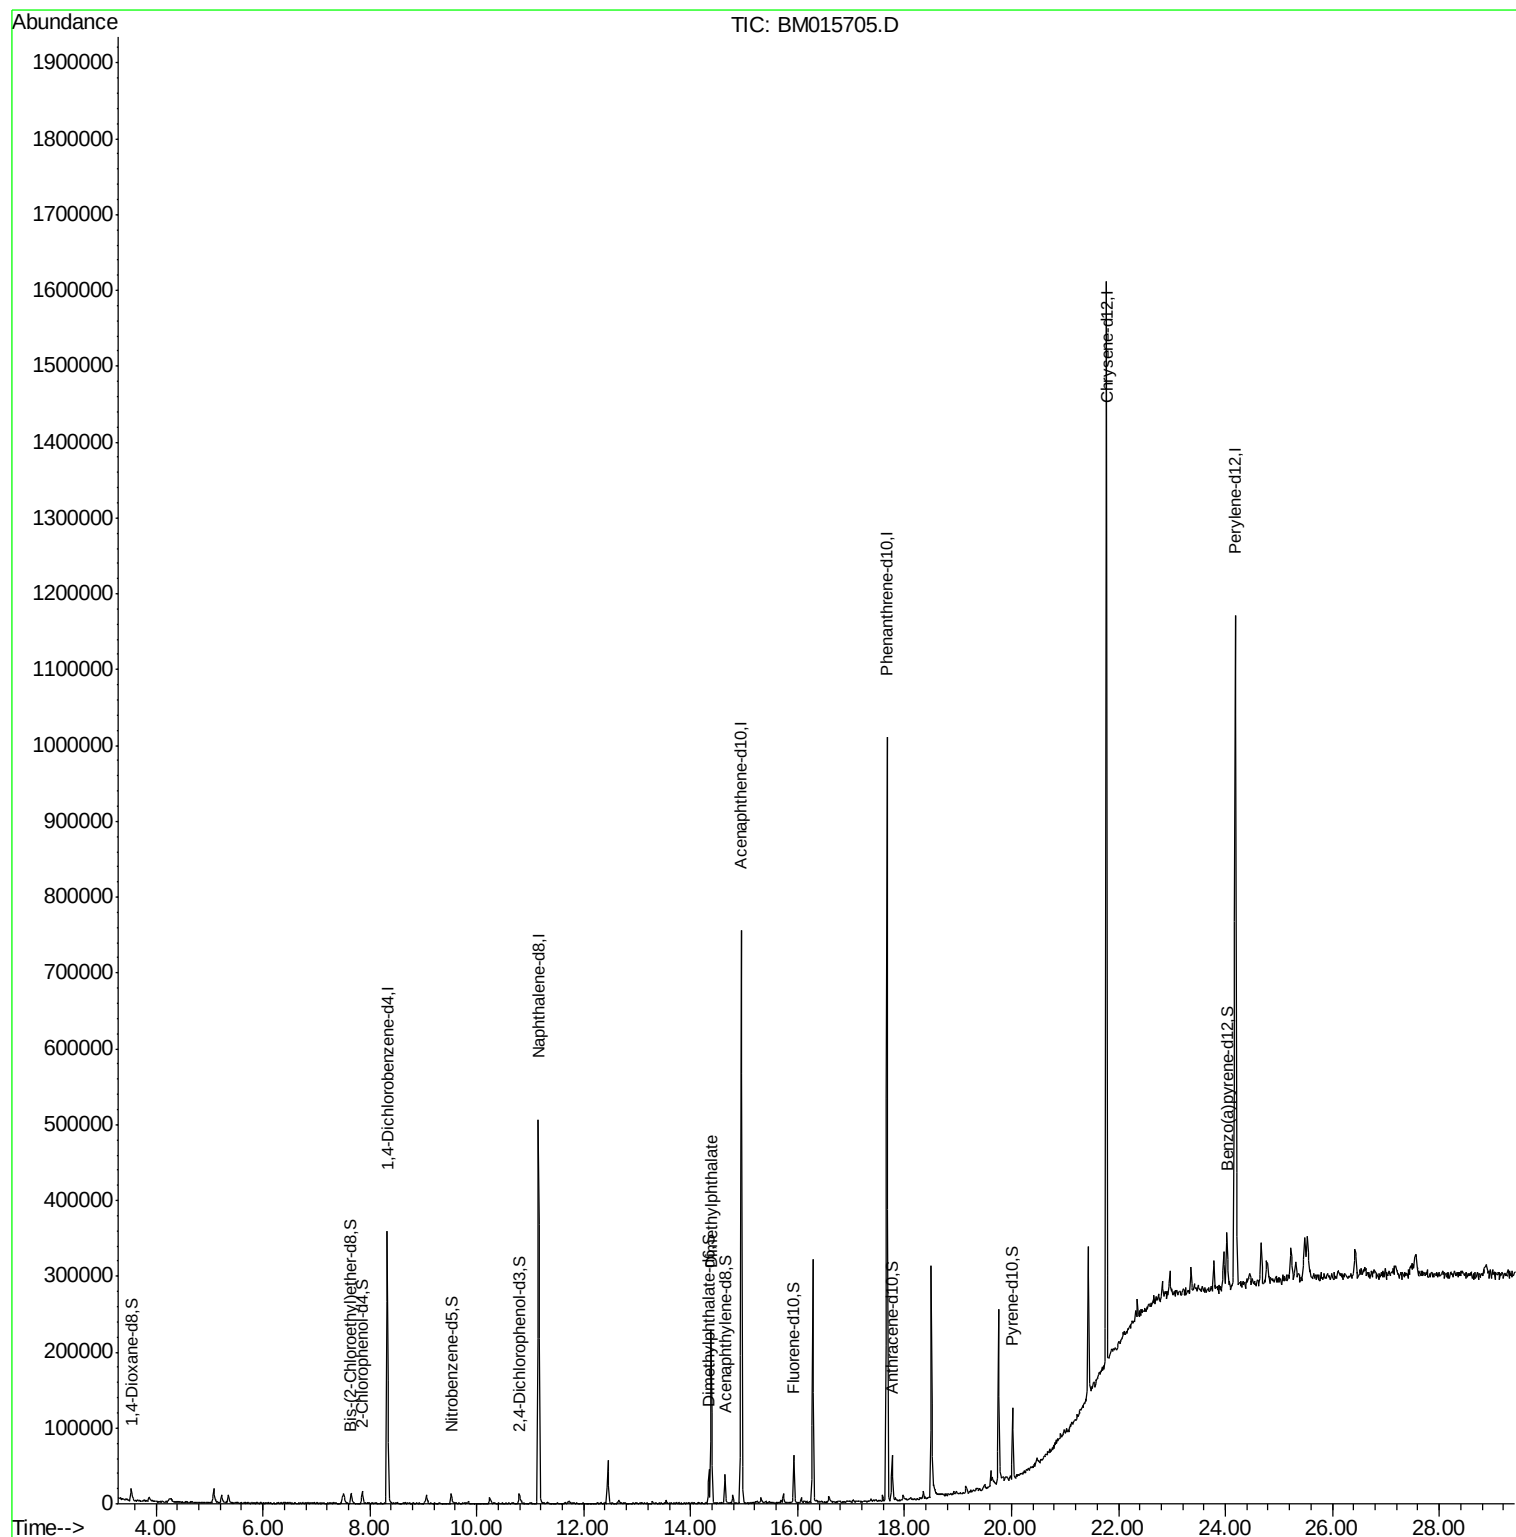

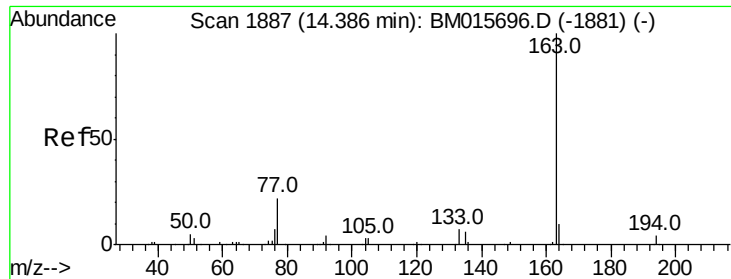

#44
 Dimethylphthalate
 Concen: 6.972 ng/ul
 RT: 14.39 min Scan# 1887
 Delta R.T. 0.00 min
 Lab File: BM015705.D
 Acq: 18 Jun 2018 23:04

Instrument :
 BNA_M
 ClientSampleId :
 DAXQ1

Tot Ion:	163	Resp:	134242
Ion Ratio	Lower	Upper	
163	100		
194	3.7	3.2	4.8
164	10.1	7.8	11.8

Manual Integrations
 APPROVED

Sohil
 6/19/2018 6:02:43 PM

