

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
 Data File : BM015710.D
 Acq On : 19 Jun 2018 02:48
 Operator : SJ/JU
 Sample : J3527-10 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DAXS4

Quant Time: Jun 19 05:12:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 19 05:11:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	88837	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	386121	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	222560	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.67	188	529346	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	626077	20.00	ng/ul	0.00
85) Perylene-d12	24.19	264	683228	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	808	0.44	ng/uL	0.00
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	7.66	67	1366	0.28	ng/ul	0.02
9) 2-Chlorophenol-d4	7.87	132	1392	0.23	ng/ul	0.02
13) 4-Methylphenol-d8	9.07	113	426	0.06	ng/ul	0.03
19) Nitrobenzene-d5	9.54	128	153	0.06	ng/ul	0.03
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	10.82	165	732	0.13	ng/ul	0.04
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	14.34	166	6499	0.35	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	6149	0.31	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.93	176	6206	0.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.77	188	9194	0.38	ng/ul	0.00
78) Pyrene-d10	20.02	212	9912	0.37	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	12576	0.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.39	163	19762	1.050	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061818\
Data File : BM015710.D
Acq On : 19 Jun 2018 02:48
Operator : SJ/JU
Sample : J3527-10 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DAXS4

Quant Time: Jun 19 05:12:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 19 05:11:15 2018
Response via : Initial Calibration

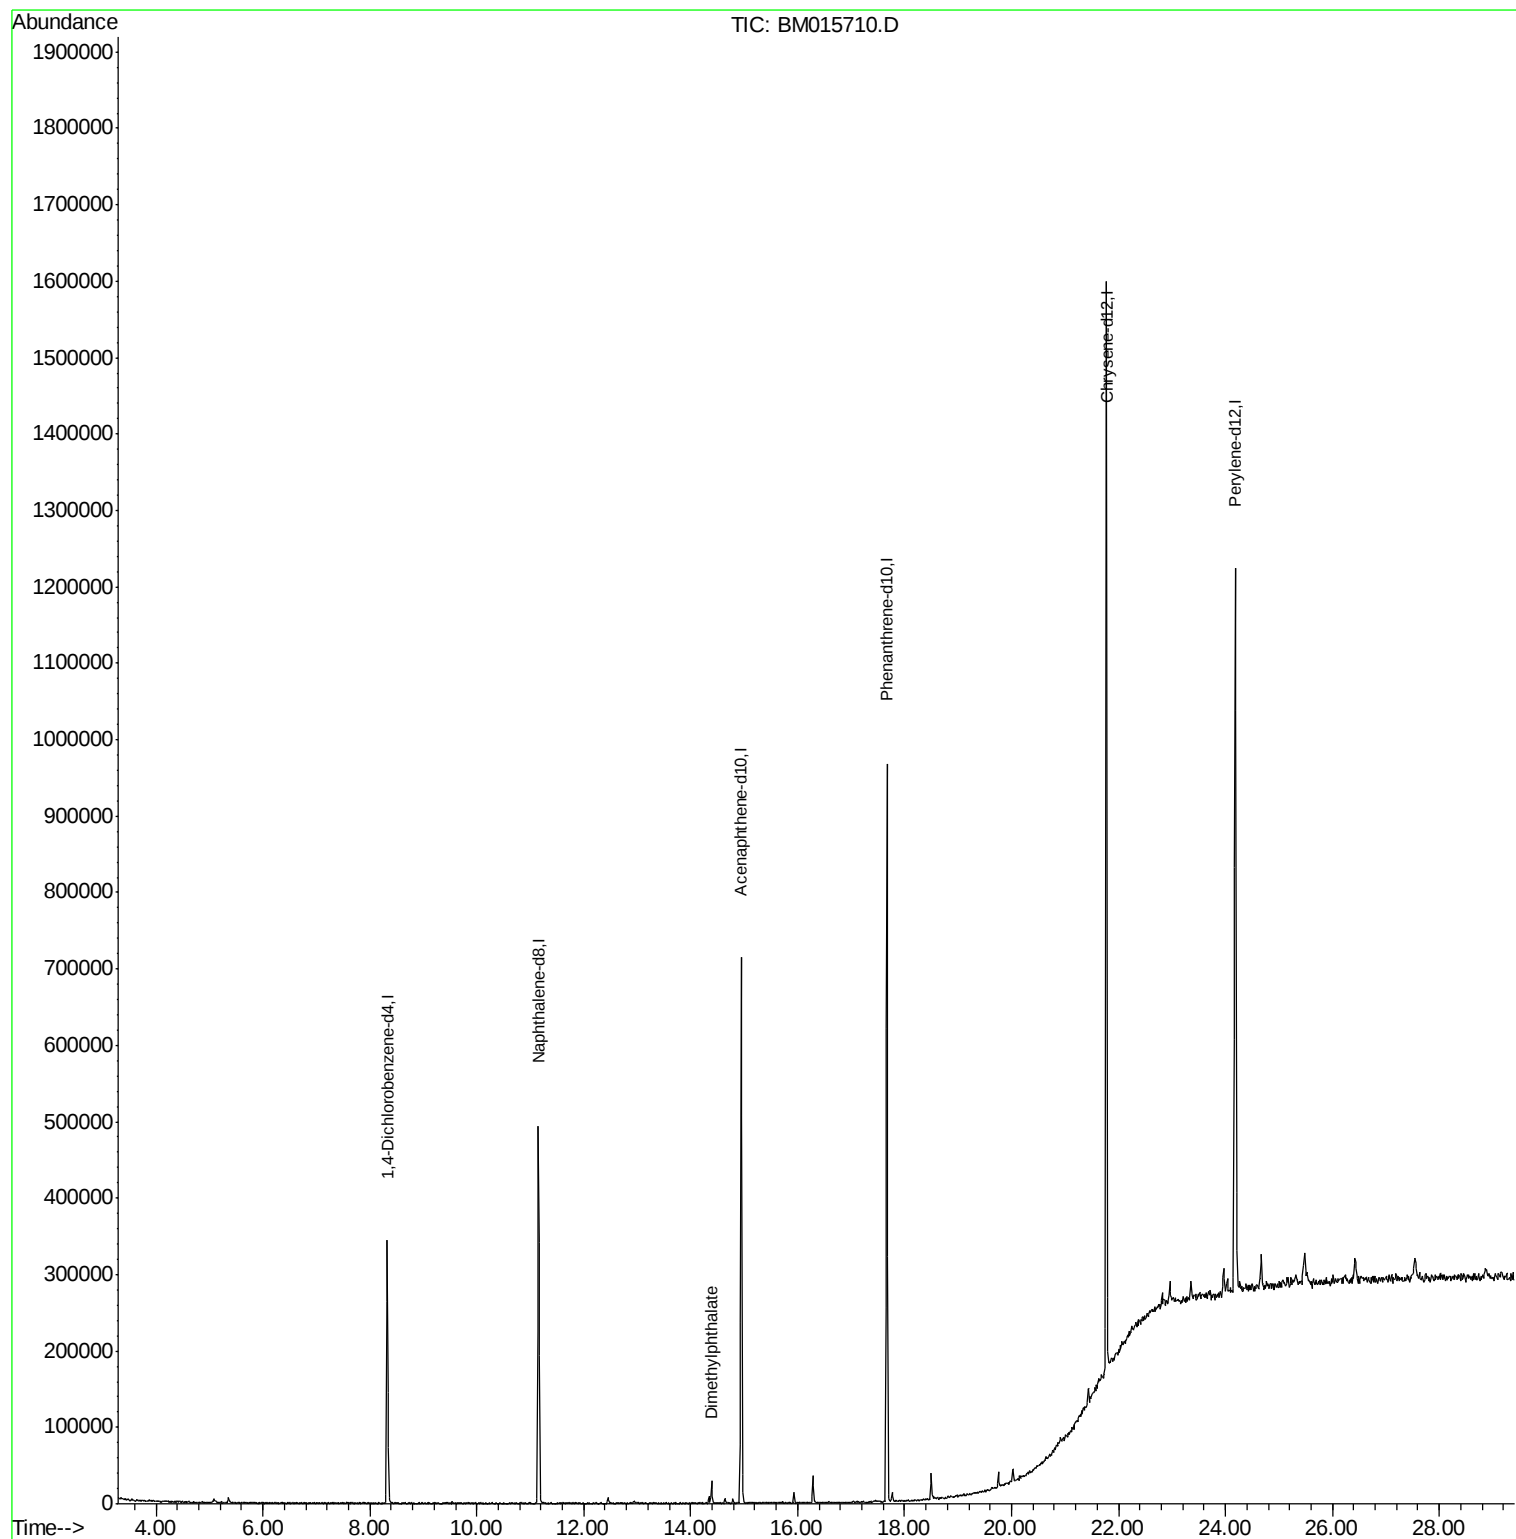

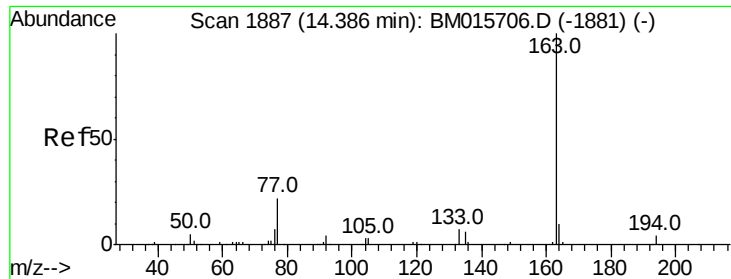

#44

Dimethylphthalate

Concen: 1.050 ng/ul

RT: 14.39 min Scan# 1888

Delta R.T. 0.01 min

Lab File: BM015710.D

Acq: 19 Jun 2018 02:48

Instrument :

BNA_M

ClientSampleId :

DAXS4


Tot Ion:163 Resp: 19762

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8

164 8.9 7.8 11.8

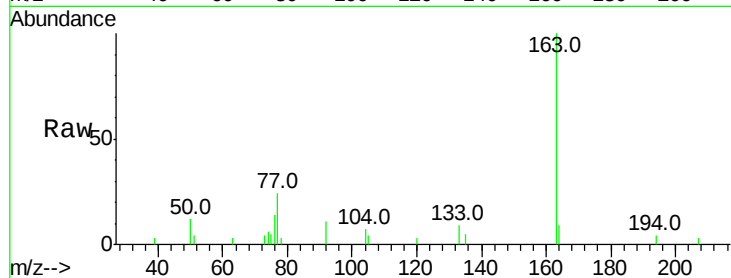

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

