

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061819\
 Data File : BM021015.D
 Acq On : 18 Jun 2019 17:08
 Operator : HP/JU
 Sample : K3353-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0JT4

Quant Time: Jun 19 00:59:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 19 00:56:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	224135	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	992425	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	678780	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1701043	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	1553642	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	1451098	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	9581	2.03	ng/uL	0.00
5) Phenol-d5	6.95	99	184825	9.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	365363	31.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	437002	27.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	333525	20.48	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	272075	33.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	307804	34.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	587152	32.28	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	741583	39.09	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	2191156	35.73	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	2485927	33.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	85540	8.57	ng/ul	0.00
57) Fluorene-d10	15.42	176	1895047	35.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	294215	28.14	ng/ul	0.00
70) Anthracene-d10	17.27	188	3220443	36.43	ng/ul	0.00
78) Pyrene-d10	19.57	212	3675116	39.42	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.49	264	3219623	37.61	ng/ul	0.00


Target Compounds					Qvalue	
17) Hexachloroethane	8.89	117	8840	1.420	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061819\
Data File : BM021015.D
Acq On : 18 Jun 2019 17:08
Operator : HP/JU
Sample : K3353-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0JT4

Quant Time: Jun 19 00:59:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 19 00:56:26 2019
Response via : Initial Calibration

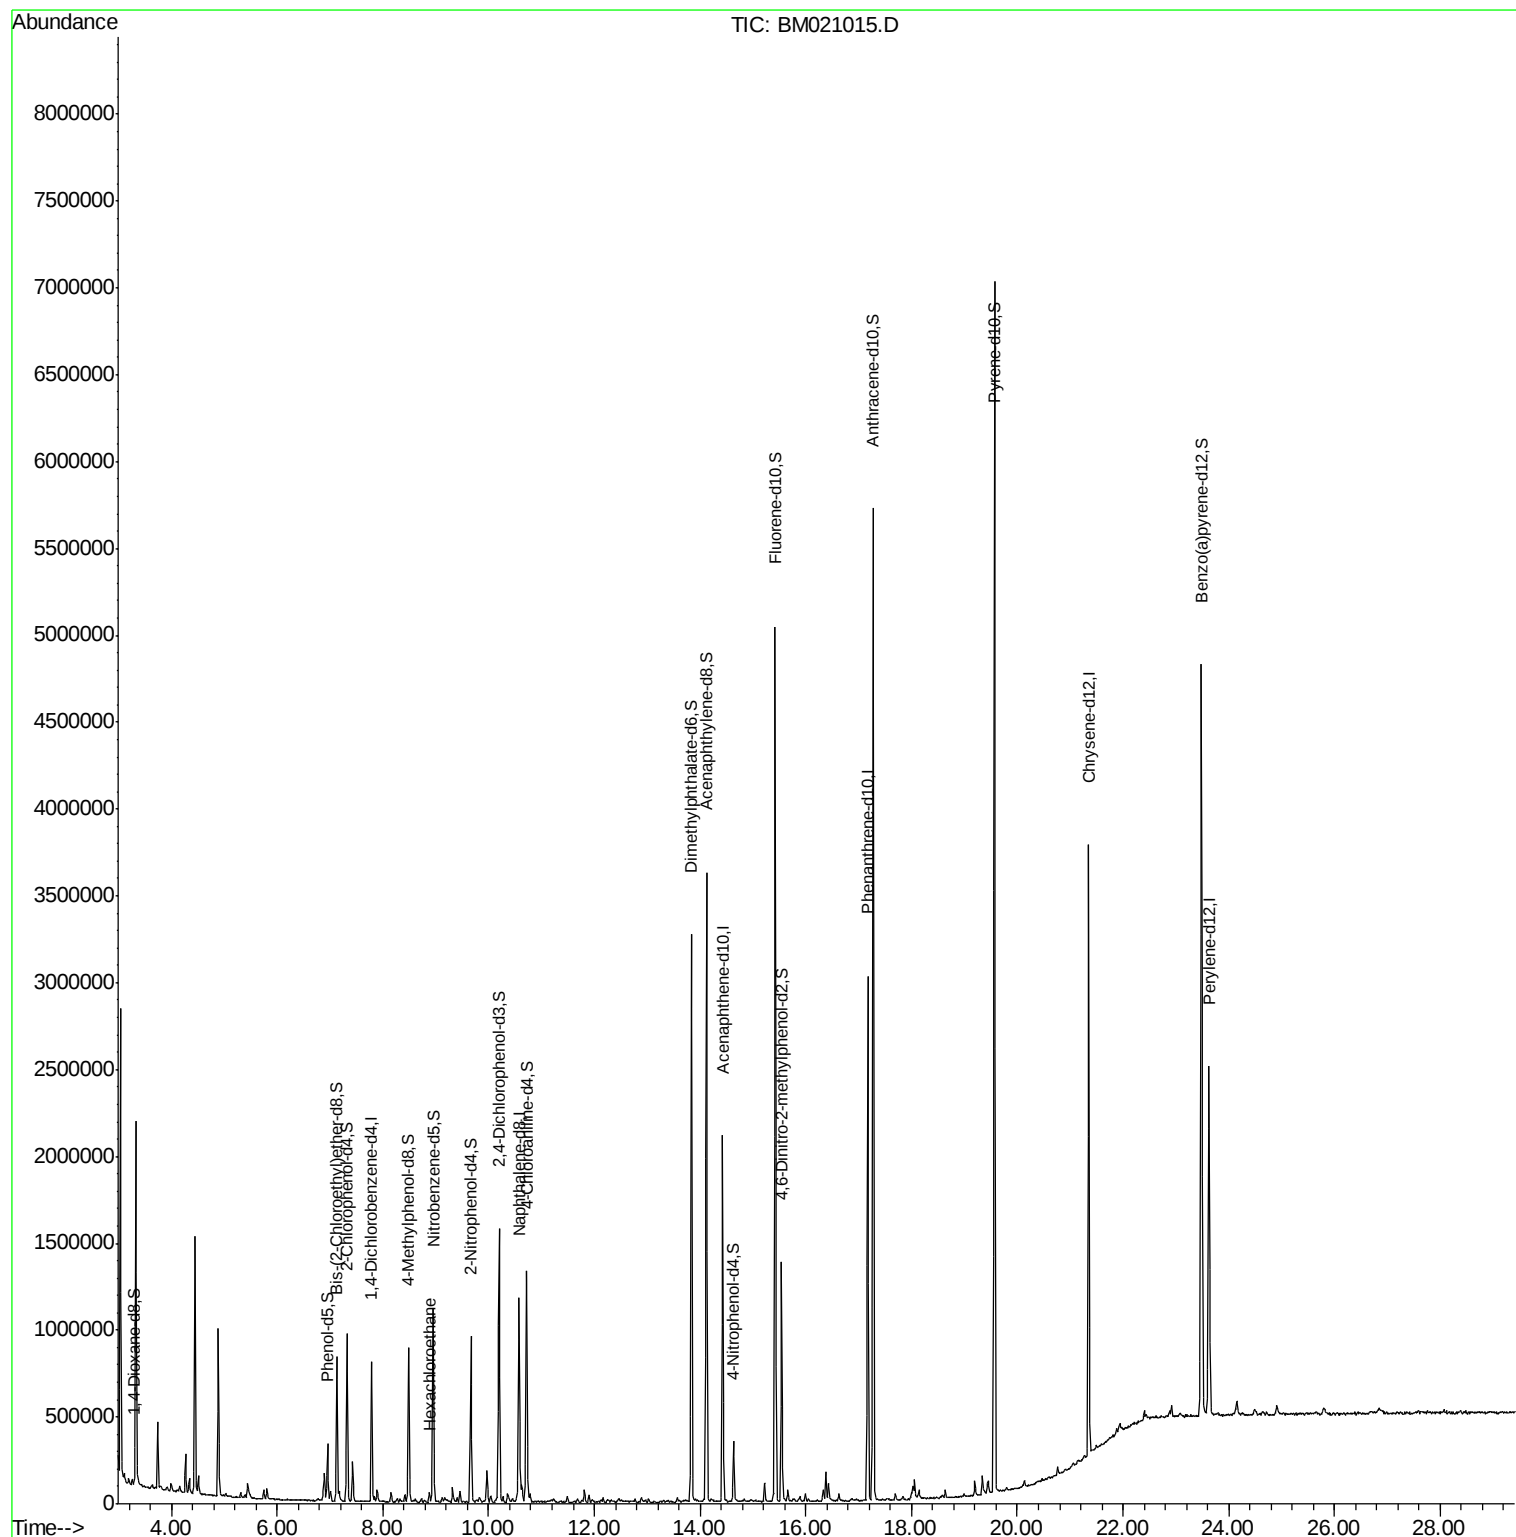

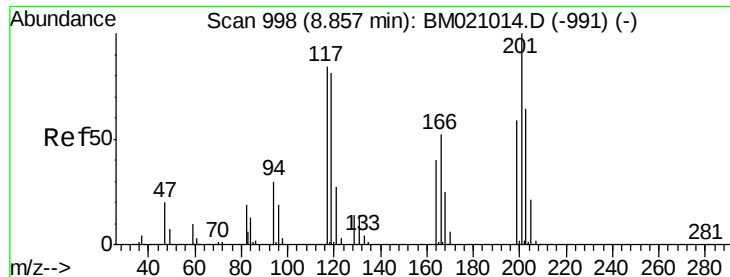

#17
 Hexachloroethane
 Concen: 1.420 ng/ul
 RT: 8.89 min Scan# 1003
 Delta R.T. 0.03 min
 Lab File: BM021015.D
 Acq: 18 Jun 2019 17:08

Instrument :
 BNA_M
 ClientSampleId :
 C0JT4

Tgt Ion:117 Resp: 8840
 Ion Ratio Lower Upper
 117 100
 201 0.0 93.9 140.9#
 199 0.0 57.8 86.8#

