

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061819\
 Data File : BM021025.D
 Acq On : 18 Jun 2019 23:10
 Operator : HP/JU
 Sample : K3332-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4227

Quant Time: Jun 19 01:00:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 19 00:56:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	237335	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1065479	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	705272	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1672364	20.00	ng/ul	0.00
77) Chrysene-d12	21.35	240	1388267	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	1429586	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	17895	3.58	ng/uL	0.00
5) Phenol-d5	6.95	99	385728	18.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	252362	20.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	329694	19.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	329563	19.11	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	174209	20.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	192590	20.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	376232	19.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	432324	21.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1388324	21.79	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1595906	20.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	151205	14.59	ng/ul	0.00
57) Fluorene-d10	15.42	176	1206445	21.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	145643	14.17	ng/ul	0.00
70) Anthracene-d10	17.27	188	1835787	21.12	ng/ul	0.00
78) Pyrene-d10	19.56	212	1970484	23.65	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.48	264	1795438	21.29	ng/ul	0.00


Target Compounds					Qvalue	
44) Dimethylphthalate	13.89	163	314530	5.422	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061819\
Data File : BM021025.D
Acq On : 18 Jun 2019 23:10
Operator : HP/JU
Sample : K3332-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4227

Quant Time: Jun 19 01:00:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 19 00:56:26 2019
Response via : Initial Calibration

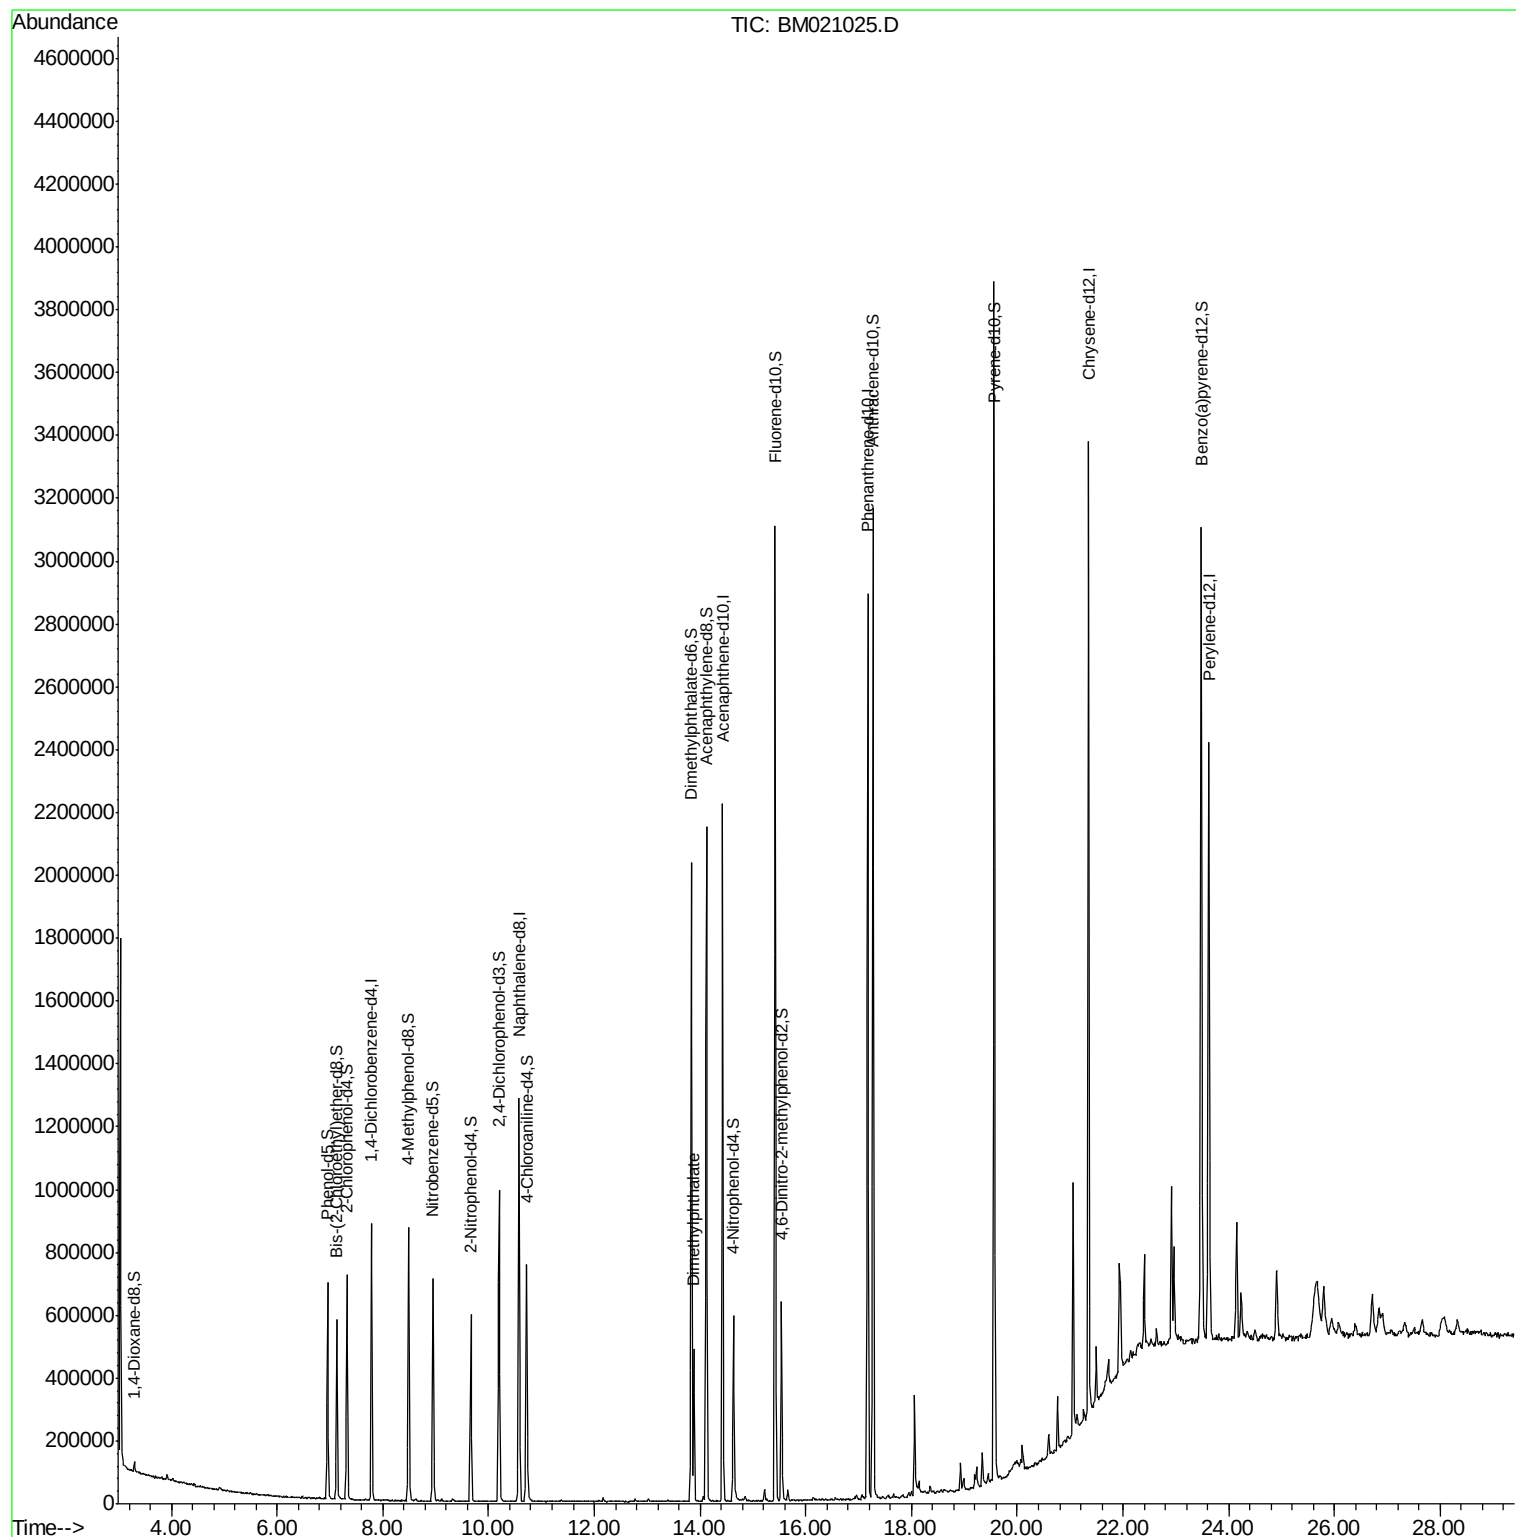

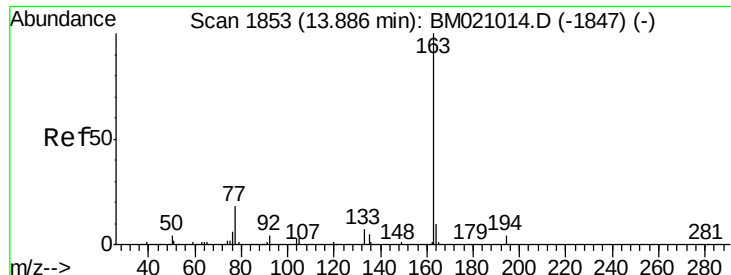

#44

Dimethylphthalate

Concen: 5.422 ng/ul

RT: 13.89 min Scan# 1853

Delta R.T. -0.00 min

Lab File: BM021025.D

Acq: 18 Jun 2019 23:10

Instrument :

BNA_M

ClientSampleId :

A4227

Tgt Ion:163 Resp: 314530

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 10.4 7.7 11.5

