

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061819\
 Data File : BM021005.D
 Acq On : 18 Jun 2019 10:02
 Operator : HP/JU
 Sample : K3332-14
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4222

Quant Time: Jun 18 17:38:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 18 05:54:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	215692	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	969835	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	644820	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1535943	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	1272092	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	1296684	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	16141	3.55	ng/uL	0.00
5) Phenol-d5	6.95	99	327986	17.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	221041	19.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	280052	18.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	271643	17.33	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	154397	19.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	168025	19.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	320945	18.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	380455	20.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1270744	21.81	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1432833	20.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	99800	10.53	ng/ul	0.00
57) Fluorene-d10	15.42	176	1089339	21.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	104913	11.11	ng/ul	0.00
70) Anthracene-d10	17.27	188	1729673	21.67	ng/ul	0.00
78) Pyrene-d10	19.57	212	1837334	24.07	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.49	264	1632002	21.33	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.89	163	232405	4.382	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061819\
Data File : BM021005.D
Acq On : 18 Jun 2019 10:02
Operator : HP/JU
Sample : K3332-14
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A4222

Quant Time: Jun 18 17:38:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 18 05:54:28 2019
Response via : Initial Calibration

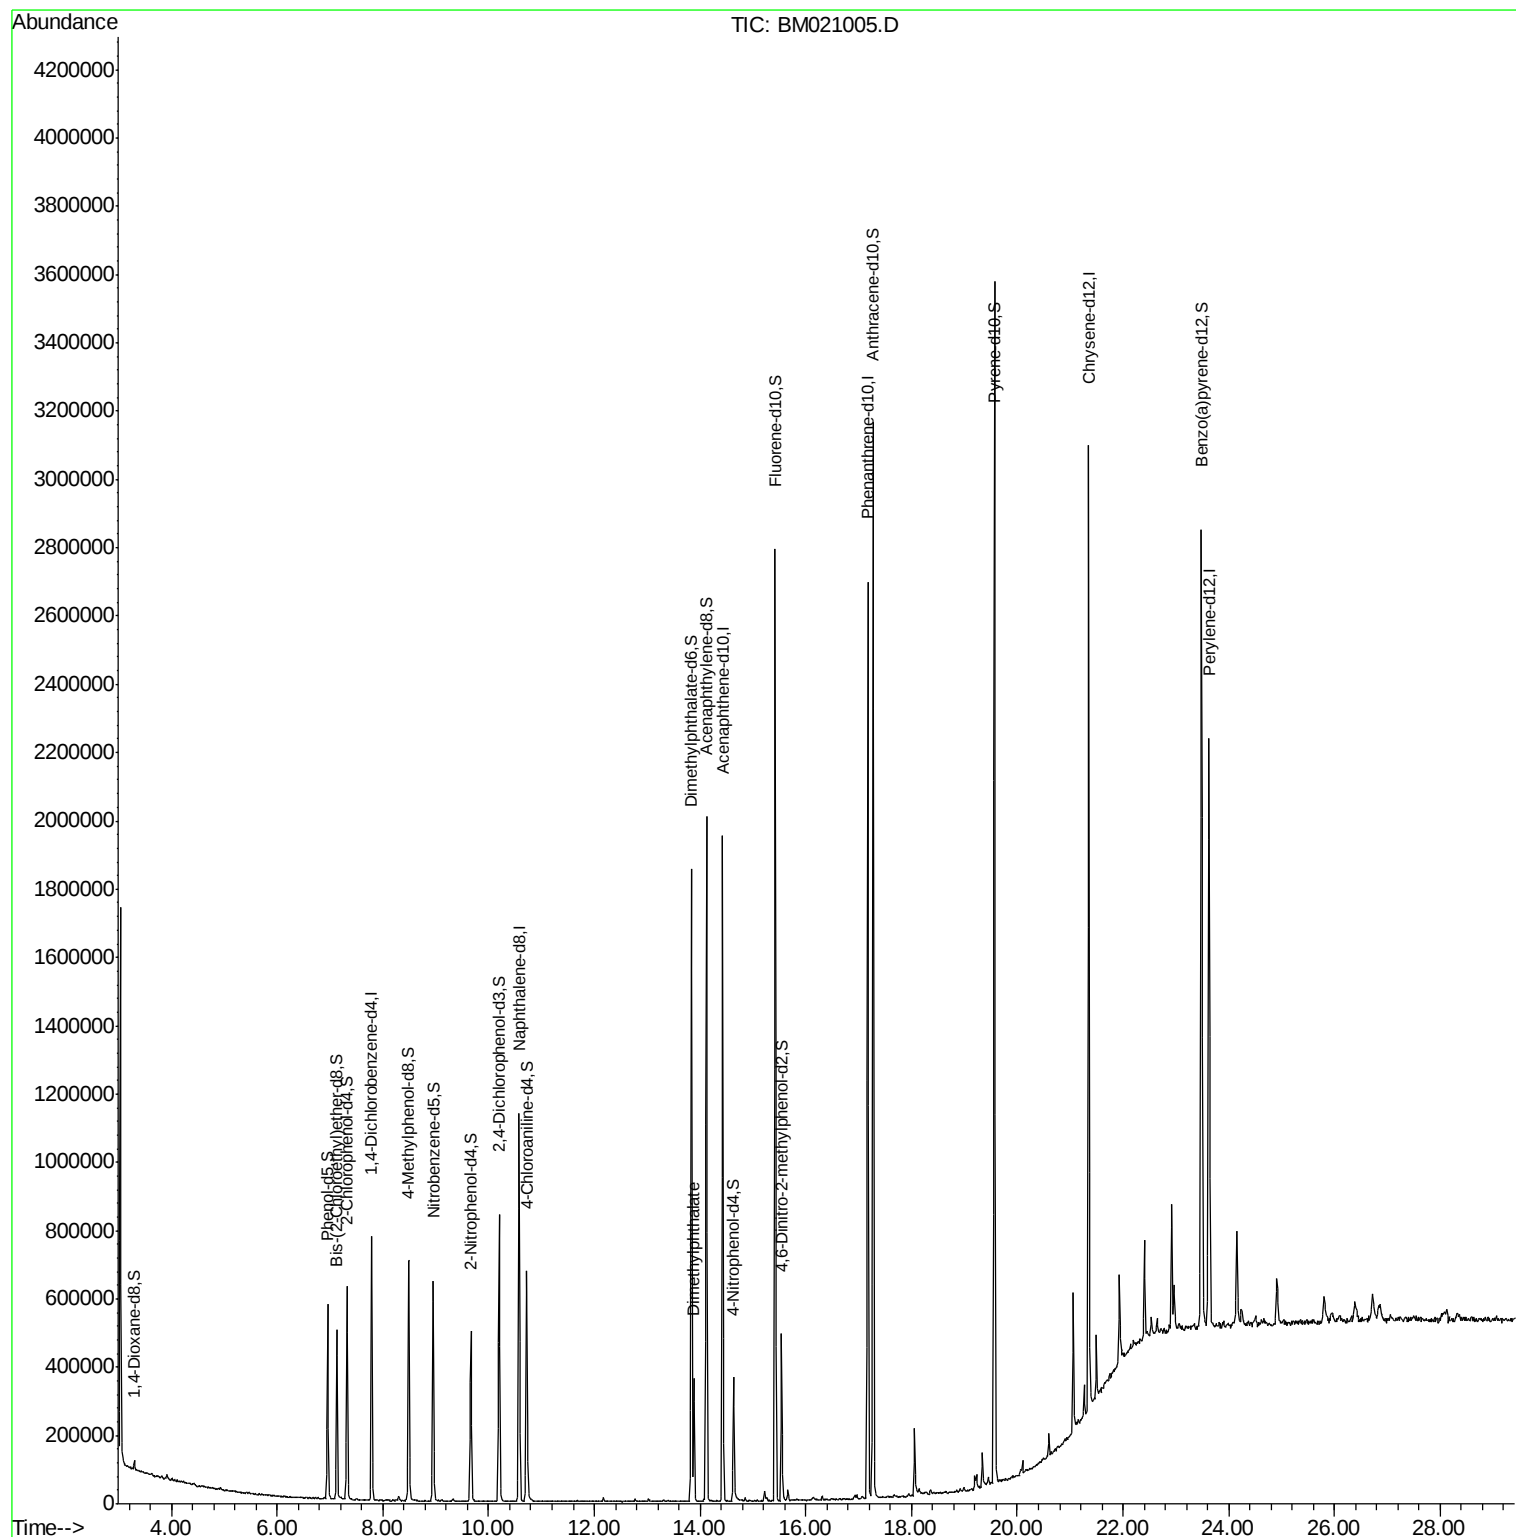

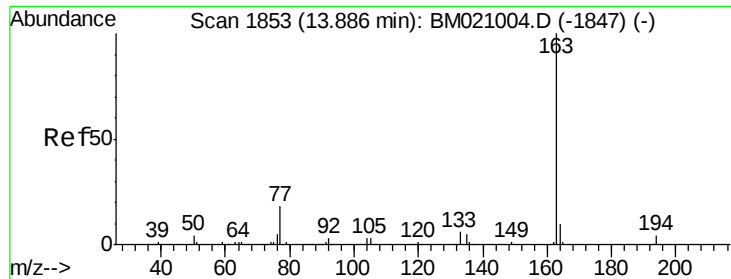

#44

Dimethylphthalate

Concen: 4.382 ng/ul

RT: 13.89 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BM021005.D

Acq: 18 Jun 2019 10:02

Instrument :

BNA_M

ClientSampleId :

A4222


Tot Ion:163 Resp: 232405

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.2

164 9.8 7.7 11.5

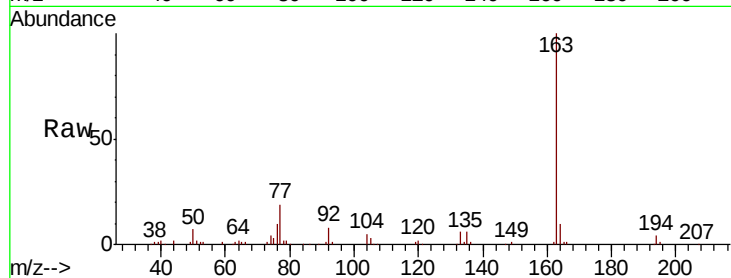

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

