

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061819\
 Data File : BM021009.D
 Acq On : 18 Jun 2019 13:31
 Operator : HP/JU
 Sample : K3353-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0JS9

Quant Time: Jun 18 17:43:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 18 05:54:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	225973	20.00	ng/ul	0.00
18) Naphthalene-d8	10.58	136	994272	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	678188	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1714100	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	1797708	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	1789843	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.30	96	10565	2.22	ng/uL	0.01
5) Phenol-d5	6.96	99	219959	11.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	407726	34.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	493547	30.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	379239	23.10	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	297542	36.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	344637	38.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	636417	34.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	812706	42.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	2349790	38.35	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	2656129	35.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	107689	10.80	ng/ul	0.00
57) Fluorene-d10	15.42	176	2062165	38.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	286008	27.14	ng/ul	0.00
70) Anthracene-d10	17.27	188	3528740	39.61	ng/ul	0.00
78) Pyrene-d10	19.57	212	4110519	38.10	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.49	264	4307684	40.79	ng/ul	0.00


Target Compounds					Ovalue	
83) Bis(2-ethylhexyl)phthalate	21.27	149	194763	2.908	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061819\
Data File : BM021009.D
Acq On : 18 Jun 2019 13:31
Operator : HP/JU
Sample : K3353-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0JS9

Quant Time: Jun 18 17:43:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 18 05:54:28 2019
Response via : Initial Calibration

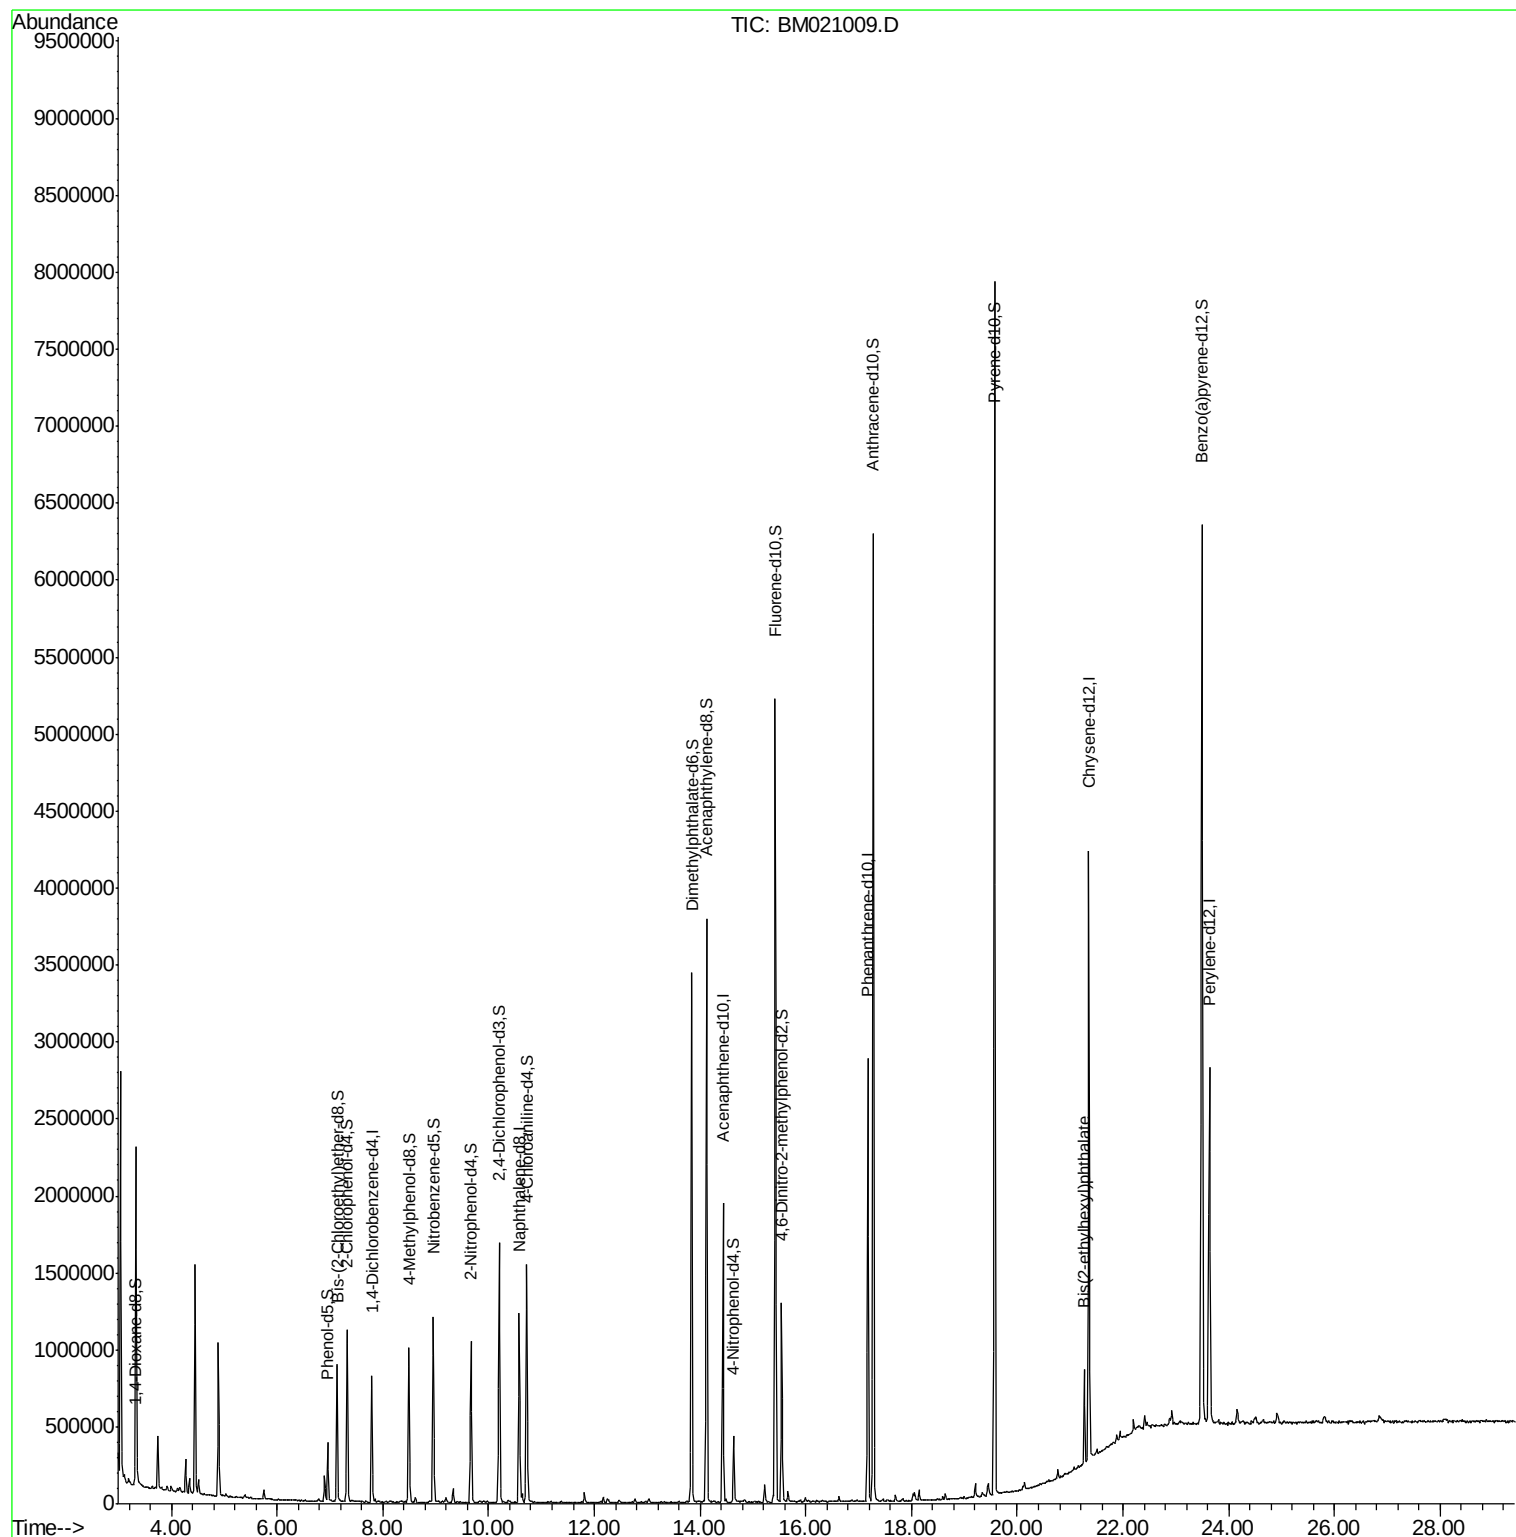

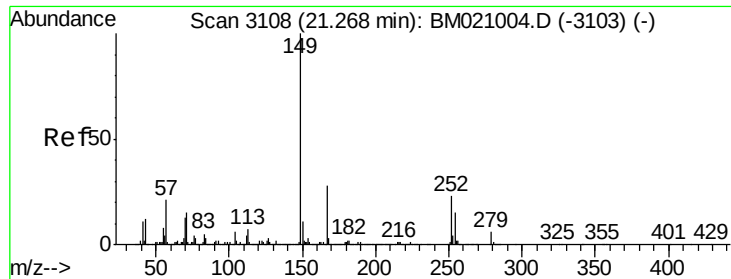

#83

Bis(2-ethylhexyl)phthalate

Concen: 2.908 ng/ul

RT: 21.27 min Scan# 3108

Delta R.T. 0.01 min

Lab File: BM021009.D

Acq: 18 Jun 2019 13:31

Instrument :

BNA_M

ClientSampleId :

C0JS9


Tot Ion:149 Resp: 194763

Ion Ratio Lower Upper

149 100

167 26.8 22.3 33.5

279 5.0 3.8 5.6

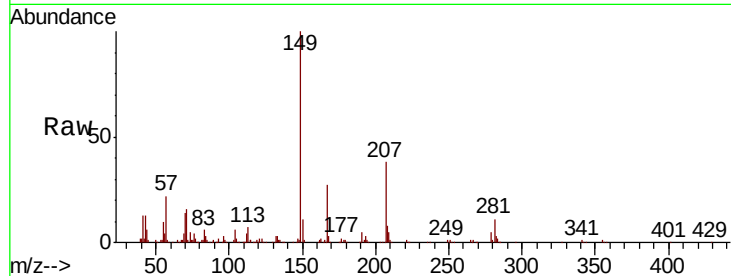

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

