

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061819\
 Data File : BM021030.D
 Acq On : 19 Jun 2019 02:10
 Operator : HP/JU
 Sample : PB120551BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	5	8	15	rVB2	44457	60900	0.75%	0.074%
2	3.293	49	52	61	rBV2	67534	104405	1.29%	0.127%
3	6.951	667	674	688	rBV	1237136	1928131	23.78%	2.352%
4	7.128	697	704	715	rBV	1017155	1562062	19.26%	1.906%
5	7.316	729	736	748	rVB	1262226	2042893	25.19%	2.492%
6	7.786	808	816	825	rBV	876946	1380089	17.02%	1.684%
7	8.486	926	935	944	rBV	1641229	2596882	32.02%	3.168%
8	8.951	1004	1014	1026	rBV	1268196	2137171	26.35%	2.607%
9	9.663	1127	1135	1146	rBV	1115463	1837638	22.66%	2.242%
10	10.192	1218	1225	1240	rBV	1748897	2939587	36.25%	3.586%
11	10.575	1279	1290	1298	rBV	1354136	2216437	27.33%	2.704%
12	10.716	1307	1314	1334	rBV	1679482	2964309	36.55%	3.616%
13	12.174	1554	1562	1568	rVB2	24370	48449	0.60%	0.059%
14	13.386	1763	1768	1773	rBV2	4883	8397	0.10%	0.010%
15	13.839	1838	1845	1853	rBV	3610771	4917471	60.64%	5.999%
16	14.115	1884	1892	1902	rBV	3832665	5919758	72.99%	7.222%
17	14.427	1938	1945	1955	rBV2	2211129	3348526	41.29%	4.085%
18	14.627	1972	1979	1995	rBV	1297758	1950531	24.05%	2.380%
19	15.221	2073	2080	2086	rBV	34327	45396	0.56%	0.055%
20	15.421	2107	2114	2124	rBV	5318556	7421895	91.52%	9.055%
21	15.545	2129	2135	2146	rVV	1152844	1596786	19.69%	1.948%
22	15.662	2150	2155	2161	rVB	58249	86171	1.06%	0.105%
23	16.204	2244	2247	2251	rVB2	7609	9462	0.12%	0.012%
24	16.374	2271	2276	2281	rVB6	4582	8623	0.11%	0.011%
25	16.956	2371	2375	2380	rVB3	10137	14348	0.18%	0.018%
26	17.174	2405	2412	2422	rBV	2837791	3935663	48.53%	4.802%
27	17.274	2422	2429	2442	rBV	5321942	7622345	93.99%	9.299%
28	17.556	2476	2477	2484	rVB4	6862	8134	0.10%	0.010%
29	19.198	2752	2756	2761	rVV	48133	62051	0.77%	0.076%
30	19.450	2796	2799	2803	rVB	43848	48157	0.59%	0.059%
31	19.568	2812	2819	2829	rBV	5851972	8109904	100.00%	9.894%
32	21.350	3117	3122	3130	rBV	3019099	3745437	46.18%	4.569%
33	23.485	3477	3485	3496	rVB	4086990	7633755	94.13%	9.313%
34	23.627	3503	3509	3521	rVB	1954226	3654935	45.07%	4.459%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061819\
Data File : BM021030.D
Acq On : 19 Jun 2019 02:10
Operator : HP/JU
Sample : PB120551BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 81966698

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061819\
Data File : BM021030.D
Acq On : 19 Jun 2019 02:10
Operator : HP/JU
Sample : PB120551BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

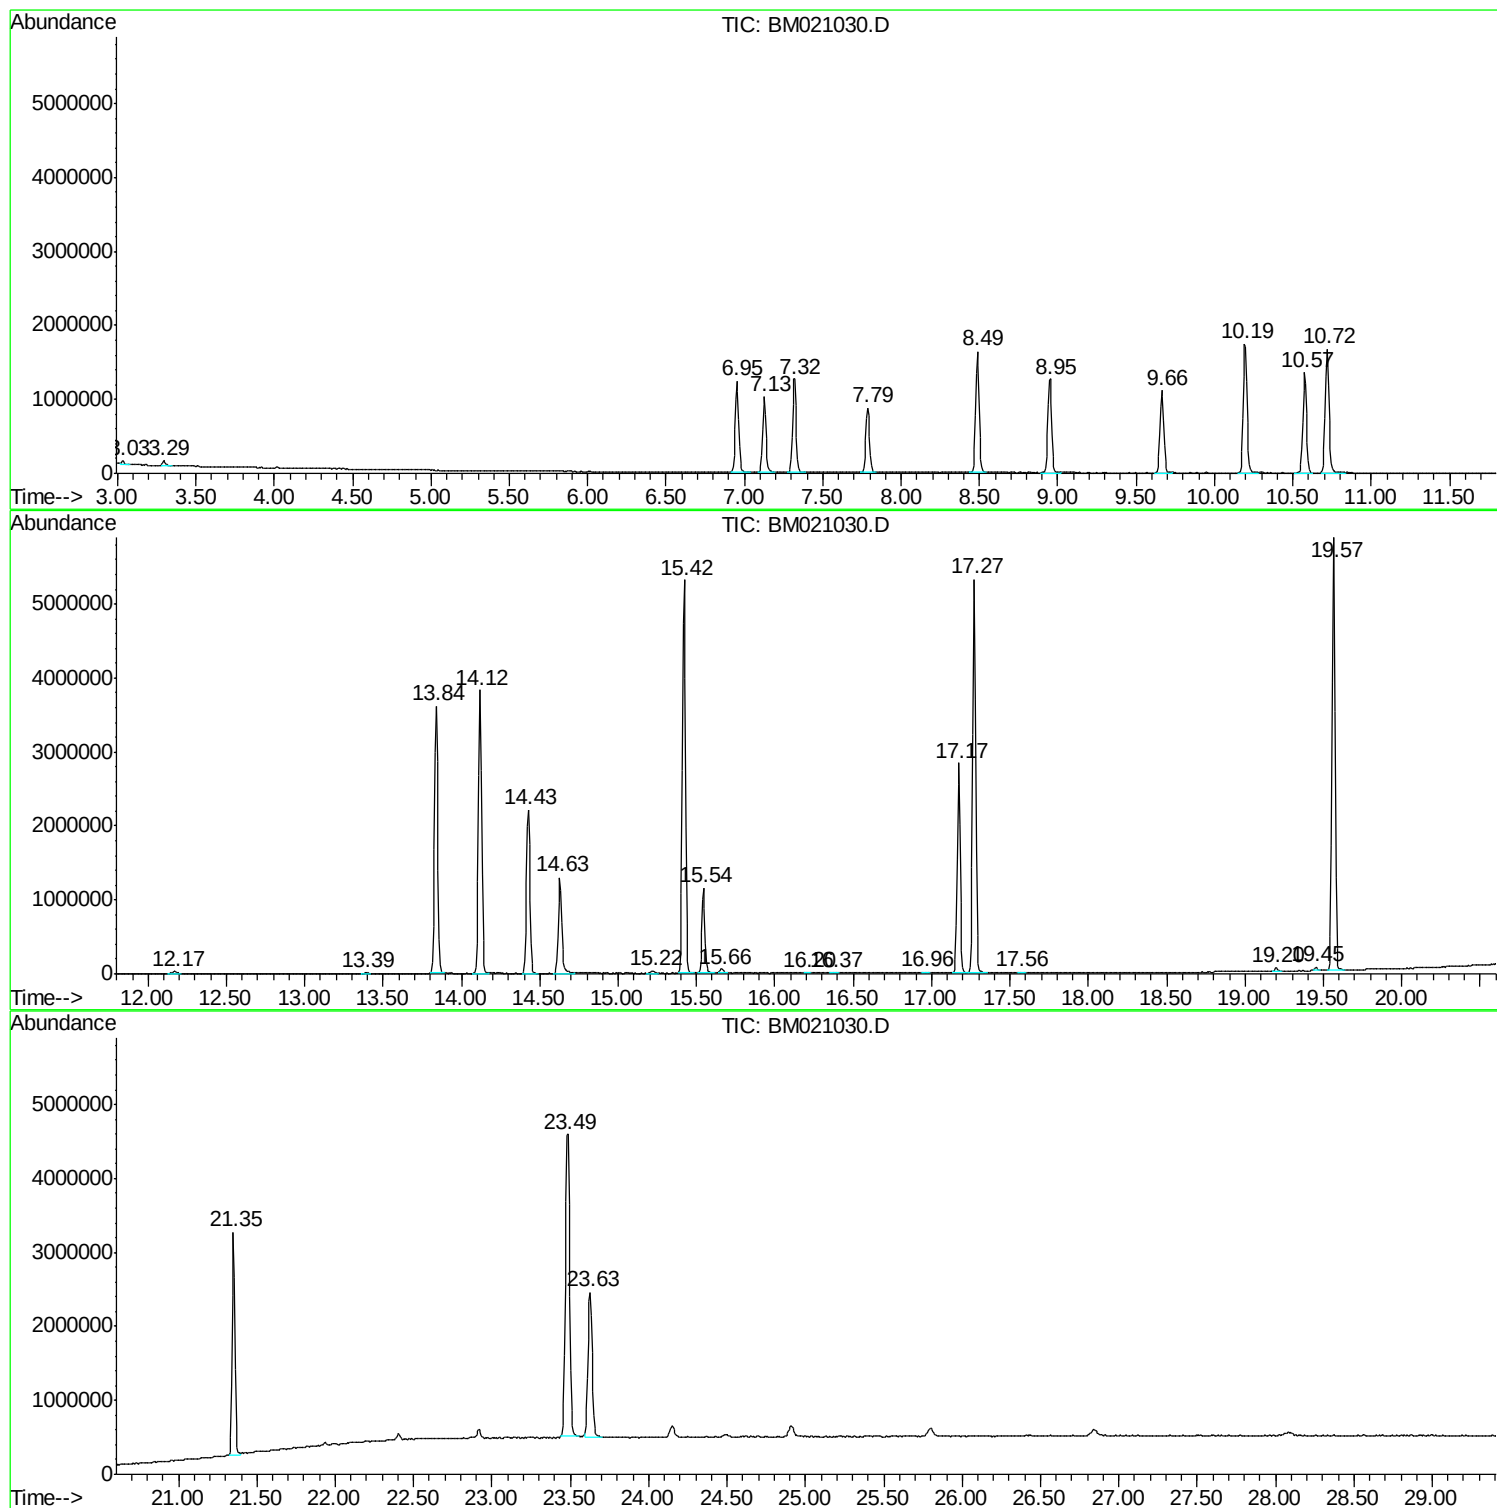

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061819\
Data File : BM021030.D
Acq On : 19 Jun 2019 02:10
Operator : HP/JU
Sample : PB120551BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061819\
Data File : BM021030.D
Acq On : 19 Jun 2019 02:10
Operator : HP/JU
Sample : PB120551BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK51

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc