

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061919\
 Data File : BM021034.D
 Acq On : 19 Jun 2019 09:47
 Operator : HP/JU
 Sample : K3332-06
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4231

Quant Time: Jun 19 12:36:21 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 19 00:56:26 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	212144	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	948399	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	630237	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1527525	20.00	ng/ul	0.00
77) Chrysene-d12	21.35	240	1286413	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	1282126	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.30	96	18898	4.23	ng/uL	0.00
5) Phenol-d5	6.95	99	421887	22.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	261190	23.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	347044	23.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	355277	23.05	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	184413	23.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	206745	24.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	413524	23.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	438029	24.16	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1551003	27.24	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1770666	25.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	197127	21.28	ng/ul	0.00
57) Fluorene-d10	15.42	176	1347931	27.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	173807	18.51	ng/ul	0.00
70) Anthracene-d10	17.27	188	2134430	26.89	ng/ul	0.00
78) Pyrene-d10	19.56	212	2281892	29.56	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.48	264	2007135	26.53	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	13.89	163	171852	3.315	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061919\
Data File : BM021034.D
Acq On : 19 Jun 2019 09:47
Operator : HP/JU
Sample : K3332-06
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4231

Quant Time: Jun 19 12:36:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 19 00:56:26 2019
Response via : Initial Calibration

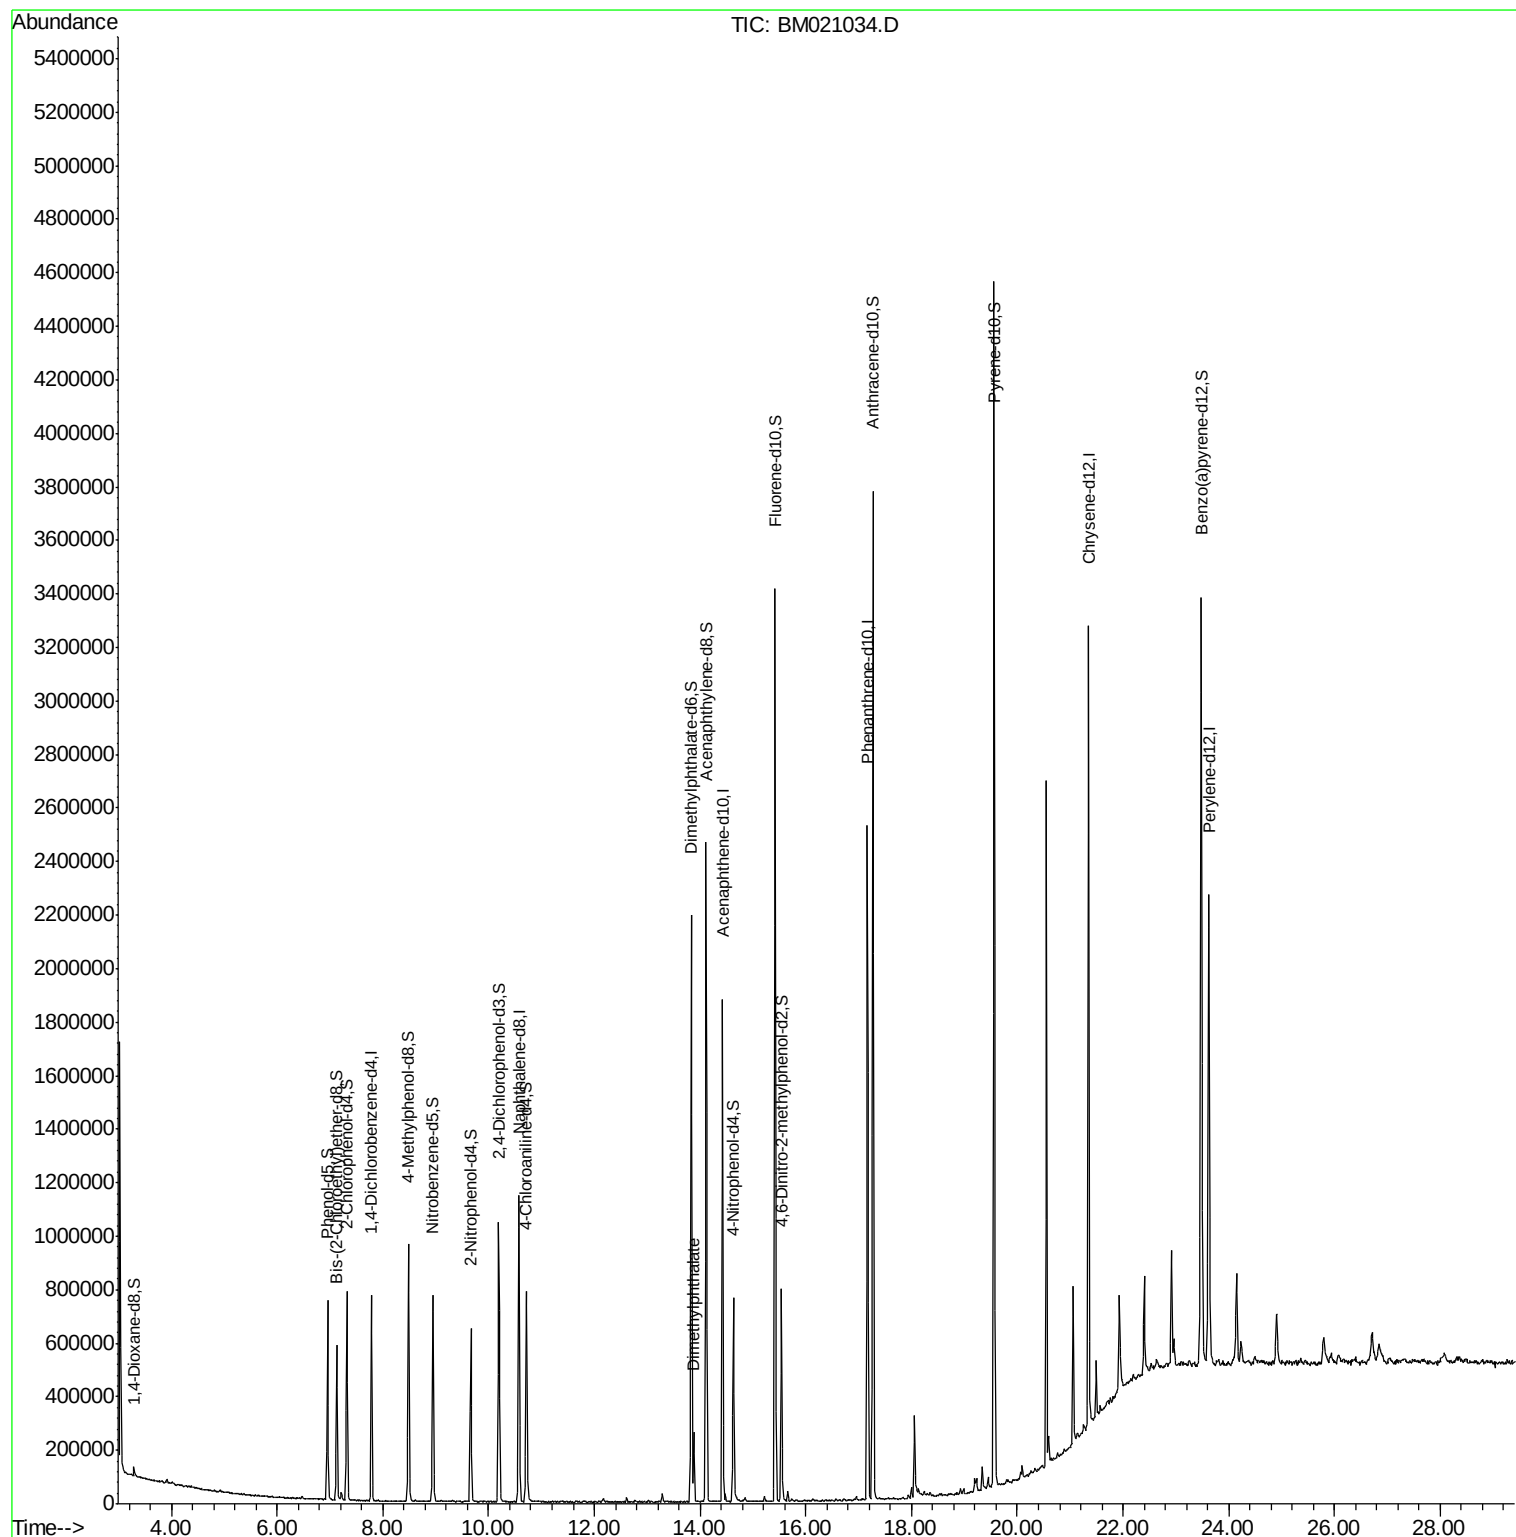

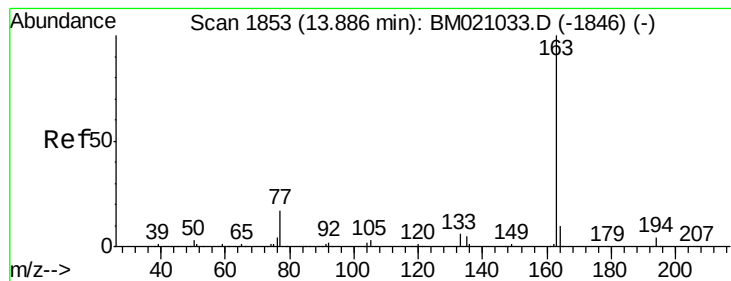

#44

Dimethylphthalate

Concen: 3.315 ng/ul

RT: 13.89 min Scan# 1853

Delta R.T. -0.00 min

Lab File: BM021034.D

Acq: 19 Jun 2019 09:47

Instrument :

BNA_M

ClientSampleId :

A4231


Tot Ion:163 Resp: 171852

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 9.4 7.7 11.5

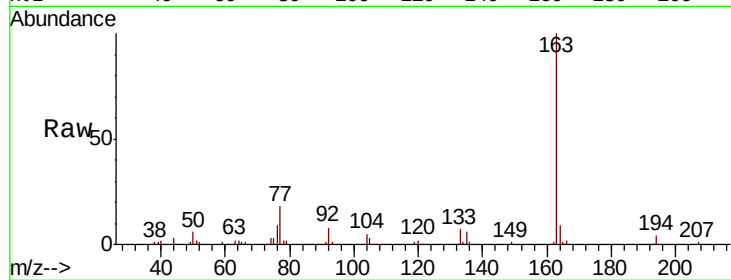

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

