

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061919\
 Data File : BM021036.D
 Acq On : 19 Jun 2019 14:06
 Operator : HP/JU
 Sample : K3332-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4233

Quant Time: Jun 19 15:03:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 19 00:56:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	236416	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1069401	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	707811	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1672195	20.00	ng/ul	0.00
77) Chrysene-d12	21.36	240	1407715	20.00	ng/ul	0.00
85) Perylene-d12	23.63	264	1418132	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	17274	3.47	ng/uL	0.00
5) Phenol-d5	6.95	99	393708	19.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	243738	19.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	321242	19.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	324035	18.86	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	173317	19.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	198891	20.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	389902	19.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	426590	20.87	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1440547	22.52	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1670632	21.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	169450	16.29	ng/ul	0.00
57) Fluorene-d10	15.42	176	1238389	22.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	161274	15.69	ng/ul	0.00
70) Anthracene-d10	17.27	188	1921349	22.11	ng/ul	0.00
78) Pyrene-d10	19.56	212	2063173	24.42	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.49	264	1835307	21.94	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.89	163	281418	4.834	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061919\
Data File : BM021036.D
Acq On : 19 Jun 2019 14:06
Operator : HP/JU
Sample : K3332-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4233

Quant Time: Jun 19 15:03:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 19 00:56:26 2019
Response via : Initial Calibration

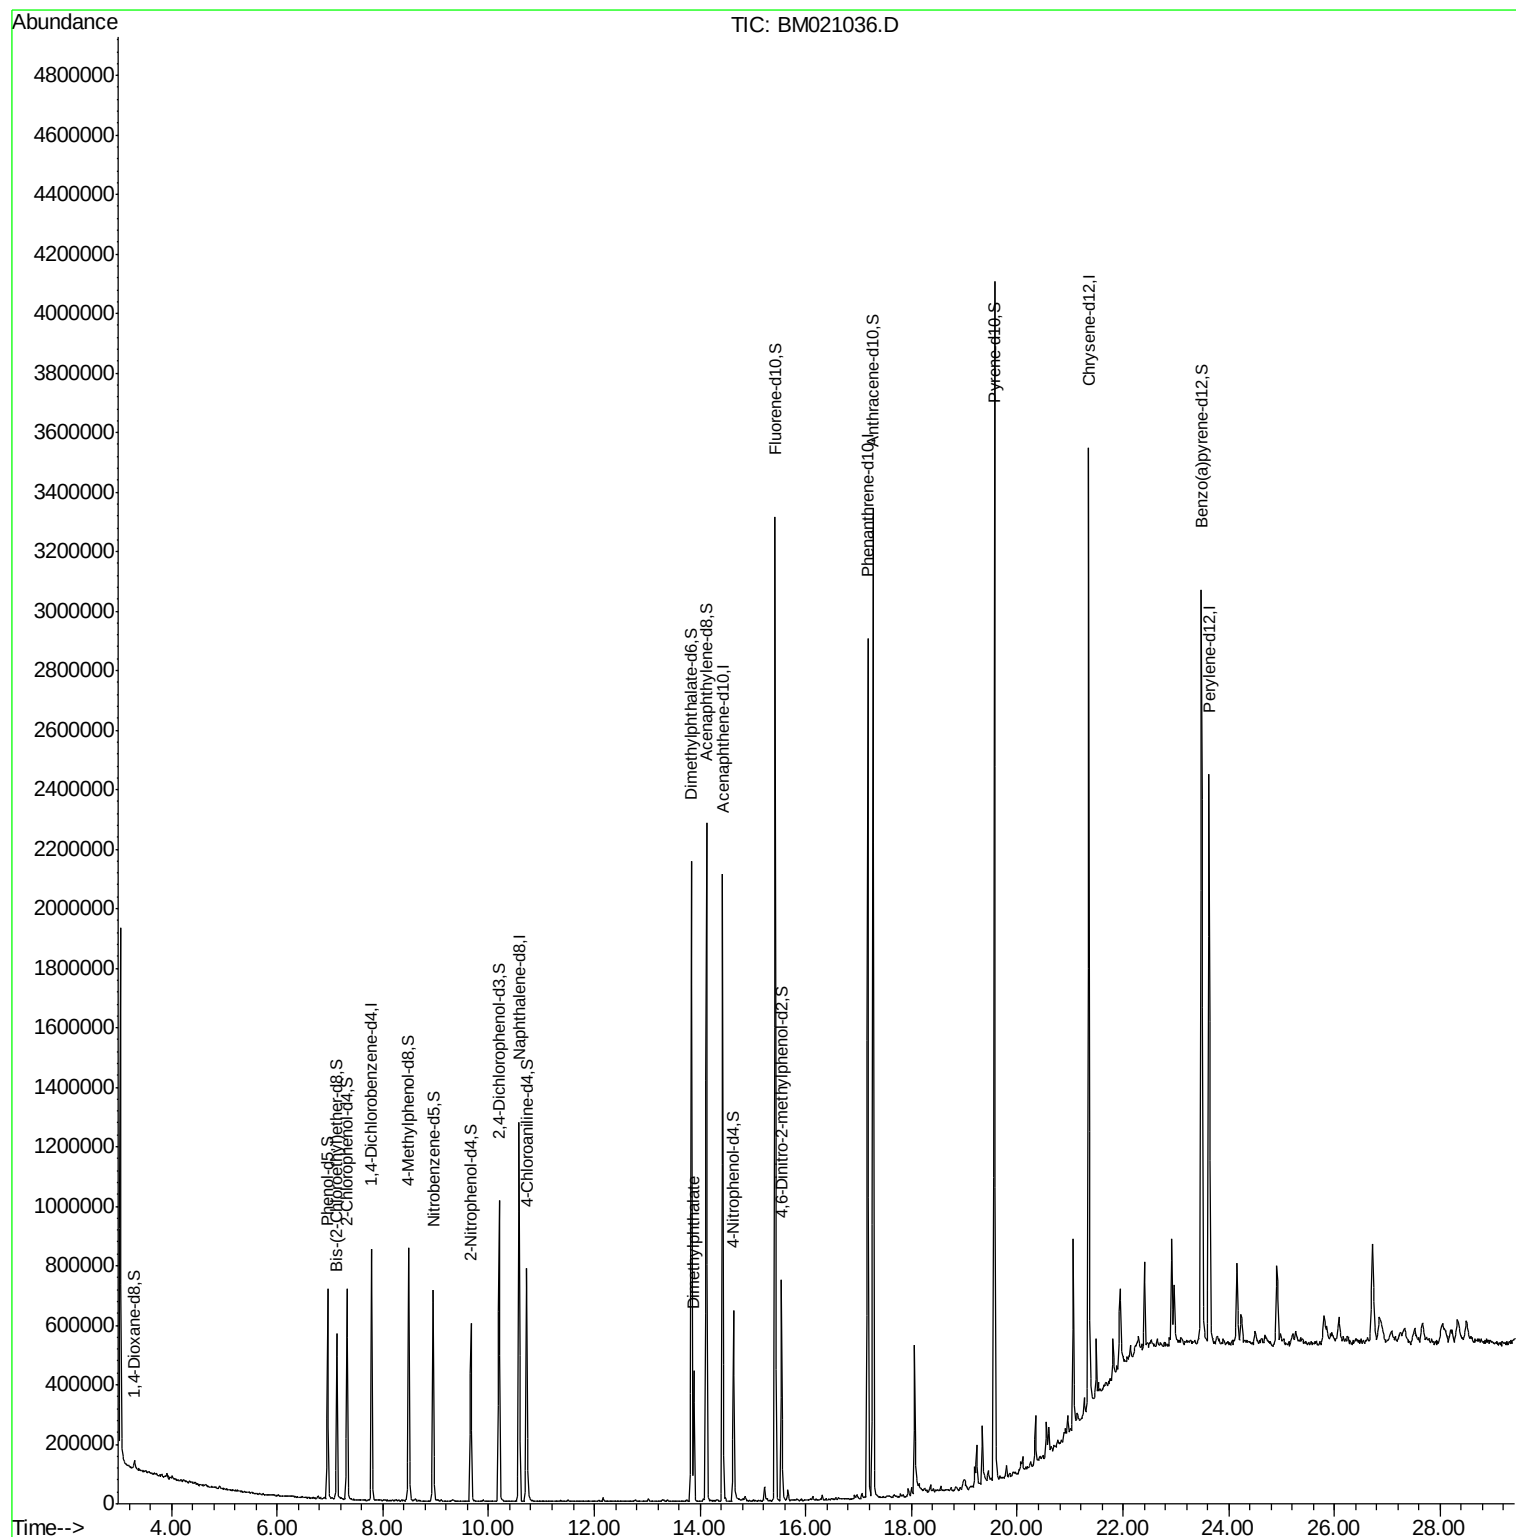

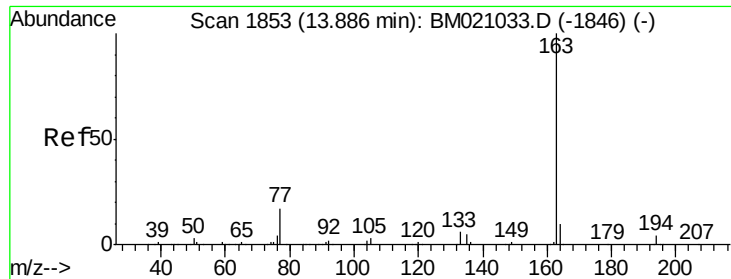

#44

Dimethylphthalate

Concen: 4.834 ng/ul

RT: 13.89 min Scan# 1853

Delta R.T. 0.00 min

Lab File: BM021036.D

Acq: 19 Jun 2019 14:06

Instrument :

BNA_M

ClientSampleId :

A4233

Tot Ion:163 Resp: 281418

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.1 7.7 11.5

