

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061923\
 Data File : BM040308.D
 Acq On : 19 Jun 2023 11:11
 Operator : MA/JU
 Sample : PB153382BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK382

Quant Time: Jun 20 00:12:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 15 00:31:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	7750	0.400	ng/ul	0.00
4) Naphthalene-d8	10.777	136	29830	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.603	164	16815	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.348	188	32920	0.400	ng/ul	0.00
17) Chrysene-d12	21.525	240	26335	0.400	ng/ul	# 0.00
23) Perylene-d12	23.945	264	35074	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.342	96	60919	6.366	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.360	152	13116	0.346	ng/ul	-0.01
18) Fluoranthene-d10	19.369	212	24267	0.369	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.593	166	4356	0.078	ng/ul#	15
20) Pyrene	19.736	202	4946	0.053	ng/ul#	1
26) Benzo(a)pyrene	23.796	252	9606	0.091	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061923\
Data File : BM040308.D
Acq On : 19 Jun 2023 11:11
Operator : MA/JU
Sample : PB153382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK382

Quant Time: Jun 20 00:12:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 00:31:16 2023
Response via : Initial Calibration

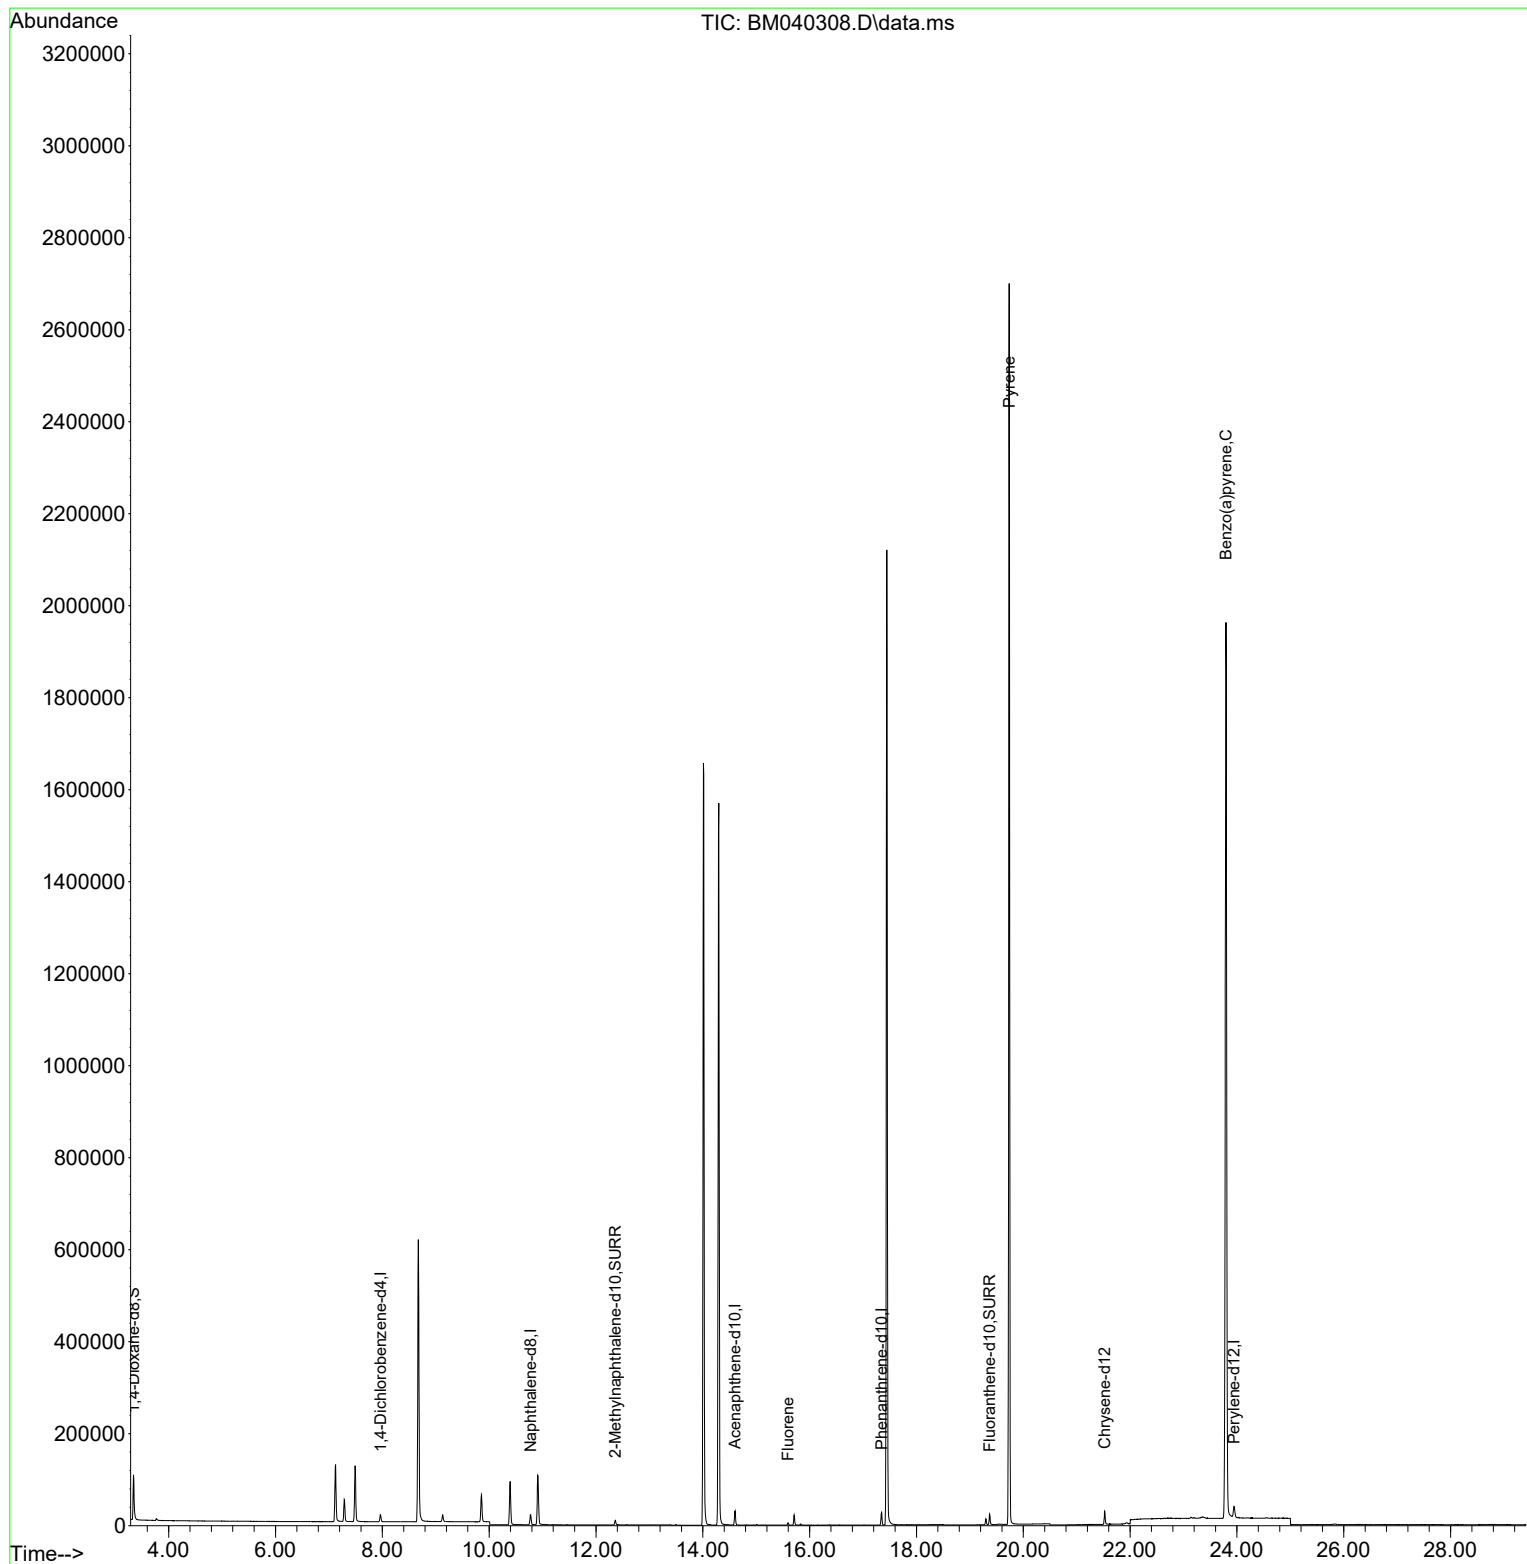

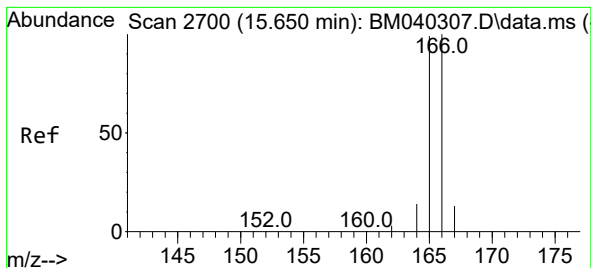

#12

Fluorene

Concen: 0.078 ng/ul

RT: 15.593 min Scan# 2

Delta R.T. -0.066 min

Lab File: BM040308.D

Acq: 19 Jun 2023 11:11

Instrument :

BNA_M

ClientSampleId :

SBLK382





Tgt Ion:166 Resp: 4356

Ion Ratio Lower Upper

166 100

165 9.4 78.2 117.4#

167 34.0 11.0 16.4#

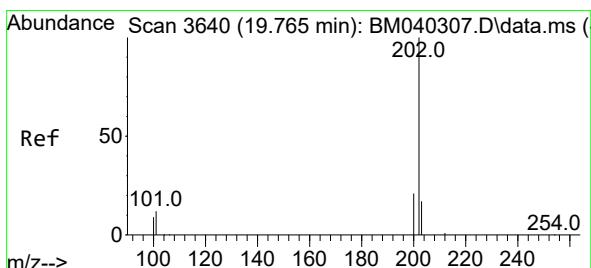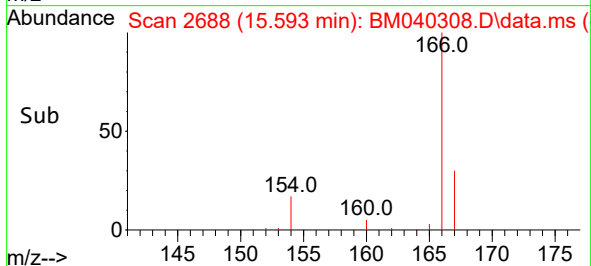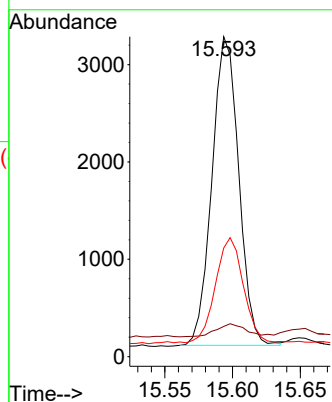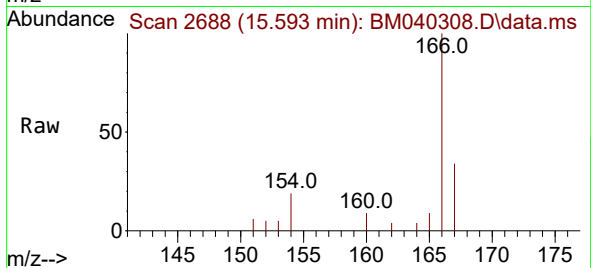

#20

Pyrene

Concen: 0.053 ng/ul

RT: 19.736 min Scan# 3634

Delta R.T. -0.034 min

Lab File: BM040308.D

Acq: 19 Jun 2023 11:11




Tgt Ion:202 Resp: 4946


Ion Ratio Lower Upper

202 100

101 165.0 11.8 17.8#


100 1152.9 9.3 13.9#

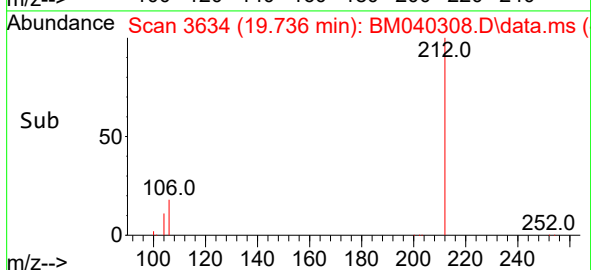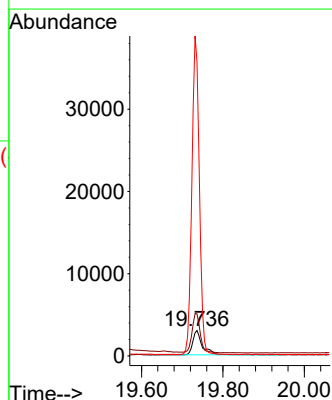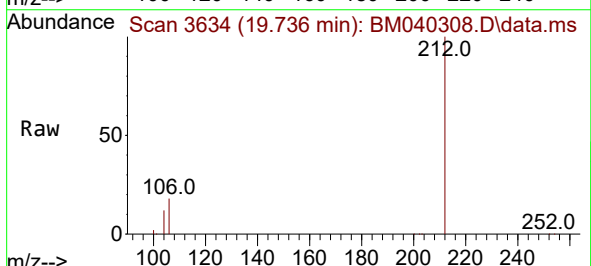

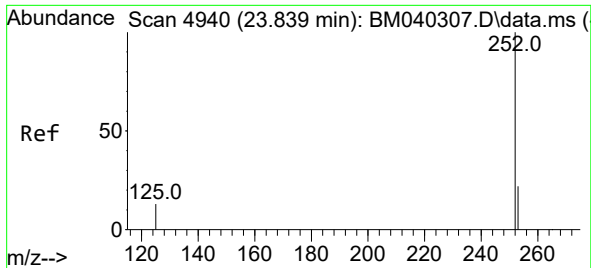

#26
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 23.796 min Scan# 4940
Delta R.T. -0.054 min
Lab File: BM040308.D
Acq: 19 Jun 2023 11:11

Instrument :
BNA_M
ClientSampleId :
SBLK382

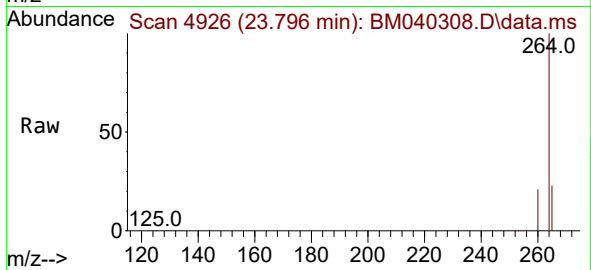

Tgt Ion:252 Resp: 9606
Ion Ratio Lower Upper
252 100
253 59.2 23.4 35.0#
125 63.3 19.7 29.5#

