

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062019\
 Data File : BM021068.D
 Acq On : 20 Jun 2019 19:14
 Operator : HP/JU
 Sample : PB120267BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120267BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	399	405	420	rVB	3239892	4601055	28.21%	6.157%
2	6.951	667	674	692	rVB	3299857	5220146	32.01%	6.985%
3	7.310	728	735	747	rBV	3322305	5311429	32.57%	7.107%
4	7.781	808	815	824	rVB	827101	1323086	8.11%	1.770%
5	8.098	861	869	876	rBV	2502121	4029661	24.71%	5.392%
6	8.939	1005	1012	1029	rBV	1887449	3142748	19.27%	4.205%
7	10.569	1279	1289	1300	rBV	1092505	1832706	11.24%	2.452%
8	13.039	1701	1709	1723	rBV	5963891	9036260	55.40%	12.092%
9	14.421	1937	1944	1955	rBV2	1843579	2864337	17.56%	3.833%
10	15.910	2190	2197	2213	rBV	5436466	7802336	47.84%	10.440%
11	17.168	2404	2411	2421	rBV2	2797973	3944321	24.18%	5.278%
12	19.792	2851	2857	2865	rBV	13462540	16309730	100.00%	21.824%
13	21.350	3117	3122	3129	rBV	3843631	4702001	28.83%	6.292%
14	23.627	3502	3509	3521	rVB2	2371913	4612457	28.28%	6.172%


Sum of corrected areas: 74732273

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062019\
Data File : BM021068.D
Acq On : 20 Jun 2019 19:14
Operator : HP/JU
Sample : PB120267BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120267BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

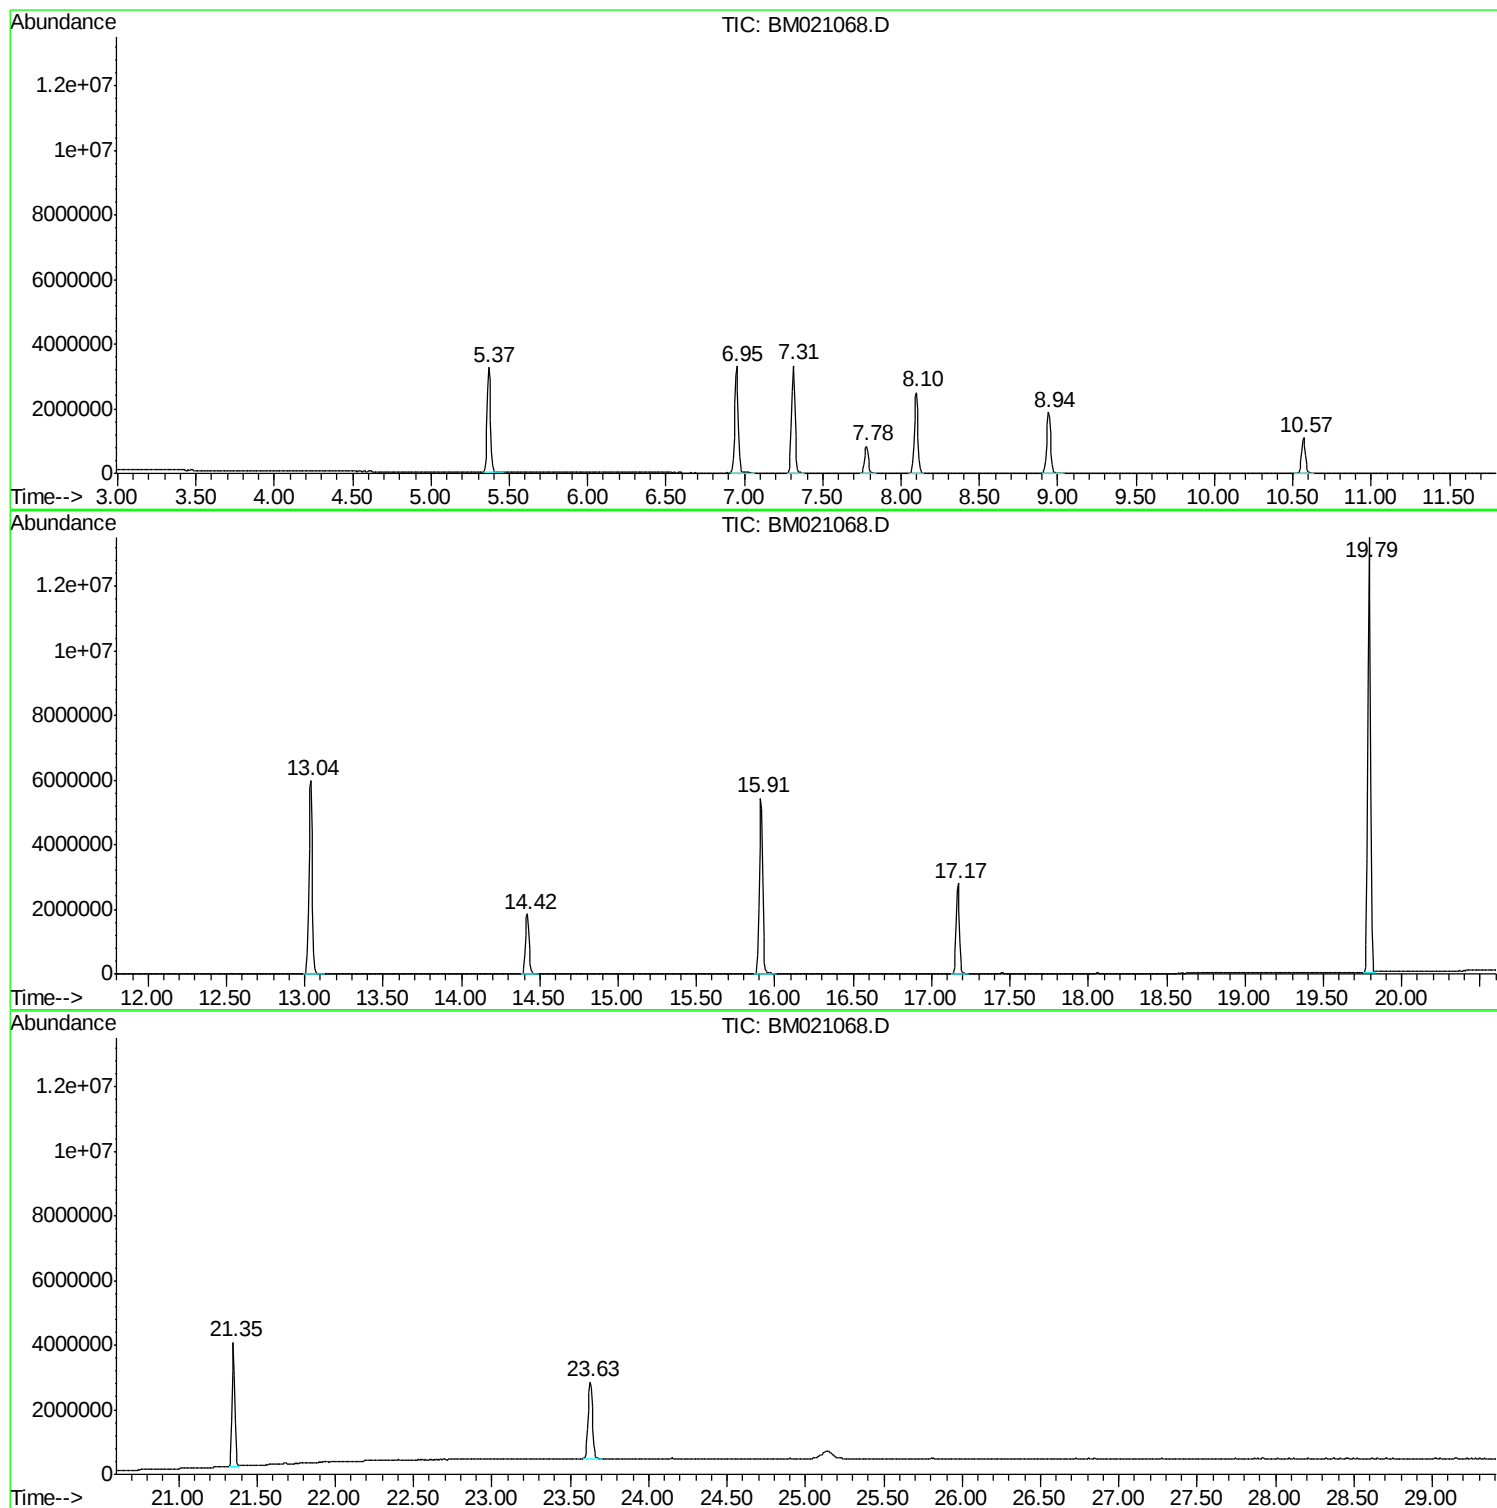

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062019\
Data File : BM021068.D
Acq On : 20 Jun 2019 19:14
Operator : HP/JU
Sample : PB120267BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120267BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.31	80.29 ng	5311430	1,4-Dichlorobenzene-d4	7.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

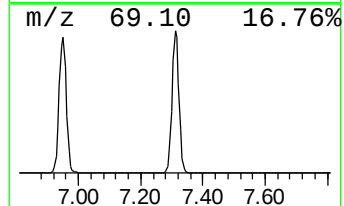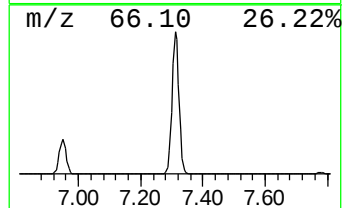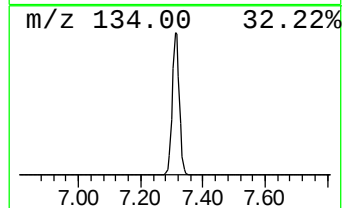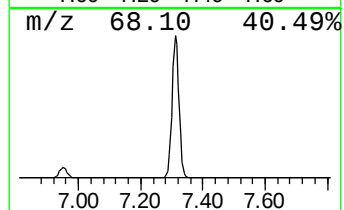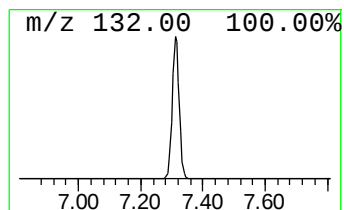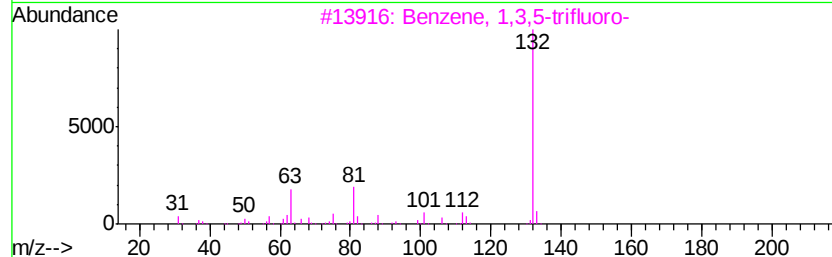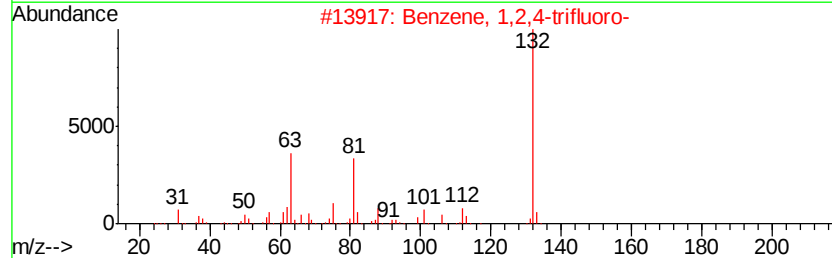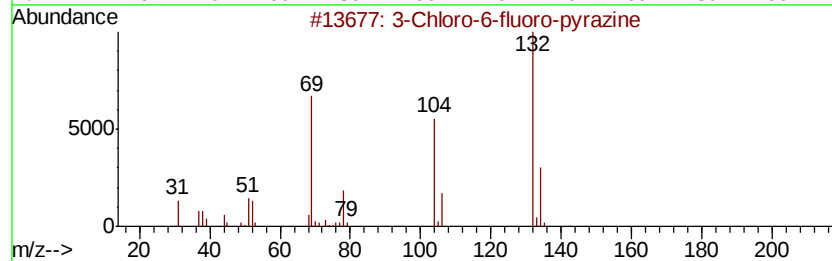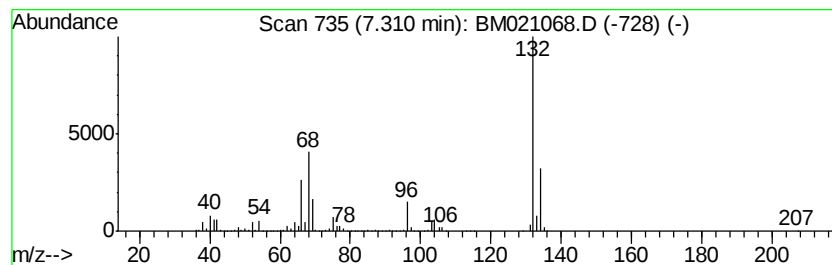

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062019\
Data File : BM021068.D
Acq On : 20 Jun 2019 19:14
Operator : HP/JU
Sample : PB120267BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120267BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.31	80.3	ng	5311430	1	7.78	1323090	20.0