


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062019\
 Data File : BM021057.D
 Acq On : 20 Jun 2019 09:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 20 15:39:58 2019

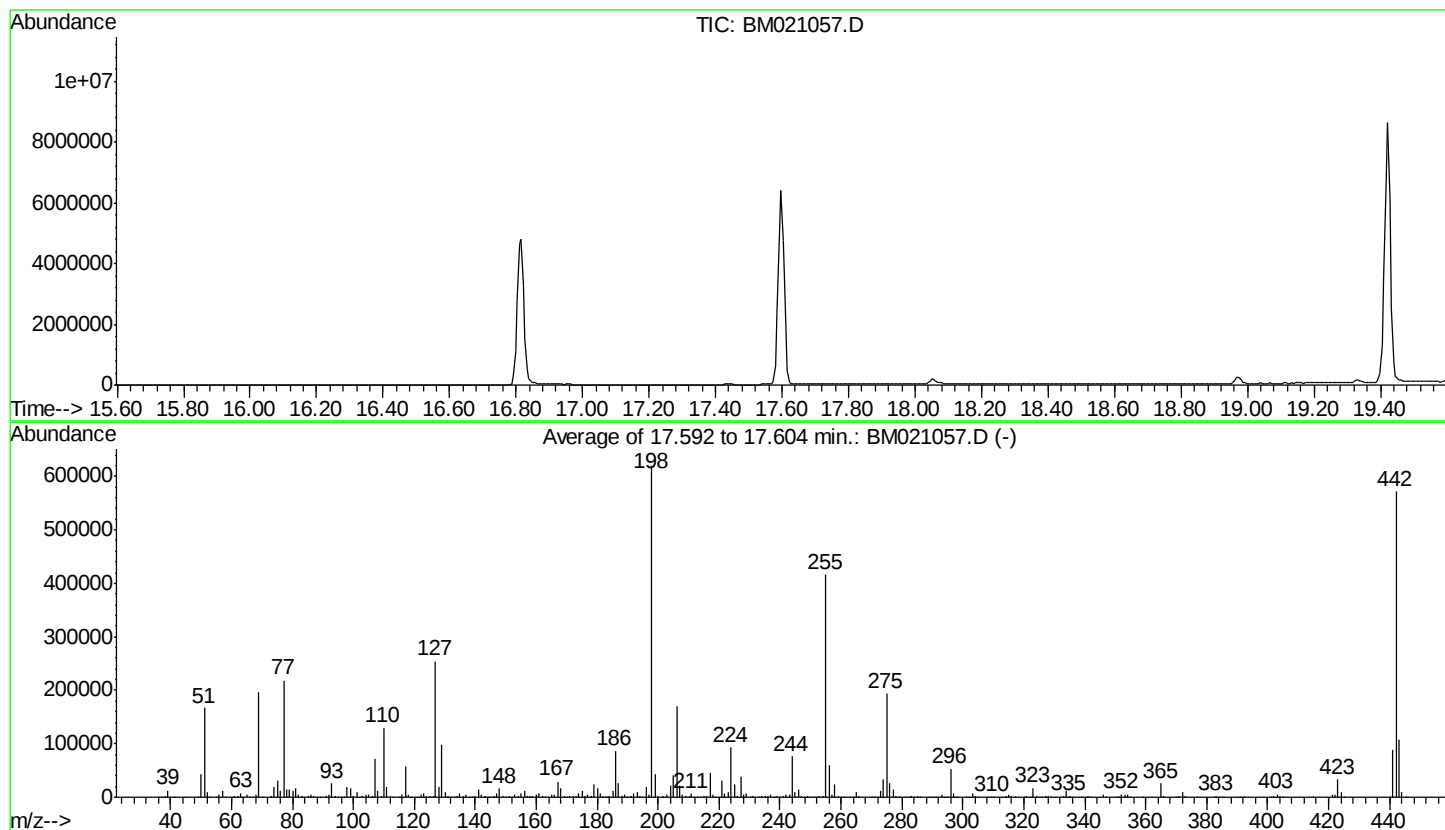

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	166909	PASS
68	69	0.00	2	1.9	3730	PASS
69	198	0.00	100	31.6	195816	PASS
70	69	0.00	2	0.6	1082	PASS
127	198	10	80	41.0	254314	PASS
197	198	0.00	2	0.8	4935	PASS
198	198	100	100	100.0	619989	PASS
199	198	5	9	7.0	43250	PASS
275	198	10	60	31.1	192810	PASS
365	198	1	100	4.1	25624	PASS
441	198	0.01	100	14.3	88557	PASS
442	198	50	100	92.2	571370	PASS
443	442	15	24	19.0	108480	PASS