


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062019\
 Data File : BM021066.D
 Acq On : 20 Jun 2019 18:01
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 20 15:39:58 2019

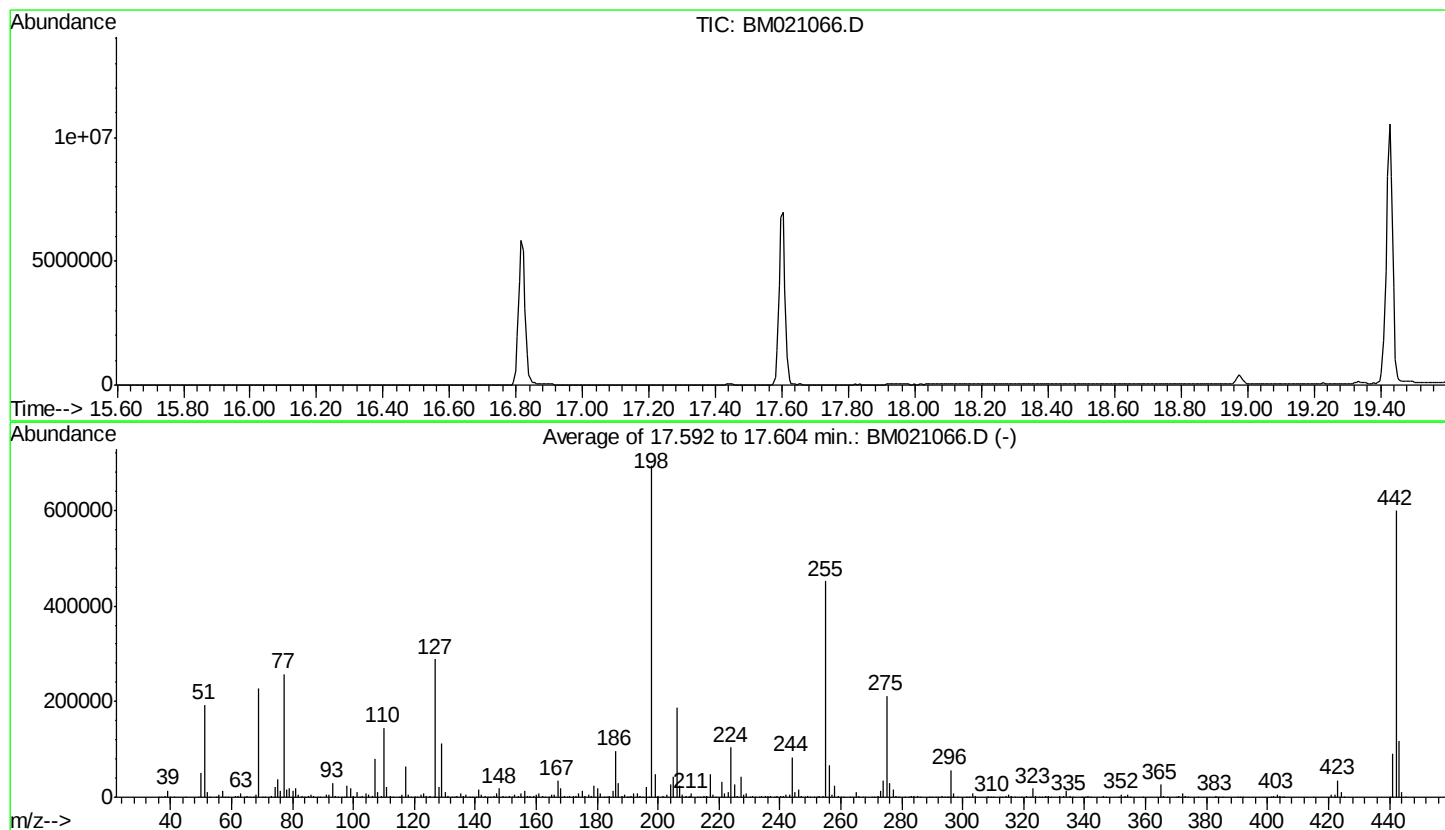

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	193642	PASS
68	69	0.00	2	1.9	4360	PASS
69	198	0.00	100	32.9	228291	PASS
70	69	0.00	2	0.4	915	PASS
127	198	10	80	41.6	288725	PASS
197	198	0.00	2	0.2	1220	PASS
198	198	100	100	100.0	693312	PASS
199	198	5	9	6.9	47672	PASS
275	198	10	60	30.6	212485	PASS
365	198	1	100	3.8	26466	PASS
441	198	0.01	100	13.2	91432	PASS
442	198	50	100	86.4	599125	PASS
443	442	15	24	19.7	118138	PASS