




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

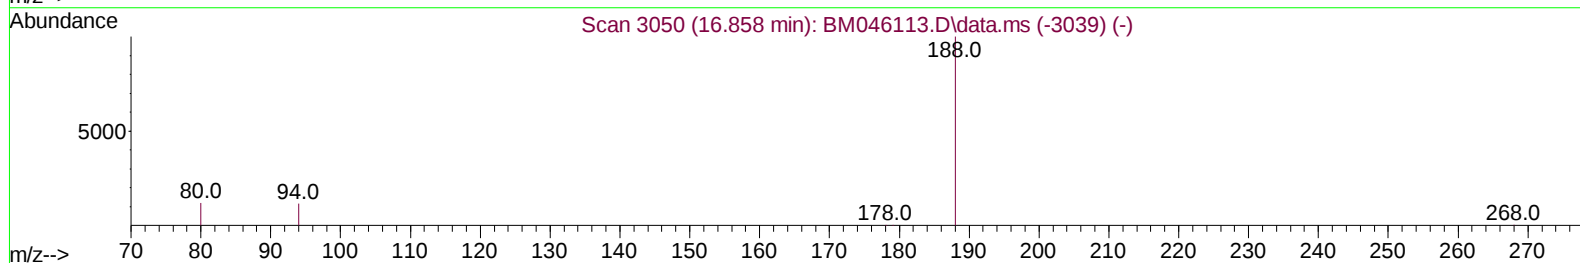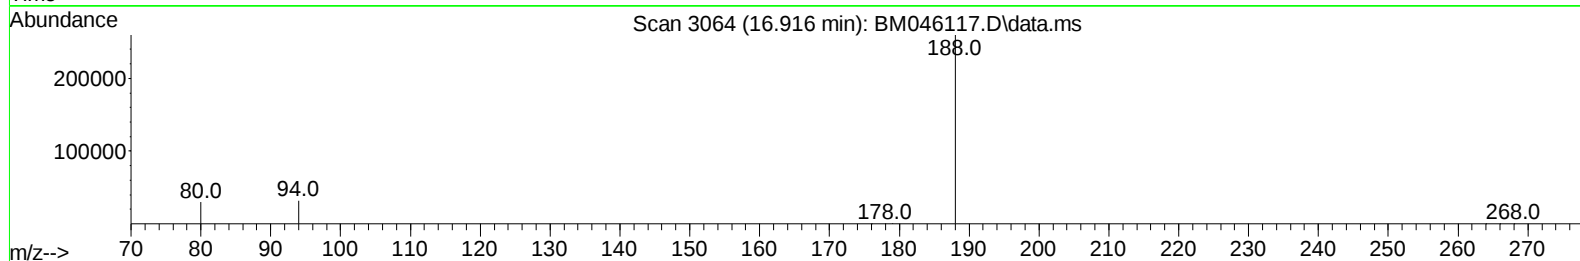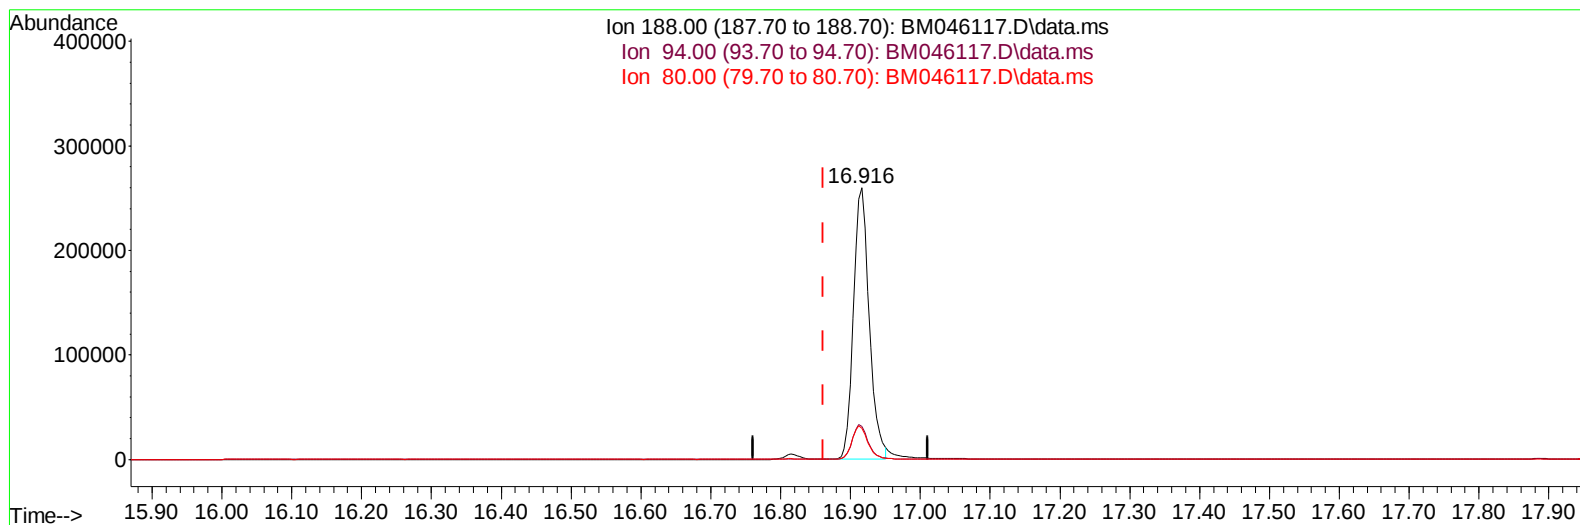

TIC: BM046117.D\data.ms

(13) Phenanthrene-d10 (I)

16.916min (+ 0.055) 0.40 ng/u1

response 407614

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	12.08
80.00	15.20	11.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

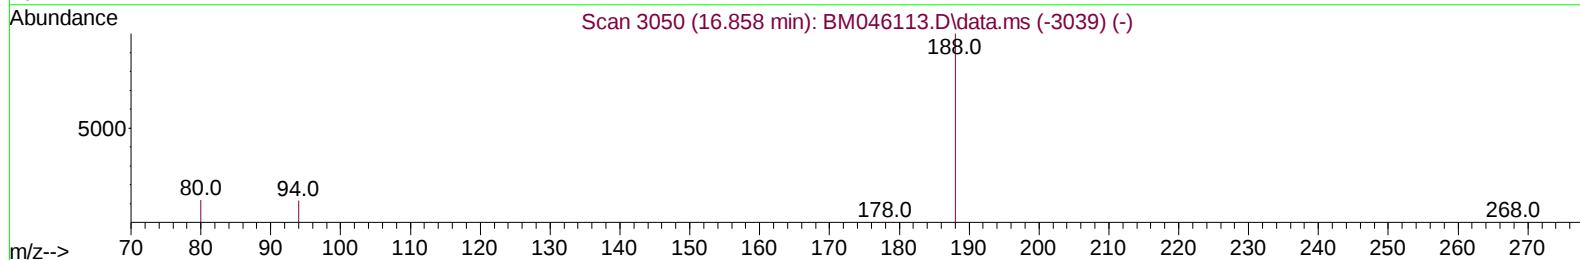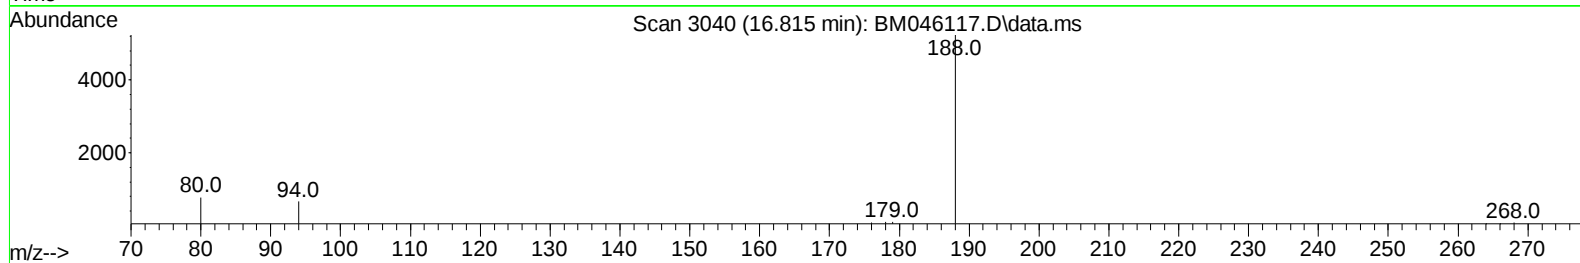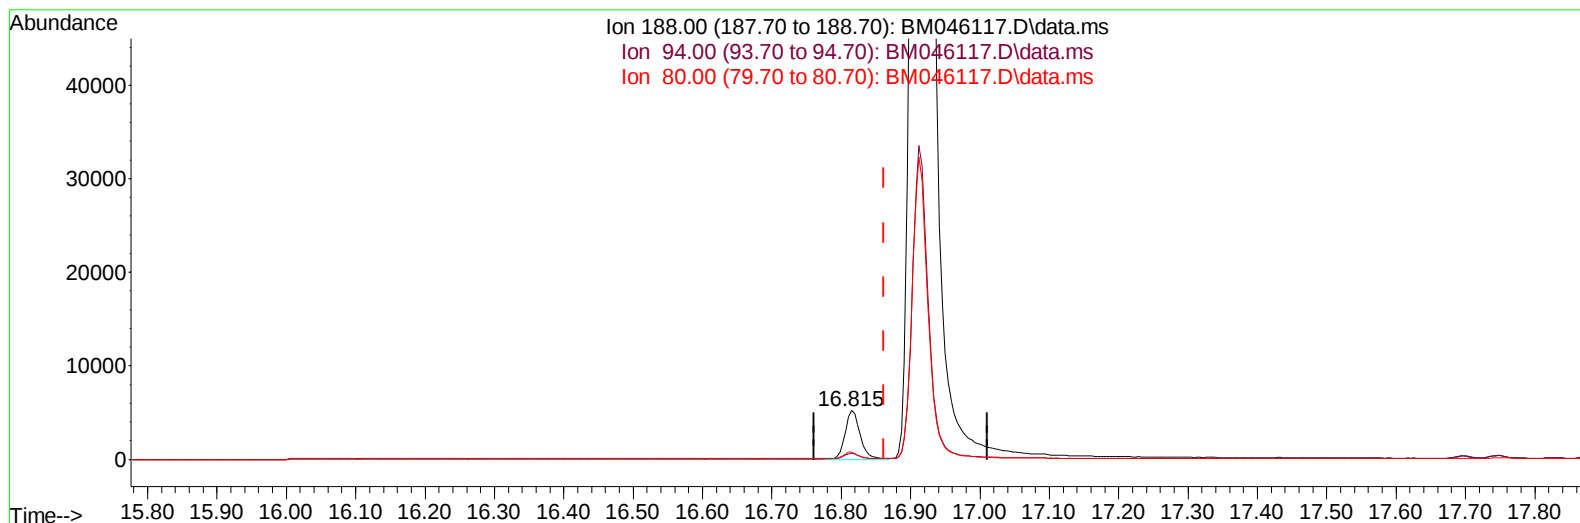

TIC: BM046117.D\data.ms

(13) Phenanthrene-d10 (I)

16.815min (-0.046) 0.40 ng/u1 m

response 7930

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	12.61
80.00	15.20	14.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

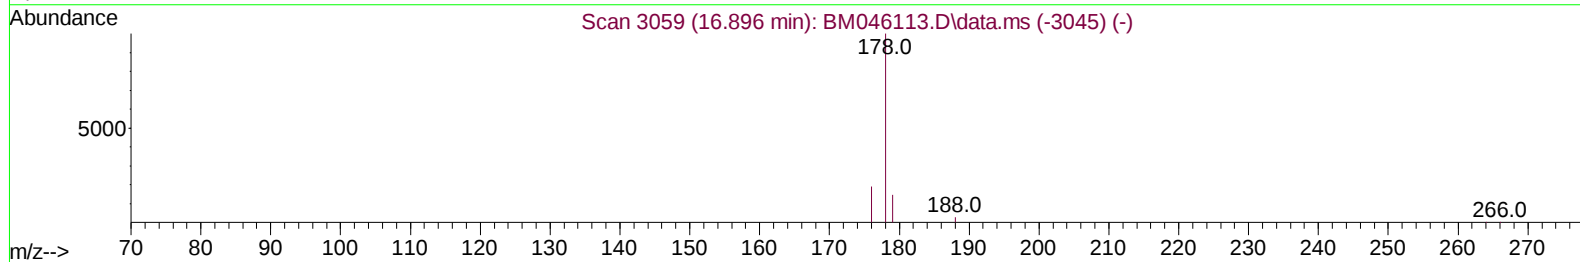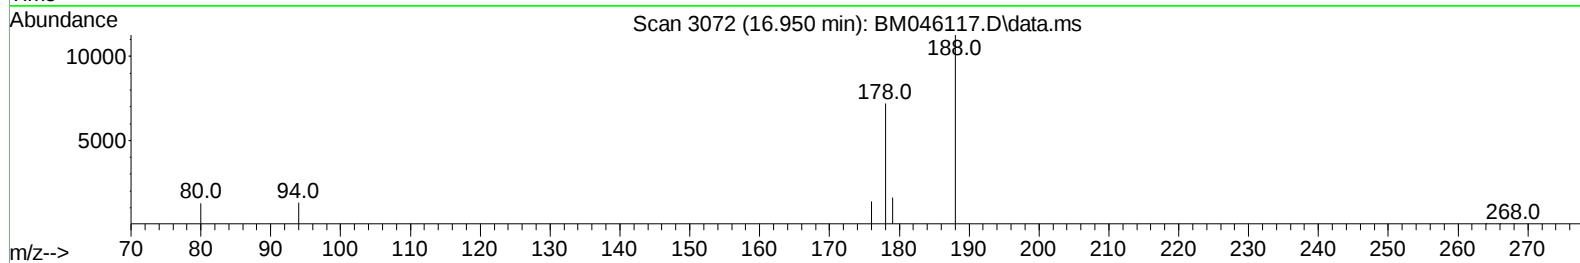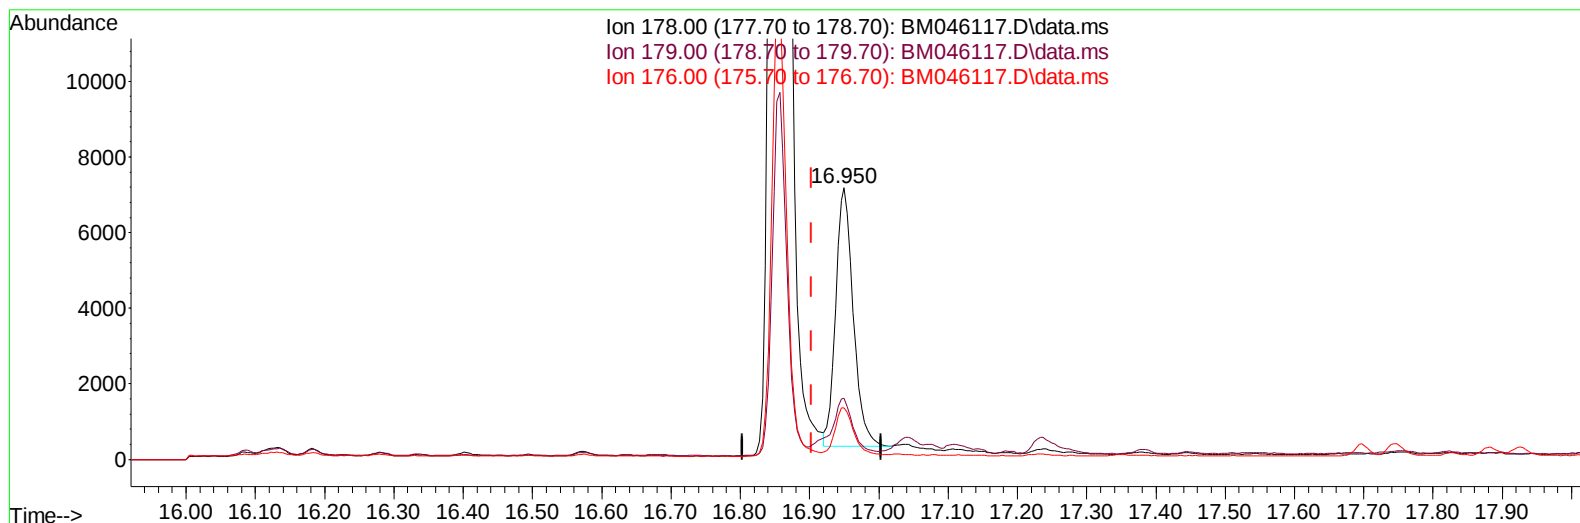

TIC: BM046117.D\data.ms

(15) Phenanthrene

16.950min (+ 0.047) 0.54 ng/u1

response 11977

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	22.43#
176.00	21.40	19.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

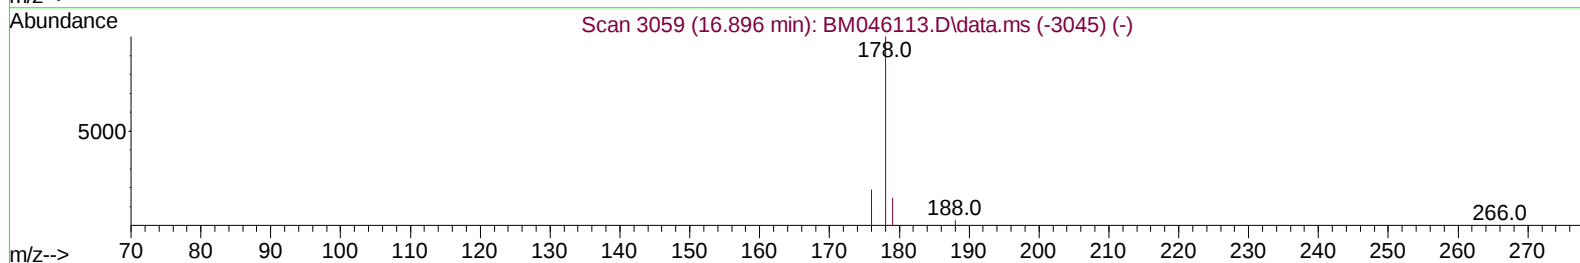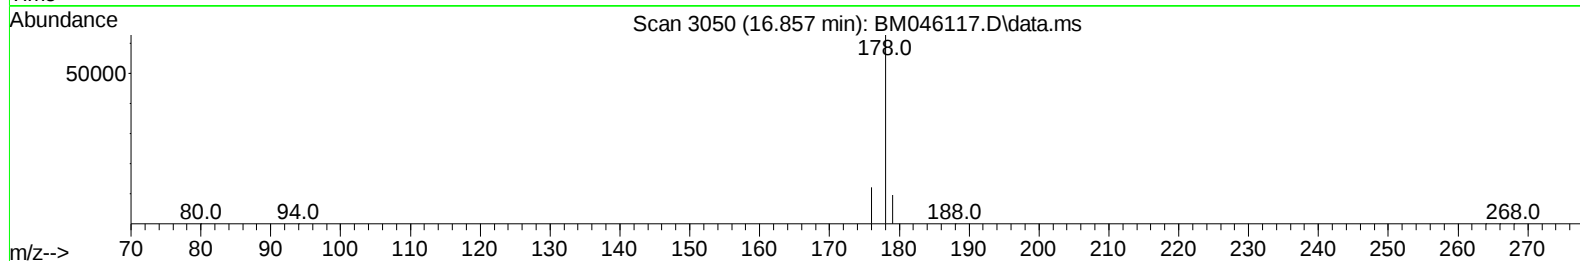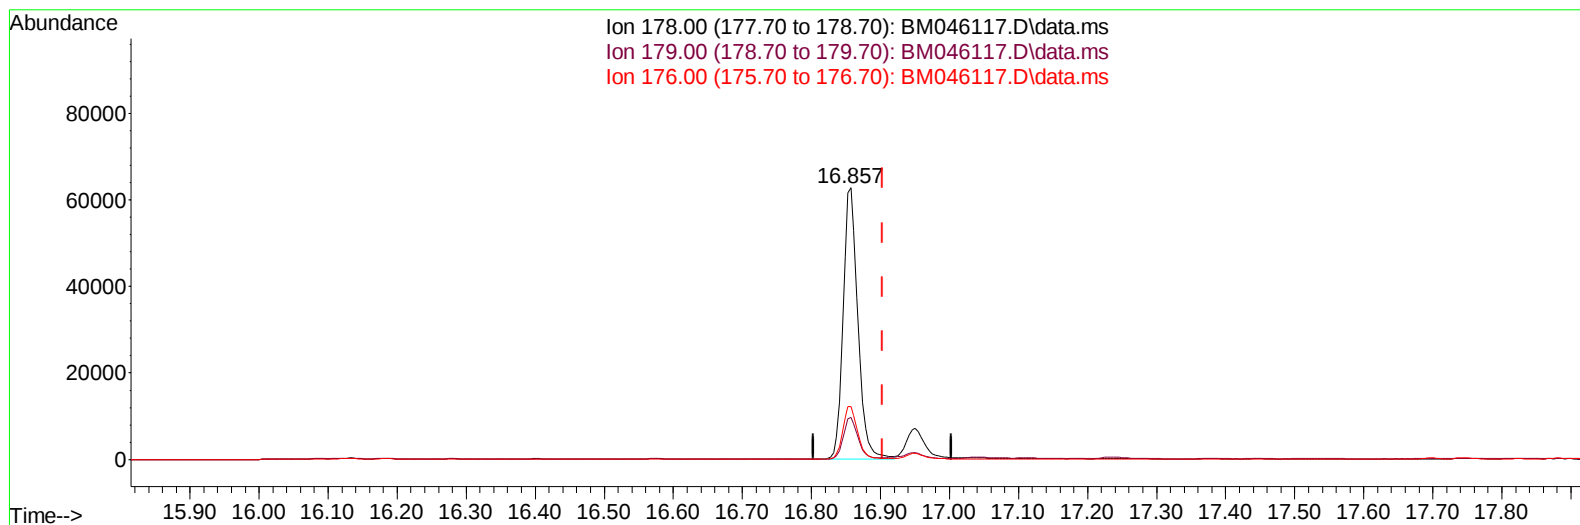

TIC: BM046117.D\data.ms

(15) Phenanthrene

16.857min (-0.046) 4.17 ng/u1 m

response 92875

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	15.46
176.00	21.40	19.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

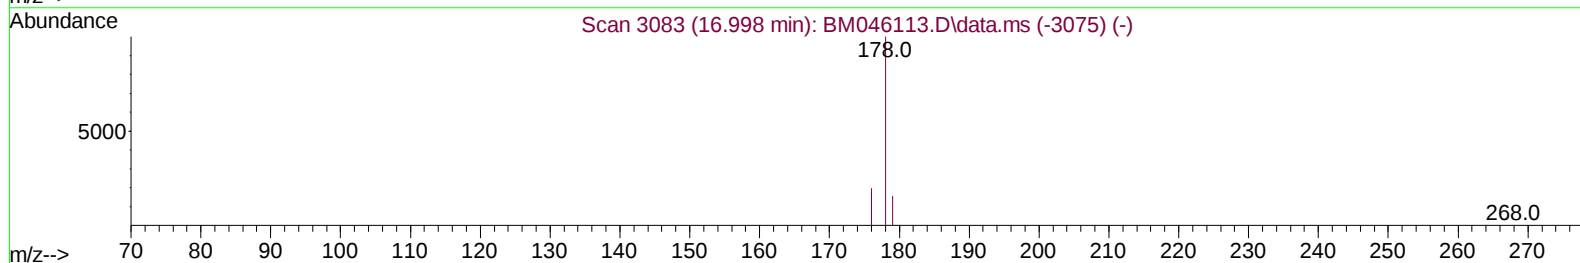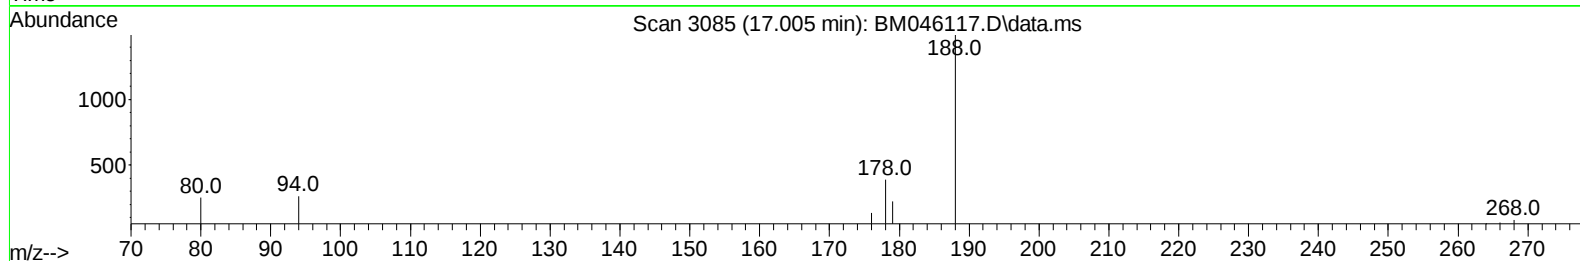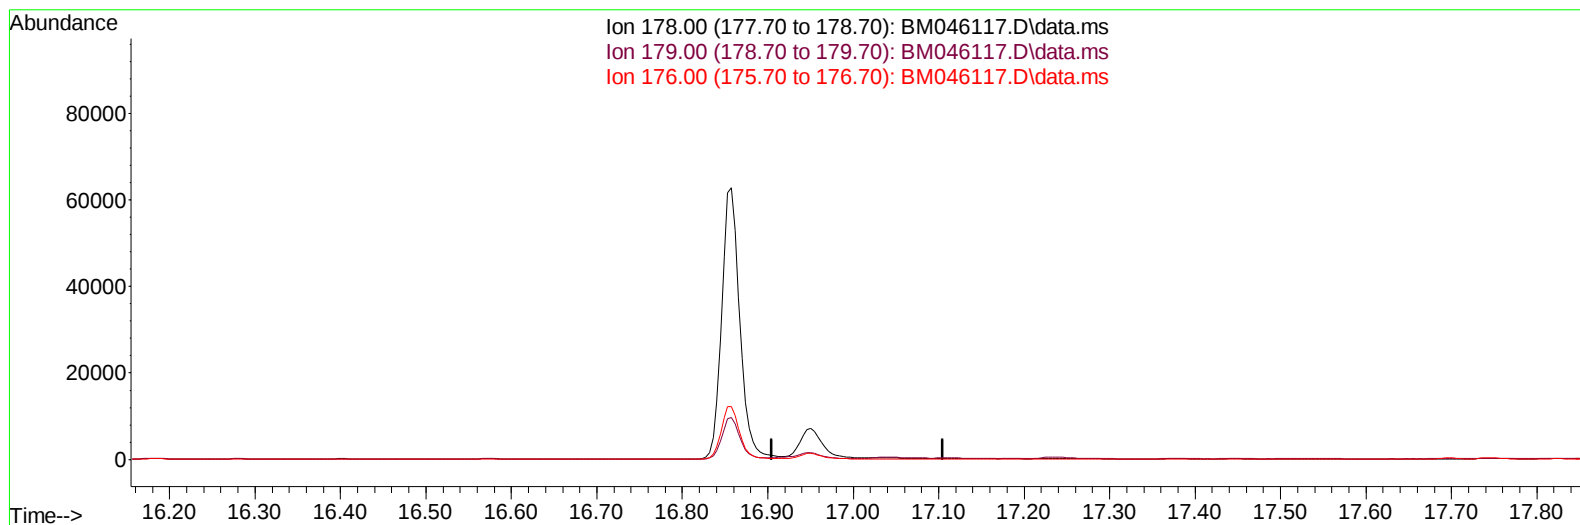

TIC: BM046117.D\data.ms

(16) Anthracene

17.005min (-17.005) 0.00 ng/u1

response 0

Ion	Exp%	Act%
178.00	100.00	0.00
179.00	18.60	0.00#
176.00	21.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

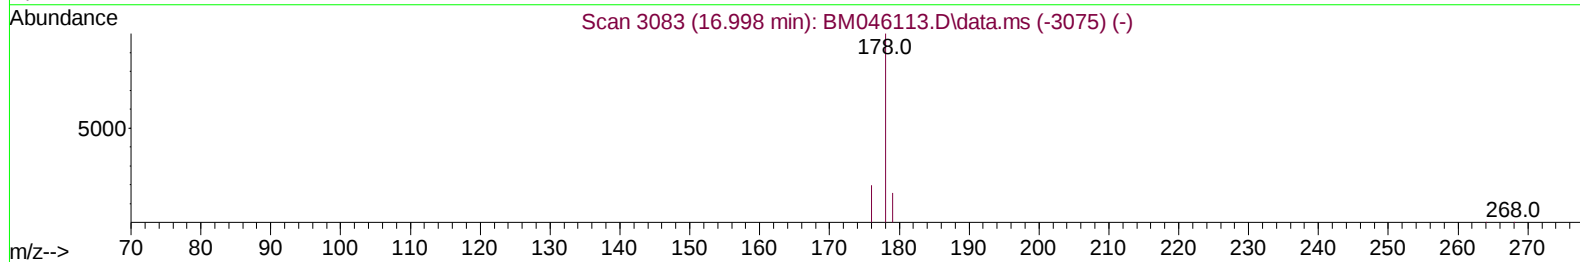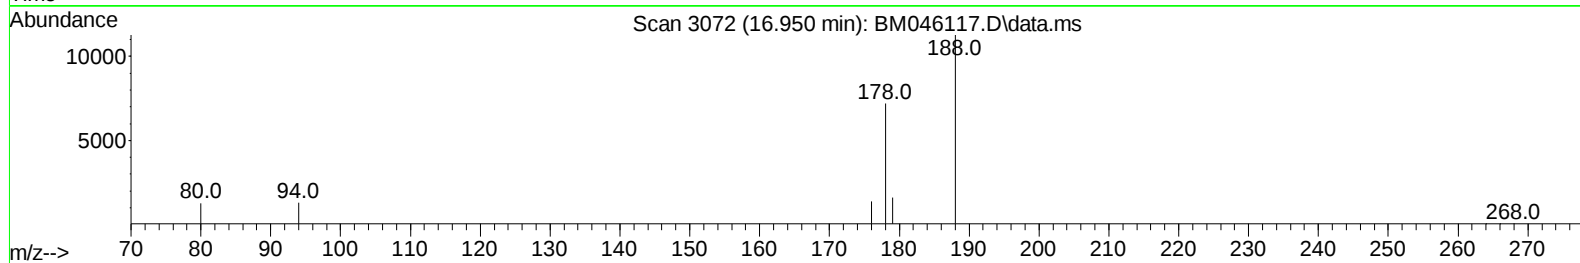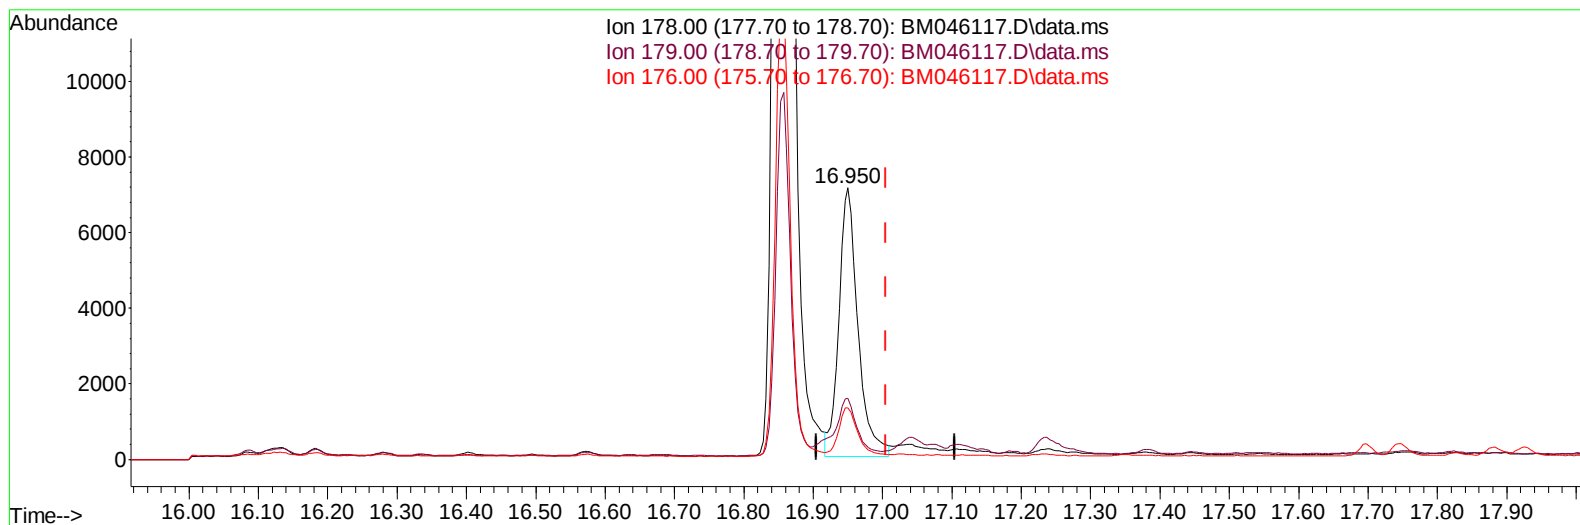

TIC: BM046117.D\data.ms

(16) Anthracene

16.950min (-0.055) 0.82 ng/u1 m

response 13548

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.60	22.43#
176.00	21.20	19.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

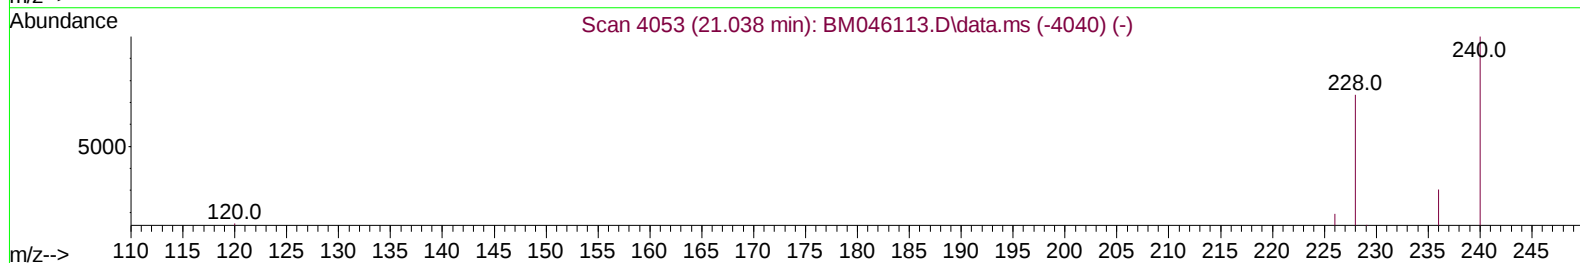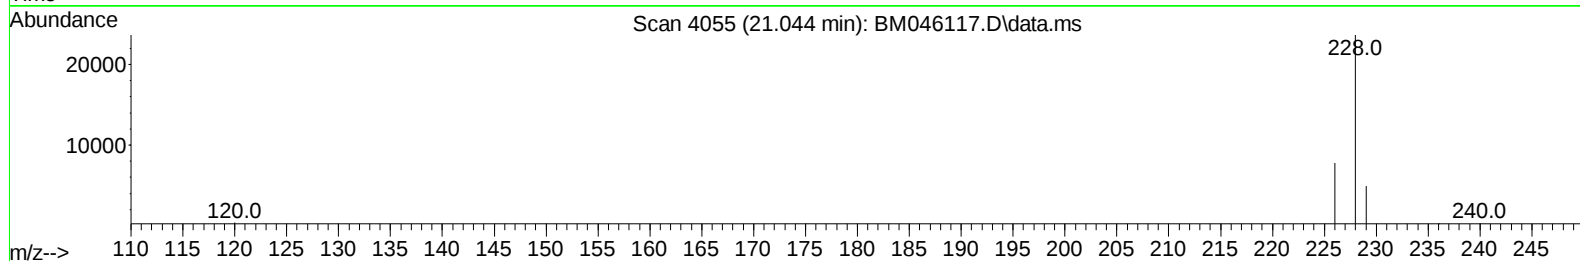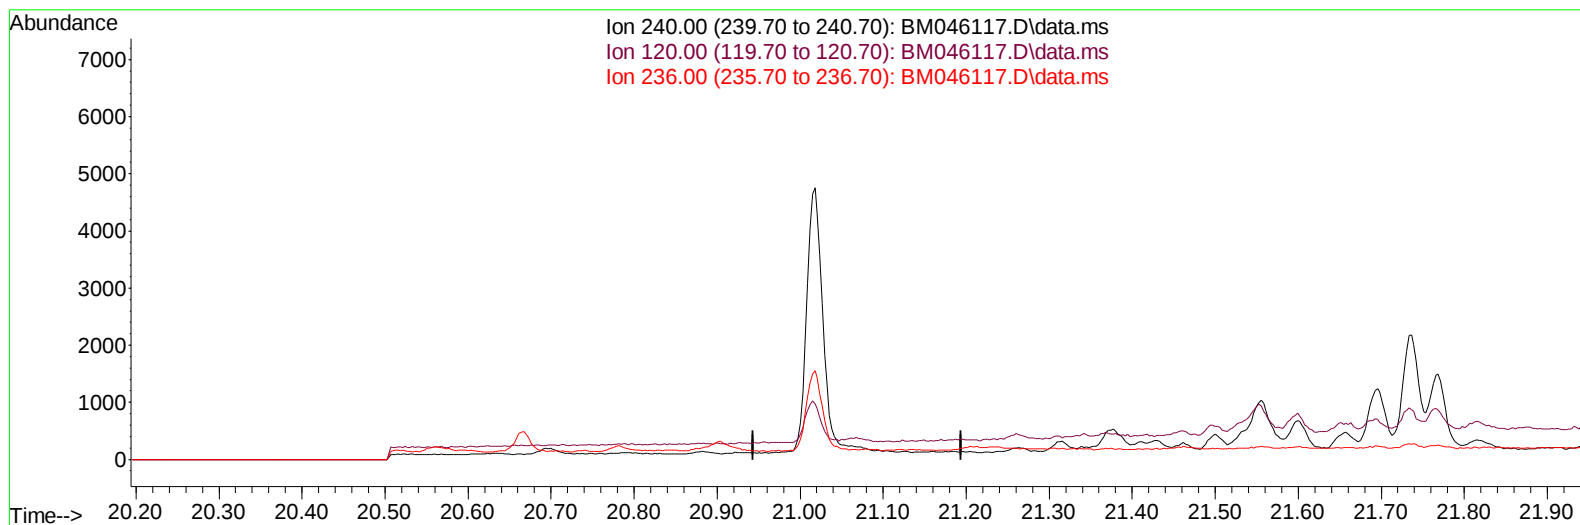

TIC: BM046117.D\data.ms

(17) Chrysene-d12

21.044min (-21.044) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	23.50	0.00#
236.00	33.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

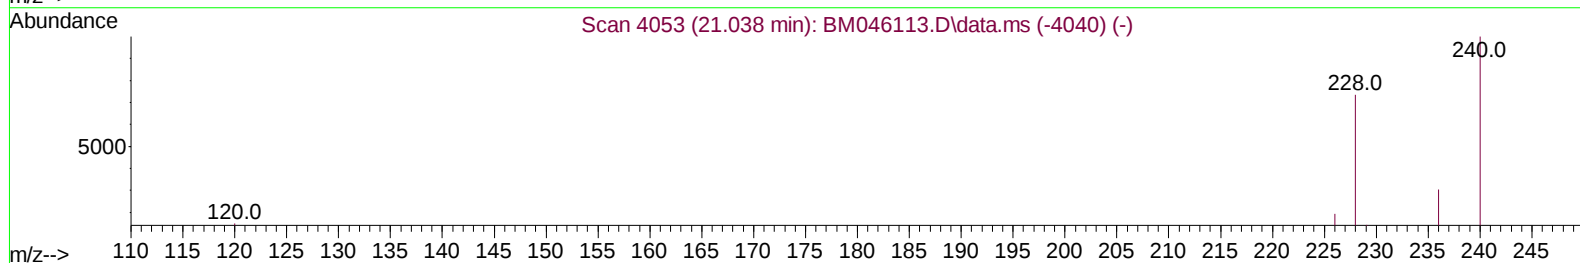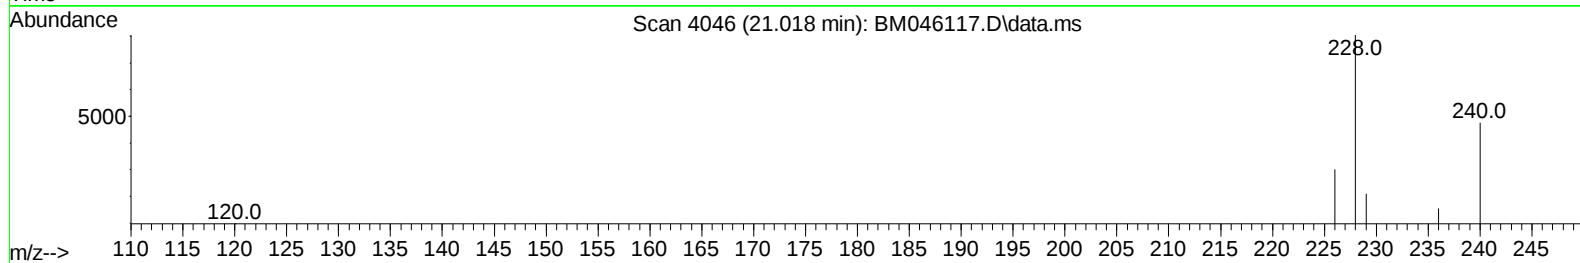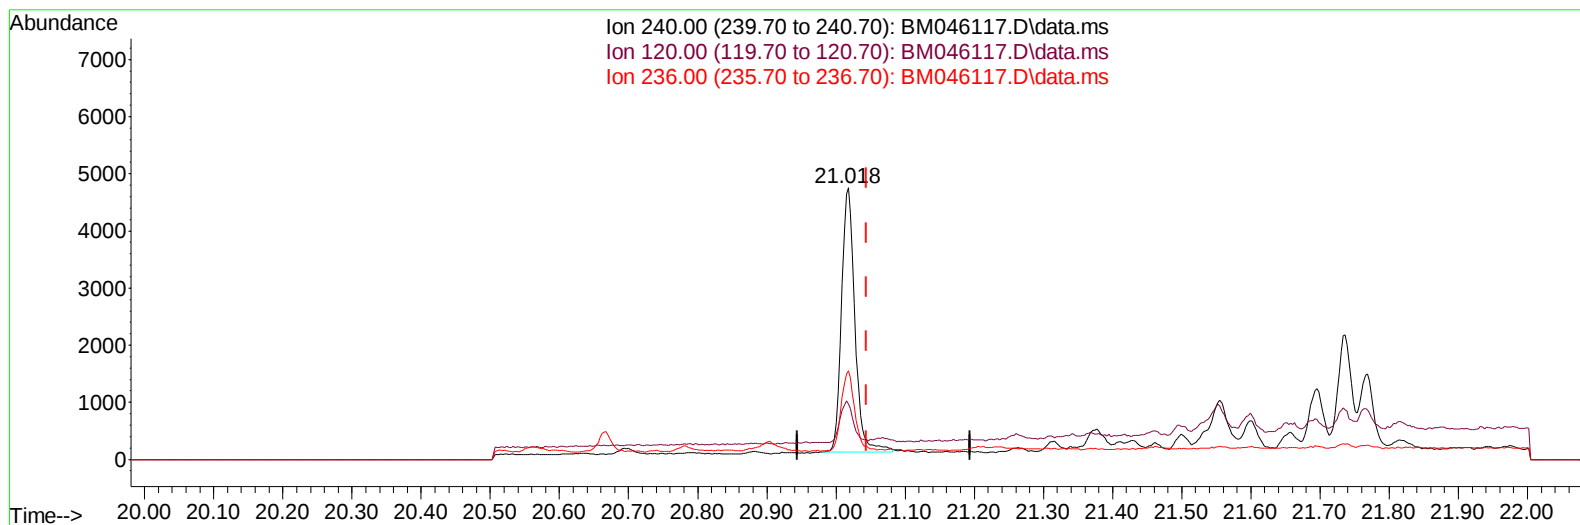

TIC: BM046117.D\data.ms

(17) Chrysene-d12

21.018min (-0.026) 0.40 ng/ul m

response 6271

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	23.50	20.41
236.00	33.60	32.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

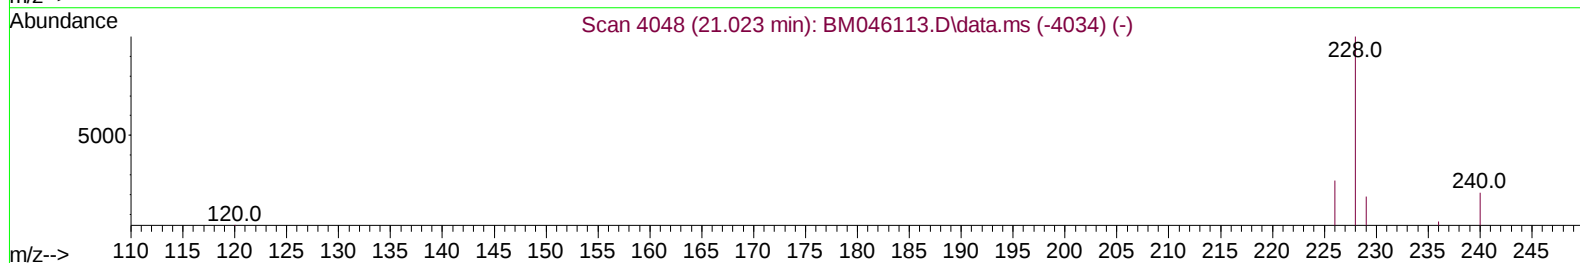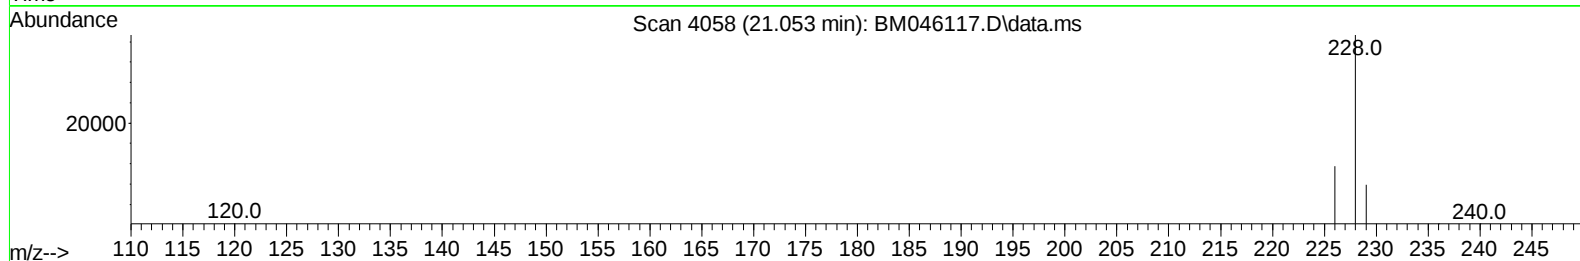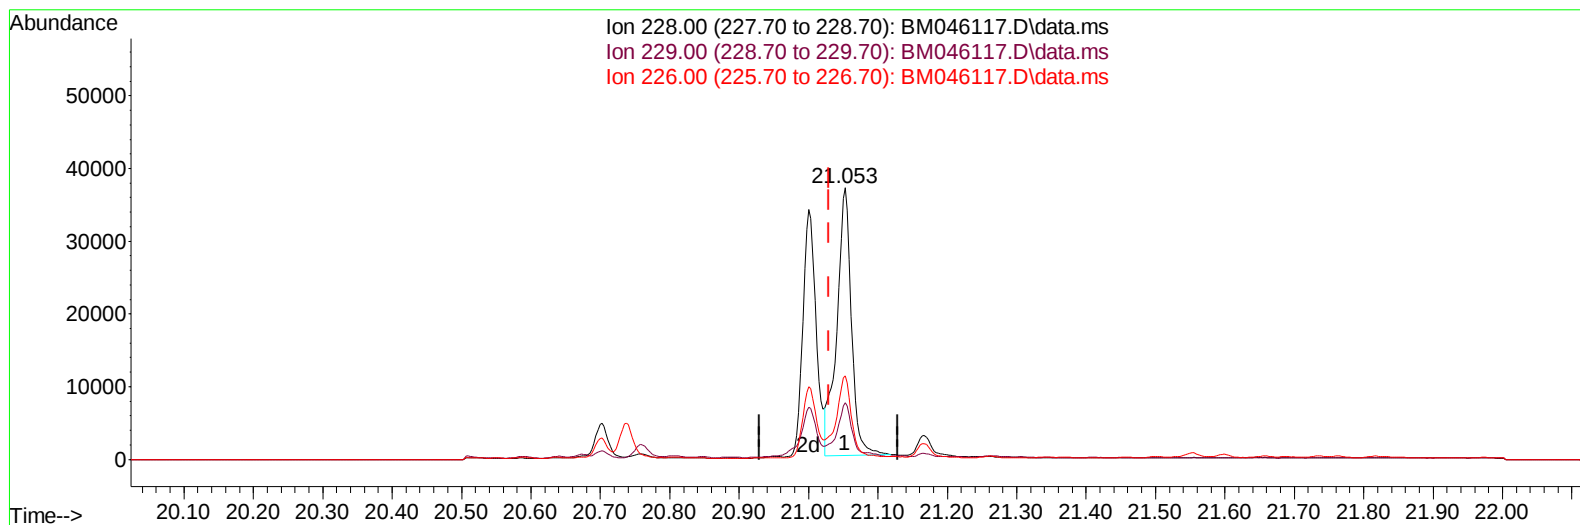

TIC: BM046117.D\data.ms

(21) Benzo(a)anthracene

21.053min (+ 0.023) 2.23 ng/u1

response 53974

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.50	20.95
226.00	29.30	30.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

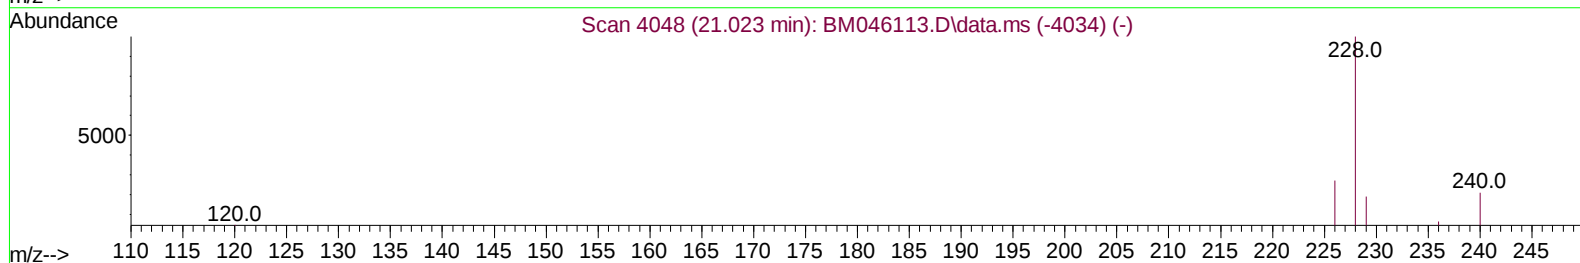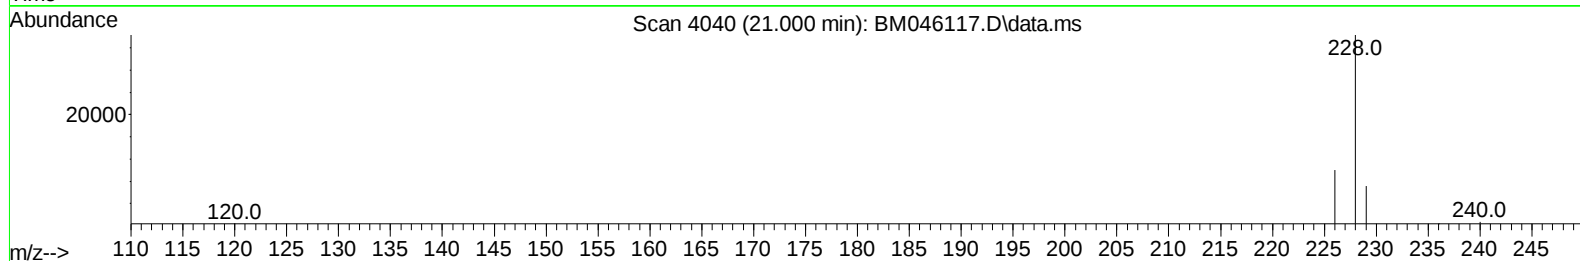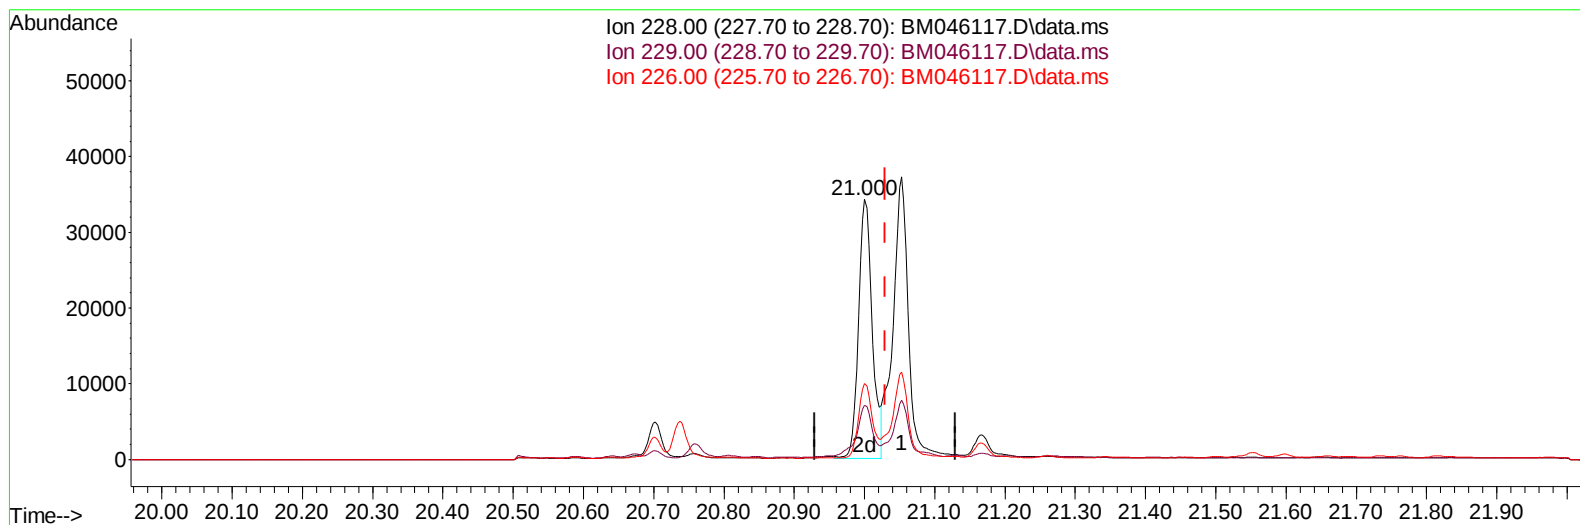

TIC: BM046117.D\data.ms

(21) Benzo(a)anthracene

21.000min (-0.029) 1.92 ng/u1 m

response 46554

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.50	20.94
226.00	29.30	29.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

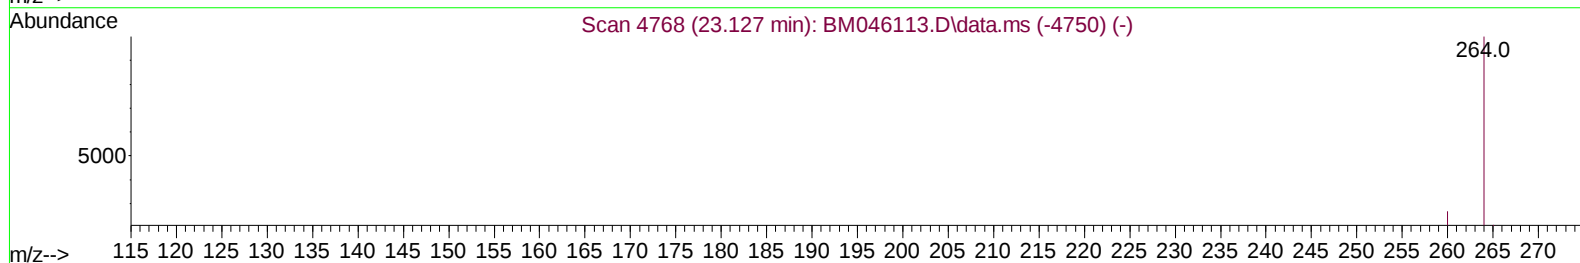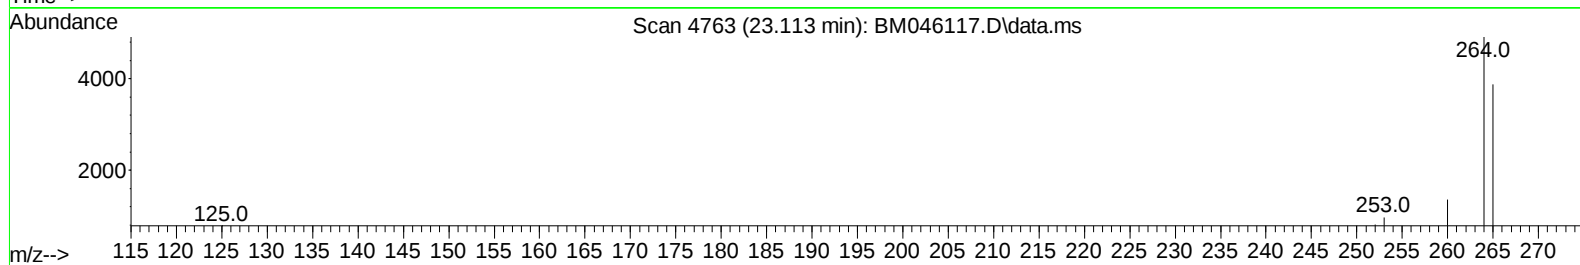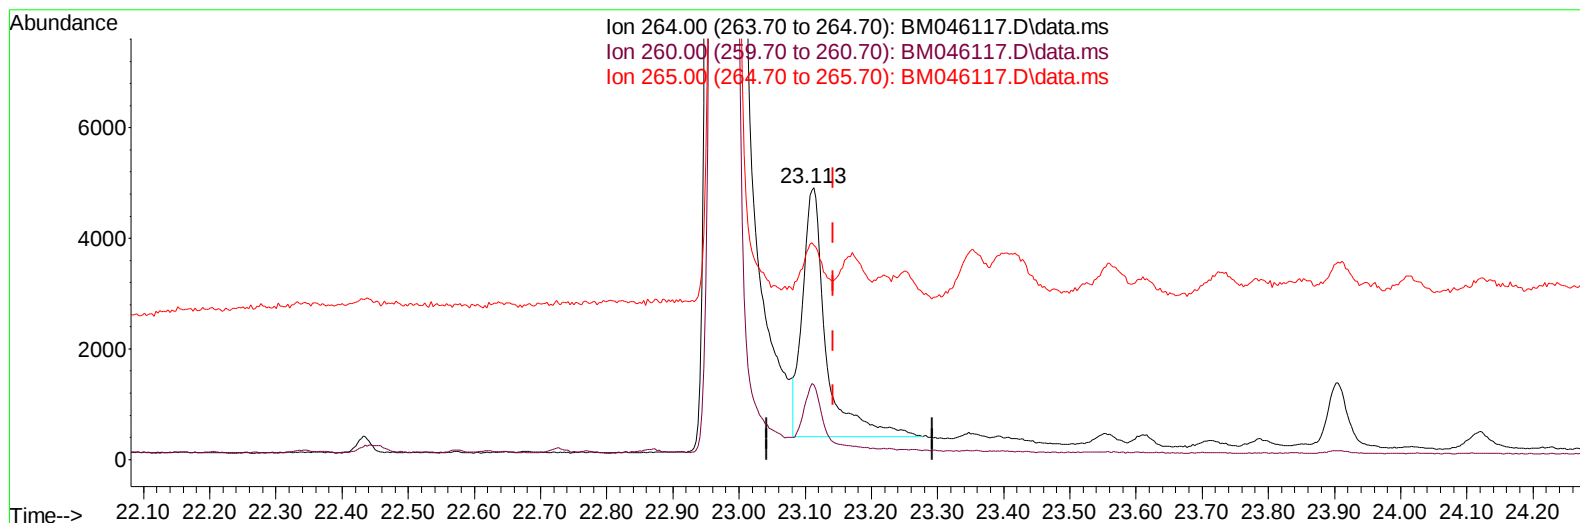

TIC: BM046117.D\data.ms

(23) Perylene-d12 (I)

23.113min (-0.029) 0.40 ng/u1

response 11161

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	27.59
265.00	110.60	78.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

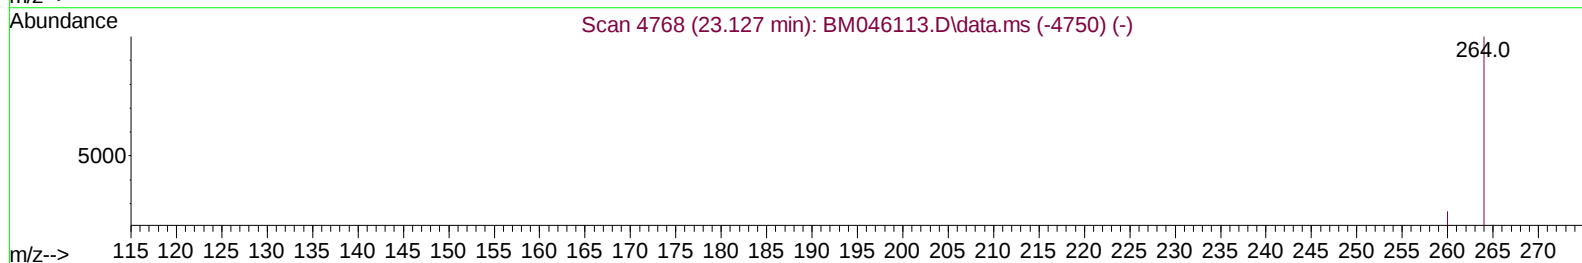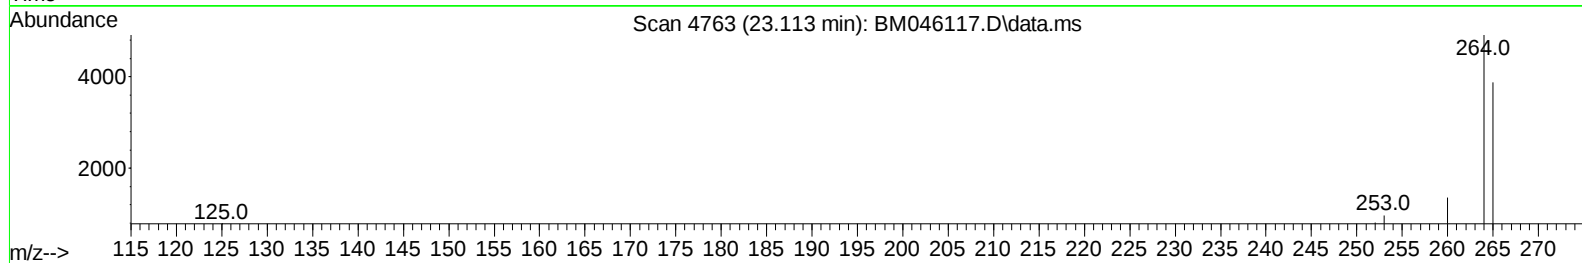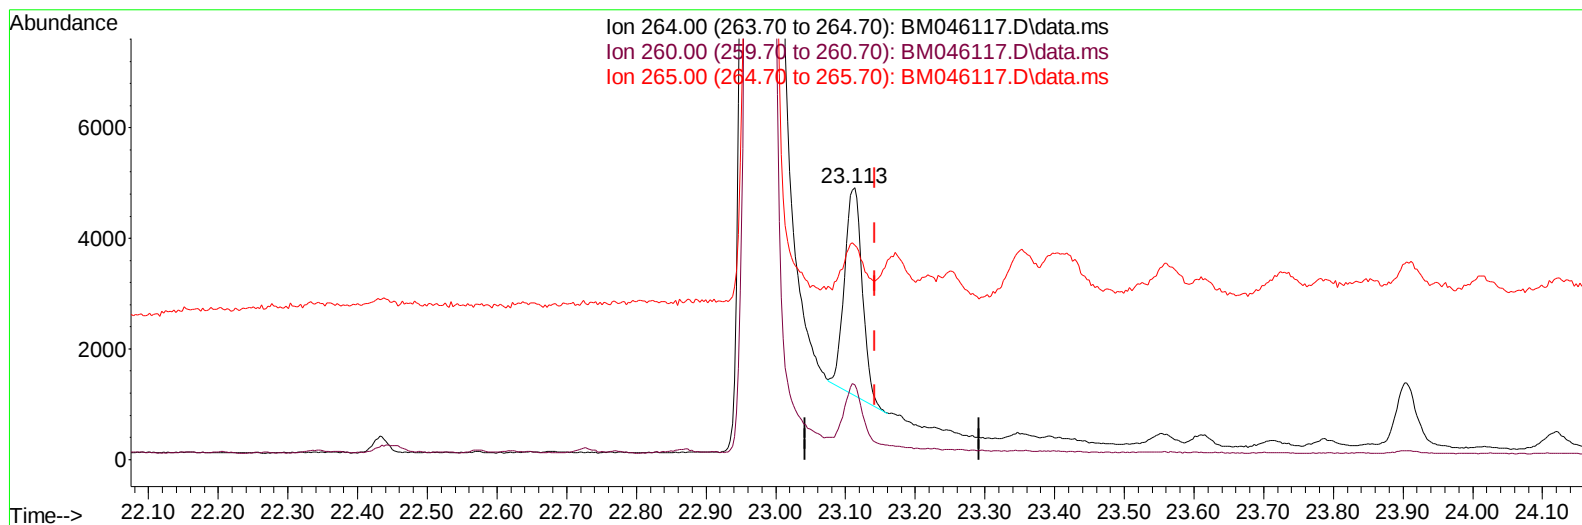

TIC: BM046117.D\data.ms

(23) Perylene-d12 (I)

23.113min (-0.029) 0.40 ng/ul m

response 6634

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	27.59
265.00	110.60	78.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
 Data File : BM046117.D
 Acq On : 20 Jun 2024 11:28
 Operator : MA/JU
 Sample : P2710-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 13:58:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
 Supervised By :mohammad ahmed 06/24/2024

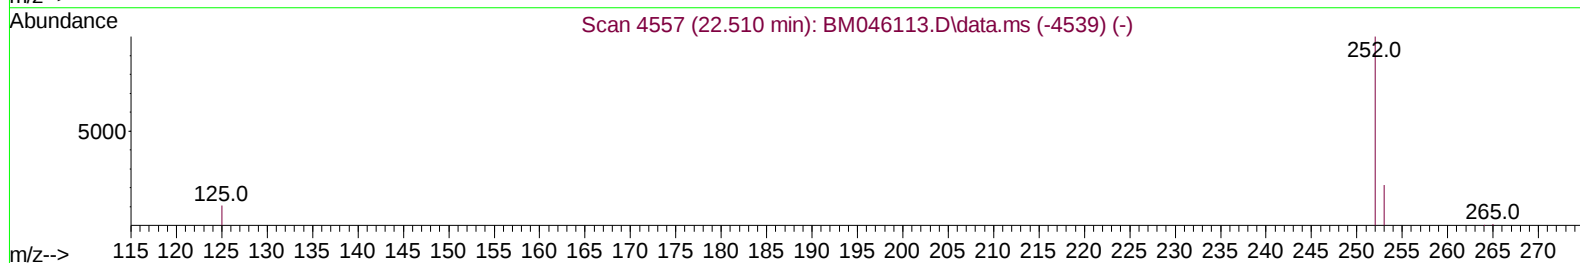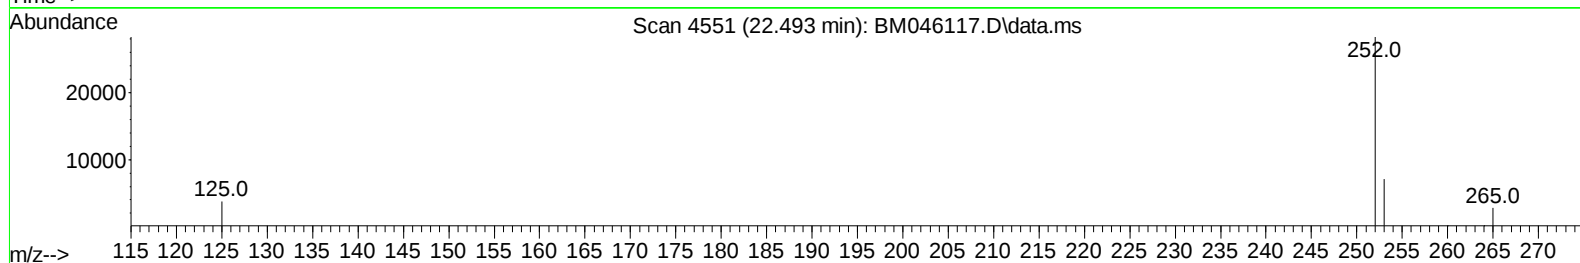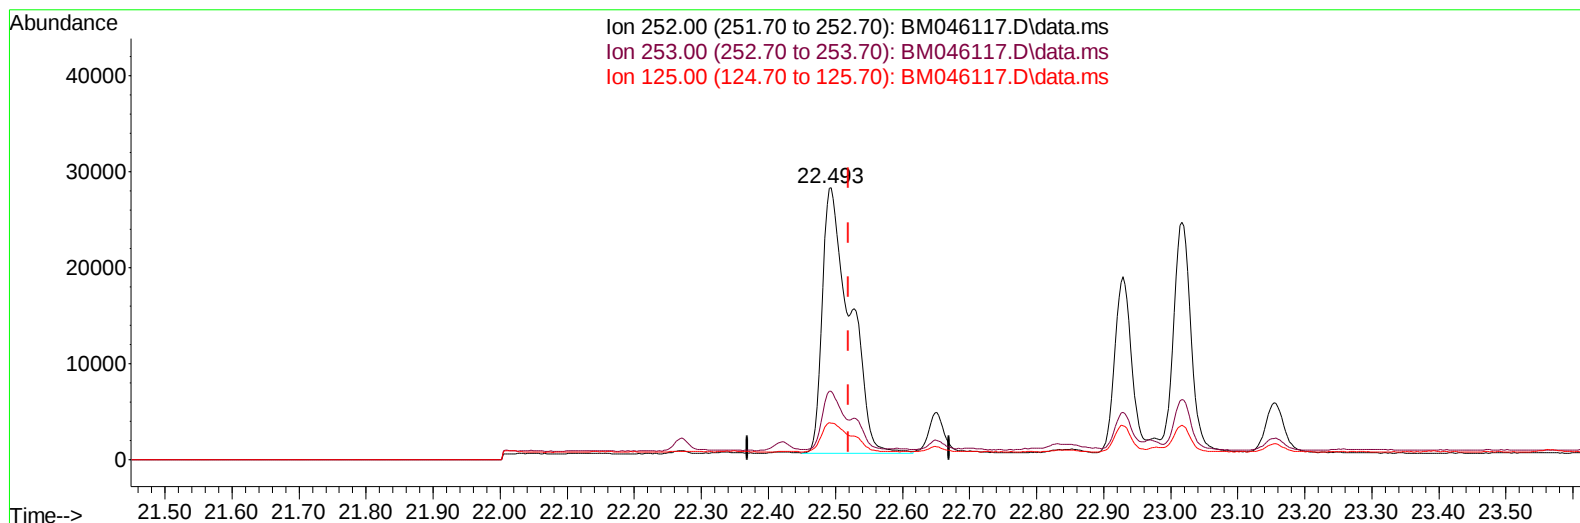

TIC: BM046117.D\data.ms

(24) Benzo(b)fluoranthene

22.493min (-0.026) 3.29 ng/u1

response 78741

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	25.07
125.00	20.10	13.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

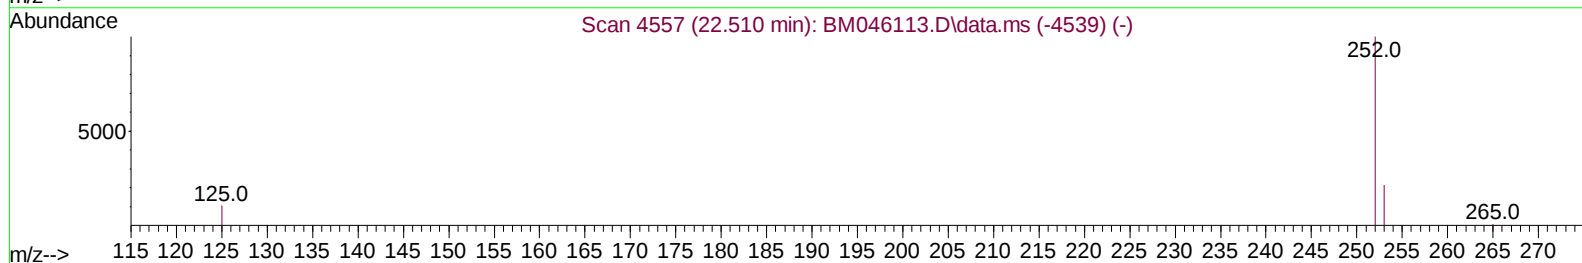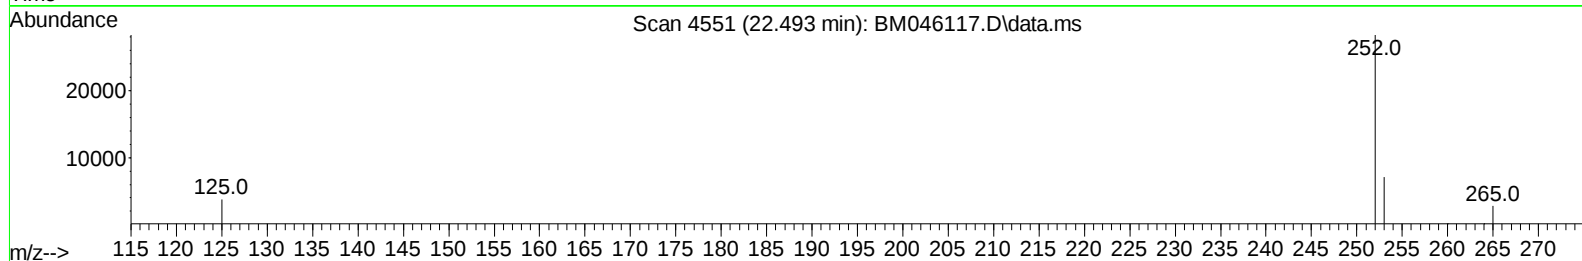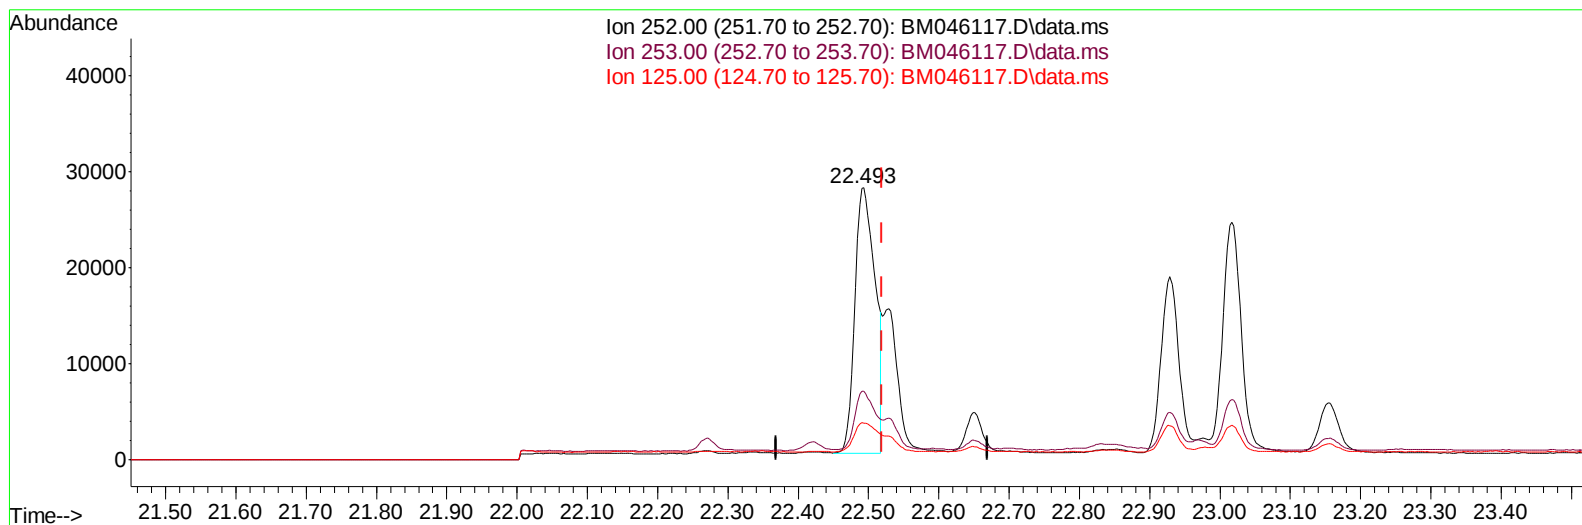

TIC: BM046117.D\data.ms

(24) Benzo(b)fluoranthene

22.493min (-0.026) 2.31 ng/u1 m

response 55107

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	25.07
125.00	20.10	13.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

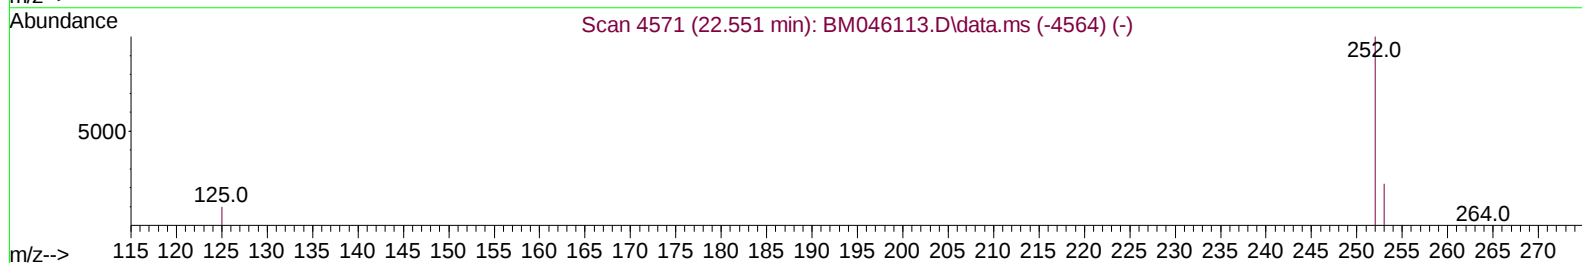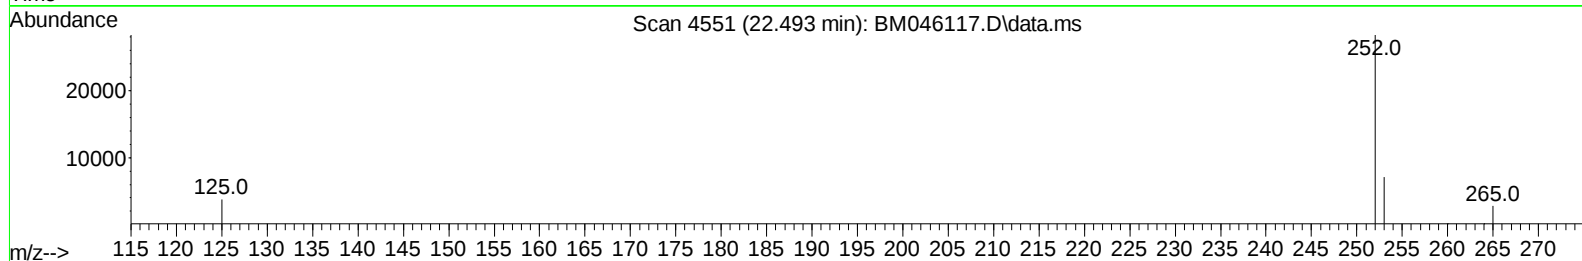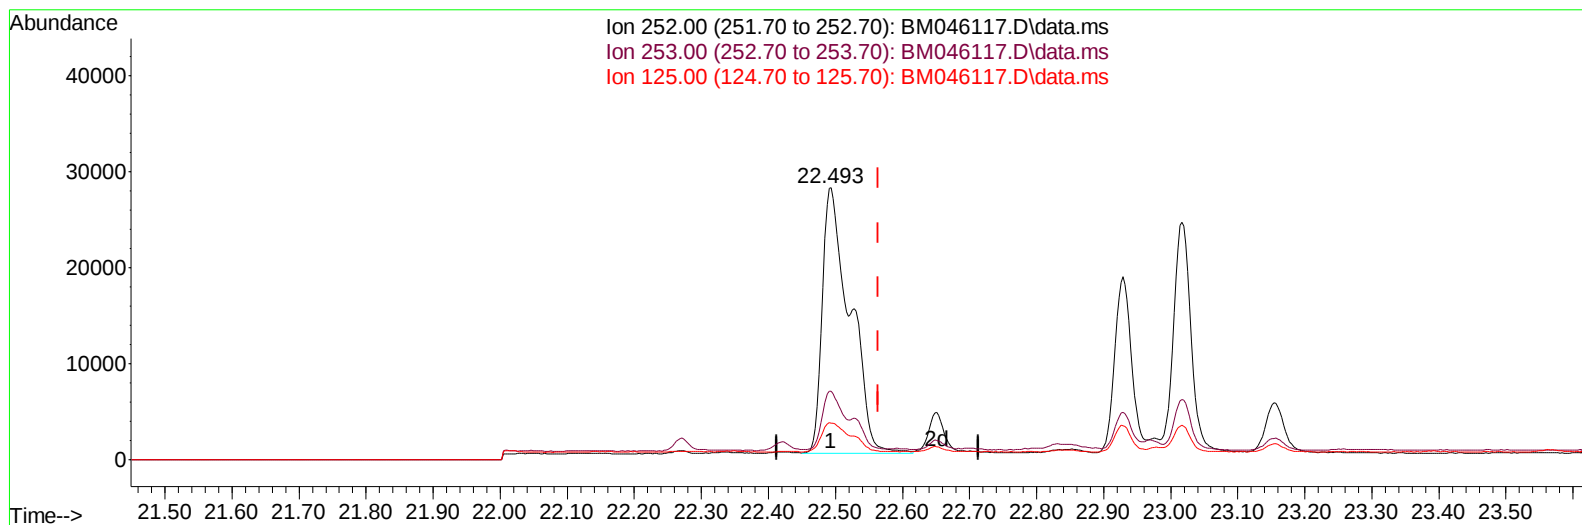

TIC: BM046117.D\data.ms

(25) Benzo(k)fluoranthene

22.493min (-0.070) 2.77 ng/u1

response 78741

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	25.07#
125.00	20.80	13.42#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

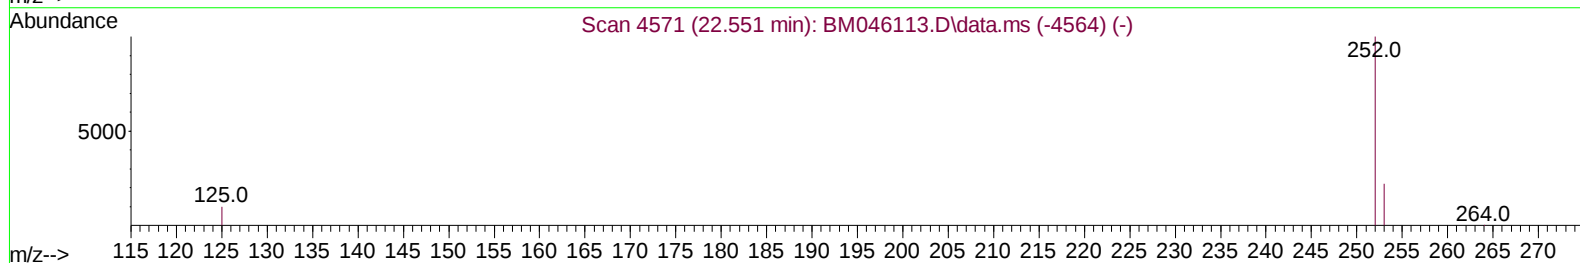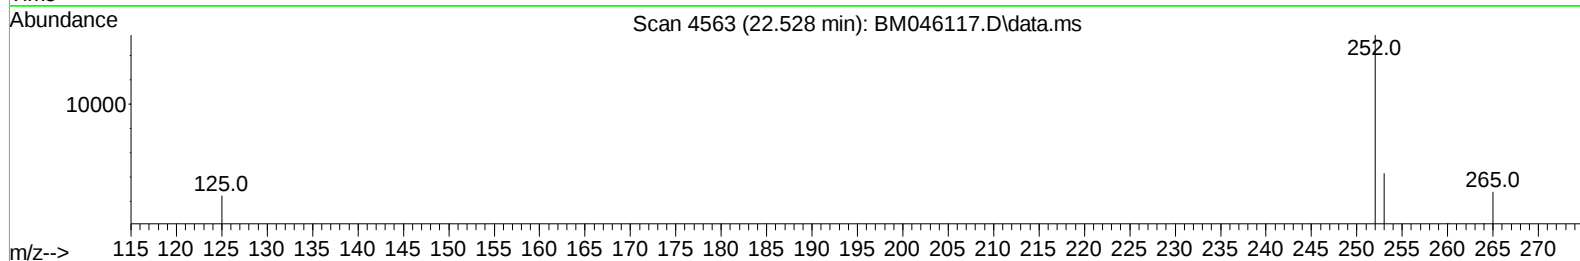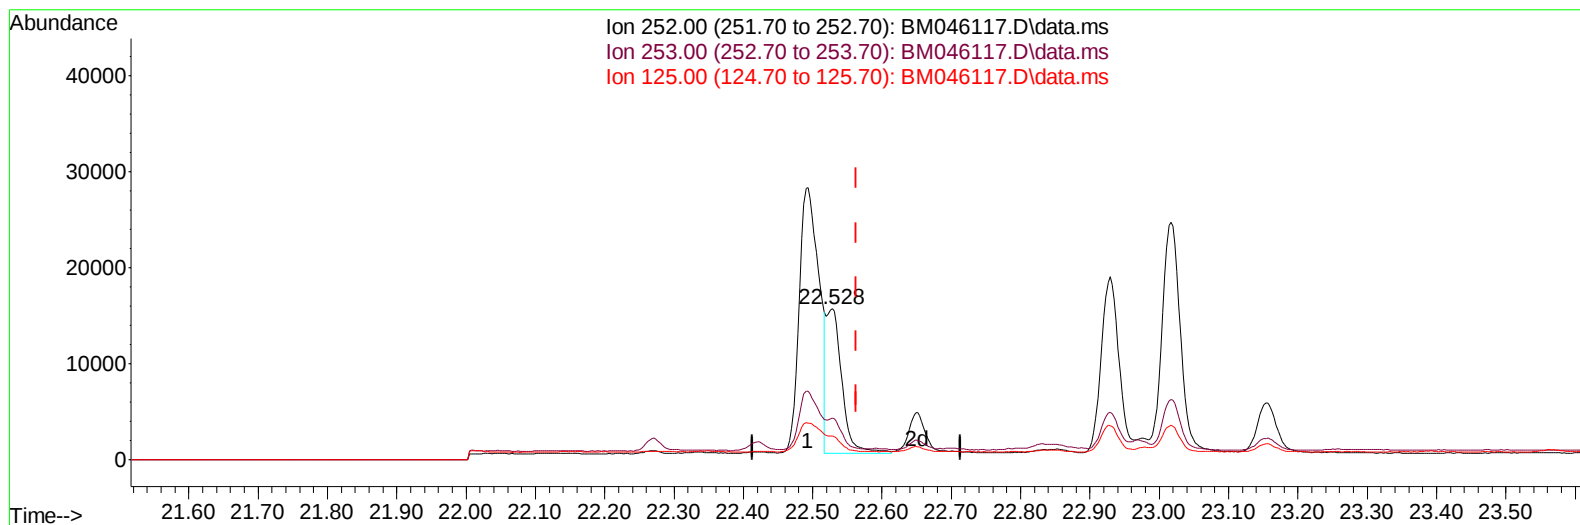

TIC: BM046117.D\data.ms

(25) Benzo(k)fluoranthene

22.528min (-0.035) 0.84 ng/u1 m

response 23790

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	27.50
125.00	20.80	15.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

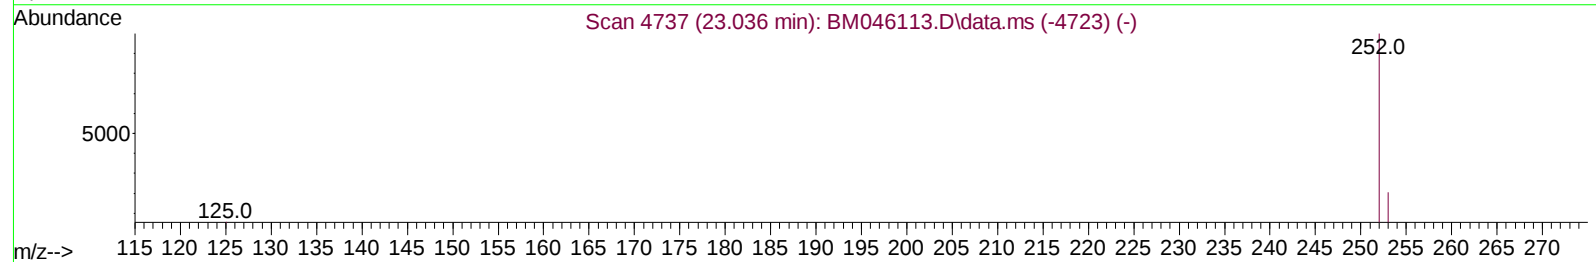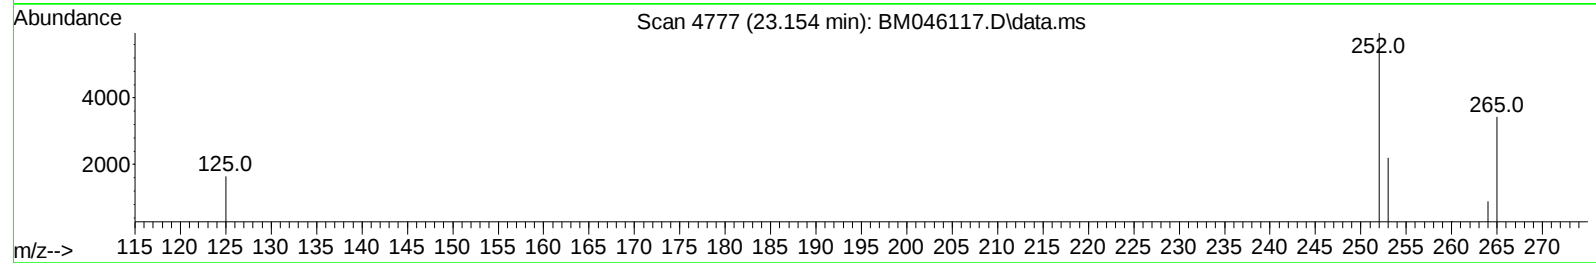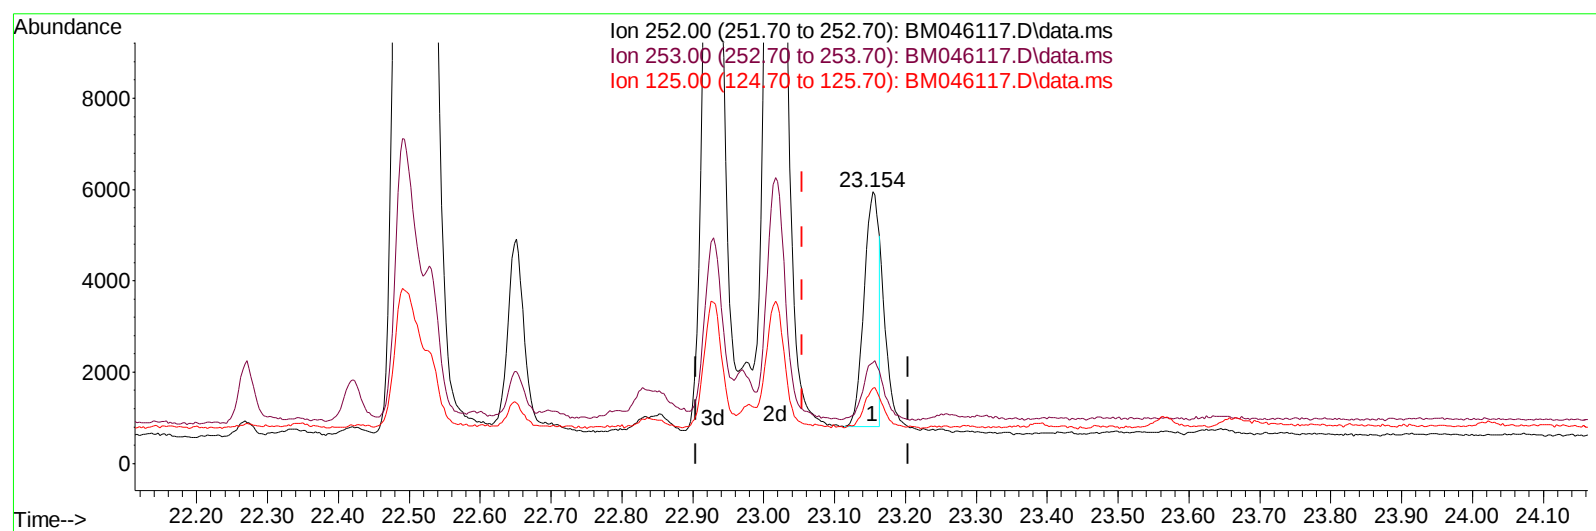

TIC: BM046117.D\data.ms

(26) Benzo(a)pyrene (C)

23.154min (+ 0.100) 0.33 ng/u1

response 7279

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	40.10	37.10
125.00	26.50	27.61
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
 Data File : BM046117.D
 Acq On : 20 Jun 2024 11:28
 Operator : MA/JU
 Sample : P2710-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 13:58:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
 Supervised By :mohammad ahmed 06/24/2024

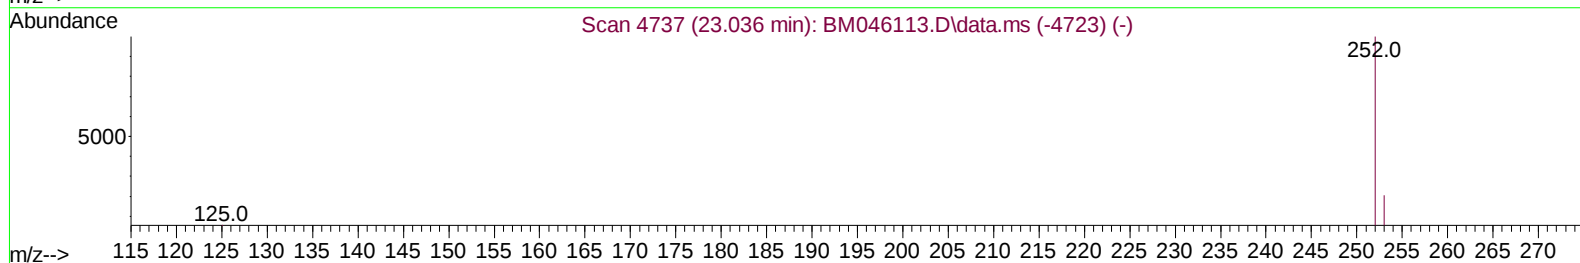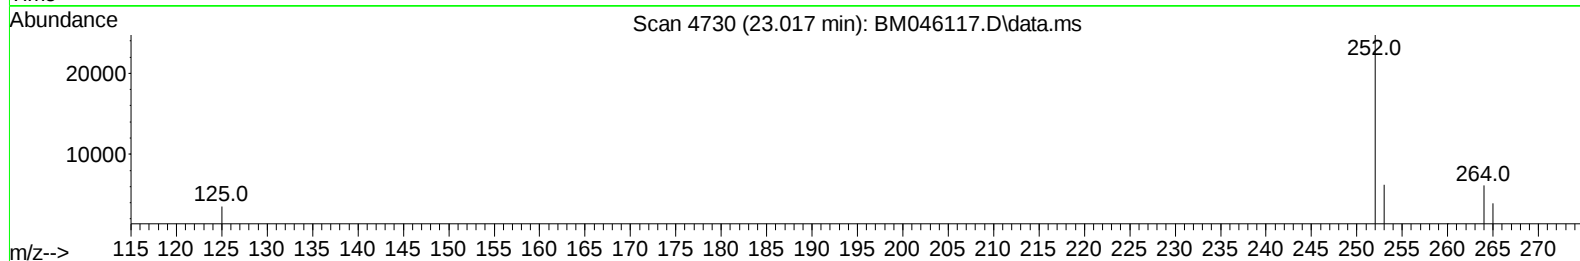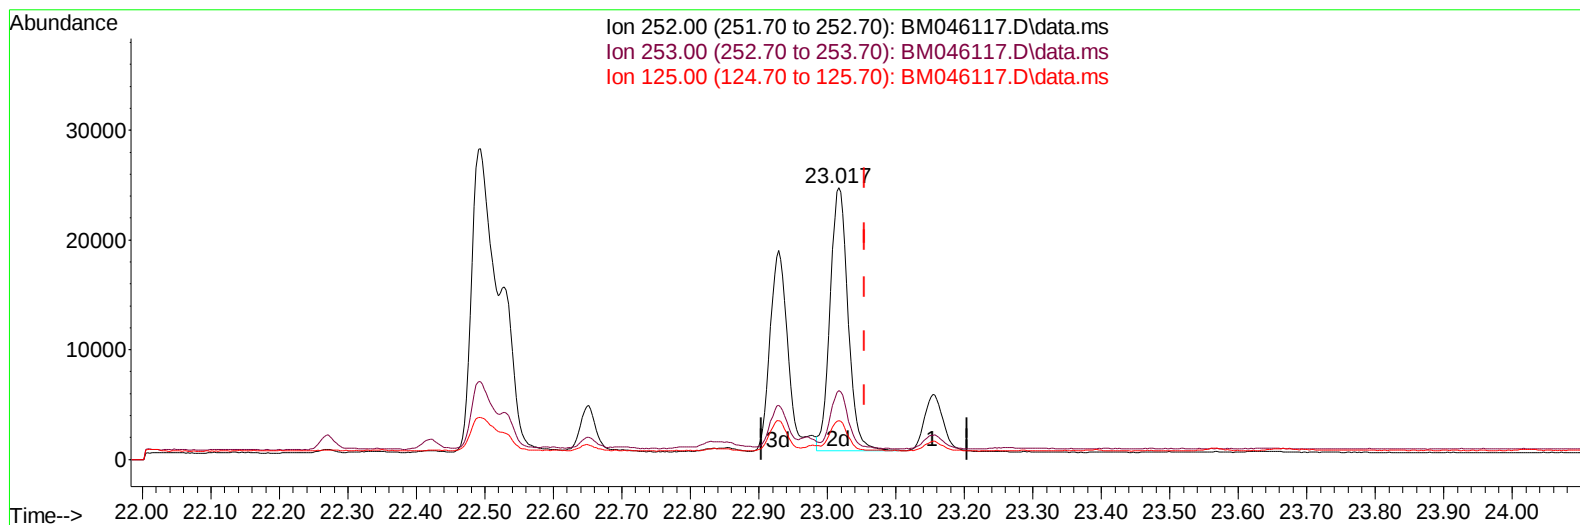

TIC: BM046117.D\data.ms

(26) Benzo(a)pyrene (C)

23.017min (-0.038) 1.98 ng/u1 m

response 43742

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	40.10	25.29#
125.00	26.50	14.38#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
 Data File : BM046117.D
 Acq On : 20 Jun 2024 11:28
 Operator : MA/JU
 Sample : P2710-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4B27

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2024
 Supervised By :mohammad ahmed 06/24/2024

Quant Time: Jun 20 12:25:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 13:58:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.426	152	2375	0.400	ng/ul	#-0.04
4) Naphthalene-d8	10.198	136	6669	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.075	164	3664	0.400	ng/ul	-0.04
13) Phenanthrene-d10	16.815	188	7930m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.018	240	6271m	0.400	ng/ul	-0.03
23) Perylene-d12	23.113	264	6634m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.033	96	13519	4.149	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.832	152	2384	0.266	ng/ul	-0.03
18) Fluoranthene-d10	18.848	212	5272	0.281	ng/ul	-0.04
Target Compounds						
						Qvalue
5) Naphthalene	10.248	128	2389	0.128	ng/ul	95
7) 2-Methylnaphthalene	11.903	142	1021	0.098	ng/ul	98
8) 1-Methylnaphthalene	12.118	142	1157	0.101	ng/ul	96
10) Acenaphthylene	13.793	152	2285	0.131	ng/ul#	90
11) Acenaphthene	14.135	153	4348	0.347	ng/ul	97
12) Fluorene	15.130	166	4167	0.310	ng/ul	99
15) Phenanthrene	16.857	178	92875m	4.169	ng/ul	
16) Anthracene	16.950	178	13548m	0.817	ng/ul	
19) Fluoranthene	18.880	202	109096	4.018	ng/ul	97
20) Pyrene	19.243	202	121961	4.153	ng/ul	95
21) Benzo(a)anthracene	21.000	228	46554m	1.922	ng/ul	
22) Chrysene	21.053	228	54144	1.752	ng/ul	99
24) Benzo(b)fluoranthene	22.493	252	55107m	2.306	ng/ul	
25) Benzo(k)fluoranthene	22.528	252	23790m	0.837	ng/ul	
26) Benzo(a)pyrene	23.017	252	43742m	1.975	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.162	276	30179	0.833	ng/ul#	89
28) Dibenzo(a,h)anthracene	25.166	278	6914	0.256	ng/ul	96
29) Benzo(g,h,i)perylene	25.783	276	32790	1.055	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046117.D
Acq On : 20 Jun 2024 11:28
Operator : MA/JU
Sample : P2710-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B27

Manual IntegrationsAPPROVED

Quant Time: Jun 20 12:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

