




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

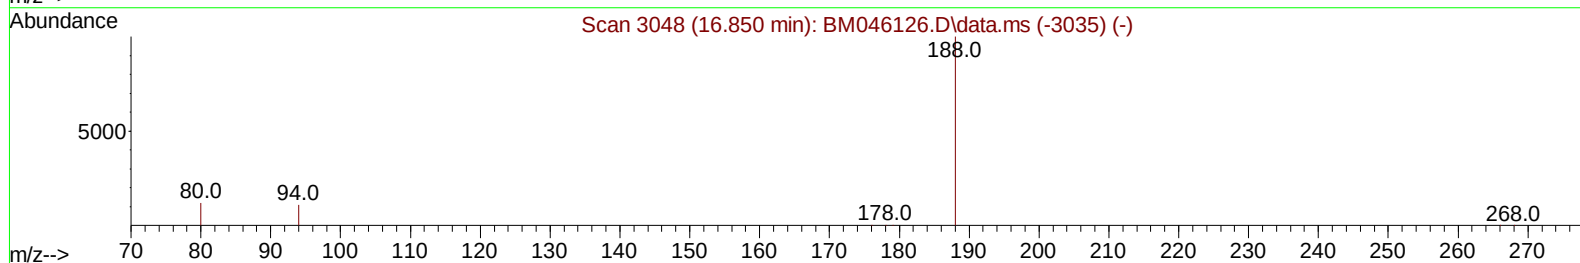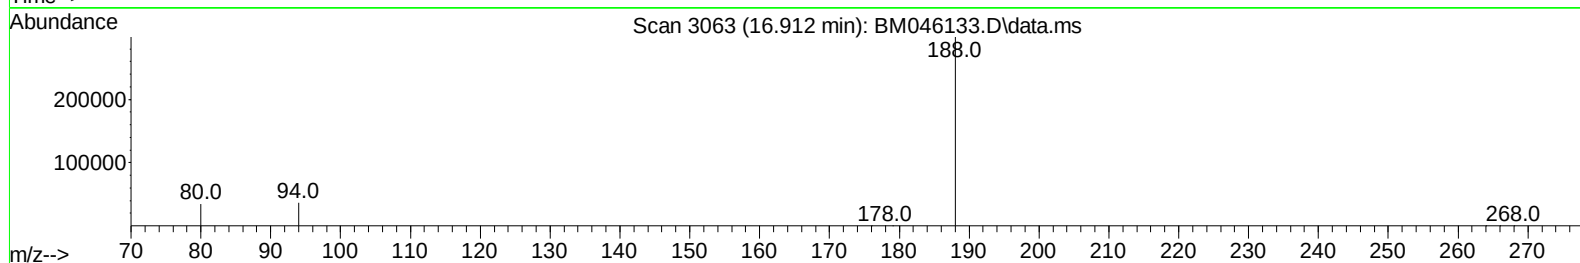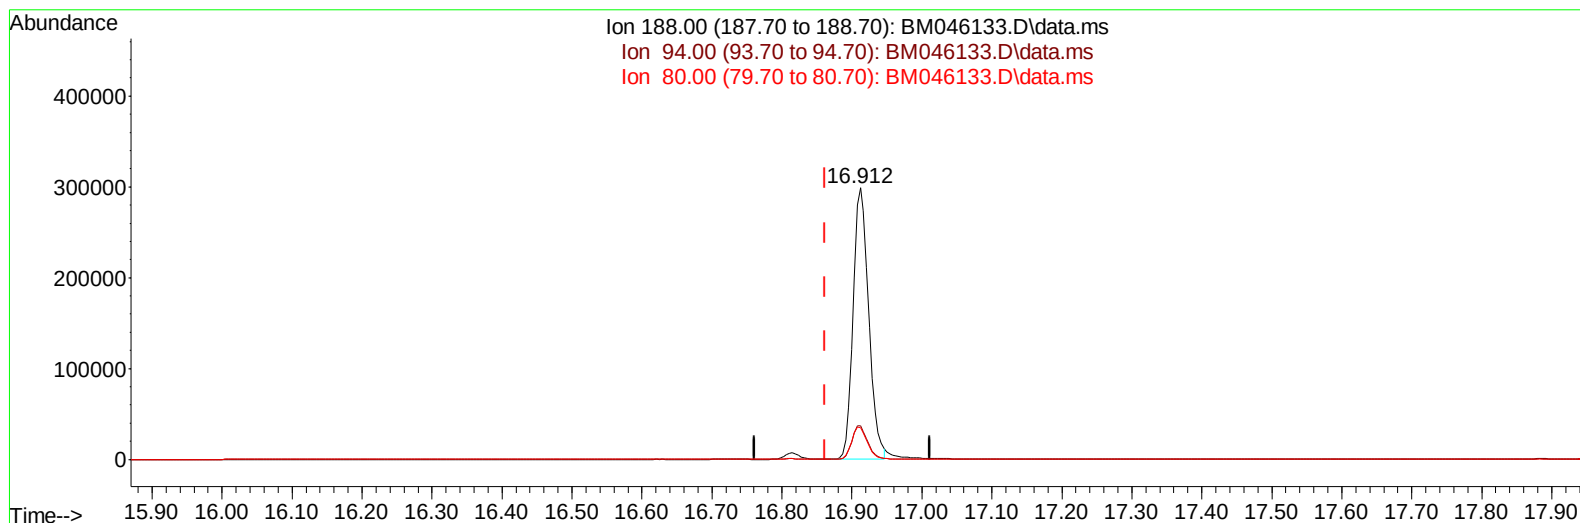

TIC: BM046133.D\data.ms

(13) Phenanthrene-d10 (I)

16.912min (+ 0.051) 0.40 ng/u1

response 459003

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	12.30
80.00	15.20	11.64#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

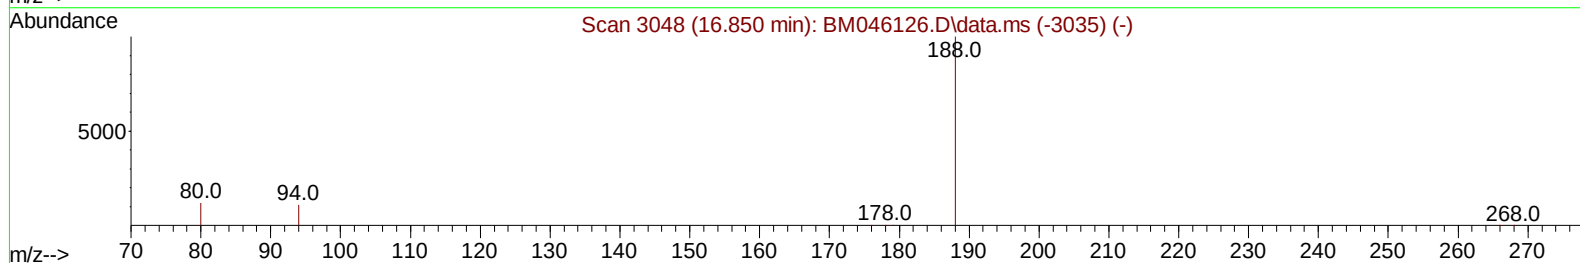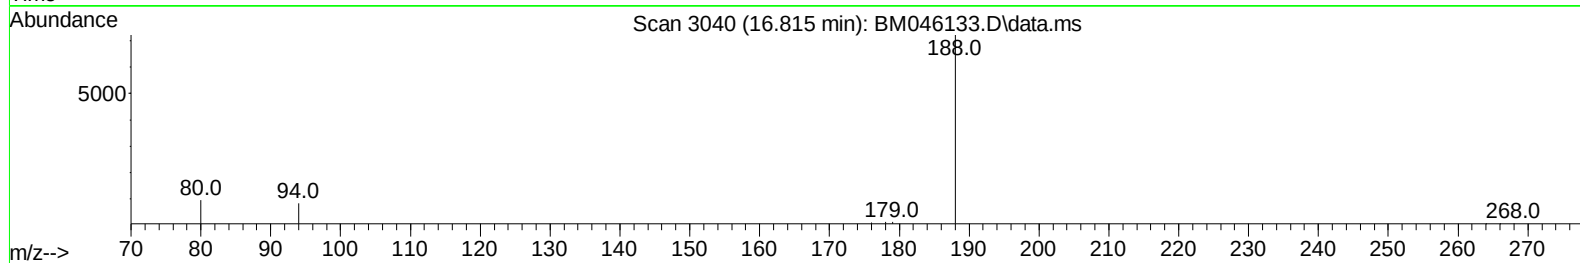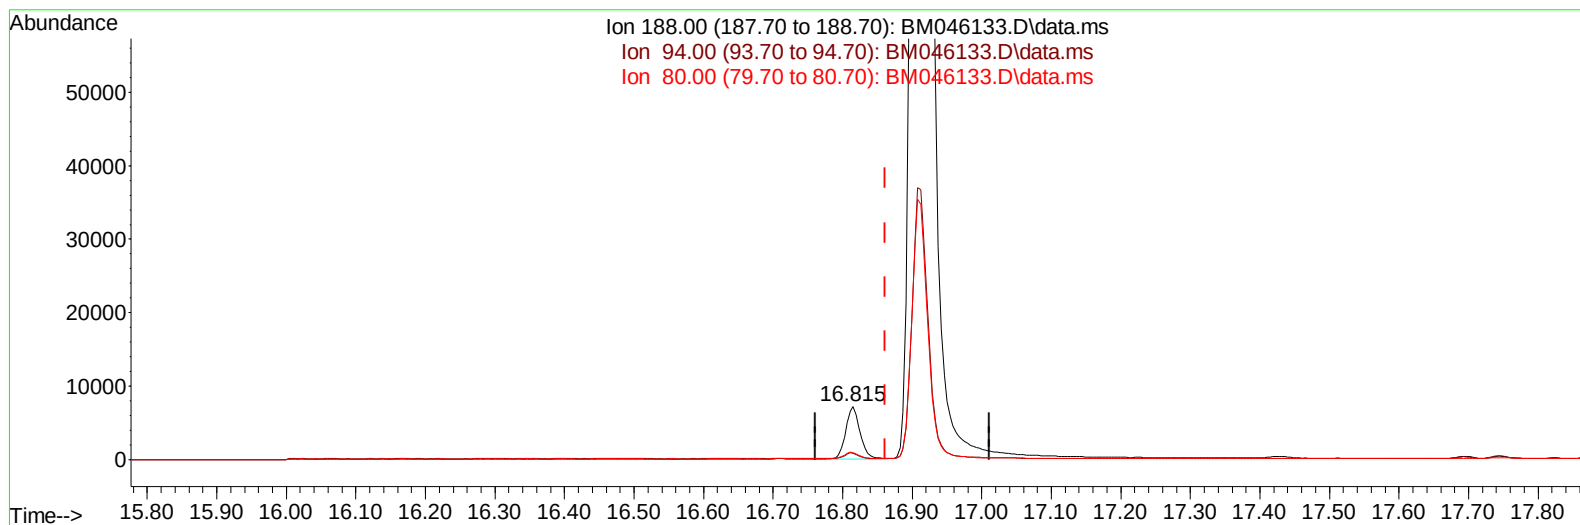

TIC: BM046133.D\data.ms

(13) Phenanthrene-d10 (I)

16.815min (-0.046) 0.40 ng/ul m

response 10276

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.80	11.62
80.00	15.20	13.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

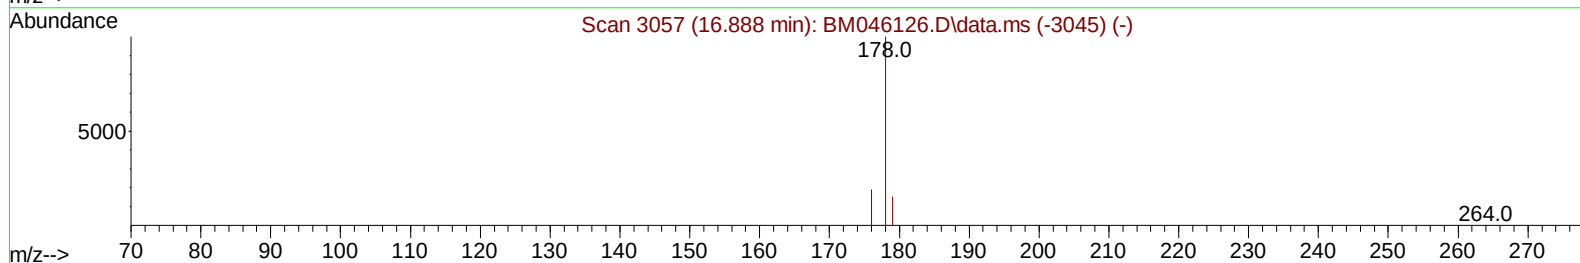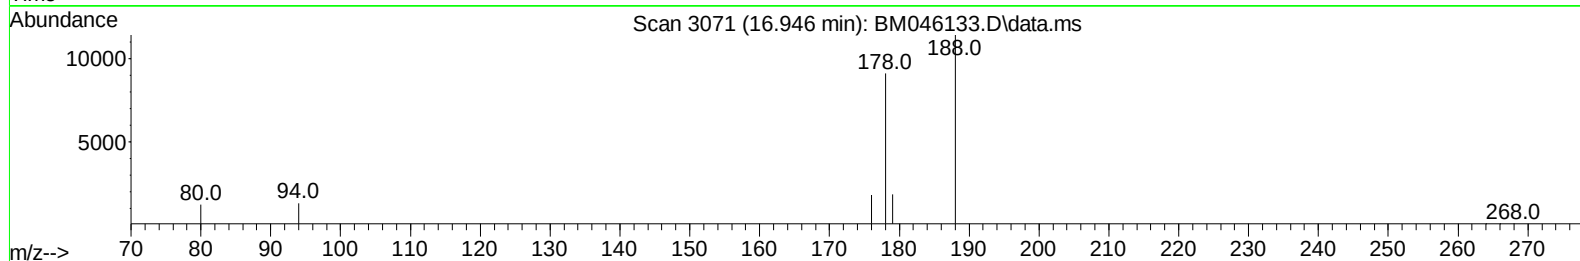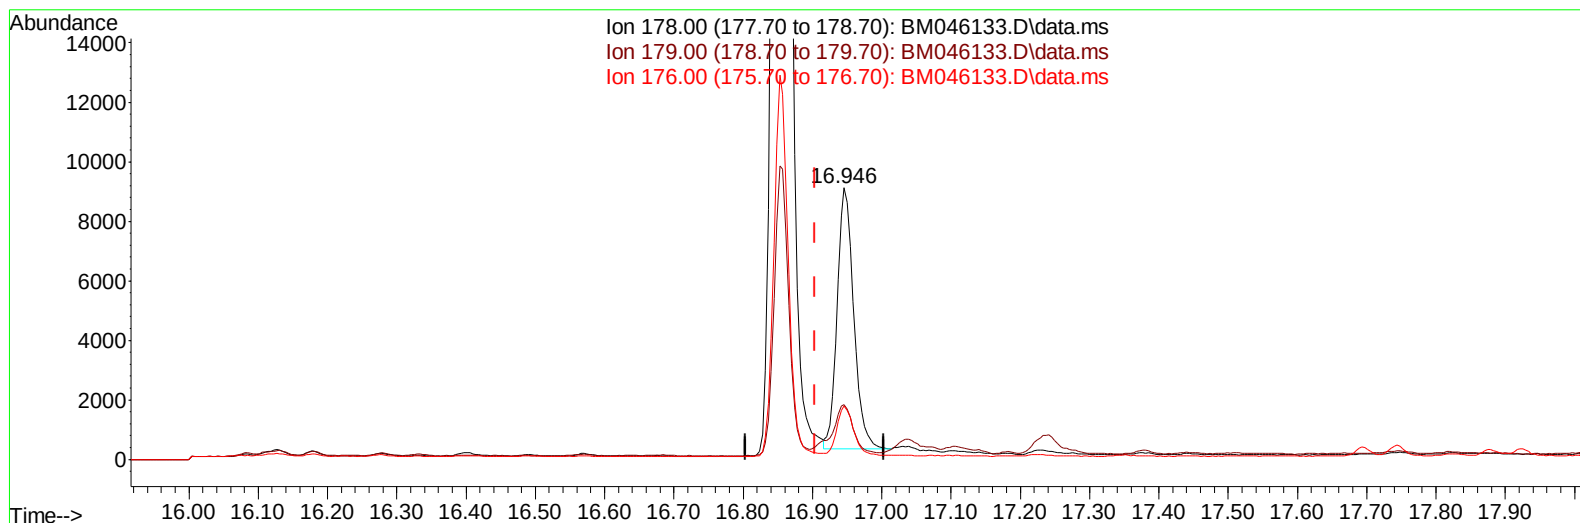

TIC: BM046133.D\data.ms

(15) Phenanthrene

16.946min (+ 0.042) 0.50 ng/u1

response 14477

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	20.26
176.00	21.40	19.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
 Data File : BM046133.D
 Acq On : 20 Jun 2024 21:14
 Operator : MA/JU
 Sample : P2710-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 13:58:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
 Supervised By :mohammad ahmed 06/24/2024

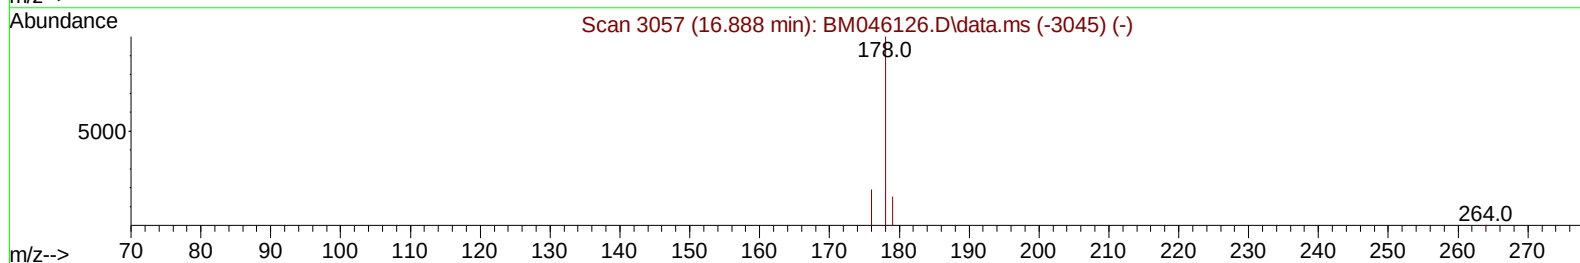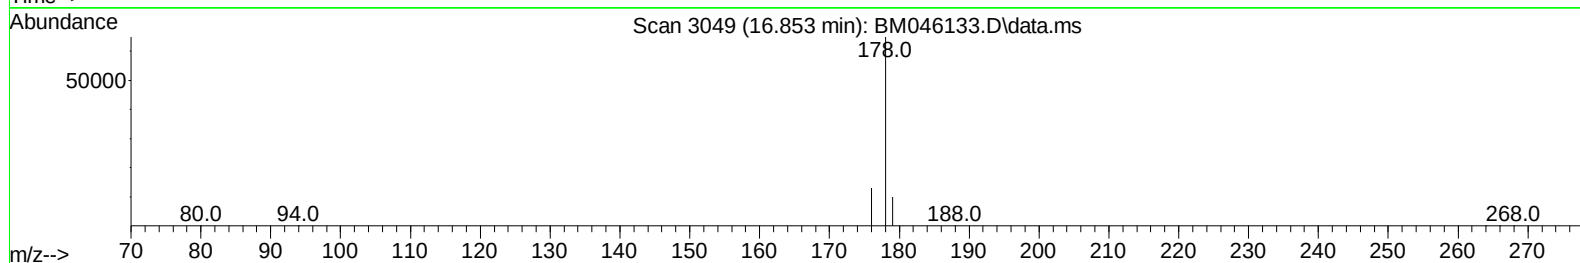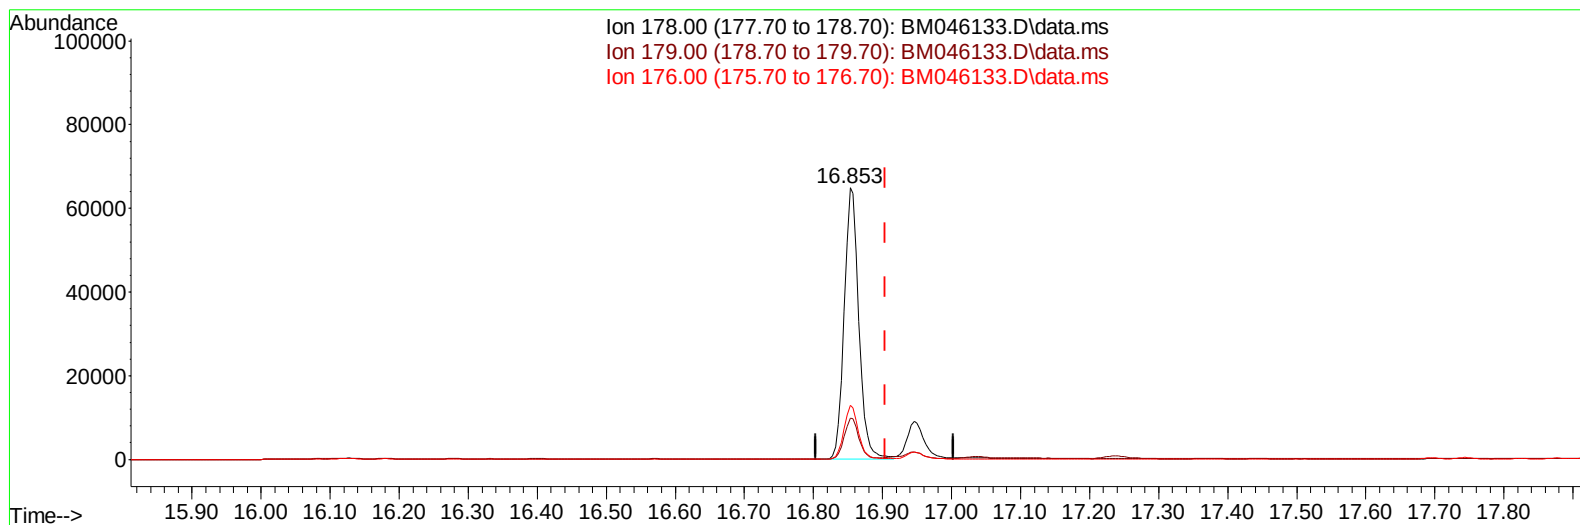

TIC: BM046133.D\data.ms

(15) Phenanthrene

16.853min (-0.051) 3.29 ng/ul m

response 94935

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	17.70	15.21
176.00	21.40	19.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

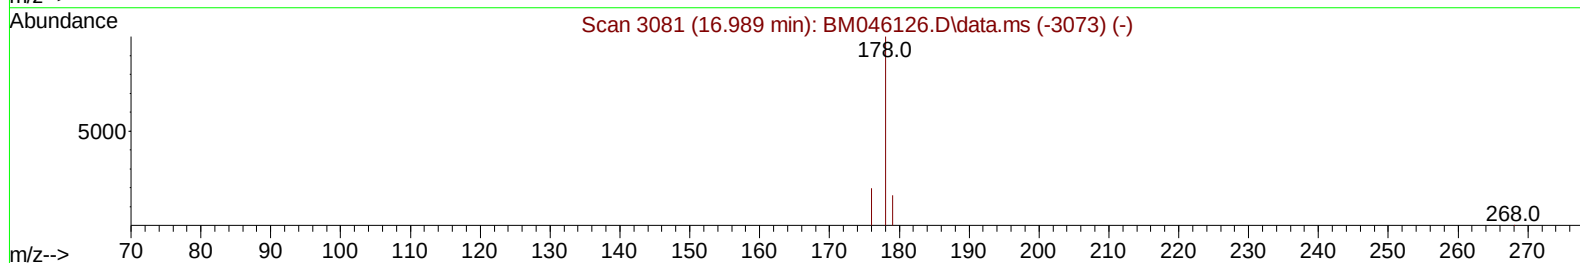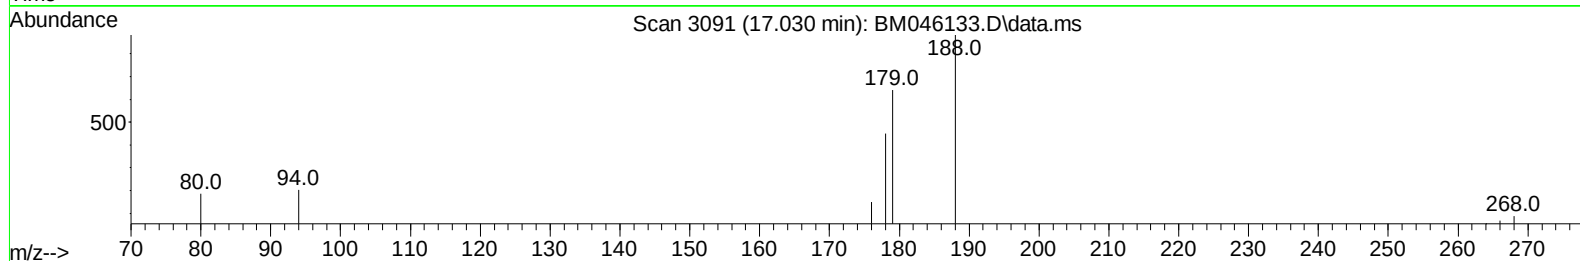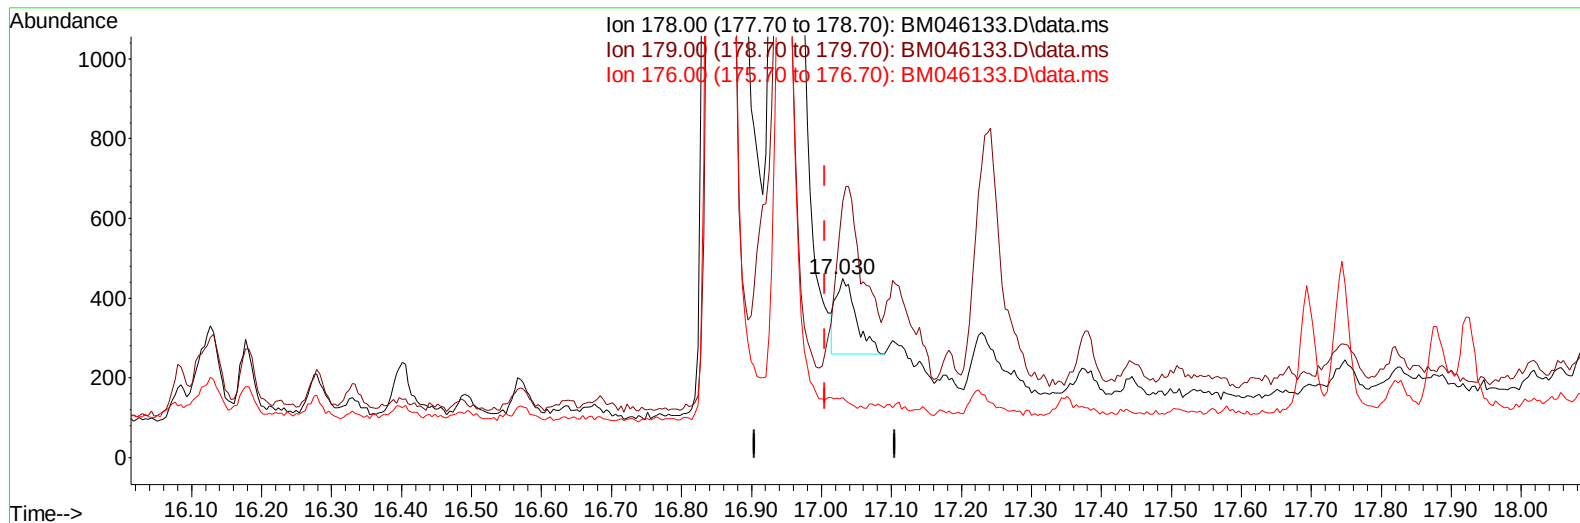

TIC: BM046133.D\data.ms

(16) Anthracene

17.030min (+ 0.025) 0.02 ng/u1

response 388

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.60	142.98#
176.00	21.20	33.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

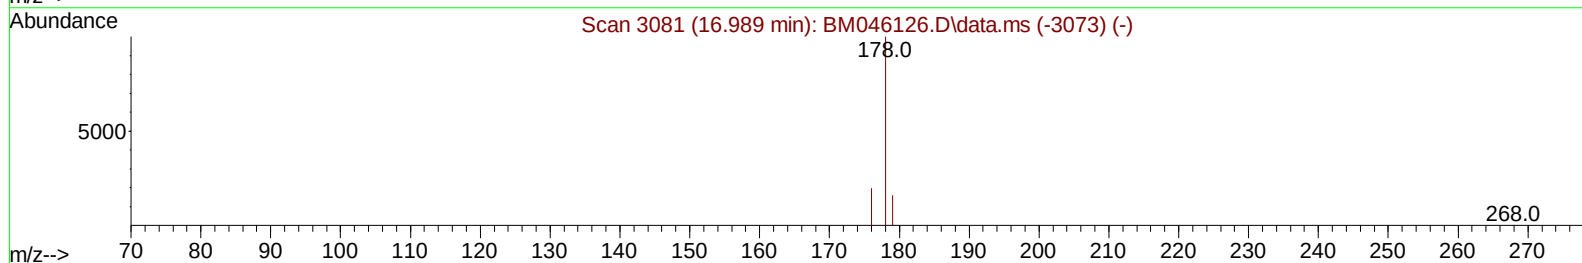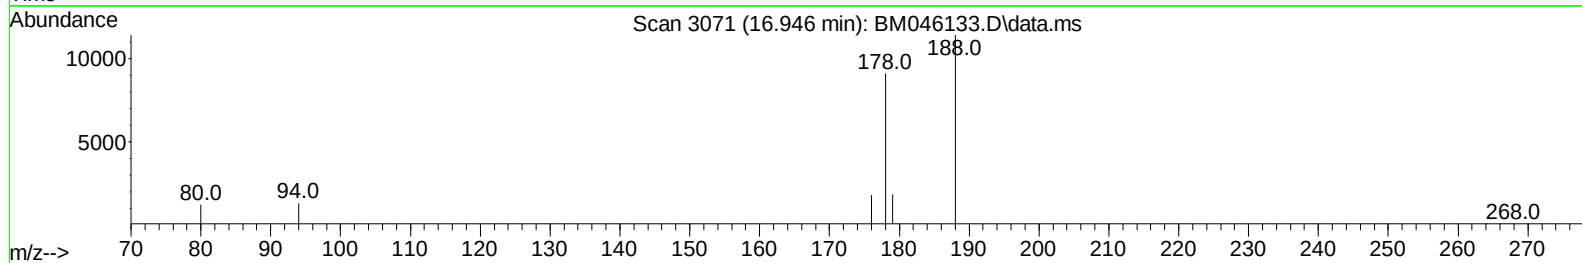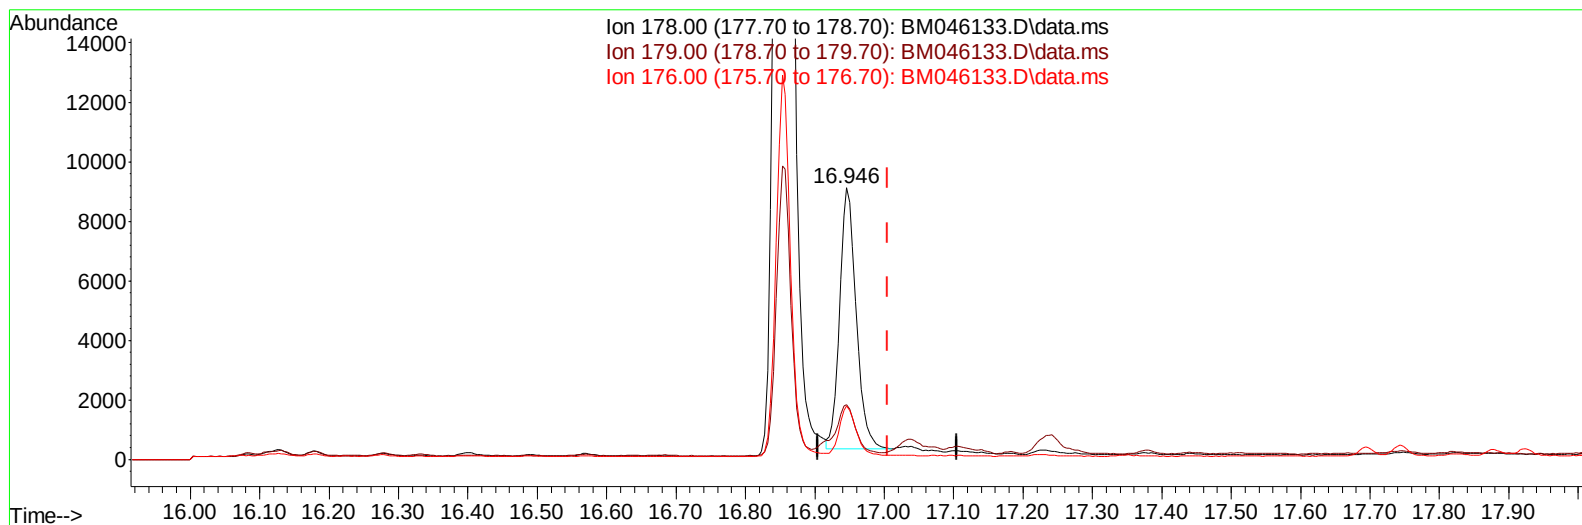

TIC: BM046133.D\data.ms

(16) Anthracene

16.946min (-0.059) 0.68 ng/ul m

response 14528

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.60	20.26
176.00	21.20	19.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

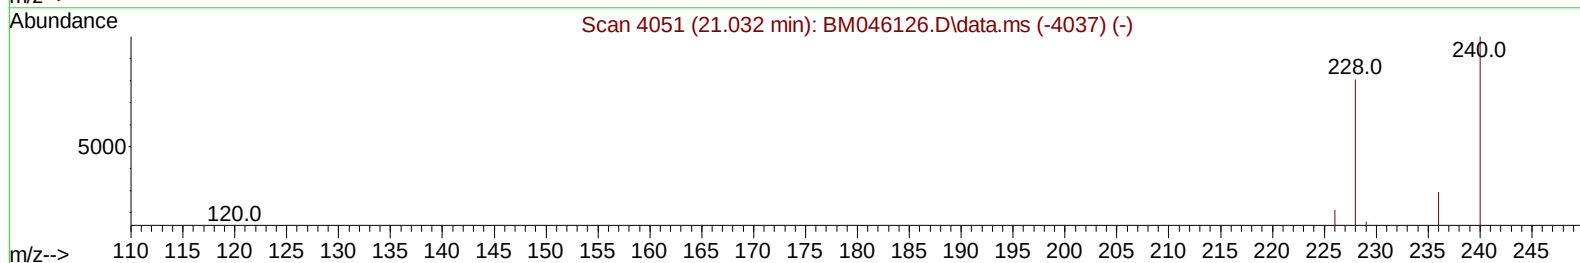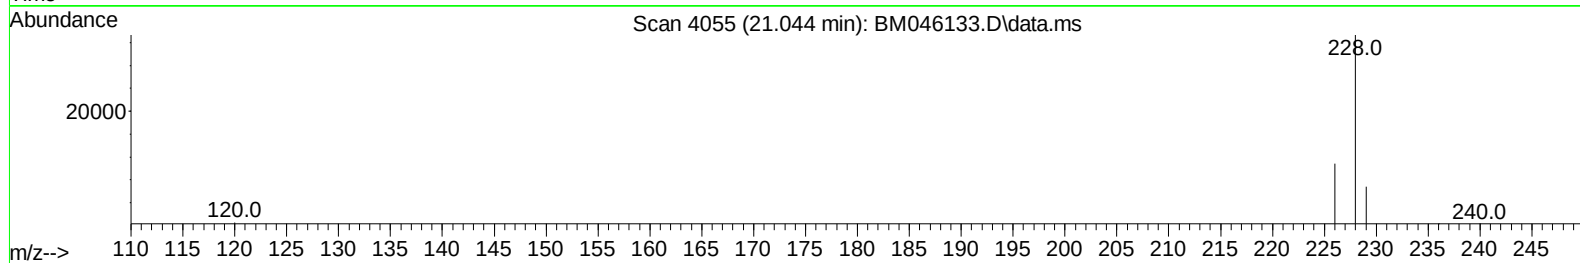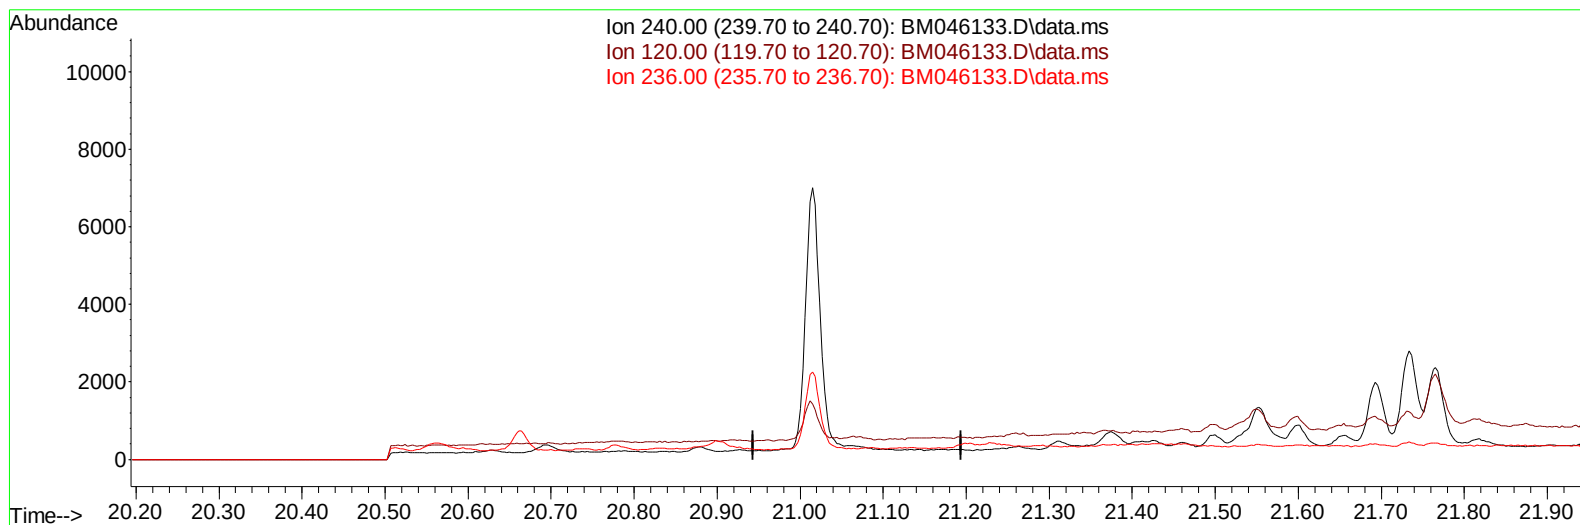

TIC: BM046133.D\data.ms

(17) Chrysene-d12

21.044min (-21.044) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	23.50	0.00#
236.00	33.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

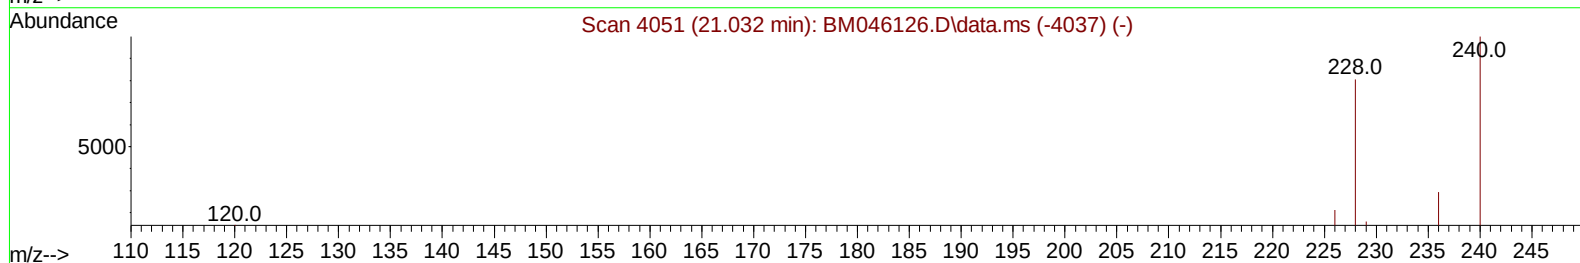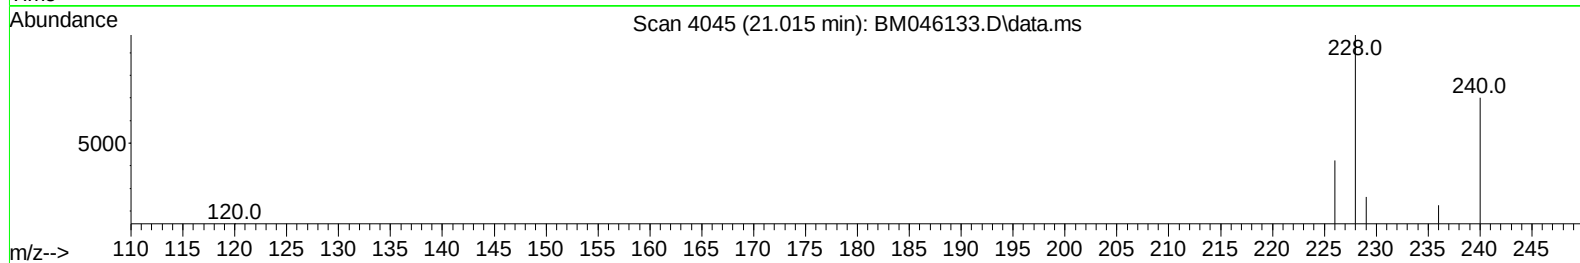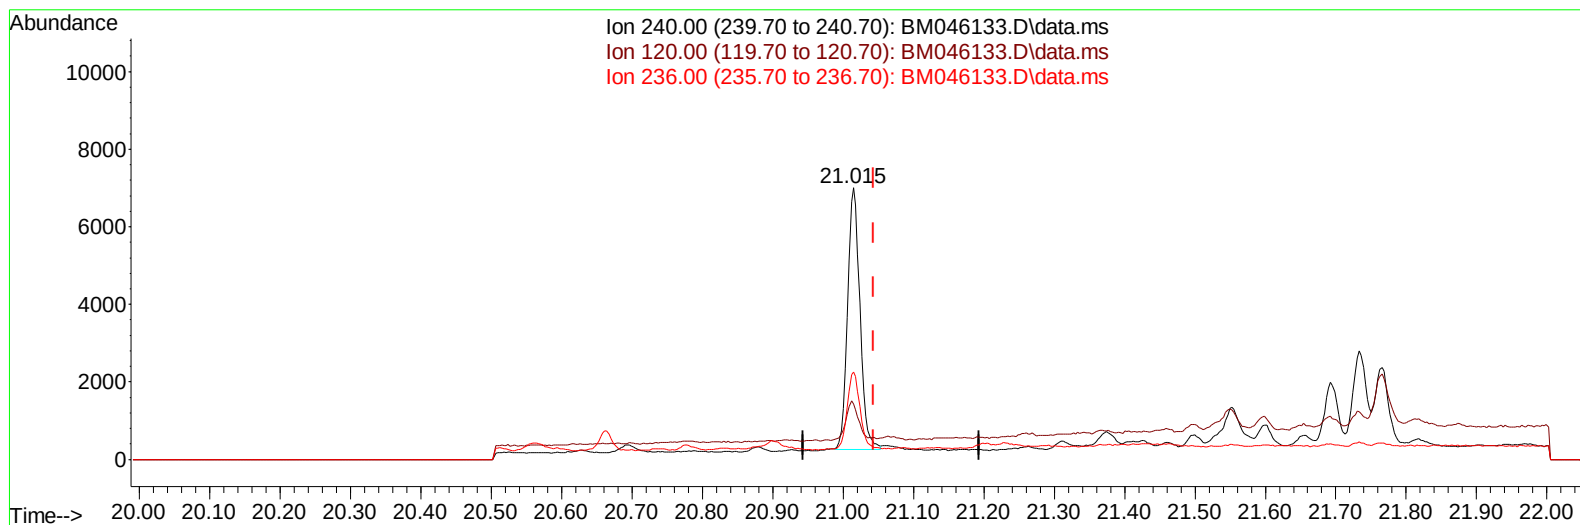

TIC: BM046133.D\data.ms

(17) Chrysene-d12

21.015min (-0.029) 0.40 ng/ul m

response 8148

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	23.50	20.47
236.00	33.60	32.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
 Data File : BM046133.D
 Acq On : 20 Jun 2024 21:14
 Operator : MA/JU
 Sample : P2710-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 13:58:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
 Supervised By :mohammad ahmed 06/24/2024

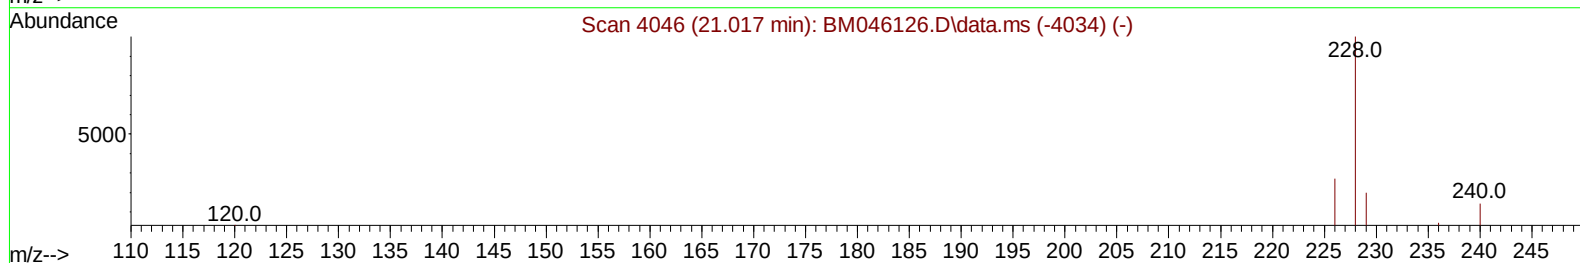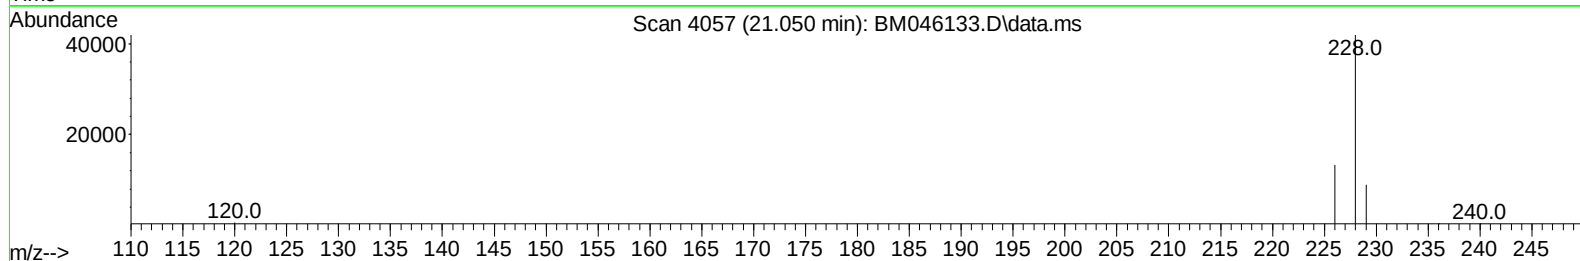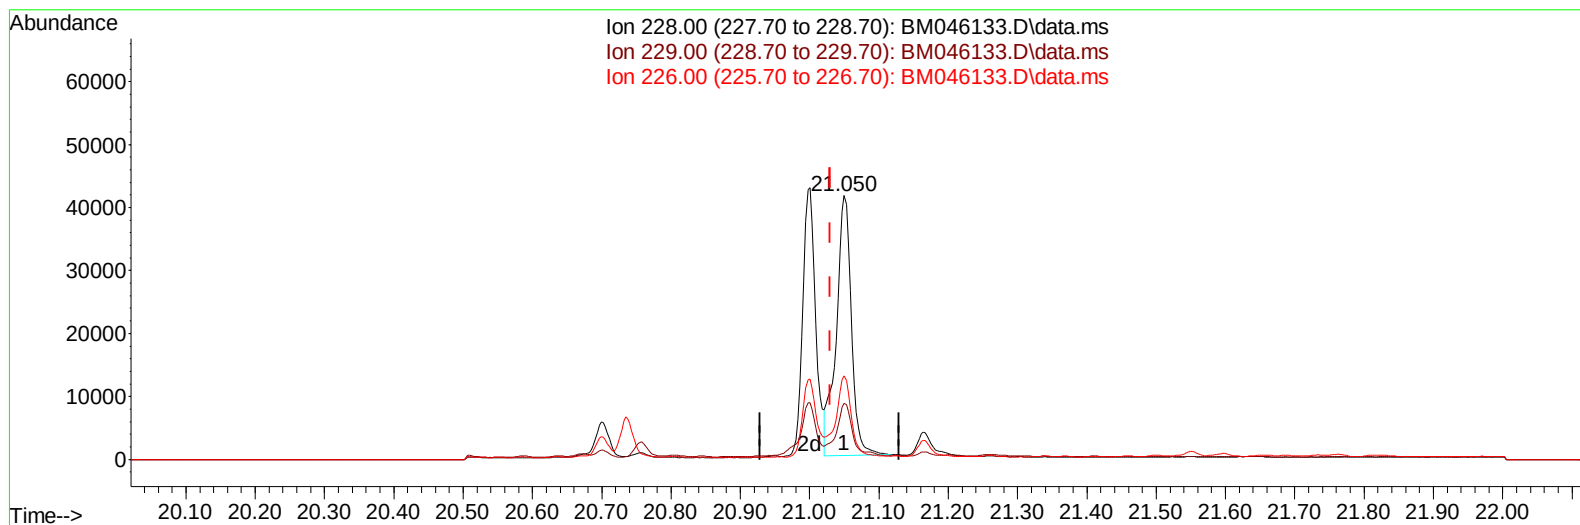

TIC: BM046133.D\data.ms

(21) Benzo(a)anthracene

21.050min (+ 0.021) 2.00 ng/u1

response 63028

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.50	21.35
226.00	29.30	31.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

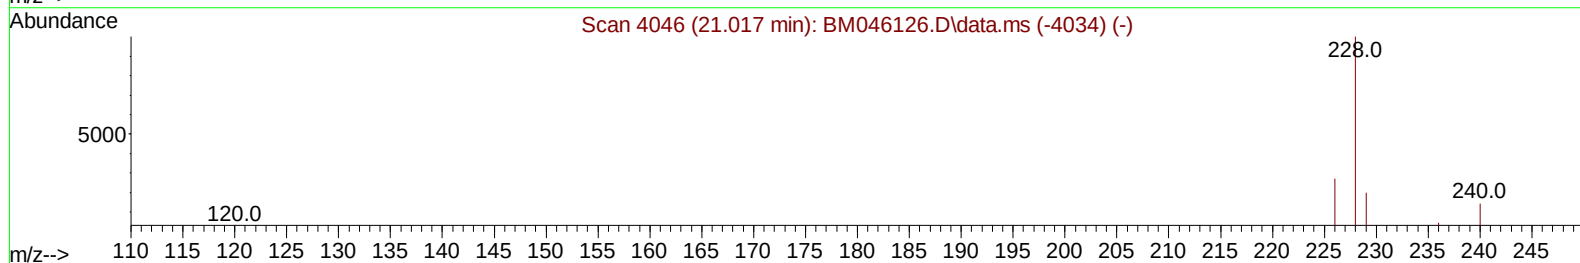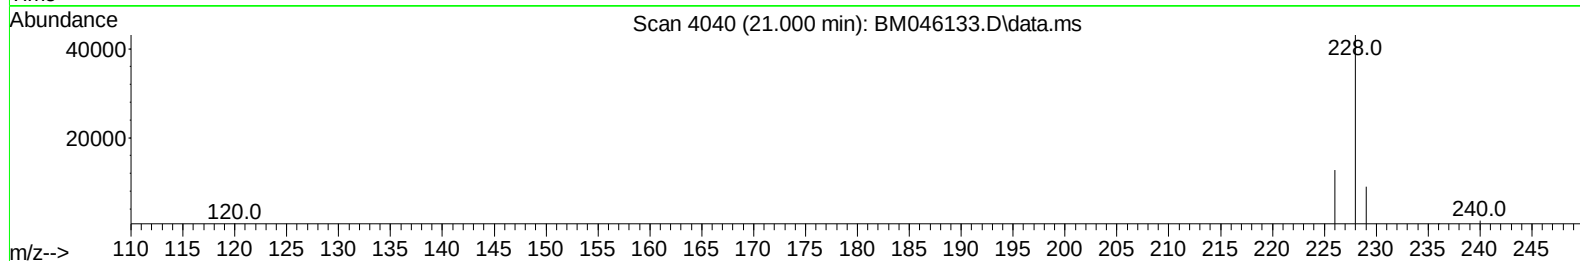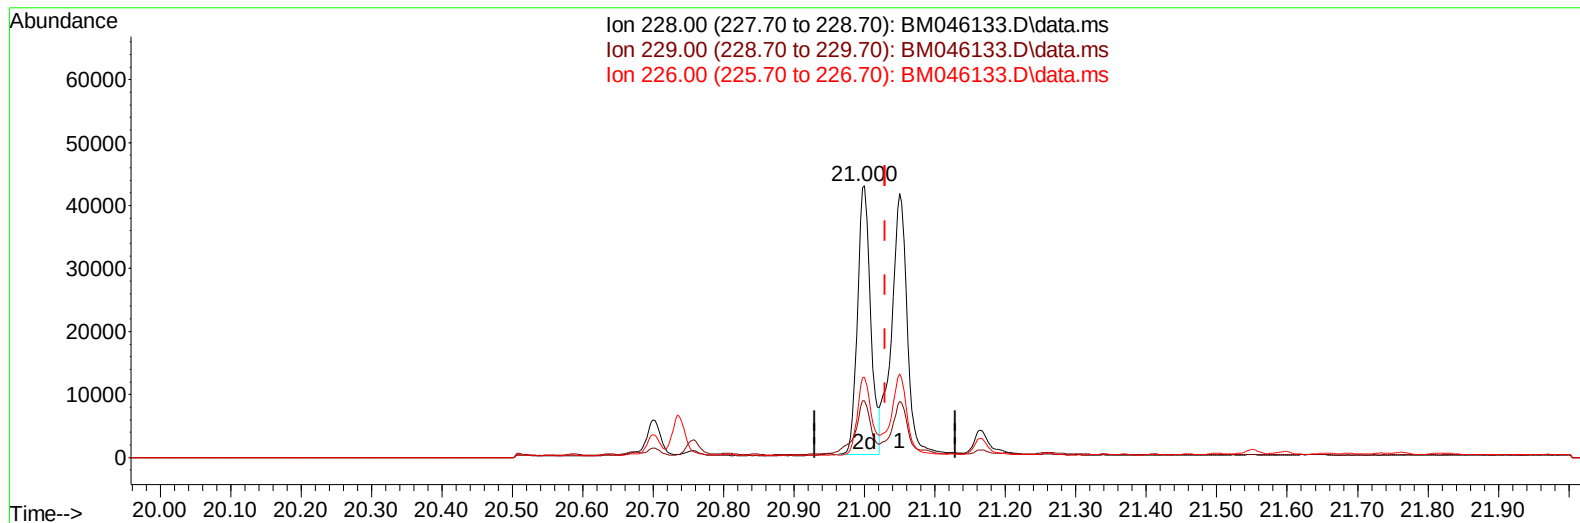

TIC: BM046133.D\data.ms

(21) Benzo(a)anthracene

21.000min (-0.029) 1.76 ng/u1 m

response 55479

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.50	20.94
226.00	29.30	29.61
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

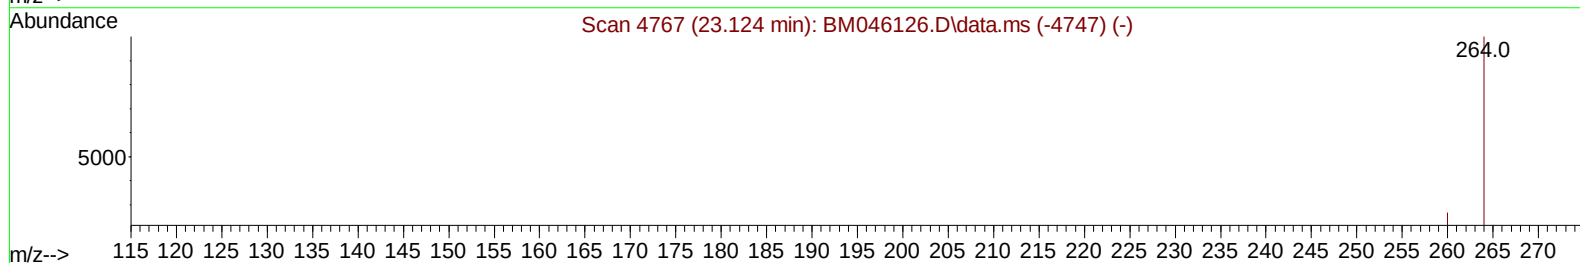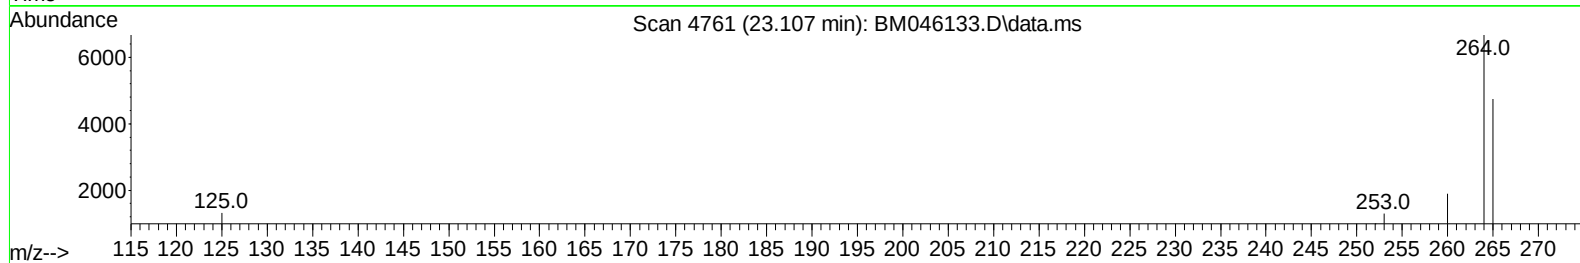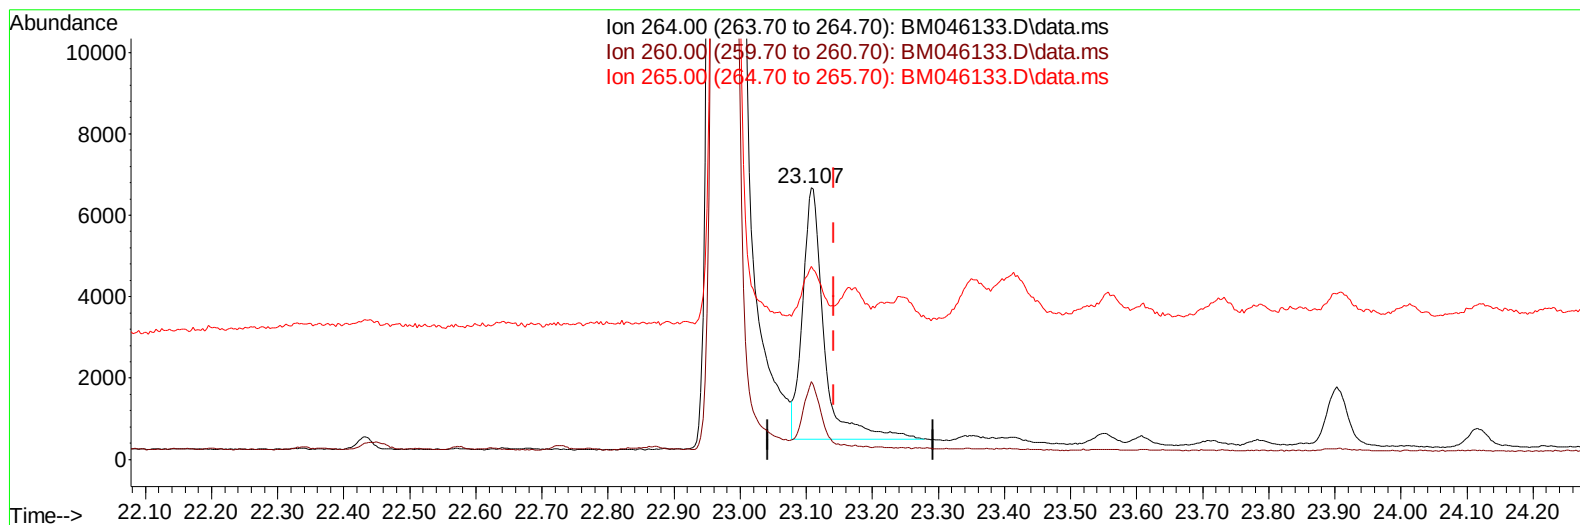

TIC: BM046133.D\data.ms

(23) Perylene-d12 (I)

23.107min (-0.035) 0.40 ng/u1

response 13712

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	28.57
265.00	110.60	71.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

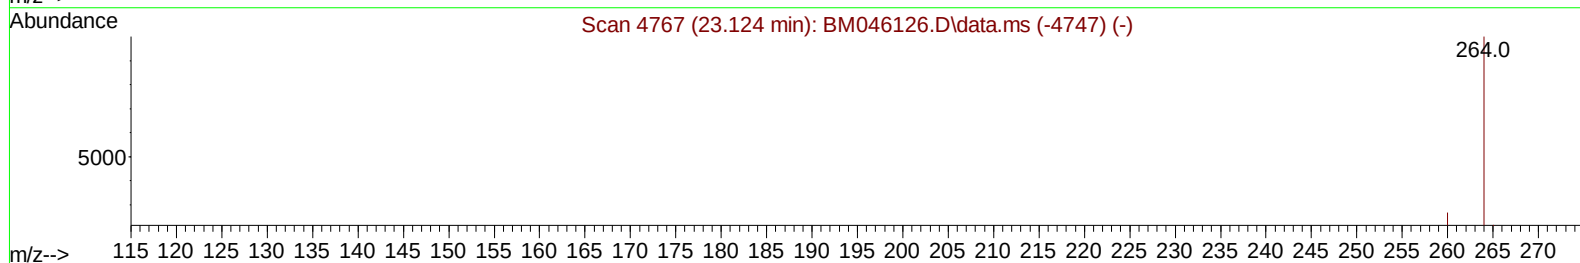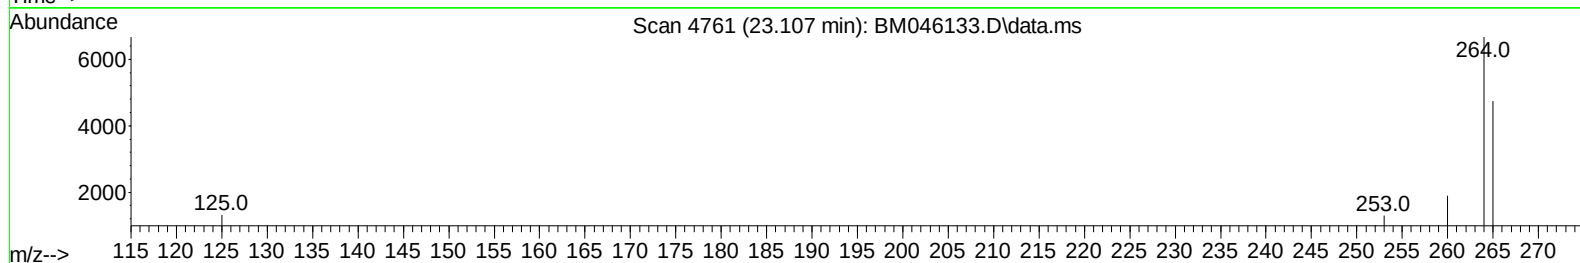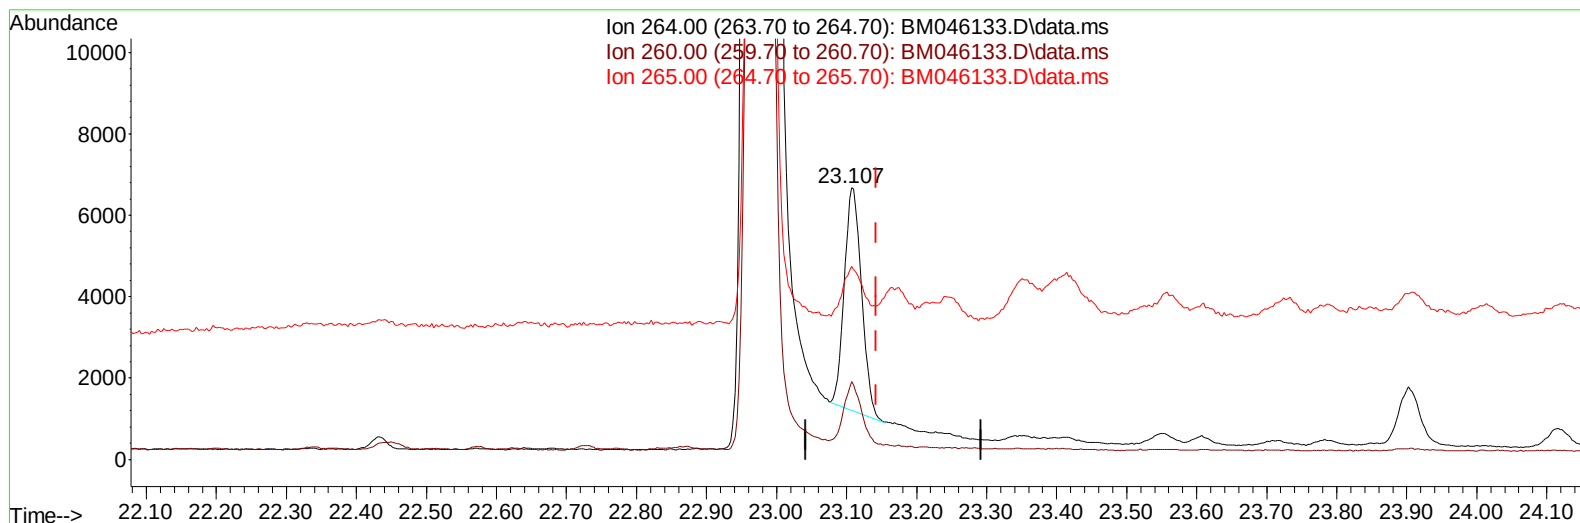

TIC: BM046133.D\data.ms

(23) Perylene-d12 (I)

23.107min (-0.035) 0.40 ng/ul m

response 9313

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	28.57
265.00	110.60	71.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

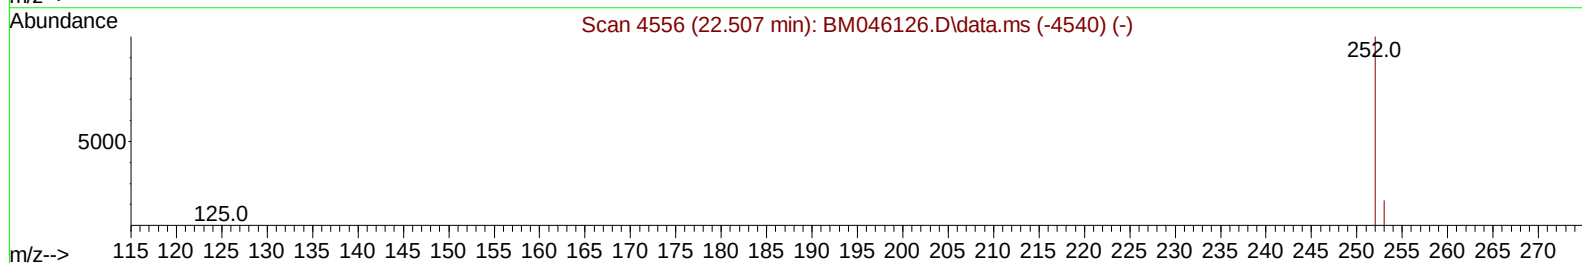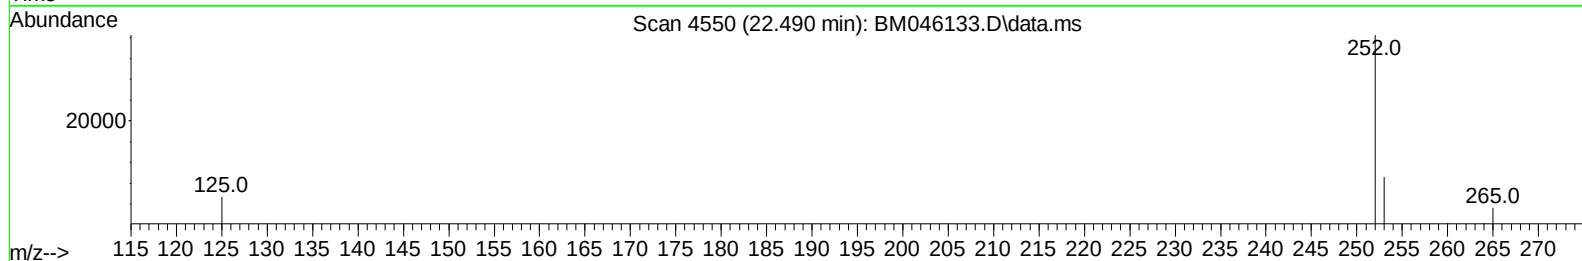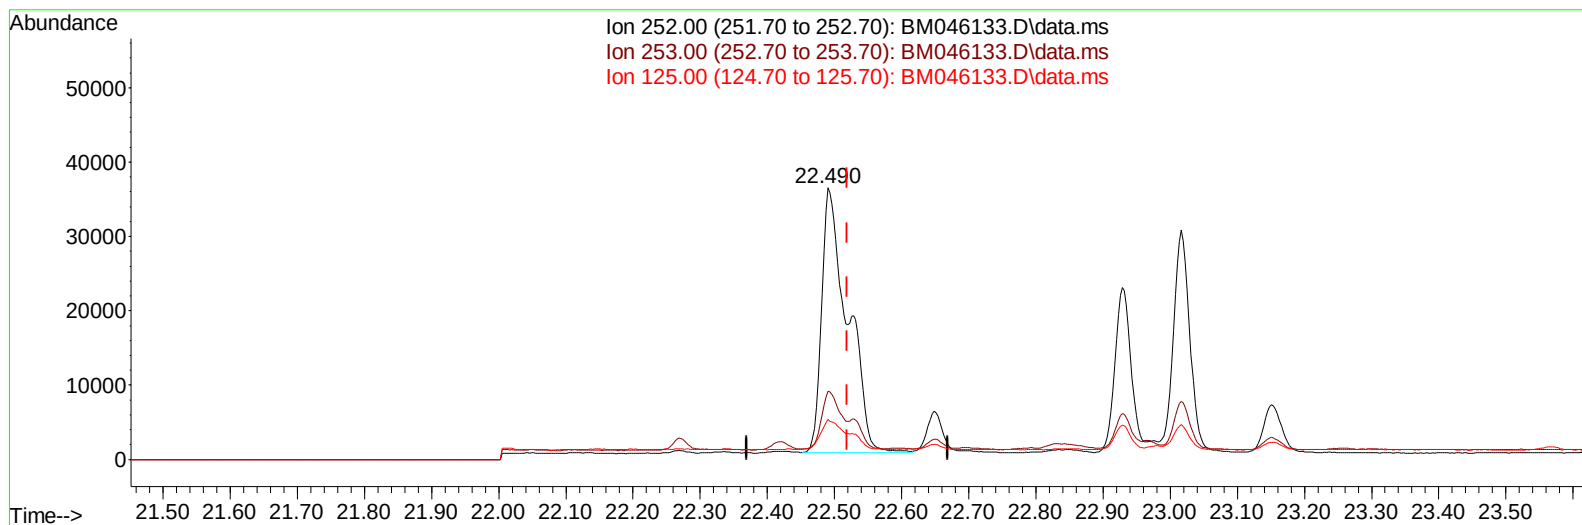

TIC: BM046133.D\data.ms

(24) Benzo(b)fluoranthene

22.490min (-0.029) 2.86 ng/u1

response 96061

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	25.11
125.00	20.10	14.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

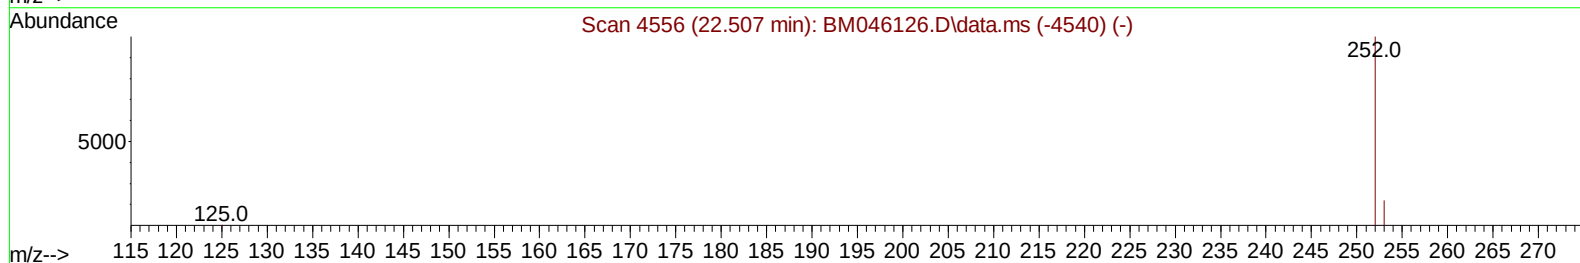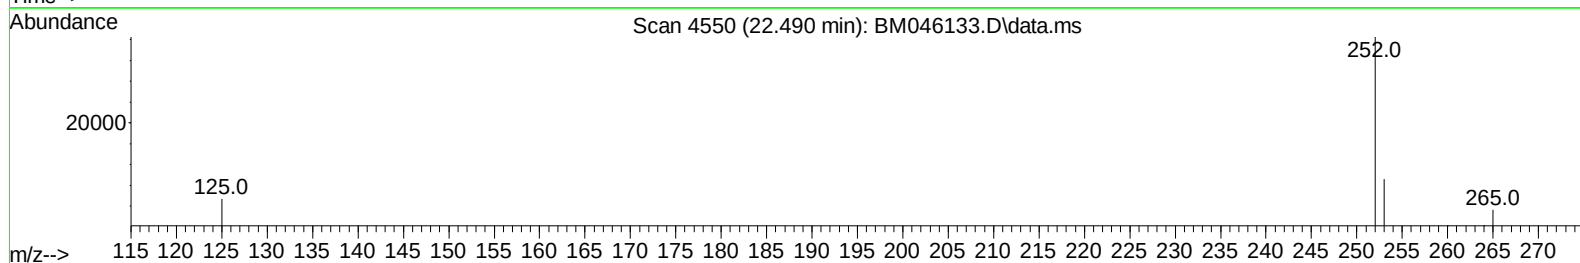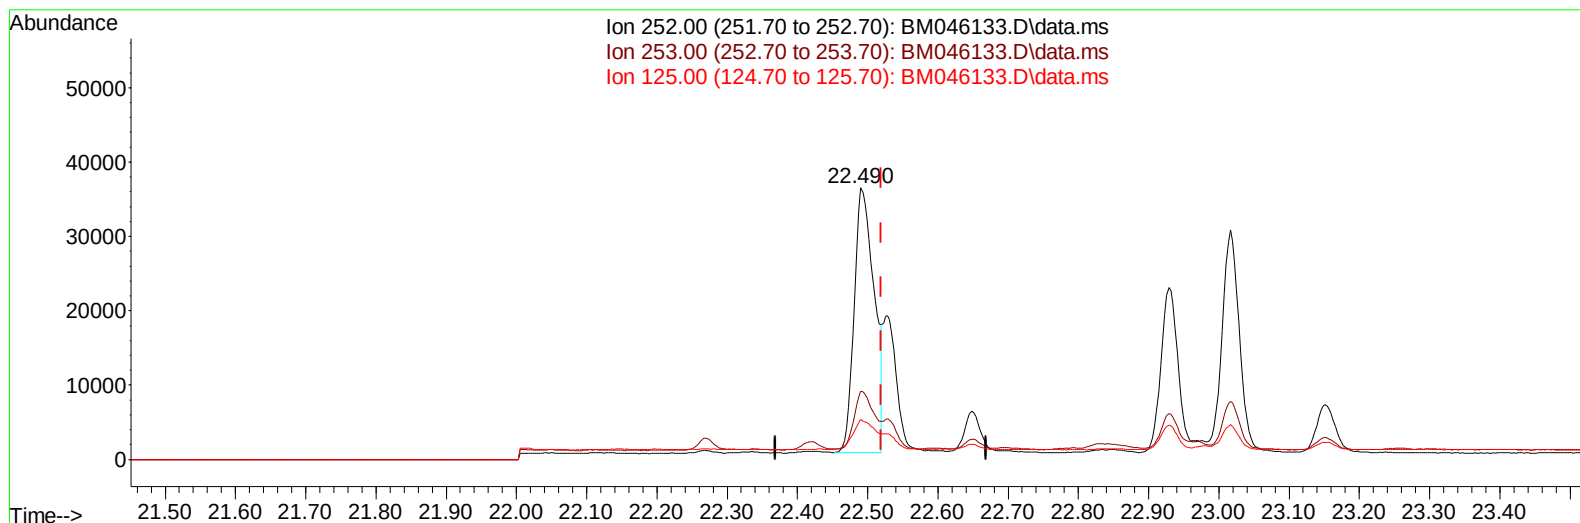

TIC: BM046133.D\data.ms

(24) Benzo(b)fluoranthene

22.490min (-0.029) 2.12 ng/ul m

response 71163

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	25.11
125.00	20.10	14.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
 Data File : BM046133.D
 Acq On : 20 Jun 2024 21:14
 Operator : MA/JU
 Sample : P2710-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 13:58:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
 Supervised By :mohammad ahmed 06/24/2024

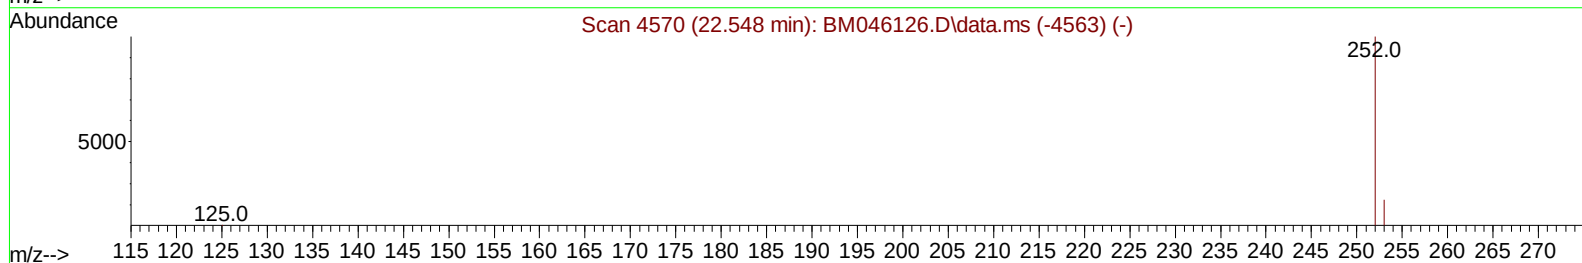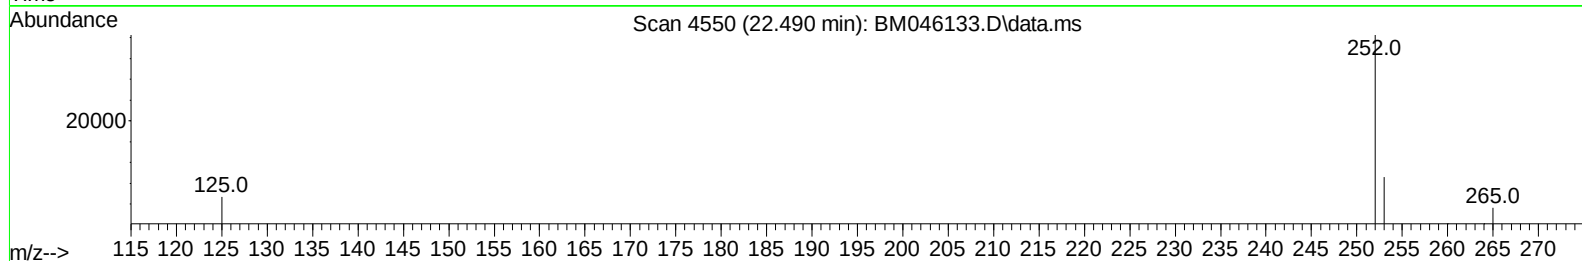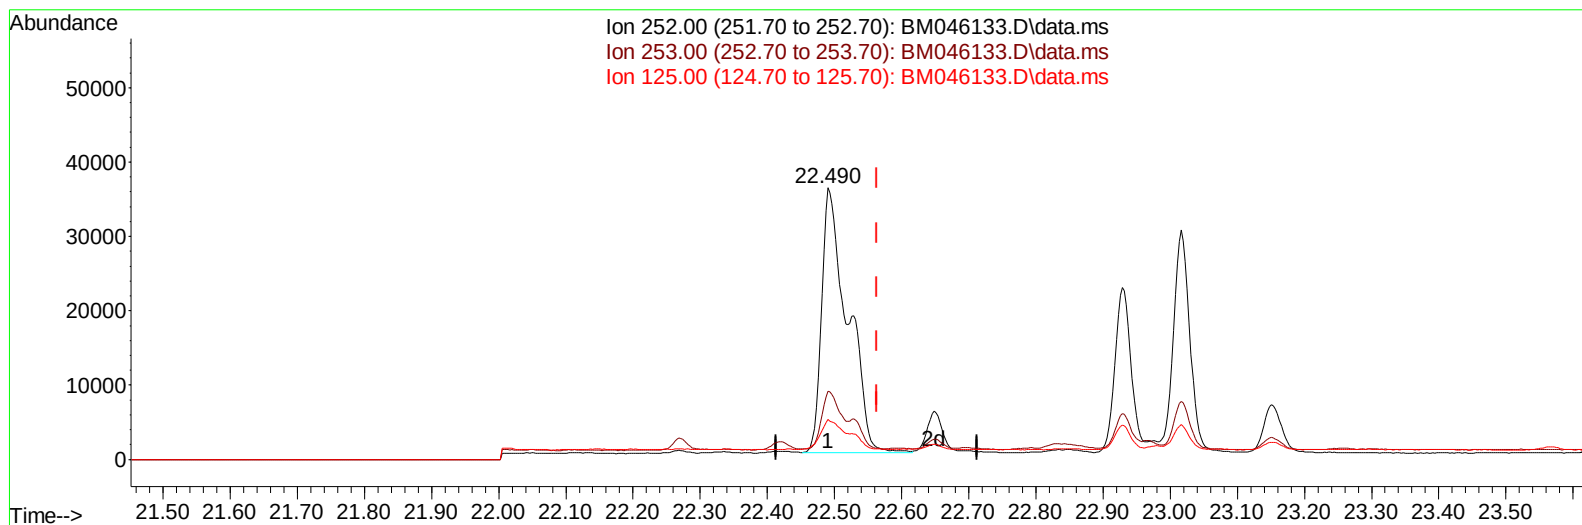

TIC: BM046133.D\data.ms

(25) Benzo(k)fluoranthene

22.490min (-0.073) 2.41 ng/u1

response 96061

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	25.11#
125.00	20.80	14.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

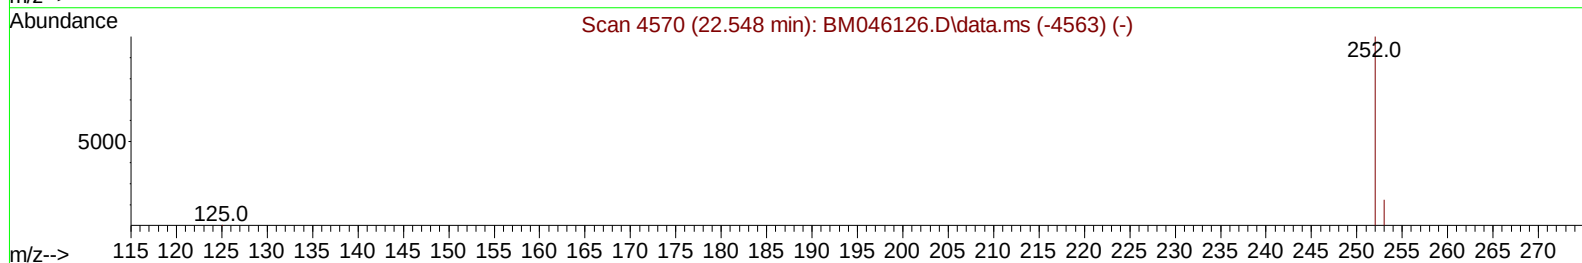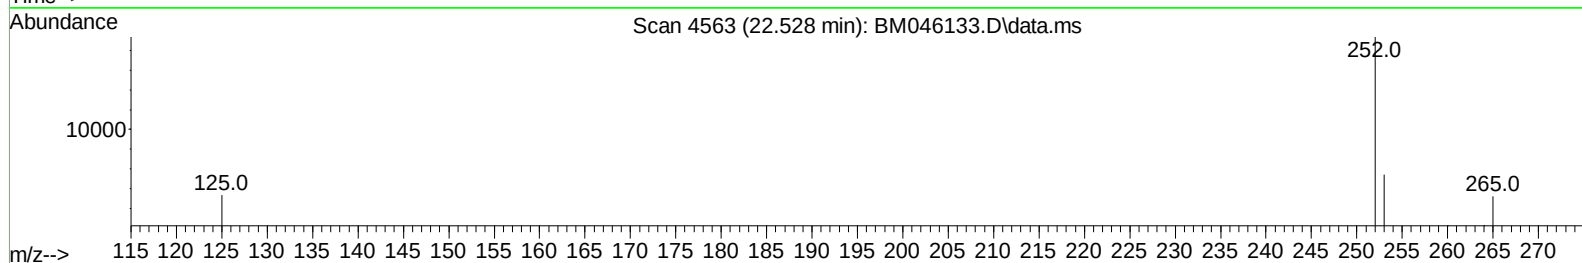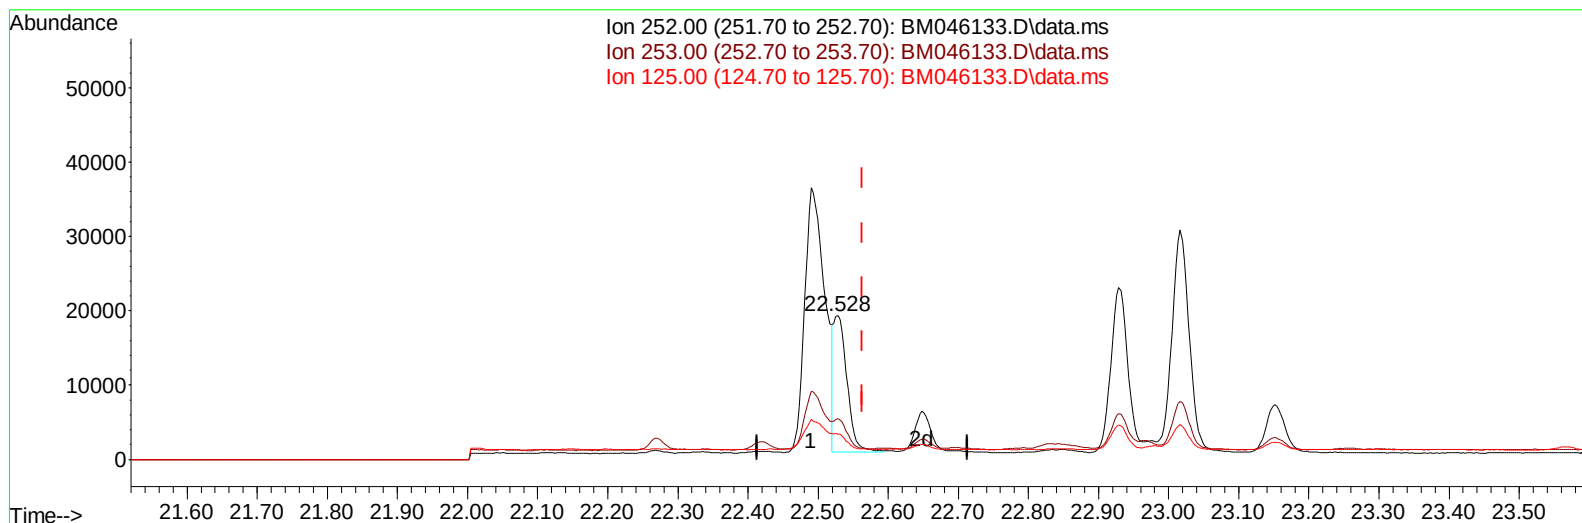

TIC: BM046133.D\data.ms

(25) Benzo(k)fluoranthene

22.528min (-0.035) 0.62 ng/ul m

response 24662

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	28.20
125.00	20.80	17.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

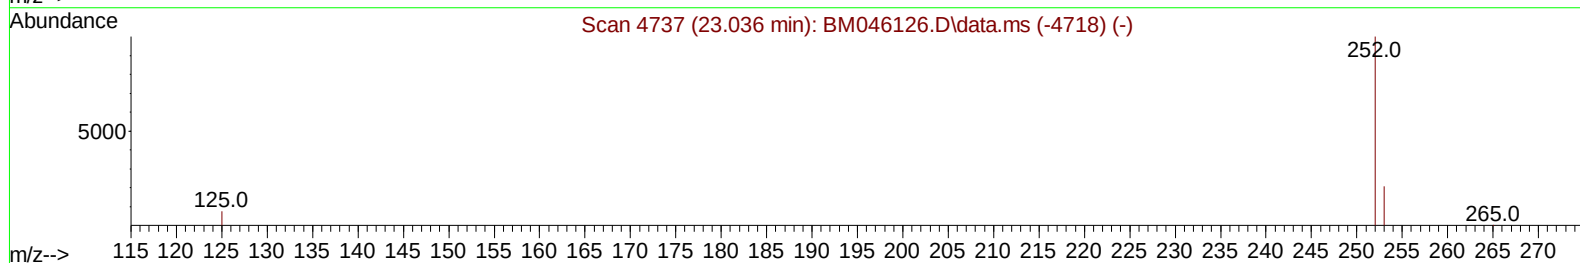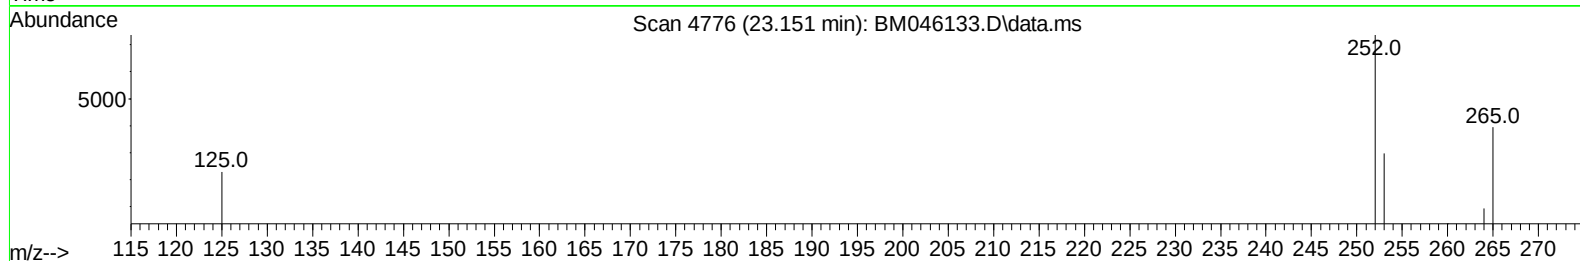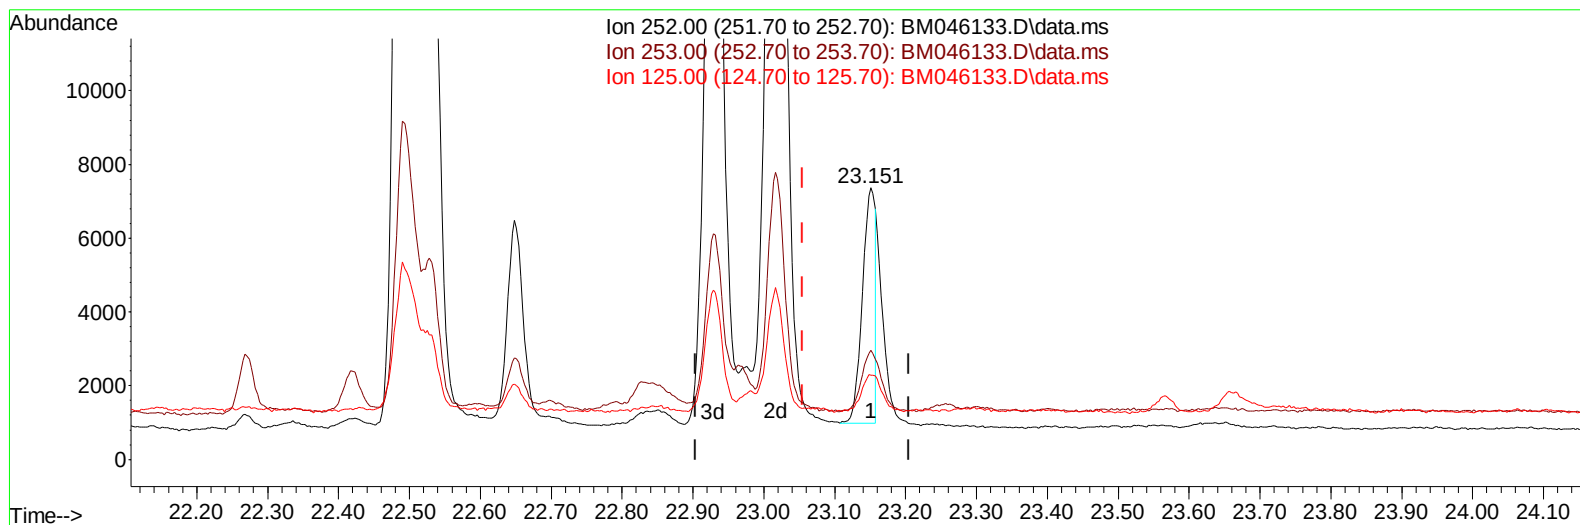

TIC: BM046133.D\data.ms

(26) Benzo(a)pyrene (C)

23.151min (+ 0.097) 0.25 ng/u1

response 7879

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	40.10	40.27
125.00	26.50	31.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

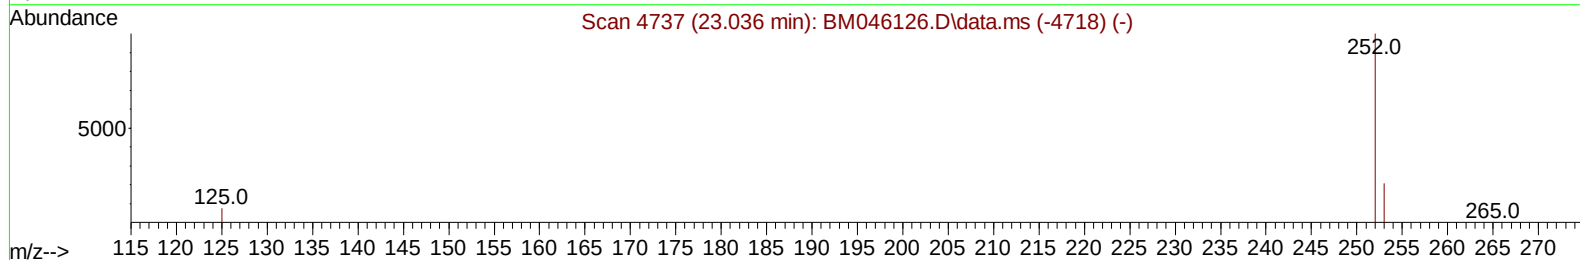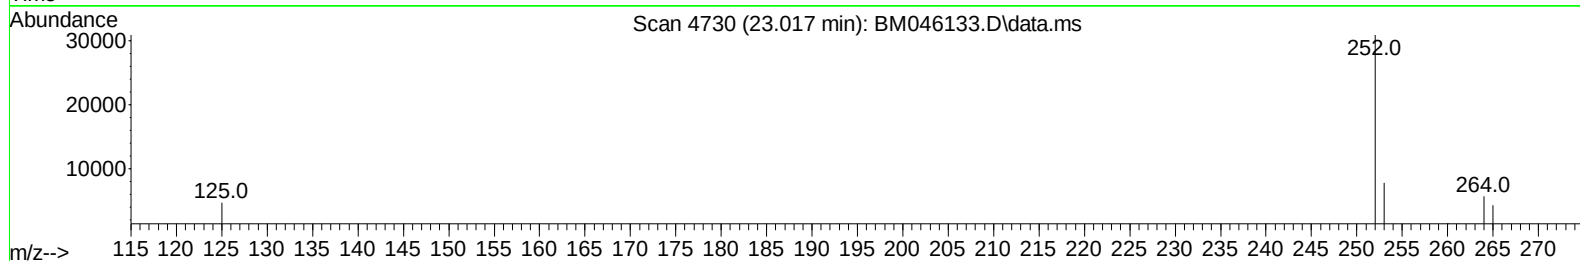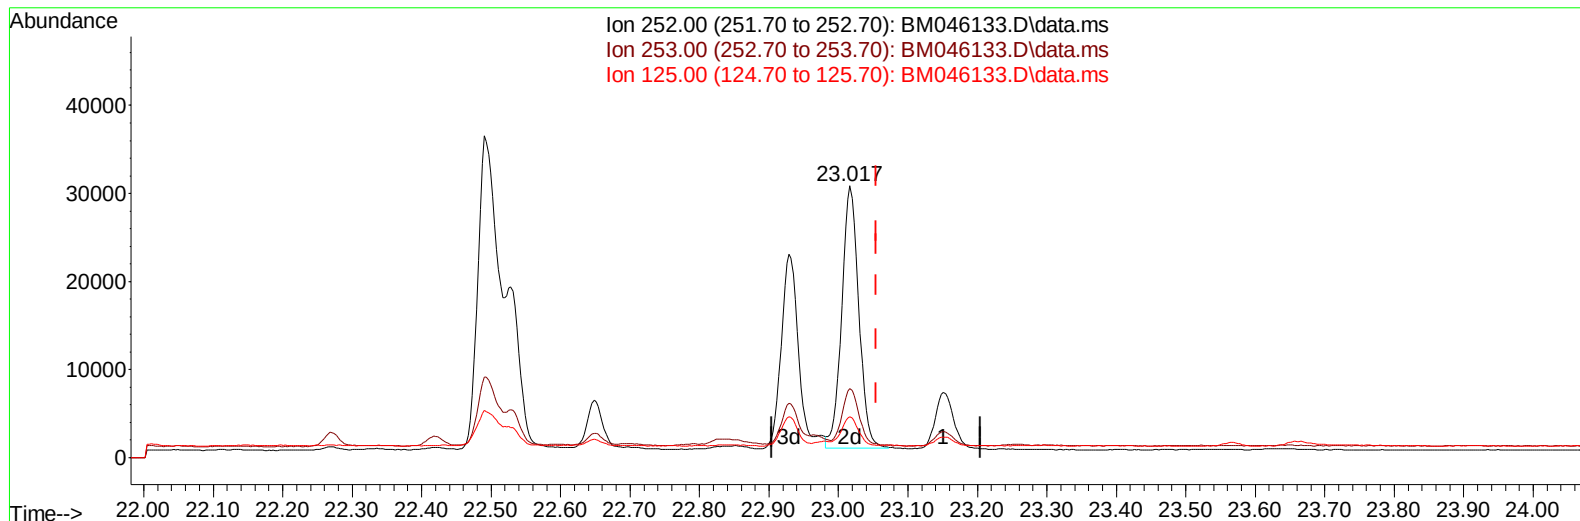

TIC: BM046133.D\data.ms

(26) Benzo(a)pyrene (C)

23.017min (-0.038) 1.63 ng/u1 m

response 50644

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	40.10	25.27#
125.00	26.50	15.10#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
 Data File : BM046133.D
 Acq On : 20 Jun 2024 21:14
 Operator : MA/JU
 Sample : P2710-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 18 13:58:29 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
 Supervised By :mohammad ahmed 06/24/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.422	152	3105	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.193	136	9030	0.400	ng/ul	#-0.06
9) Acenaphthene-d10	14.071	164	4919	0.400	ng/ul	-0.04
13) Phenanthrene-d10	16.815	188	10276m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.015	240	8148m	0.400	ng/ul	-0.03
23) Perylene-d12	23.107	264	9313m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.033	96	13934	3.271	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.821	152	2778	0.229	ng/ul	-0.04
18) Fluoranthene-d10	18.848	212	5990	0.245	ng/ul	-0.04
Target Compounds						
					Qvalue	
5) Naphthalene	10.242	128	2013	0.080	ng/ul#	93
7) 2-Methylnaphthalene	11.898	142	812	0.057	ng/ul	96
8) 1-Methylnaphthalene	12.107	142	842	0.054	ng/ul	95
10) Acenaphthylene	13.788	152	4096	0.176	ng/ul#	95
11) Acenaphthene	14.135	153	4458	0.265	ng/ul	98
12) Fluorene	15.125	166	4691	0.260	ng/ul	99
15) Phenanthrene	16.853	178	94935m	3.288	ng/ul	
16) Anthracene	16.946	178	14528m	0.676	ng/ul	
19) Fluoranthene	18.880	202	131153	3.718	ng/ul	95
20) Pyrene	19.243	202	136998	3.591	ng/ul	94
21) Benzo(a)anthracene	21.000	228	55479m	1.763	ng/ul	
22) Chrysene	21.050	228	63113	1.571	ng/ul	99
24) Benzo(b)fluoranthene	22.490	252	71163m	2.121	ng/ul	
25) Benzo(k)fluoranthene	22.528	252	24662m	0.618	ng/ul	
26) Benzo(a)pyrene	23.017	252	50644m	1.629	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.159	276	37482	0.737	ng/ul#	89
28) Dibenzo(a,h)anthracene	25.162	278	8499	0.224	ng/ul#	85
29) Benzo(g,h,i)perylene	25.783	276	38405	0.880	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062024\
Data File : BM046133.D
Acq On : 20 Jun 2024 21:14
Operator : MA/JU
Sample : P2710-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4B26

Manual IntegrationsAPPROVED

Quant Time: Jun 21 02:49:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 18 13:58:29 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2024
Supervised By :mohammad ahmed 06/24/2024

