

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
 Data File : BM015731.D
 Acq On : 21 Jun 2018 12:49
 Operator : SJ/JU
 Sample : J3470-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 22 01:27:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 22 01:26:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	98080	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	418569	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	236906	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	537157	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	579333	20.00	ng/ul	0.00
85) Perylene-d12	24.18	264	554099	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	7022	3.48	ng/uL	0.00
5) Phenol-d5	7.47	99	135292	15.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	90884	16.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.85	132	117663	17.28	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	111740	14.57	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	53516	19.01	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	56143	18.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	111283	17.75	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	149010	21.33	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	396781	20.23	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	446402	21.10	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	41166	10.87	ng/ul	0.00
57) Fluorene-d10	15.92	176	341747	20.59	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	39170	12.11	ng/ul	0.00
70) Anthracene-d10	17.76	188	535232	21.86	ng/ul	0.00
78) Pyrene-d10	20.02	212	616113	24.72	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	612663	22.06	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.39	163	103789	5.182	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
Data File : BM015731.D
Acq On : 21 Jun 2018 12:49
Operator : SJ/JU
Sample : J3470-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 22 01:27:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 22 01:26:58 2018
Response via : Initial Calibration

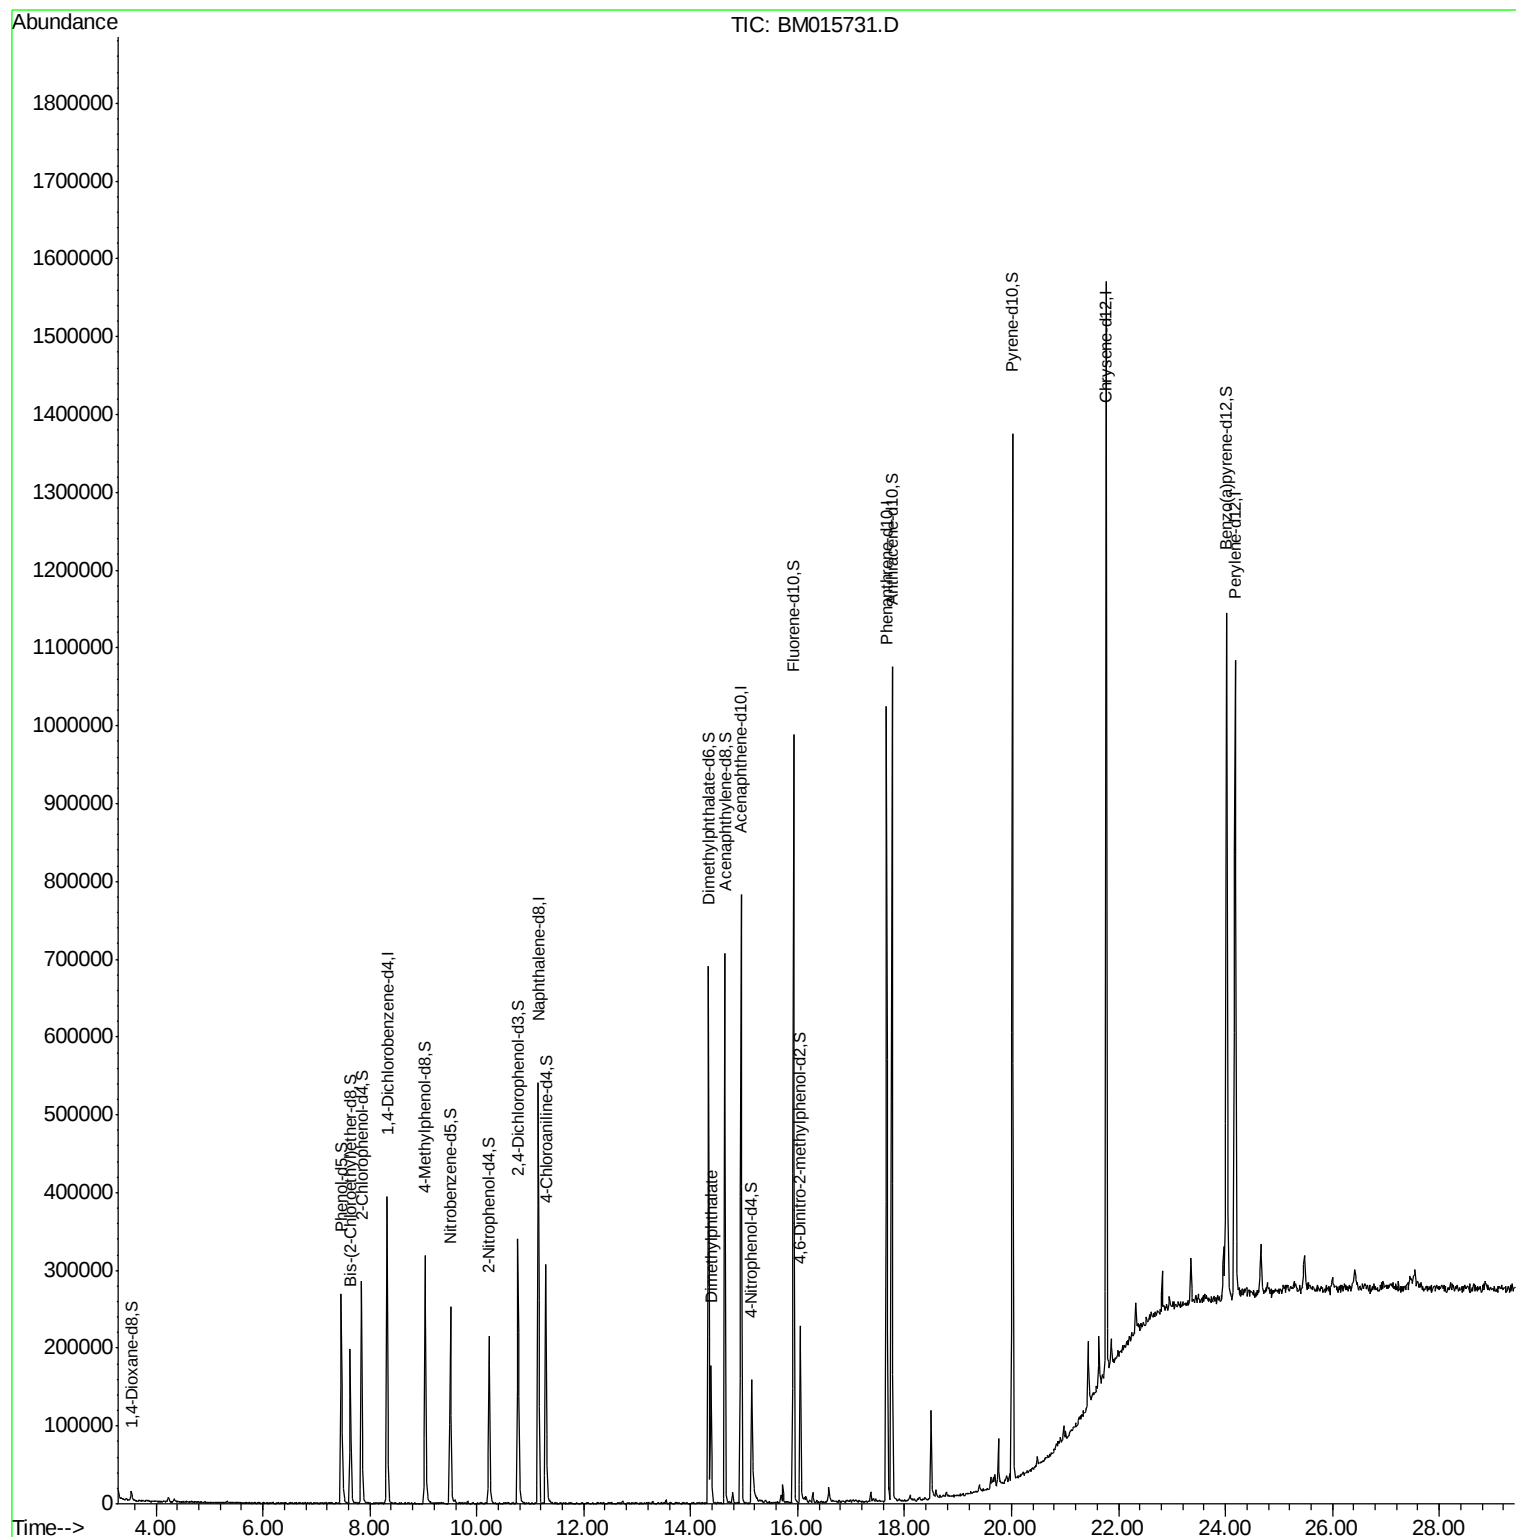

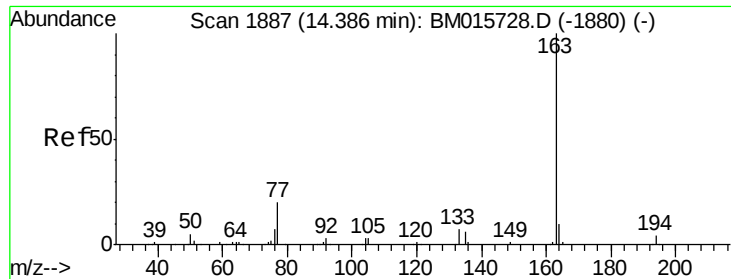

#44

Dimethylphthalate

Concen: 5.182 ng/ul

RT: 14.39 min Scan# 1887

Delta R.T. -0.00 min


Lab File: BM015731.D

Acq: 21 Jun 2018 12:49

Instrument :

BNA_M

ClientSampleId :

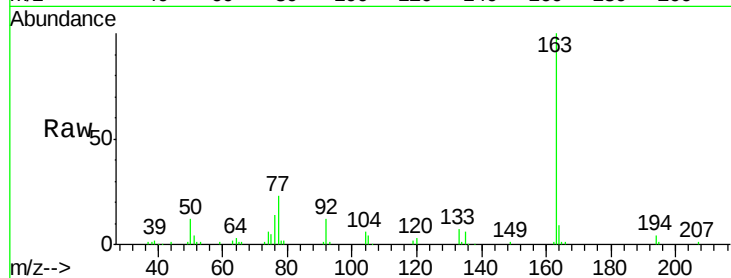

Tot Ion:	163	Resp:	103789
Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.2	4.8
164	9.2	7.8	11.8

