

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
 Data File : BM015736.D
 Acq On : 21 Jun 2018 19:57
 Operator : SJ/JU
 Sample : J3568-01RX
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 22 02:12:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 22 02:12:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	98157	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	440168	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	248636	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	565924	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	604510	20.00	ng/ul	0.00
85) Perylene-d12	24.18	264	579601	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	9375	4.64	ng/uL	0.00
5) Phenol-d5	7.46	99	173481	19.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	119122	22.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.84	132	154410	22.66	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	139445	18.17	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	71612	24.20	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	76154	23.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	143301	21.74	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	192869	26.26	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	506408	24.60	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	575060	25.90	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	55611	13.99	ng/ul	0.00
57) Fluorene-d10	15.92	176	432338	24.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	56770	16.65	ng/ul	0.00
70) Anthracene-d10	17.76	188	688072	26.67	ng/ul	0.00
78) Pyrene-d10	20.02	212	772522	29.71	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	785529	27.04	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	14.39	163	124077	5.903	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
Data File : BM015736.D
Acq On : 21 Jun 2018 19:57
Operator : SJ/JU
Sample : J3568-01RX
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 22 02:12:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 22 02:12:20 2018
Response via : Initial Calibration

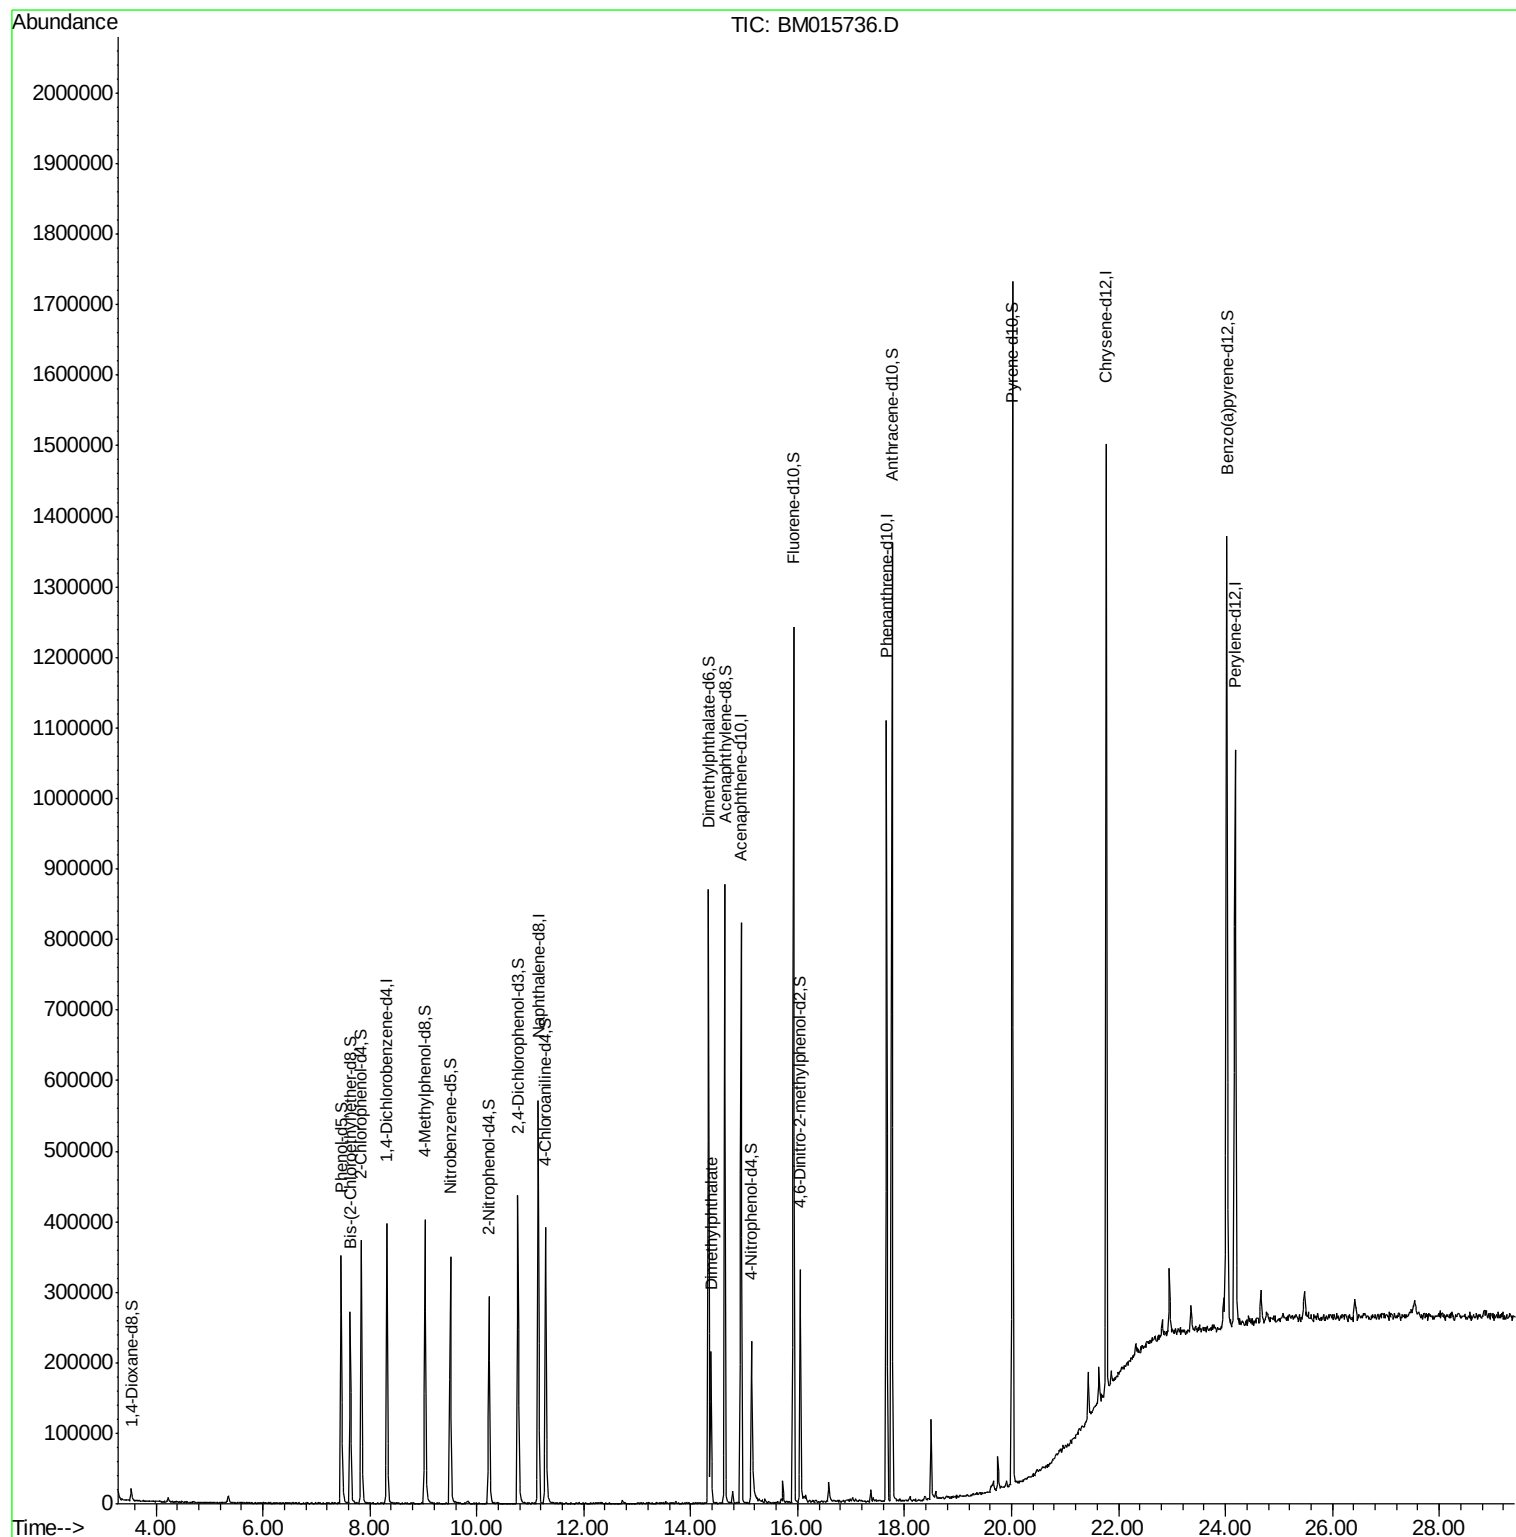

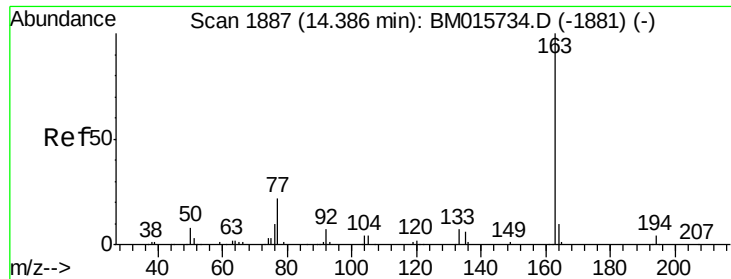

#44

Dimethylphthalate

Concen: 5.903 ng/ul

RT: 14.39 min Scan# 1887

Delta R.T. -0.00 min

Lab File: BM015736.D

Acq: 21 Jun 2018 19:57

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 124077

Ion Ratio Lower Upper

163 100

194 3.7 3.2 4.8

164 9.8 7.8 11.8

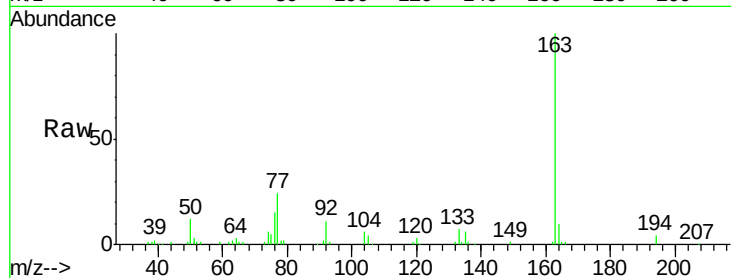

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

