

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
 Data File : BM015737.D
 Acq On : 21 Jun 2018 20:34
 Operator : SJ/JU
 Sample : J3568-02RX
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 22 02:13:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 22 02:12:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	96550	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	432776	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	247420	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	564630	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	608761	20.00	ng/ul	0.00
85) Perylene-d12	24.18	264	596186	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.53	96	5858	2.95	ng/uL	0.00
5) Phenol-d5	7.47	99	111406	12.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	77148	14.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.85	132	100227	14.95	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	90461	11.98	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	44184	15.18	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	46506	14.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	93716	14.46	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	126291	17.49	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	333000	16.26	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	366288	16.58	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	30110	7.61	ng/ul	0.00
57) Fluorene-d10	15.92	176	283484	16.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	33282	9.79	ng/ul	0.00
70) Anthracene-d10	17.76	188	453176	17.61	ng/ul	0.00
78) Pyrene-d10	20.02	212	544985	20.81	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	565852	18.93	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.39	163	80094	3.829	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
Data File : BM015737.D
Acq On : 21 Jun 2018 20:34
Operator : SJ/JU
Sample : J3568-02RX
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 22 02:13:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 22 02:12:20 2018
Response via : Initial Calibration

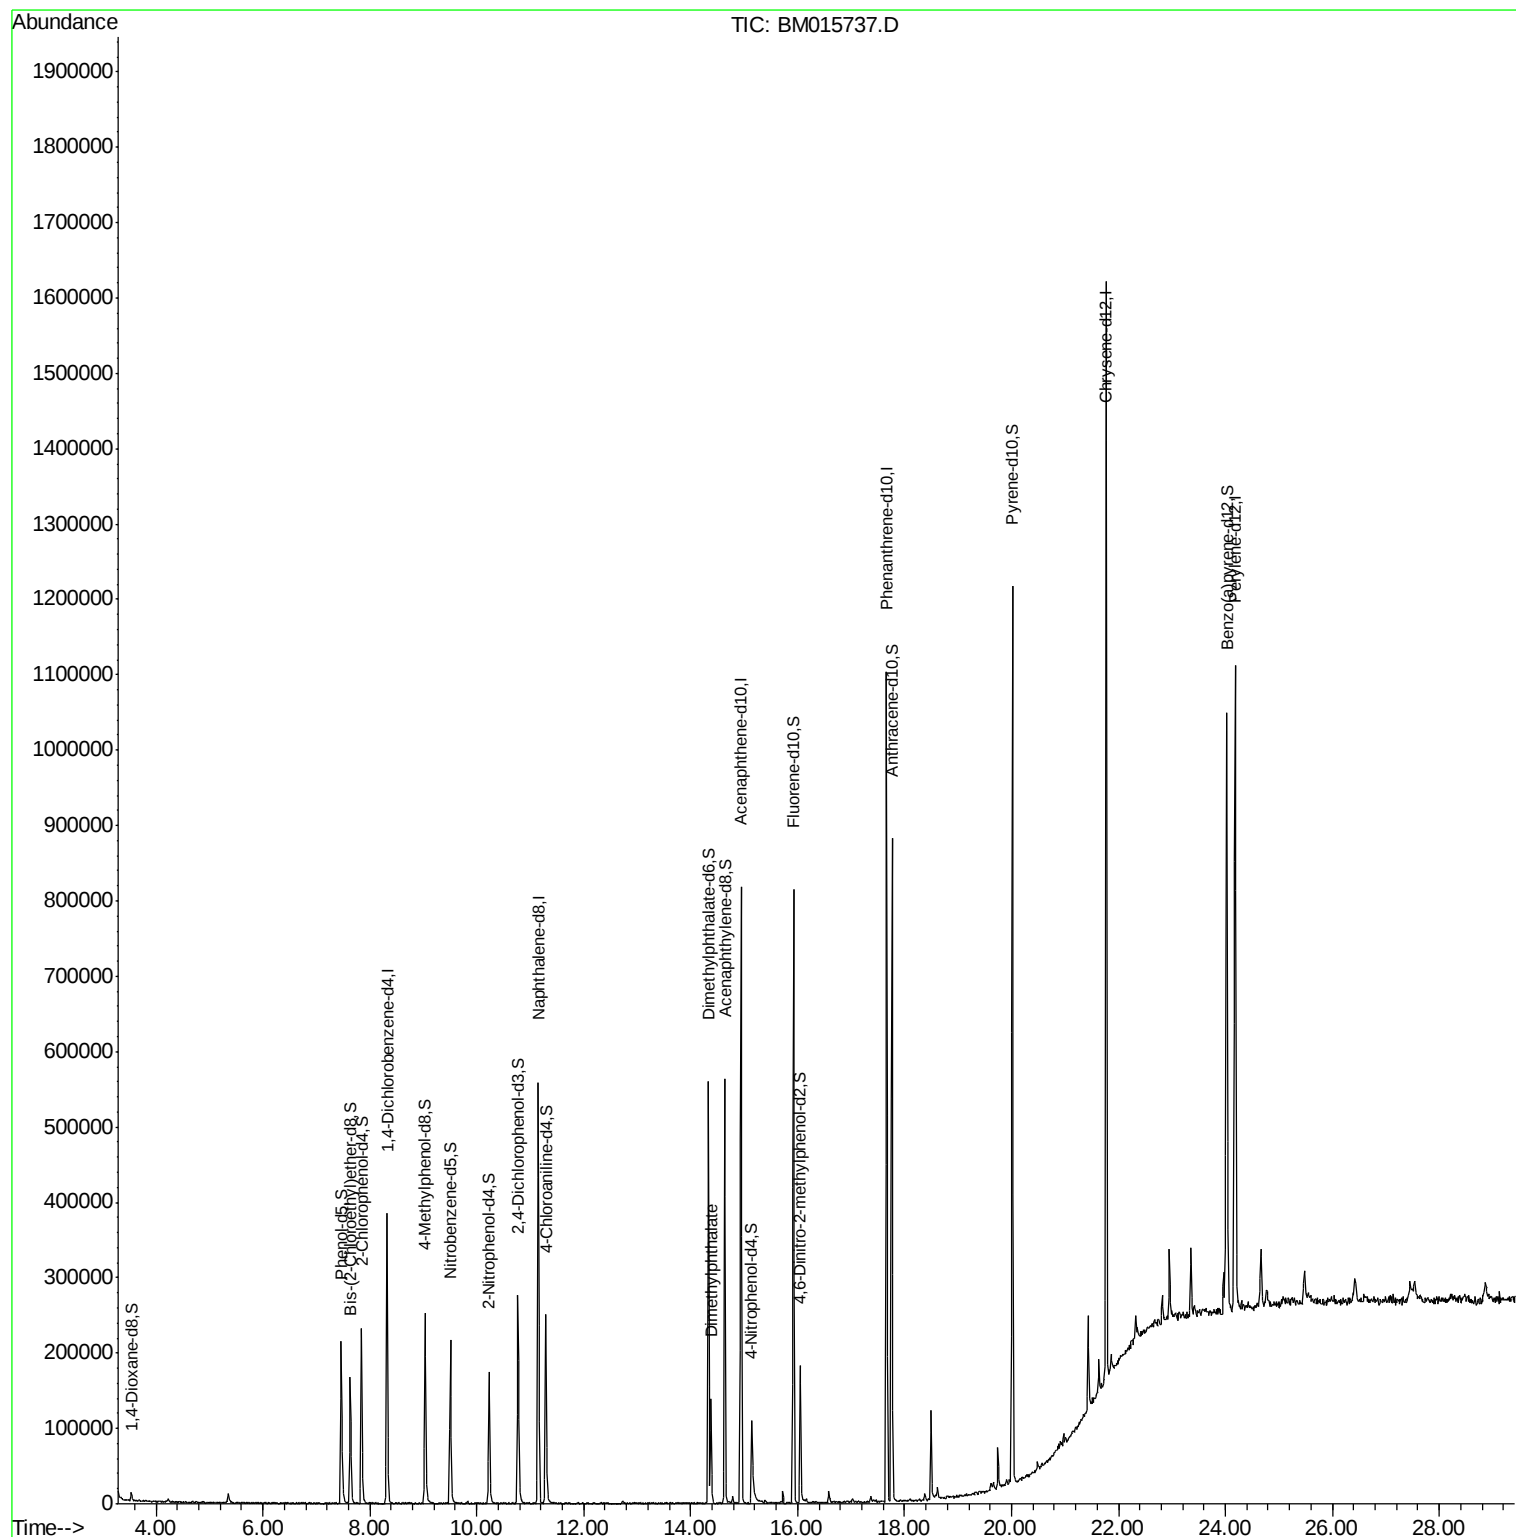

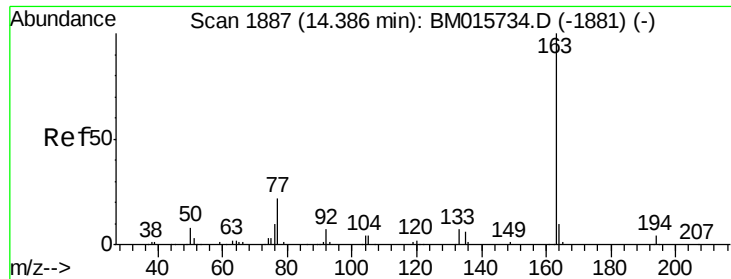

#44

Dimethylphthalate

Concen: 3.829 ng/ul

RT: 14.39 min Scan# 1887

Delta R.T. 0.00 min

Lab File: BM015737.D

Acq: 21 Jun 2018 20:34

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 80094

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8

164 10.5 7.8 11.8

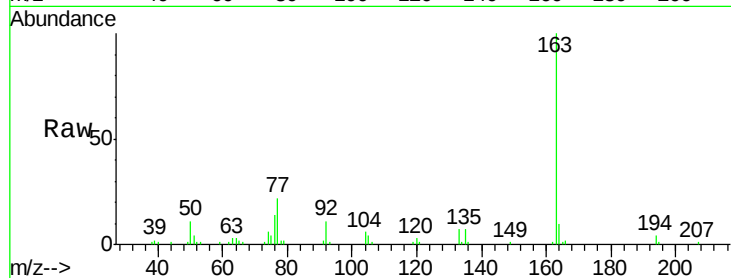

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

