

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
 Data File : BM015738.D
 Acq On : 21 Jun 2018 21:11
 Operator : SJ/JU
 Sample : J3568-03RX
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 22 02:13:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 22 02:12:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.32	152	105312	20.00	ng/ul	0.00
18) Naphthalene-d8	11.15	136	452587	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.94	164	257986	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	580388	20.00	ng/ul	0.00
77) Chrysene-d12	21.77	240	620156	20.00	ng/ul	0.00
85) Perylene-d12	24.18	264	592162	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	10446	4.82	ng/uL	0.00
5) Phenol-d5	7.46	99	211802	22.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.63	67	141433	24.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.85	132	191200	26.16	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	170276	20.67	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	82742	27.19	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	89783	27.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	176800	26.09	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	229568	30.40	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	563411	26.38	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	658123	28.57	ng/ul	0.00
51) 4-Nitrophenol-d4	15.14	143	62176	15.08	ng/ul	0.00
57) Fluorene-d10	15.92	176	481173	26.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	61631	17.63	ng/ul	0.00
70) Anthracene-d10	17.76	188	744958	28.16	ng/ul	0.00
78) Pyrene-d10	20.02	212	835710	31.33	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.03	264	838526	28.25	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	14.39	163	141034	6.467	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062118\
Data File : BM015738.D
Acq On : 21 Jun 2018 21:11
Operator : SJ/JU
Sample : J3568-03RX
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 22 02:13:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM060818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 22 02:12:20 2018
Response via : Initial Calibration

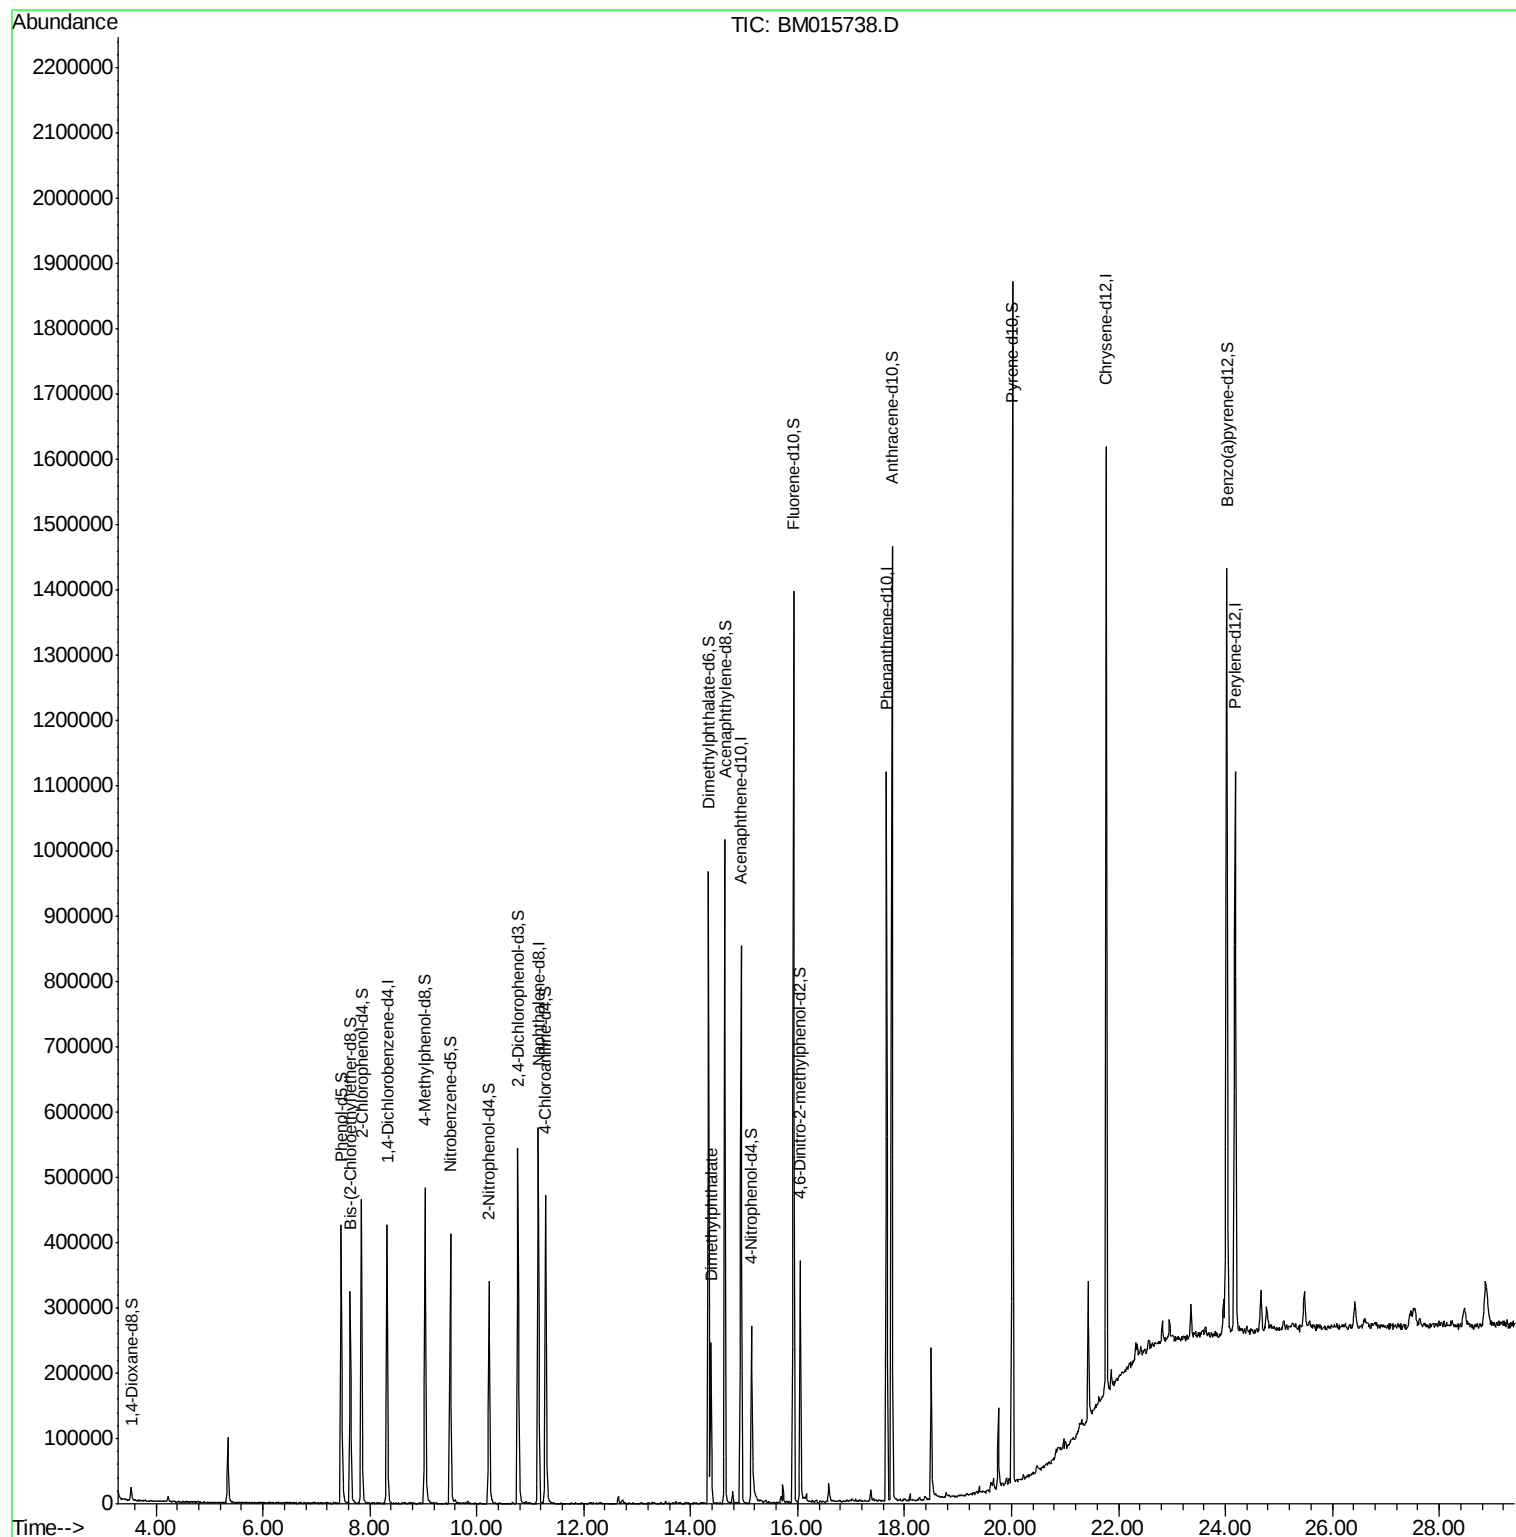

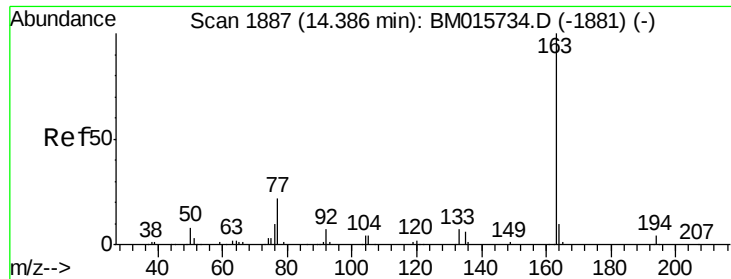

#44

Dimethylphthalate

Concen: 6.467 ng/ul

RT: 14.39 min Scan# 1887

Delta R.T. 0.00 min

Lab File: BM015738.D

Acq: 21 Jun 2018 21:11

Instrument :

BNA_M

ClientSampleId :



Tot Ion:163 Resp: 141034

Ion Ratio Lower Upper

163 100

194 3.5 3.2 4.8

164 9.1 7.8 11.8

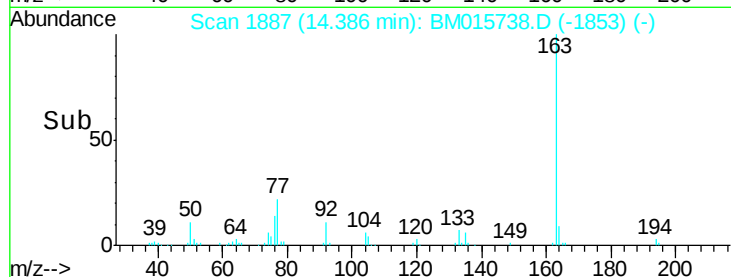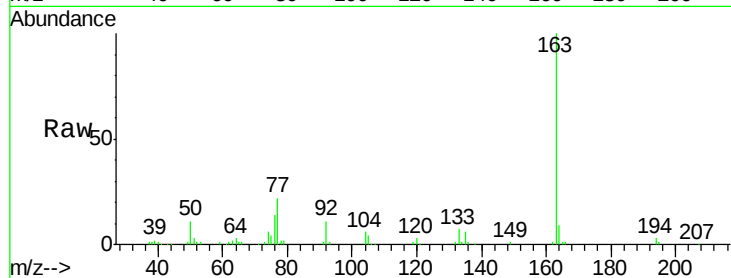

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

