

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062119\
 Data File : BM021075.D
 Acq On : 21 Jun 2019 08:41
 Operator : HP/JU
 Sample : PB120290BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120290BL

Quant Time: Jun 21 23:27:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 20 15:39:58 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	259920	20.00	ng	0.00
21) Naphthalene-d8	10.57	136	1001450	20.00	ng	0.00
39) Acenaphthene-d10	14.42	164	633689	20.00	ng	0.00
64) Phenanthrene-d10	17.17	188	1545011	20.00	ng	0.00
76) Chrysene-d12	21.35	240	1245466	20.00	ng	0.00
87) Perylene-d12	23.62	264	1241080	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	1465339	102.08	ng	0.00
7) Phenol-d6	6.95	99	2020038	96.63	ng	0.00
23) Nitrobenzene-d5	8.94	82	1198893	62.39	ng	0.00
42) 2,4,6-Tribromophenol	15.91	330	1103264	92.78	ng	0.00
45) 2-Fluorobiphenyl	13.03	172	3383209	65.62	ng	0.00
79) Terphenyl-d14	19.79	244	5223555	78.33	ng	0.00
Target Compounds						
9) Benzaldehyde	6.95	77	4055	Below Cal	Qvalue #	2


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062119\
Data File : BM021075.D
Acq On : 21 Jun 2019 08:41
Operator : HP/JU
Sample : PB120290BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120290BL

Quant Time: Jun 21 23:27:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 20 15:39:58 2019
Response via : Initial Calibration

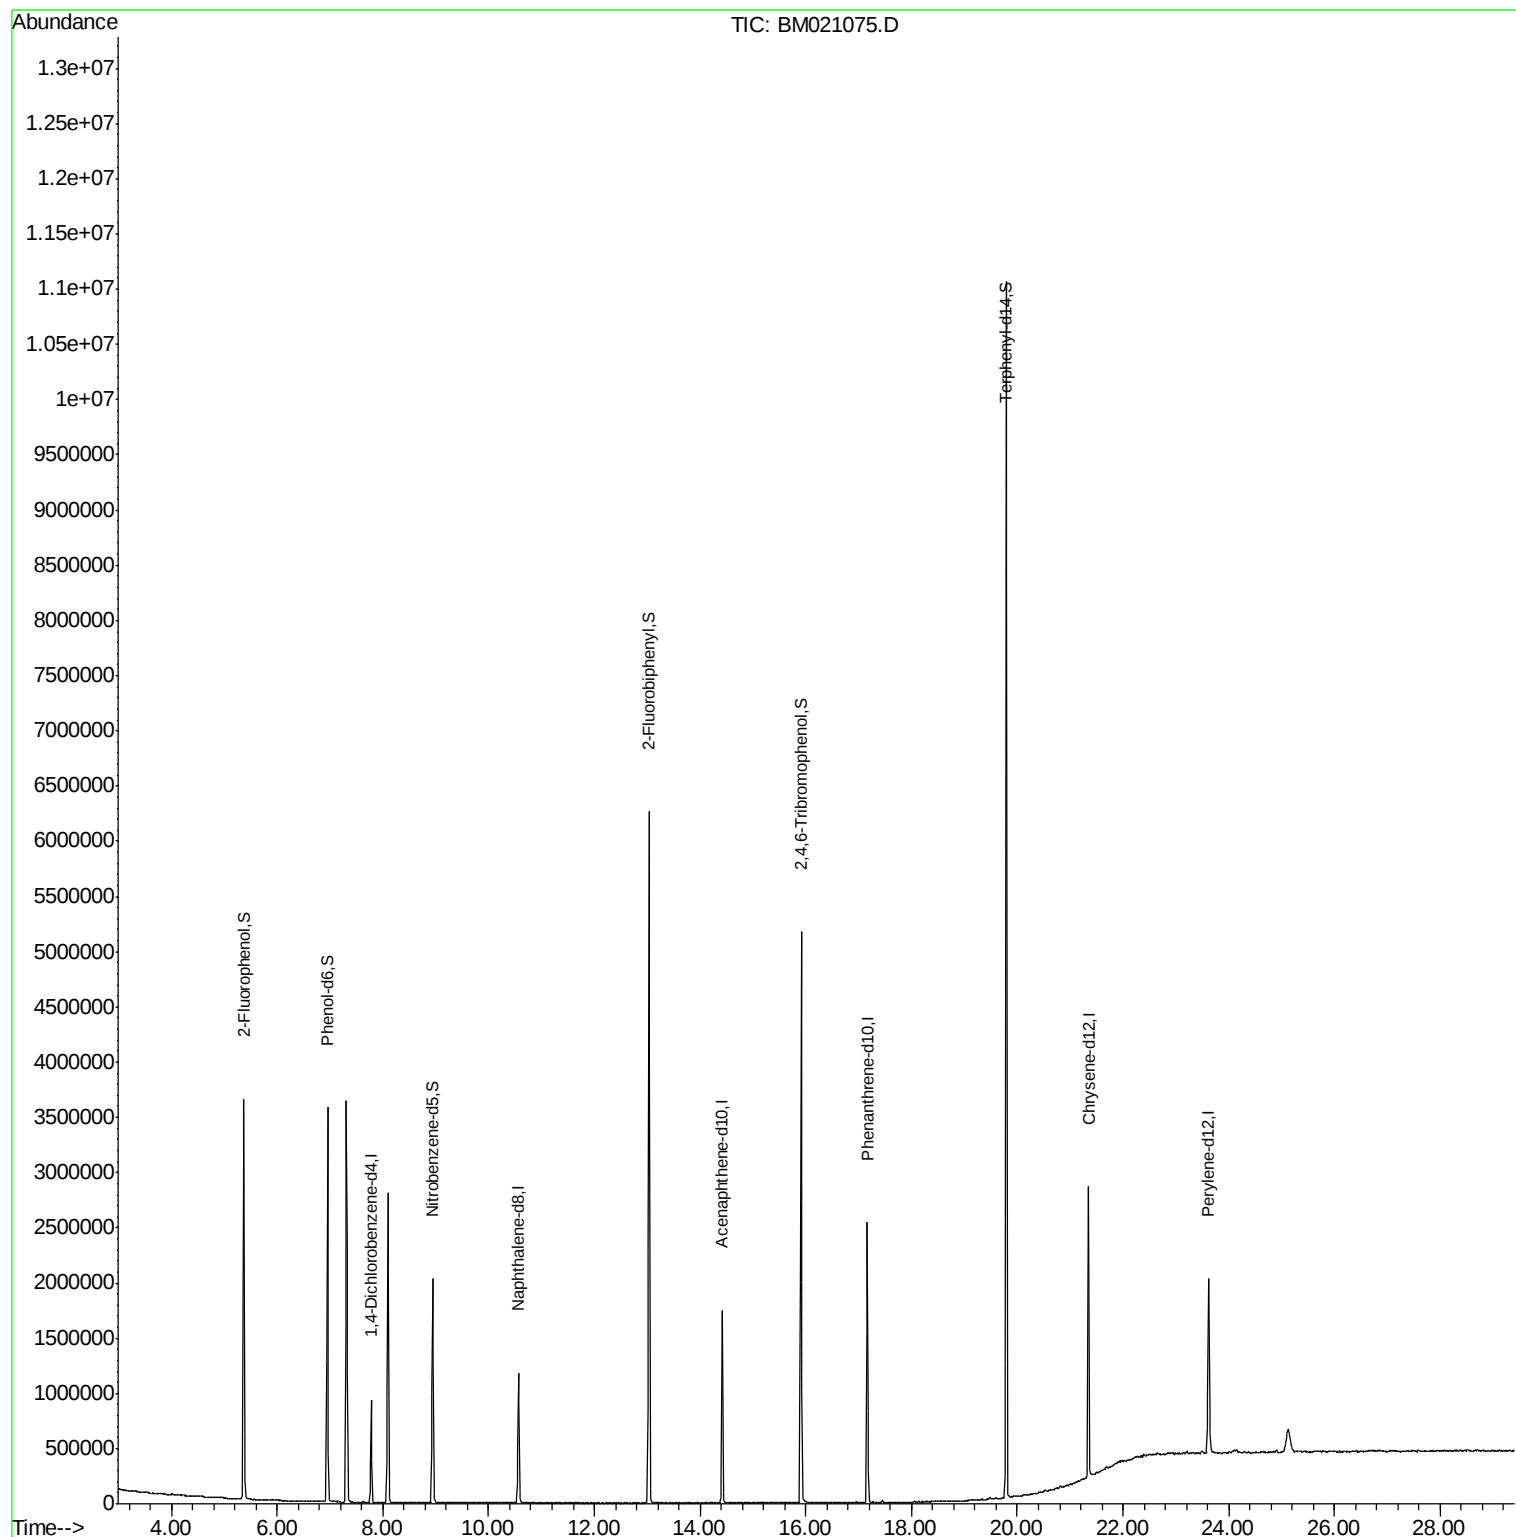

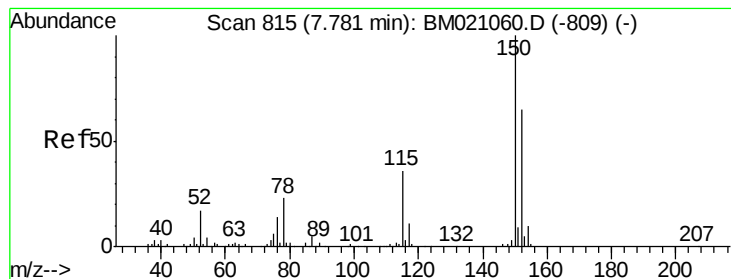


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.78 min Scan# 815
Delta R.T. -0.00 min
Lab File: BM021075.D
Acq: 21 Jun 2019 08:41

Instrument :
BNA_M
ClientSampleId :
PB120290BL

Tgt Ion	Ratio	Lower	Upper
152	100		
150	157.1	123.1	184.7
115	56.0	44.2	66.4



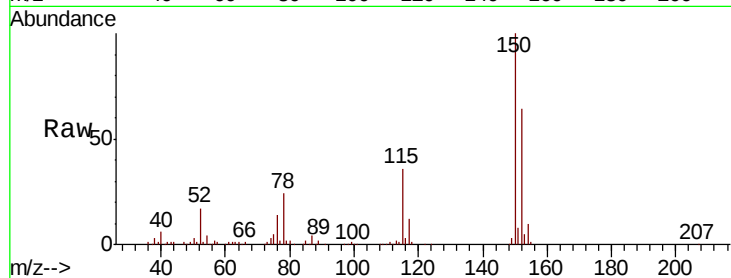


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

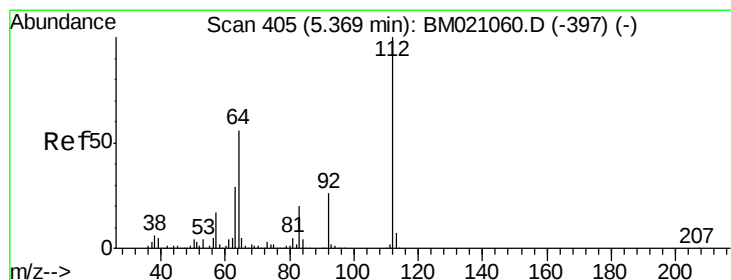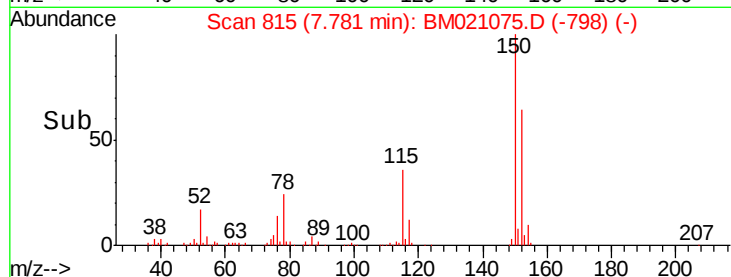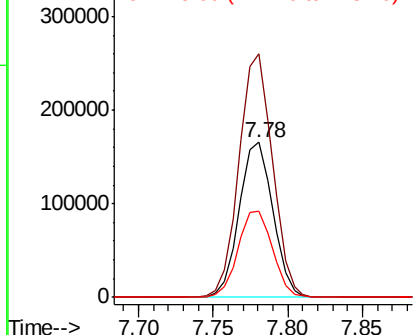

#5

2-Fluorophenol
Concen: 102.083 ng
RT: 5.37 min Scan# 405
Delta R.T. -0.00 min
Lab File: BM021075.D
Acq: 21 Jun 2019 08:41

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.7	45.2	67.8
63	30.0	23.5	35.3


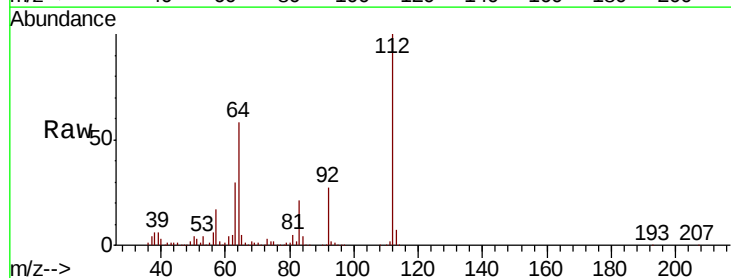



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

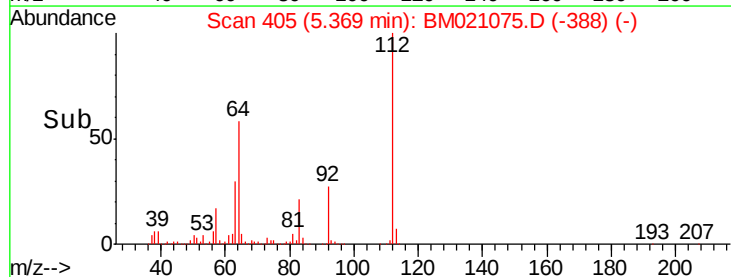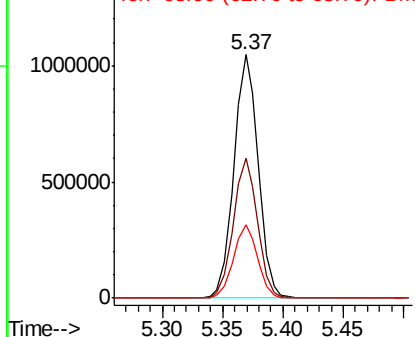

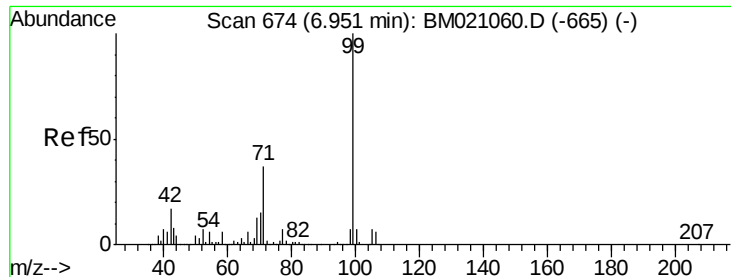

#7

Phenol-d6

Concen: 96.635 ng

RT: 6.95 min Scan# 674

Delta R.T. -0.00 min

Lab File: BM021075.D

Acq: 21 Jun 2019 08:41

Instrument :

BNA_M

ClientSampleId :

PB120290BL


Tgt Ion: 99 Resp: 2020038

Ion Ratio Lower Upper

99 100

42 16.8 13.5 20.3




71 35.9 29.3 43.9

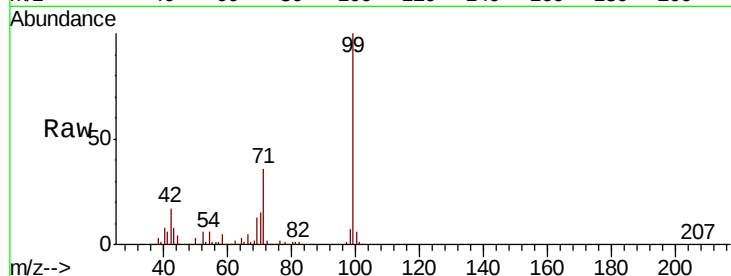

Abundance Ion 99.00 (98.70 to 99.70): BM021060.D (-665) (-)

Ion 42.00 (41.70 to 42.70): BM021060.D (-665) (-)

Ion 71.00 (70.70 to 71.70): BM021060.D (-665) (-)

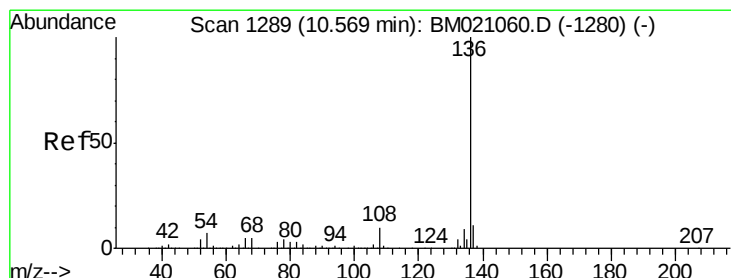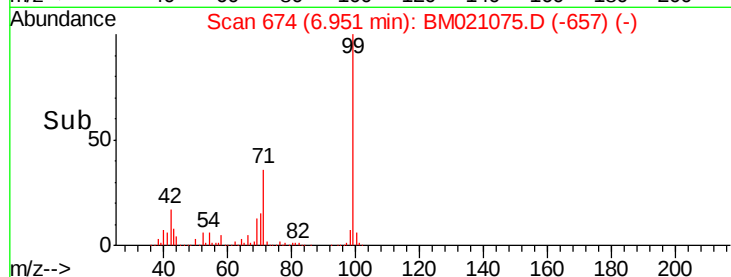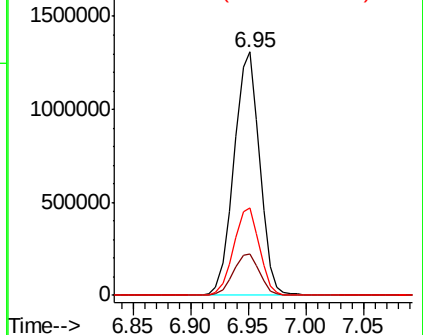

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.57 min Scan# 1289

Delta R.T. -0.00 min

Lab File: BM021075.D

Acq: 21 Jun 2019 08:41

Tgt Ion: 136 Resp: 1001450


Ion Ratio Lower Upper

136 100

137 10.4 8.6 13.0

54 6.7 5.3 7.9

68 5.1 4.4 6.6


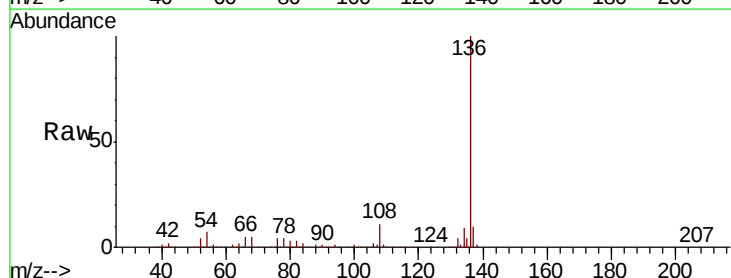



Abundance Ion 136.00 (135.70 to 136.70): BM021060.D (-1280) (-)

Ion 137.00 (136.70 to 137.70): BM021060.D (-1280) (-)

Ion 54.00 (53.70 to 54.70): BM021060.D (-1280) (-)

Ion 68.00 (67.70 to 68.70): BM021060.D (-1280) (-)

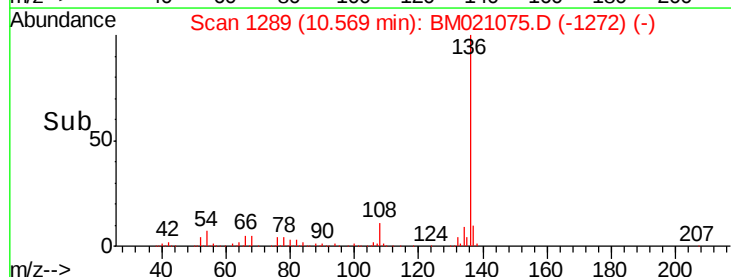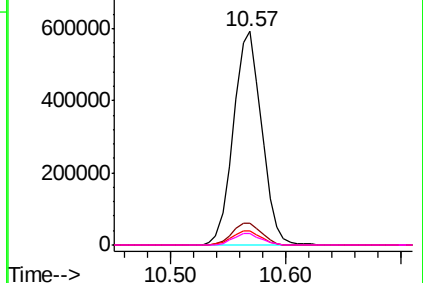




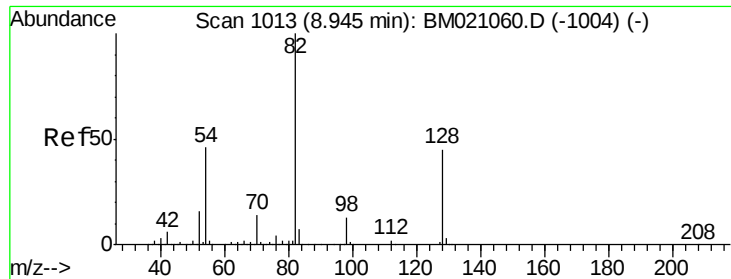


#23
 Nitrobenzene-d5
 Concen: 62.392 ng
 RT: 8.94 min Scan# 1012
 Delta R.T. -0.01 min
 Lab File: BM021075.D
 Acq: 21 Jun 2019 08:41

Instrument :
 BNA_M
 ClientSampleId :
 PB120290BL

Tgt Ion: 82 Resp: 1198893




Ion	Ratio	Lower	Upper
82	100		
128	43.7	35.9	53.9
54	45.6	36.6	55.0

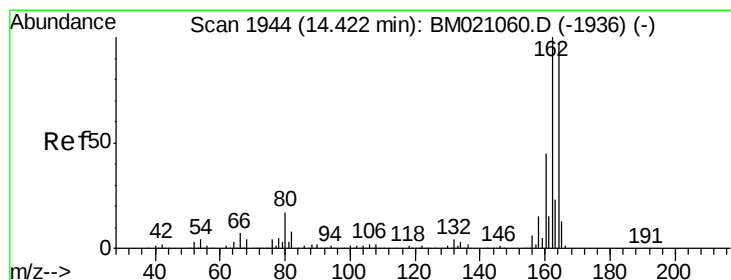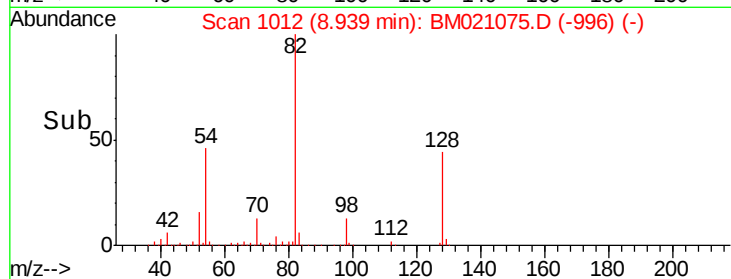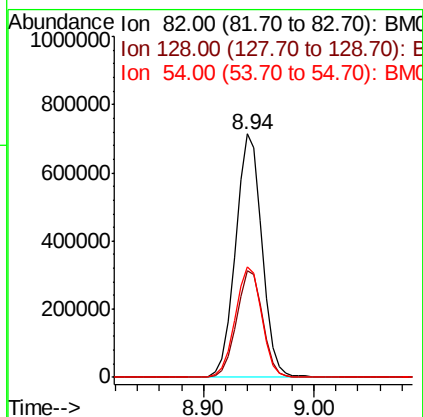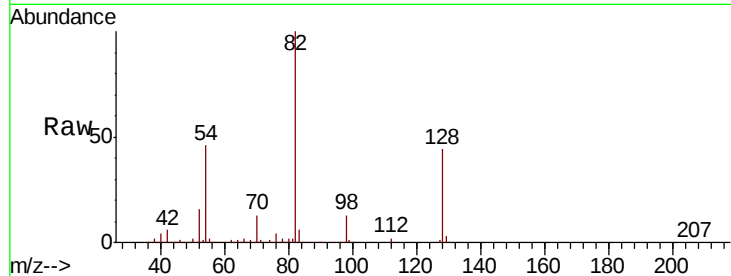


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.42 min Scan# 1943
 Delta R.T. -0.01 min
 Lab File: BM021075.D
 Acq: 21 Jun 2019 08:41

Tgt Ion: 164 Resp: 633689

Ion	Ratio	Lower	Upper
164	100		
162	104.9	82.1	123.1
160	47.0	37.1	55.7

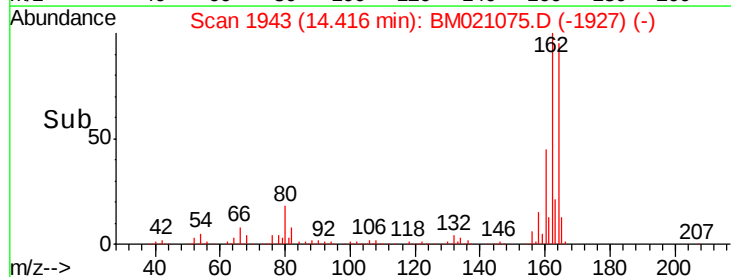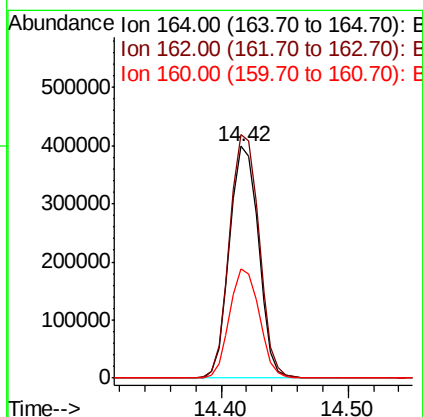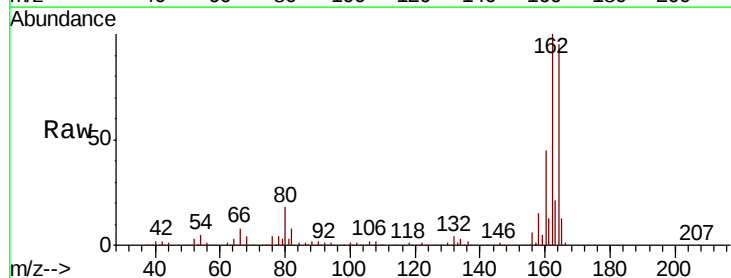


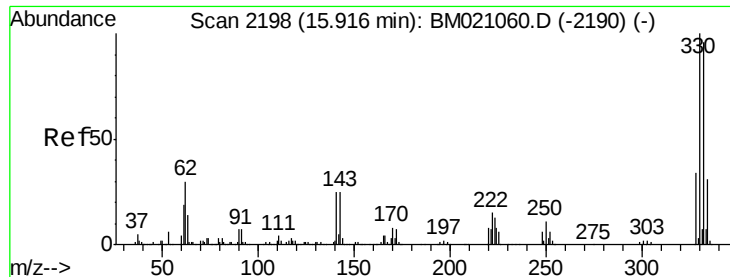




#42
 2,4,6-Tribromophenol
 Concen: 92.783 ng
 RT: 15.91 min Scan# 2197
 Delta R.T. -0.01 min
 Lab File: BM021075.D
 Acq: 21 Jun 2019 08:41

Instrument :
 BNA_M
 ClientSampleId :
 PB120290BL

Tgt Ion:330 Resp: 1103264
 Ion Ratio Lower Upper
 330 100
 332 96.5 77.1 115.7
 141 27.4 21.8 32.8

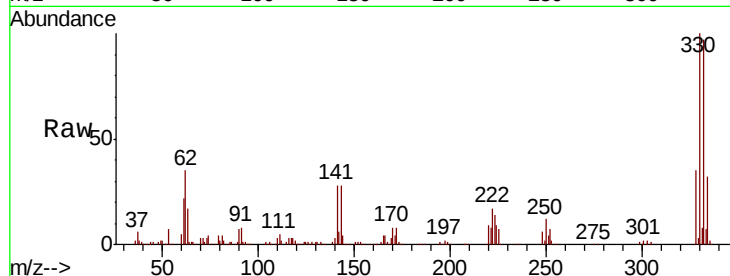


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

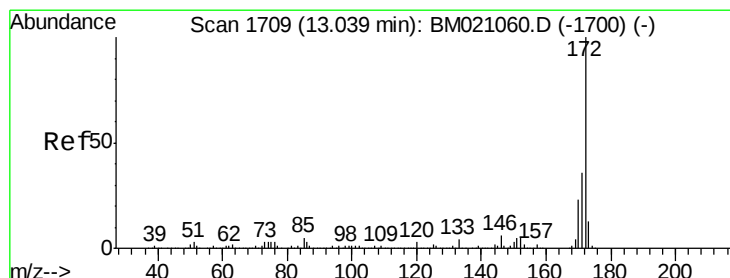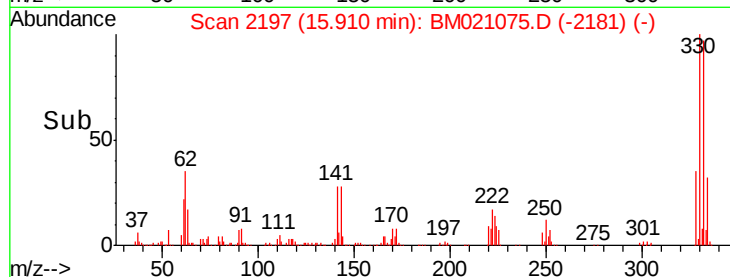
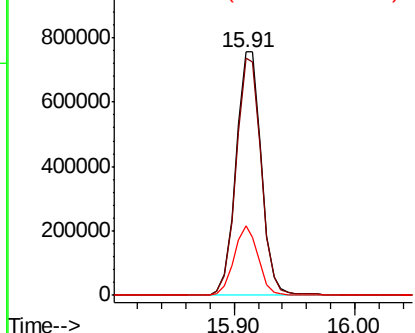



#45
 2-Fluorobiphenyl
 Concen: 65.615 ng
 RT: 13.03 min Scan# 1708
 Delta R.T. -0.01 min
 Lab File: BM021075.D
 Acq: 21 Jun 2019 08:41

Tgt Ion:172 Resp: 3383209
 Ion Ratio Lower Upper
 172 100
 171 35.5 28.6 43.0
 170 23.4 18.7 28.1

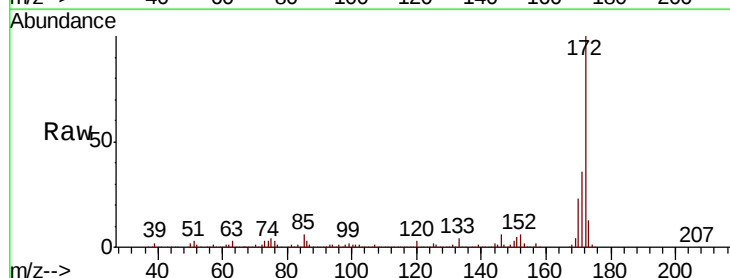

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

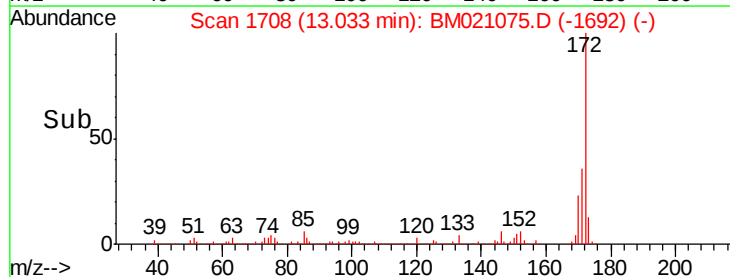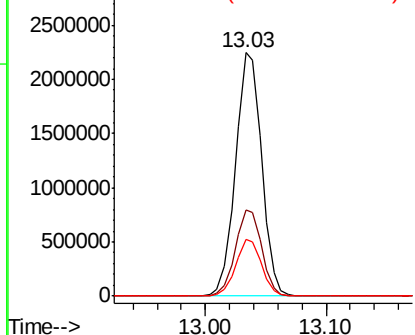


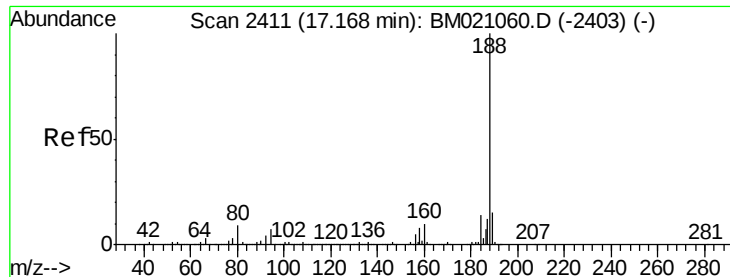




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.17 min Scan# 2411
Delta R.T. -0.00 min
Lab File: BM021075.D
Acq: 21 Jun 2019 08:41

Instrument :
BNA_M
ClientSampleId :
PB120290BL

Tgt Ion:188 Resp: 1545011
Ion Ratio Lower Upper
188 100
94 7.3 5.8 8.8
80 8.1 6.9 10.3

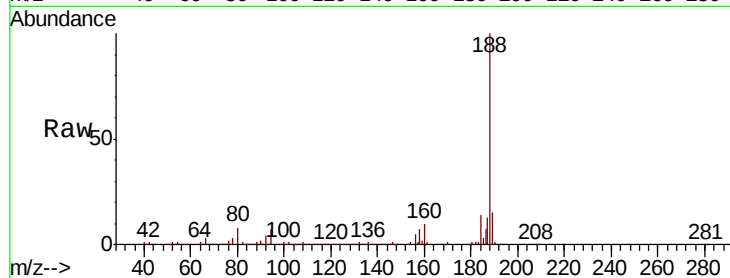


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

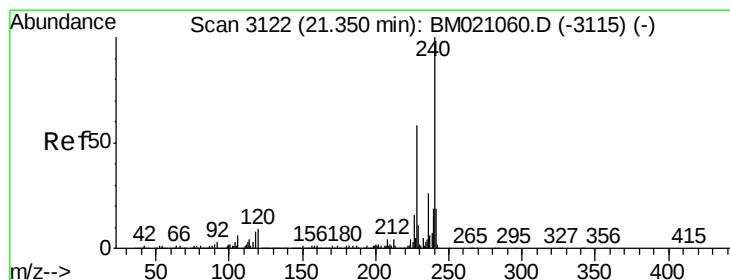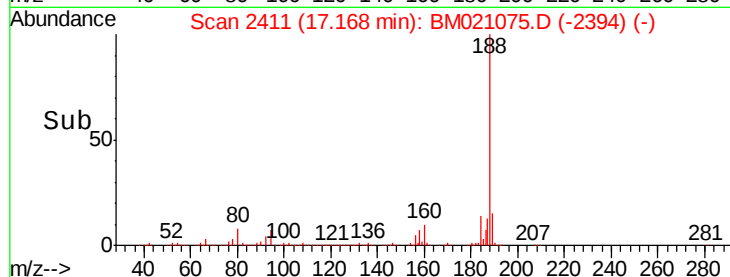
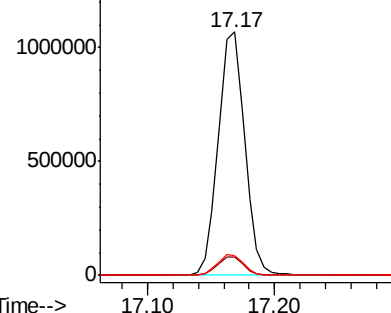



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.35 min Scan# 3122
Delta R.T. -0.00 min
Lab File: BM021075.D
Acq: 21 Jun 2019 08:41

Tgt Ion:240 Resp: 1245466
Ion Ratio Lower Upper
240 100
120 8.0 6.9 10.3
236 25.9 20.4 30.6

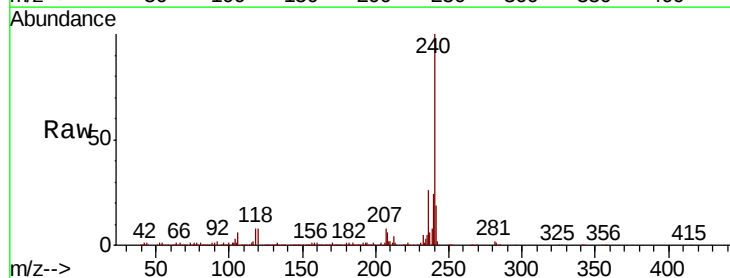

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

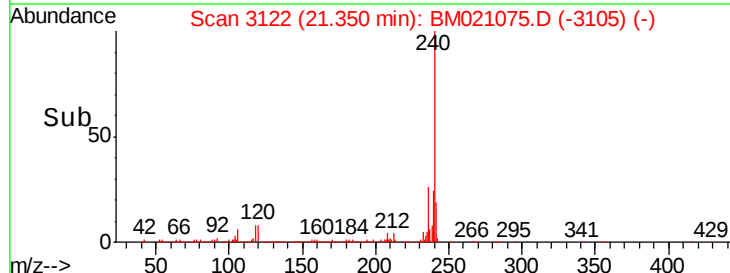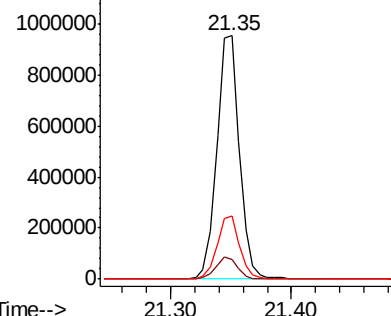

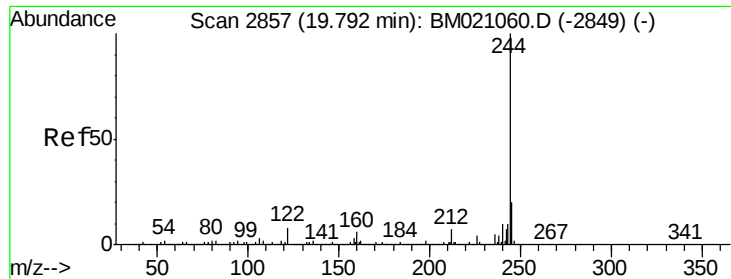

#79

Terphenyl-d14

Concen: 78.333 ng

RT: 19.79 min Scan# 2857

Delta R.T. -0.00 min

Lab File: BM021075.D

Acq: 21 Jun 2019 08:41

Instrument :

BNA_M

ClientSampleId :

PB120290BL


Tgt Ion:244 Resp: 5223555

Ion Ratio Lower Upper

244 100

212 6.6 5.3 7.9

122 8.0 6.6 9.8



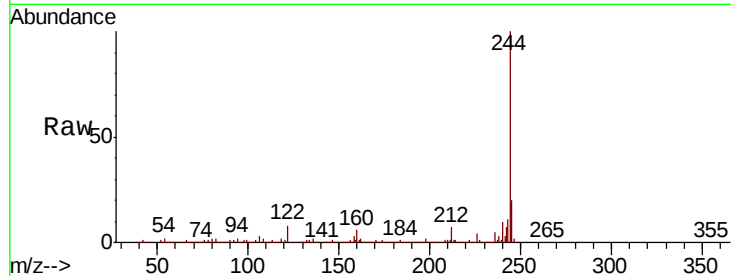


Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

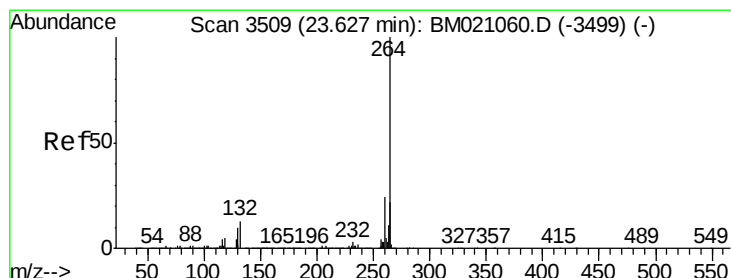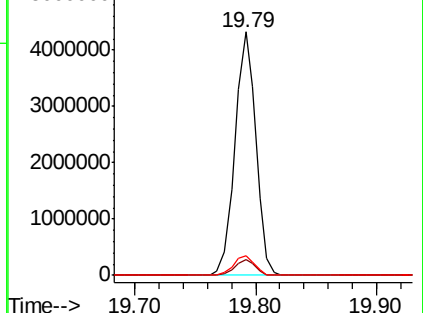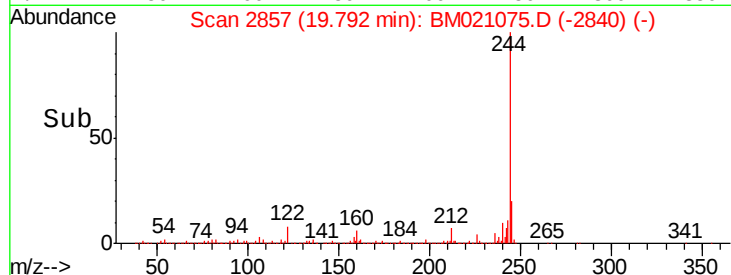

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.62 min Scan# 3508

Delta R.T. -0.01 min

Lab File: BM021075.D

Acq: 21 Jun 2019 08:41


Tgt Ion:264 Resp: 1241080

Ion Ratio Lower Upper

264 100

260 23.2 19.0 28.4

265 21.6 17.7 26.5

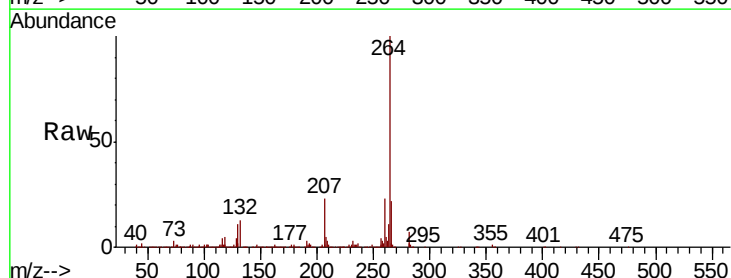

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

