

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062119\
 Data File : BM021075.D
 Acq On : 21 Jun 2019 08:41
 Operator : HP/JU
 Sample : PB120290BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120290BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	399	405	418	rVB	3622934	5051755	37.78%	7.090%
2	6.951	666	674	686	rBV	3572082	5598018	41.86%	7.856%
3	7.310	728	735	746	rBV	3630239	5798557	43.36%	8.138%
4	7.781	808	815	823	rVB	931685	1490353	11.15%	2.092%
5	8.098	861	869	877	rBV	2800796	4494512	33.61%	6.308%
6	8.939	1004	1012	1026	rBV	2028127	3429938	25.65%	4.814%
7	10.569	1281	1289	1299	rBV	1178268	1990763	14.89%	2.794%
8	13.033	1701	1708	1727	rBV	6259159	9383459	70.17%	13.169%
9	14.416	1937	1943	1953	rBV2	1749127	2909837	21.76%	4.084%
10	15.910	2191	2197	2220	rBV	5173224	7426826	55.54%	10.423%
11	17.168	2404	2411	2425	rVB2	2534844	3692540	27.61%	5.182%
12	19.792	2851	2857	2863	rBV	11015868	13371956	100.00%	18.767%
13	21.350	3116	3122	3129	rBV	2630691	3485668	26.07%	4.892%
14	23.621	3502	3508	3520	rVB	1567814	3129203	23.40%	4.392%


Sum of corrected areas: 71253385

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062119\
Data File : BM021075.D
Acq On : 21 Jun 2019 08:41
Operator : HP/JU
Sample : PB120290BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120290BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

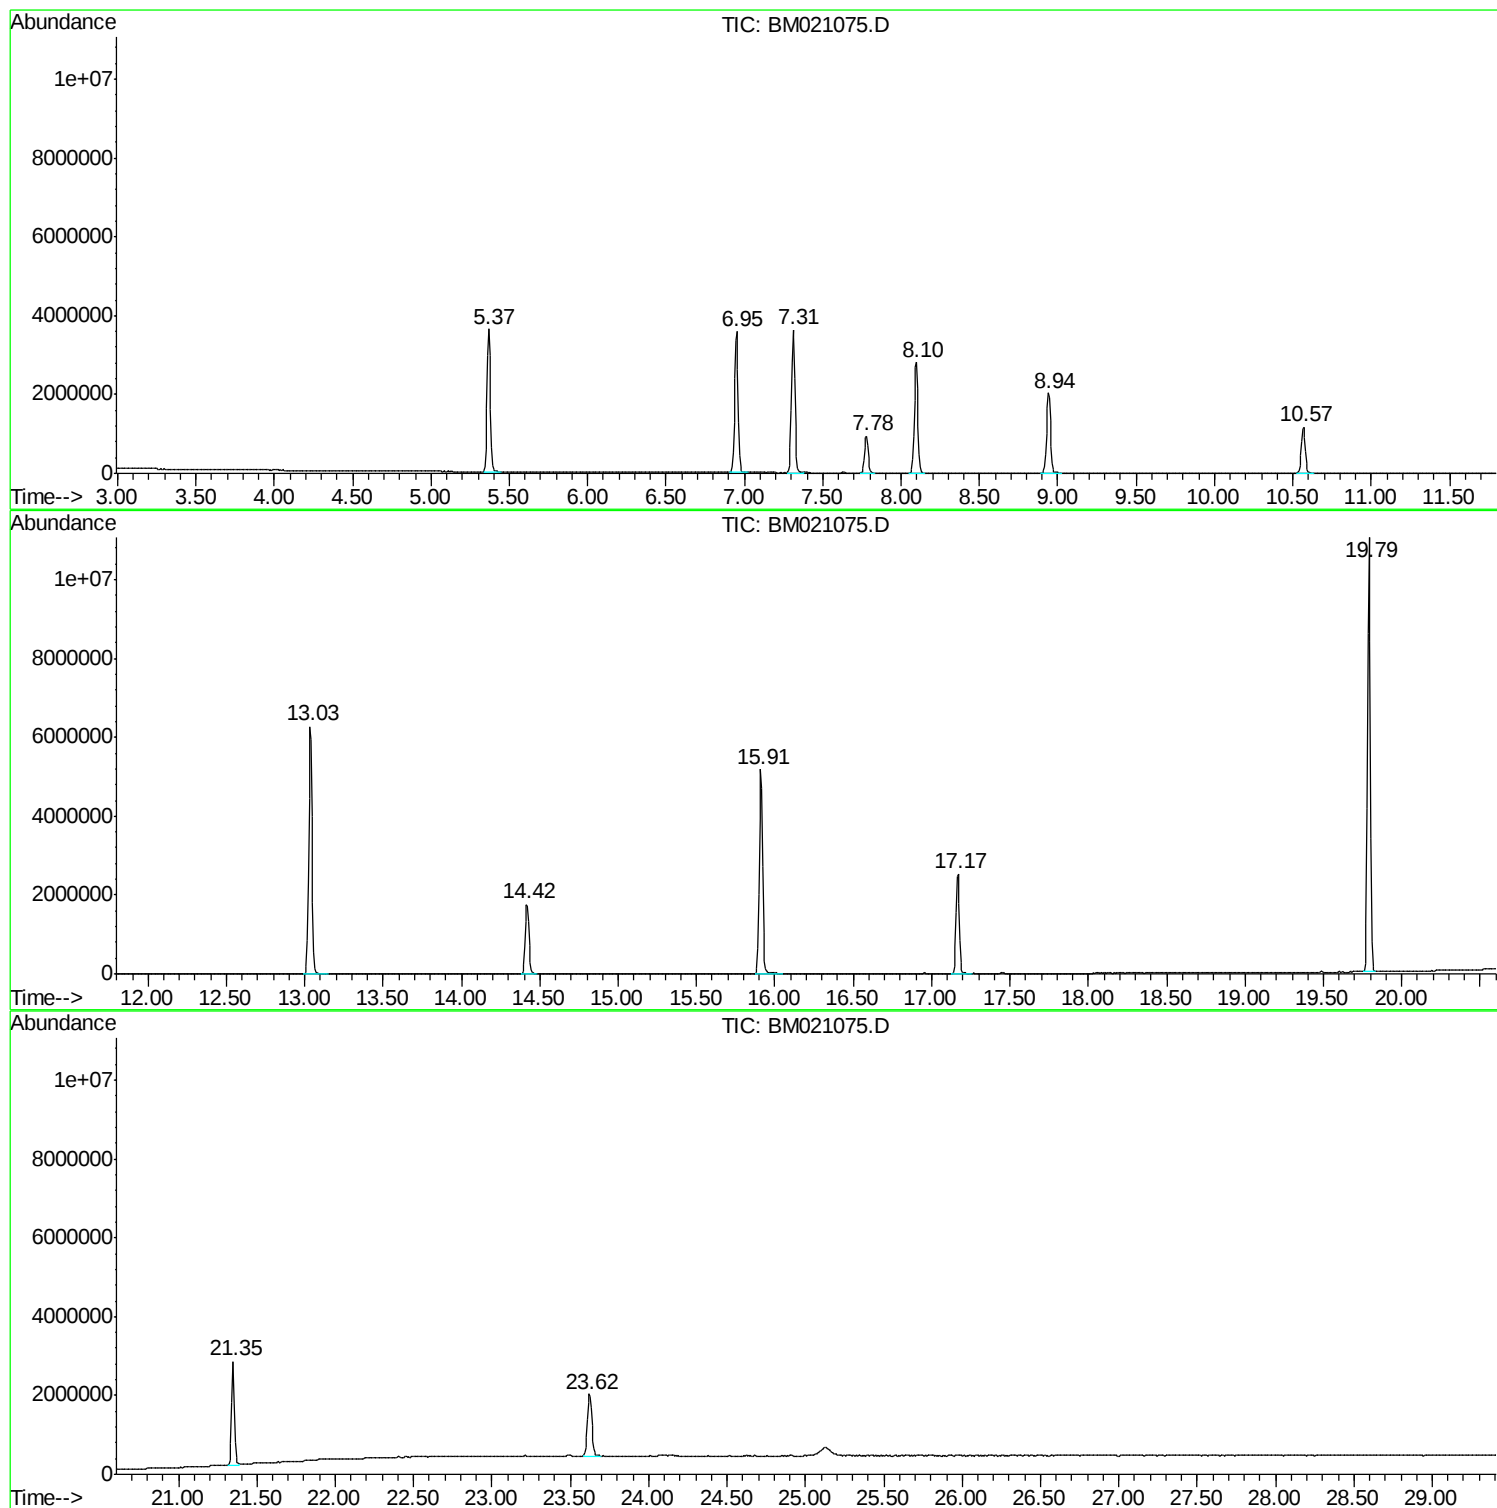

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062119\
Data File : BM021075.D
Acq On : 21 Jun 2019 08:41
Operator : HP/JU
Sample : PB120290BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120290BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.31	77.81 ng	5798560	1,4-Dichlorobenzene-d4	7.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
3		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

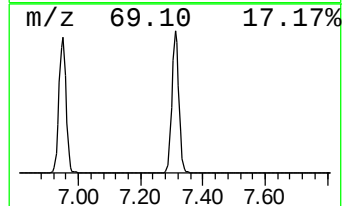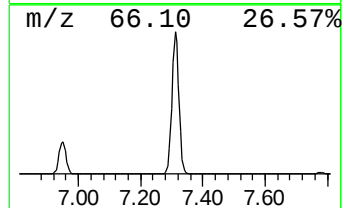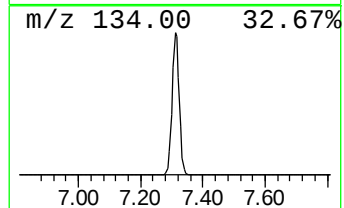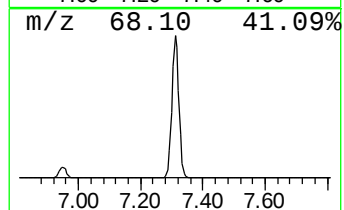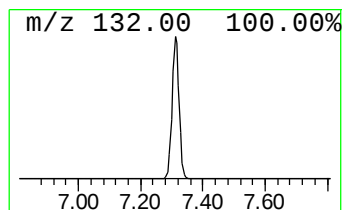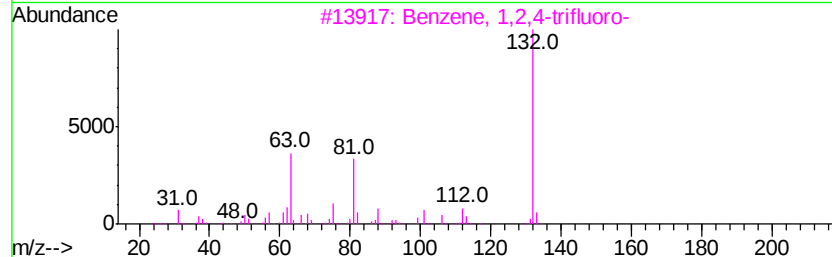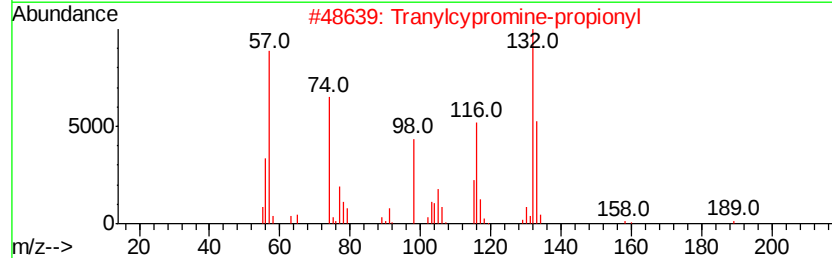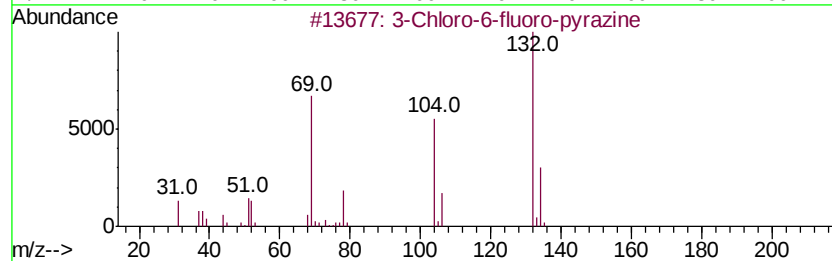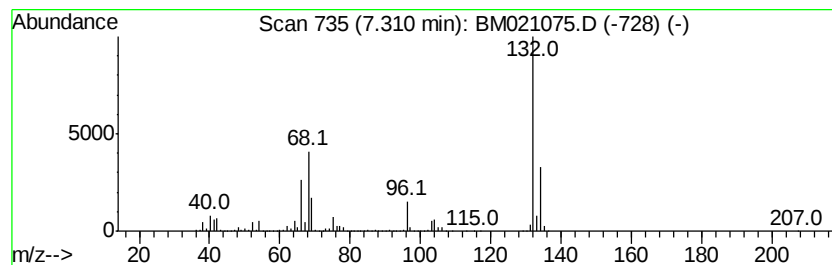

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062119\
Data File : BM021075.D
Acq On : 21 Jun 2019 08:41
Operator : HP/JU
Sample : PB120290BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120290BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.31	77.8	ng	5798560	1	7.78	1490350	20.0