

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062119\
 Data File : BM021084.D
 Acq On : 21 Jun 2019 15:34
 Operator : HP/JU
 Sample : K3309-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 LF017MW001-190610

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	3	6	20	rVB	1110412	1372191	6.52%	1.343%
2	4.452	242	249	263	rBV	6940079	10523209	50.01%	10.296%
3	5.369	399	405	420	rVB	1477296	2160990	10.27%	2.114%
4	6.946	666	673	687	rVB	1009919	1580390	7.51%	1.546%
5	7.310	728	735	744	rVB	3061011	4816159	22.89%	4.712%
6	7.775	807	814	822	rBV	886997	1417824	6.74%	1.387%
7	8.098	861	869	876	rBV	3334292	5541991	26.34%	5.422%
8	8.940	1004	1012	1021	rBV	2799010	4634275	22.02%	4.534%
9	9.028	1021	1027	1034	rVB	143000	251095	1.19%	0.246%
10	10.563	1277	1288	1296	rBV	1226501	2187650	10.40%	2.140%
11	11.857	1503	1508	1514	rVB	164660	262297	1.25%	0.257%
12	13.033	1697	1708	1717	rBV	8779013	13897810	66.05%	13.598%
13	14.416	1936	1943	1951	rVB2	2148047	3347696	15.91%	3.275%
14	15.163	2065	2070	2075	rBV	334814	439841	2.09%	0.430%
15	15.910	2190	2197	2209	rBV	6708728	10113217	48.06%	9.895%
16	16.445	2283	2288	2293	rBV	289510	397532	1.89%	0.389%
17	17.163	2404	2410	2418	rBV2	3148144	4571152	21.72%	4.472%
18	18.057	2557	2562	2571	rBV	178912	334981	1.59%	0.328%
19	18.139	2572	2576	2582	rVB	166512	246106	1.17%	0.241%
20	19.274	2765	2769	2776	rBV	1159151	1398357	6.65%	1.368%
21	19.792	2851	2857	2868	rBV	17365583	21041703	100.00%	20.587%
22	21.051	3068	3071	3077	rBV2	257449	302004	1.44%	0.295%
23	21.345	3116	3121	3128	rBV	4605470	5742236	27.29%	5.618%
24	23.621	3502	3508	3517	rVB2	2962177	5626284	26.74%	5.505%


Sum of corrected areas: 102206990

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062119\
Data File : BM021084.D
Acq On : 21 Jun 2019 15:34
Operator : HP/JU
Sample : K3309-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
LF017MW001-190610

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM062019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

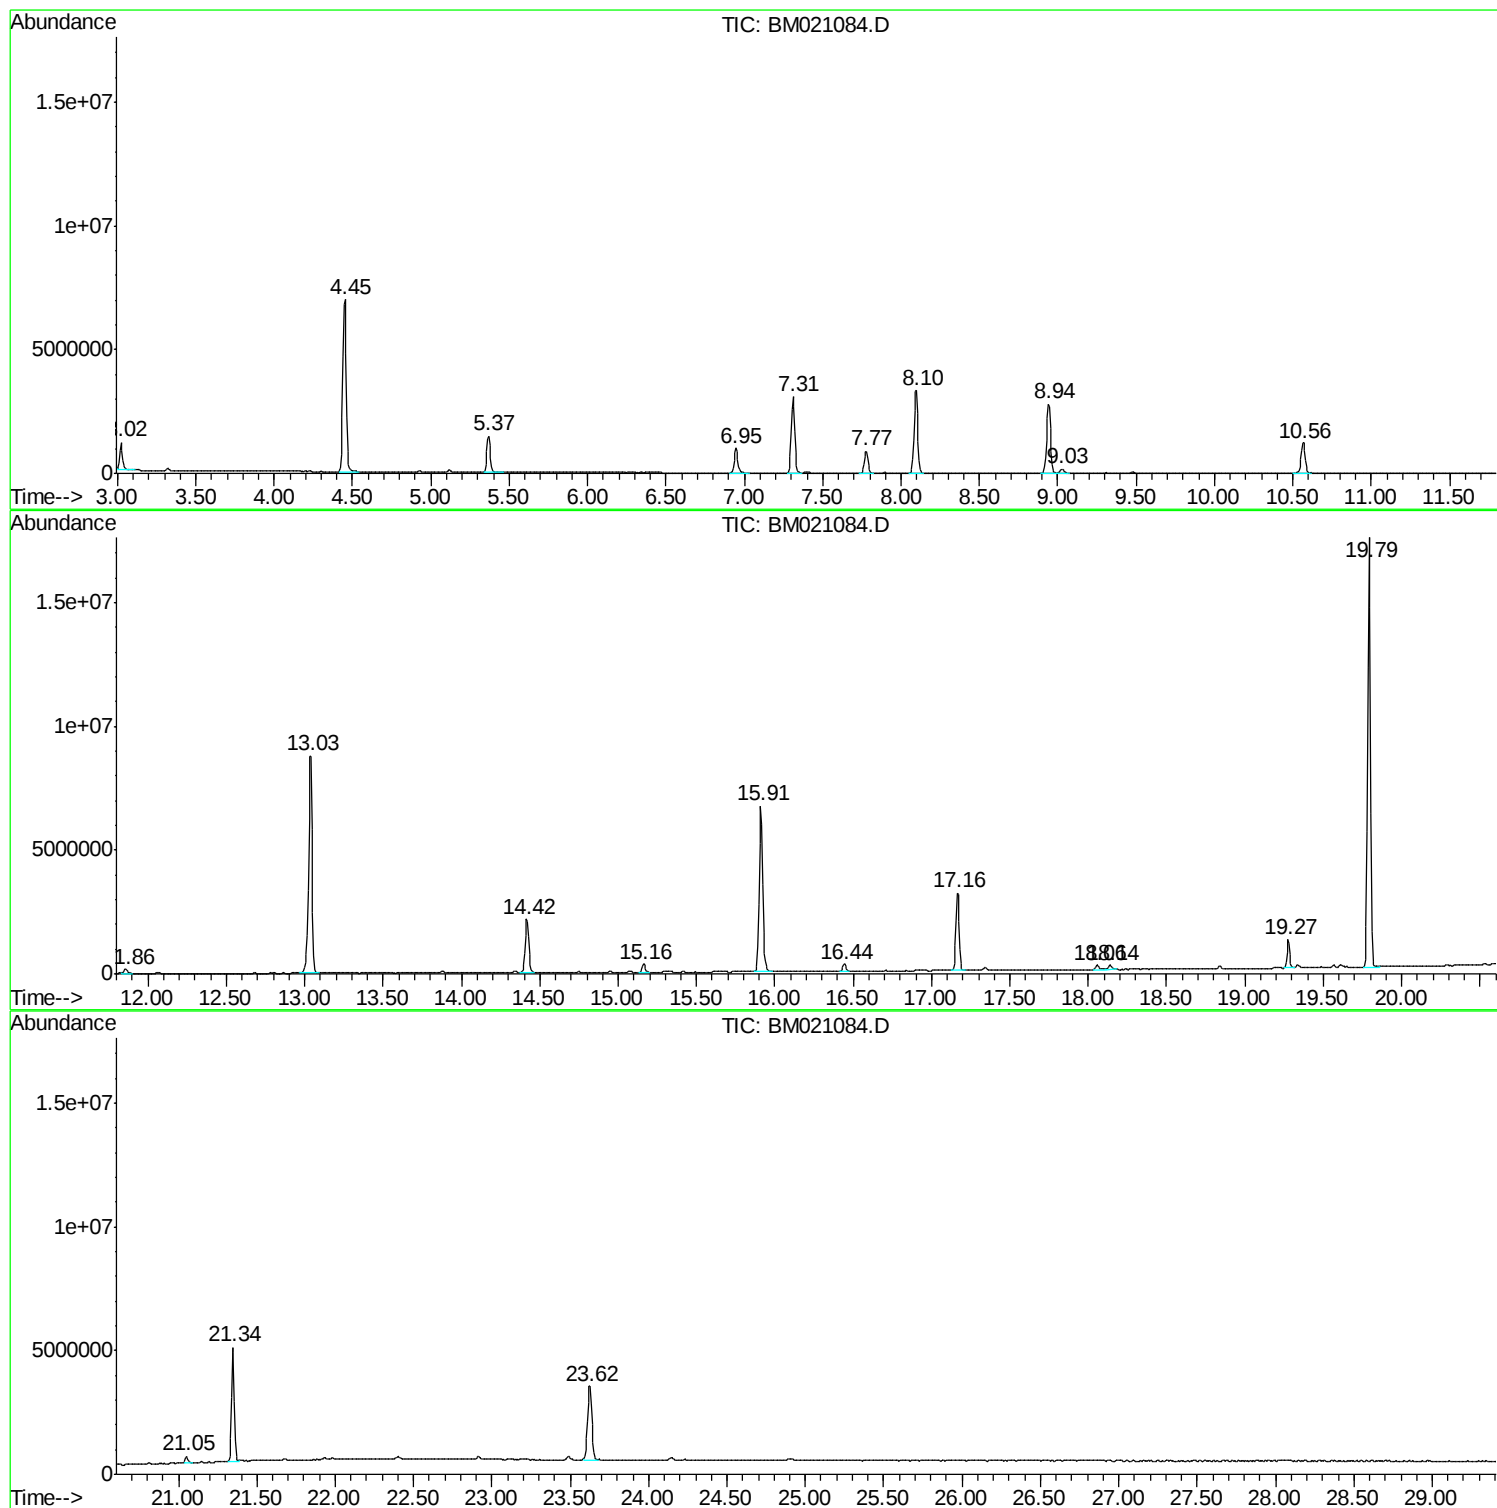

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062119\
Data_File : BM021084.D
Acq_On : 21-Jun-2019 15:344
Operator : HP/JUU
Sample : K3309-122
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
LF017MW001-190610

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
