


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062119\
 Data File : BM021073.D
 Acq On : 21 Jun 2019 07:29
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM062019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 20 15:39:58 2019

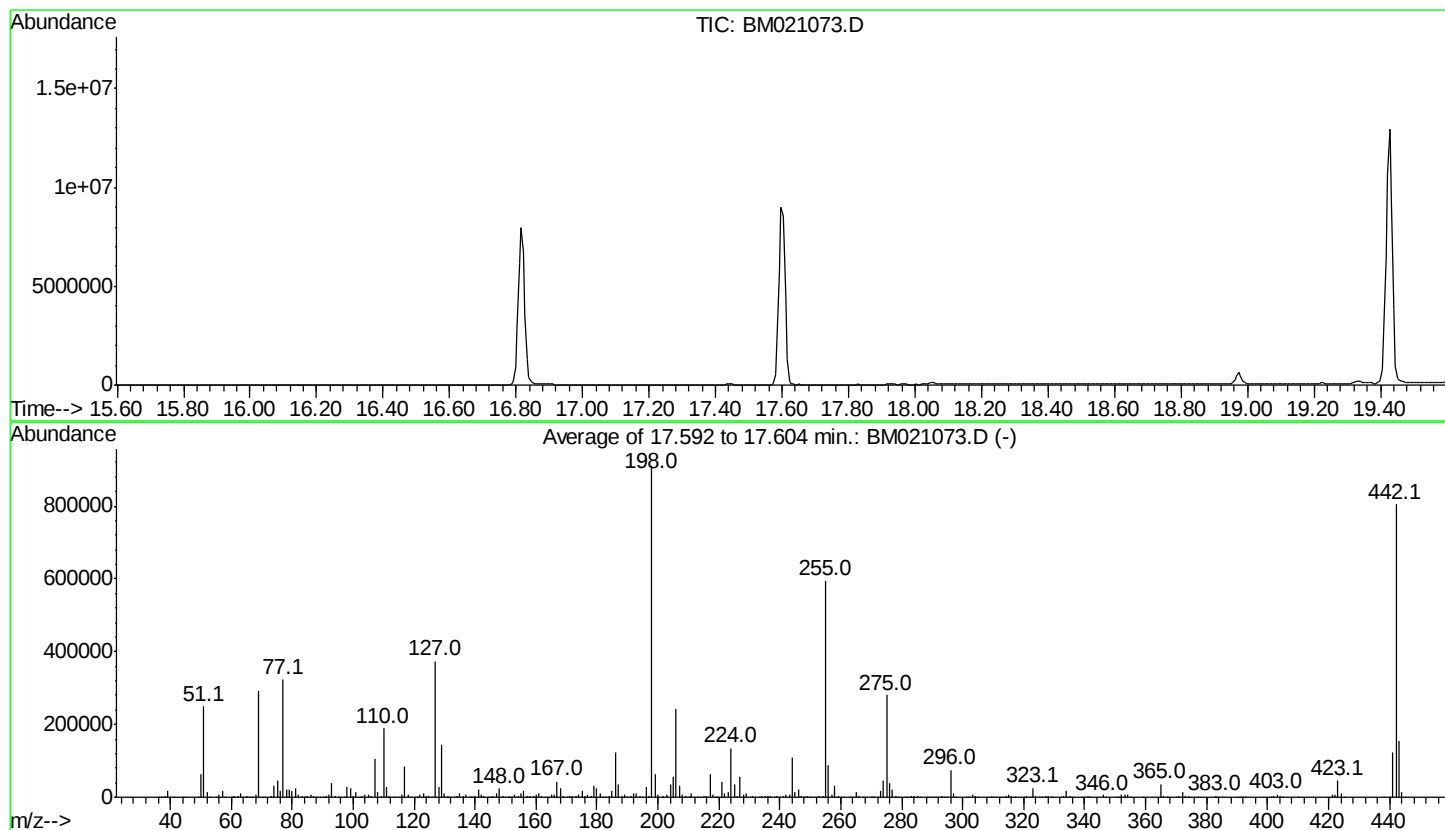

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	249301	PASS
68	69	0.00	2	1.9	5577	PASS
69	198	0.00	100	32.1	292717	PASS
70	69	0.00	2	0.5	1455	PASS
127	198	10	80	41.0	373226	PASS
197	198	0.00	2	0.4	4083	PASS
198	198	100	100	100.0	910848	PASS
199	198	5	9	6.9	63261	PASS
275	198	10	60	30.7	279680	PASS
365	198	1	100	3.9	35168	PASS
441	198	0.01	100	13.7	124552	PASS
442	198	50	100	88.3	804245	PASS
443	442	15	24	19.4	156072	PASS