

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062121\
 Data File : BM030507.D
 Acq On : 21 Jun 2021 16:42
 Operator : CG/JU
 Sample : M2697-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX82

Quant Time: Jun 21 17:12:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 21 10:48:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	180345	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	659955	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	381032	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	737620	20.000	ng/u1	0.00
79) Chrysene-d12	21.356	240	730527	20.000	ng/u1	0.00
88) Perylene-d12	23.638	264	764225	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	10215	2.163	ng/uL	0.00
4) Pyridine-d5	3.769	84	61035	4.918	ng/u1	0.02
7) Phenol-d5	6.992	99	207956	13.267	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.157	67	138702	13.711	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	174547	15.398	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	129858	10.373	ng/u1	0.00
21) Nitrobenzene-d5	8.975	128	76304	16.891	ng/u1	0.00
24) 2-Nitrophenol-d4	9.692	143	79684	17.760	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.233	165	150390	15.388	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	139226	9.319	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	430789	16.475	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	530994	16.255	ng/u1	0.00
54) 4-Nitrophenol-d4	14.651	143	38374	7.840	ng/u1	0.00
60) Fluorene-d10	15.439	176	376617	16.088	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	31550	7.410	ng/u1	0.00
73) Anthracene-d10	17.280	188	561687	16.742	ng/u1	0.00
81) Pyrene-d10	19.574	212	652416	17.063	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.491	264	681351	17.880	ng/u1	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.969	77	16208	2.206	ng/u1	98
16) Acetophenone	8.645	105	56957	2.878	ng/u1	98
86) Bis(2-ethylhexyl)phtha...	21.268	149	114068	4.822	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062121\
Data File : BM030507.D
Acq On : 21 Jun 2021 16:42
Operator : CG/JU
Sample : M2697-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLX82

Quant Time: Jun 21 17:12:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 21 10:48:13 2021
Response via : Initial Calibration




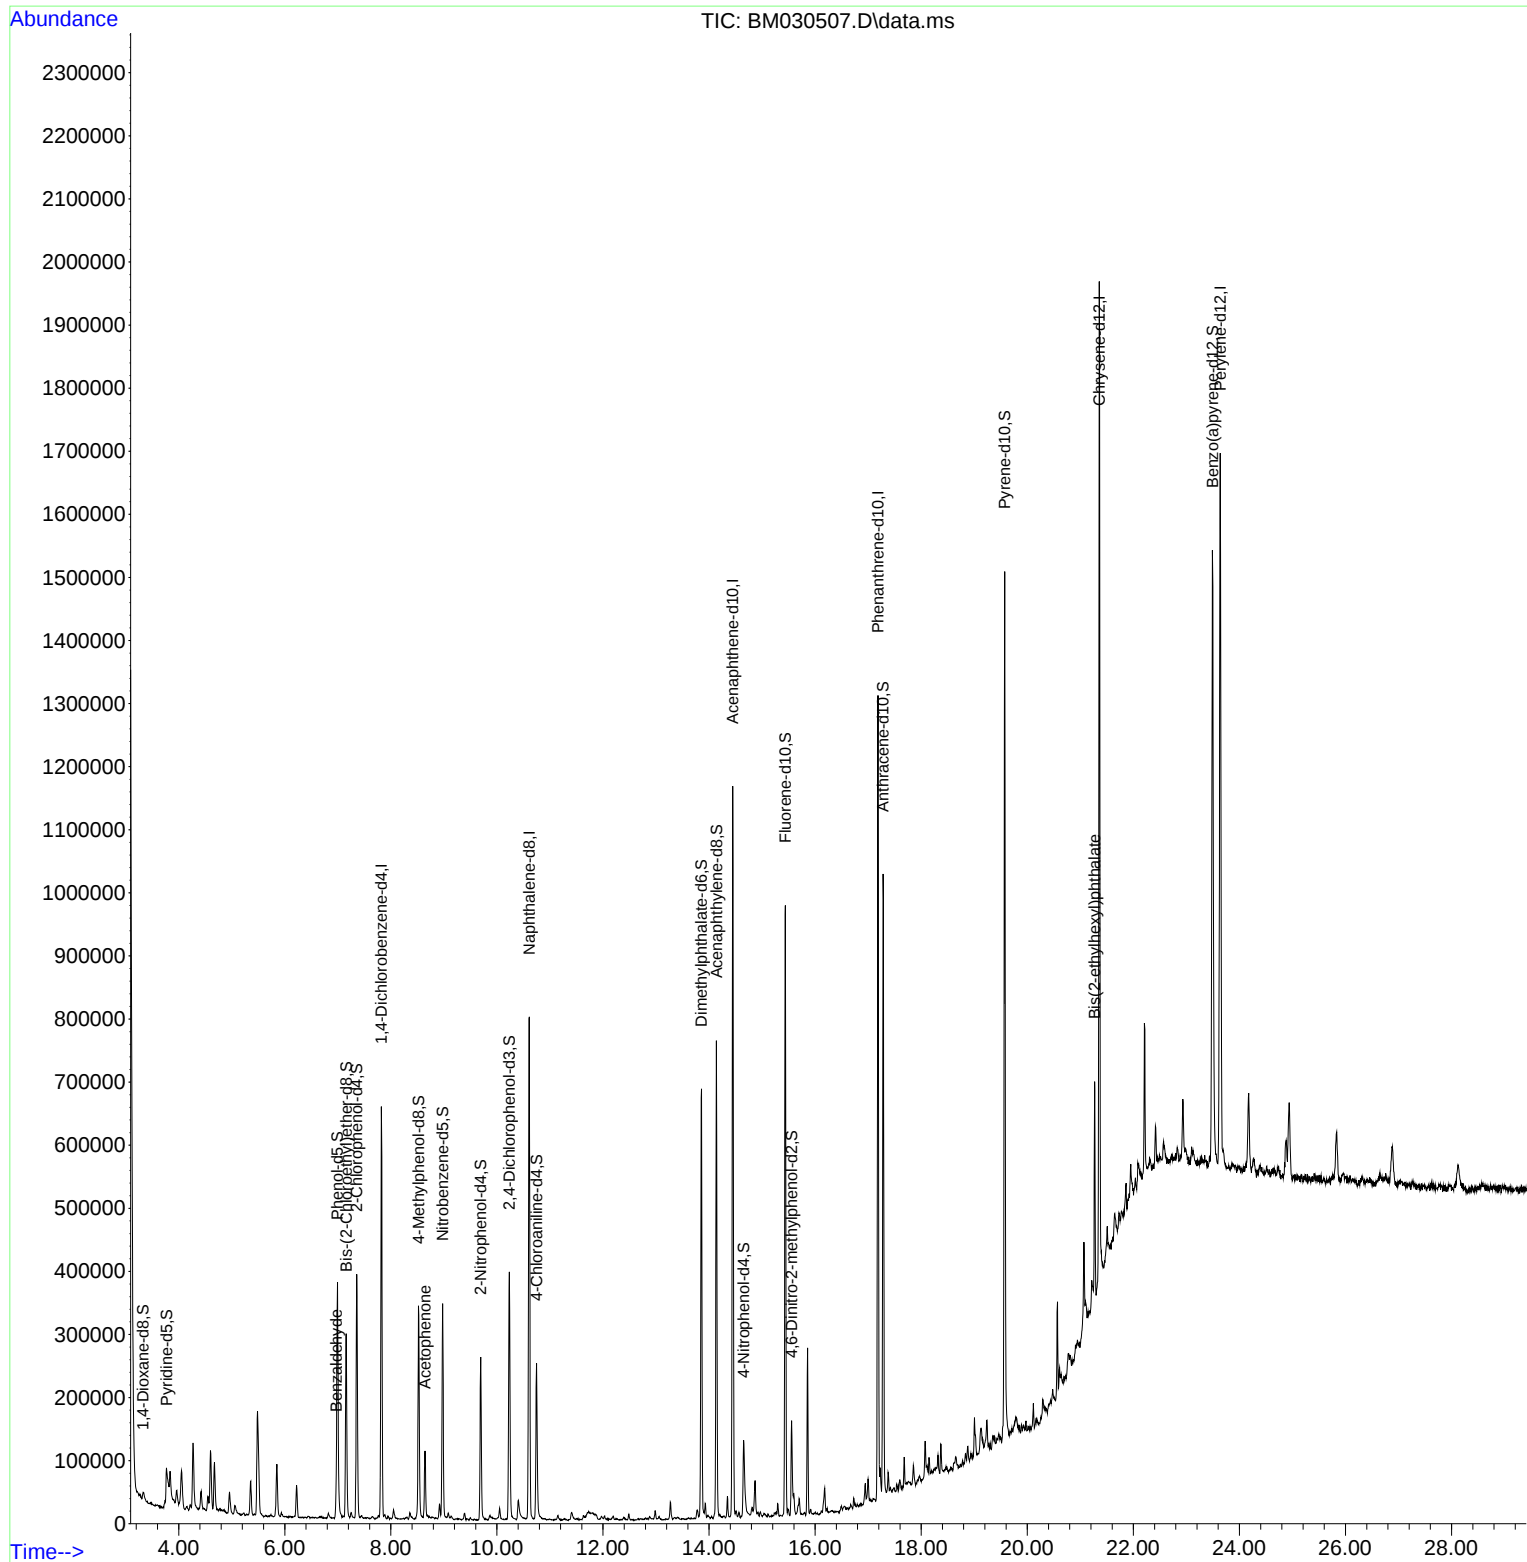


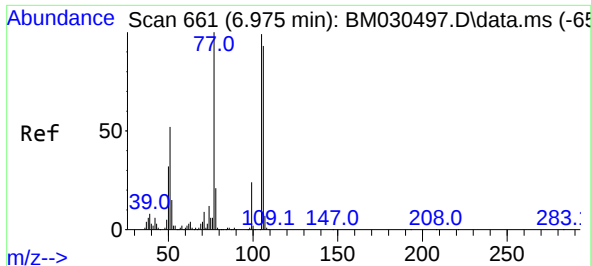

#6
Benzaldehyde
Concen: 2.206 ng/ul
RT: 6.969 min Scan# 660
Delta R.T. -0.006 min
Lab File: BM030507.D
Acq: 21 Jun 2021 16:42




Instrument :
BNA_M
ClientSampleId :
JLX82


Tgt Ion: 77 Resp: 16208
Ion Ratio Lower Upper
77 100
105 93.2 74.5 111.7
106 92.2 70.2 105.2

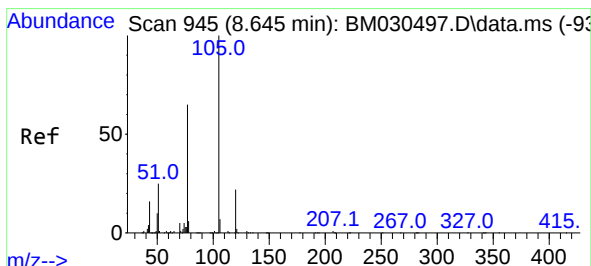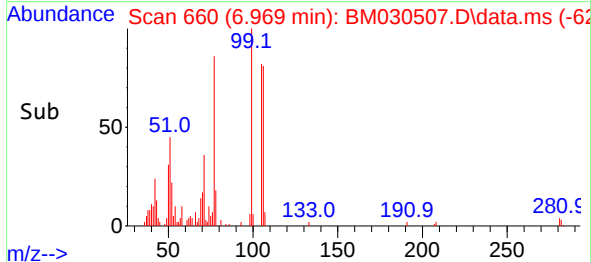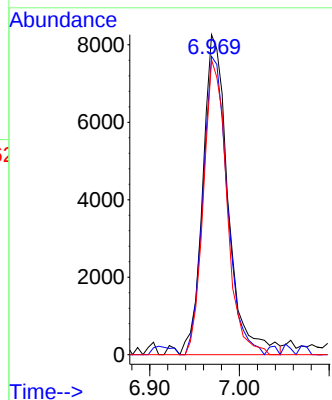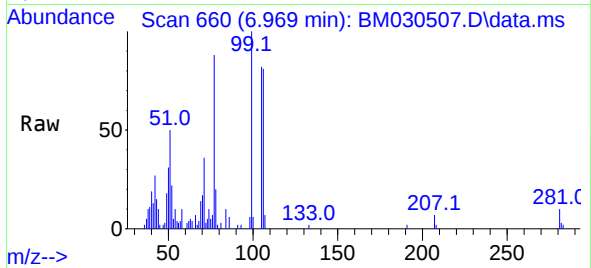

#16
Acetophenone
Concen: 2.878 ng/ul
RT: 8.645 min Scan# 945
Delta R.T. -0.000 min
Lab File: BM030507.D
Acq: 21 Jun 2021 16:42

Tgt Ion: 105 Resp: 56957
Ion Ratio Lower Upper
105 100
77 80.1 62.6 93.8
51 28.7 24.3 36.5

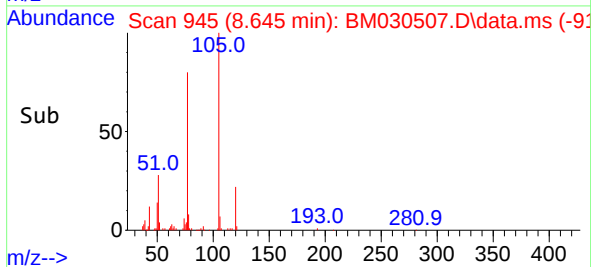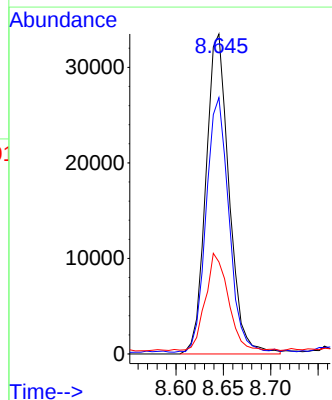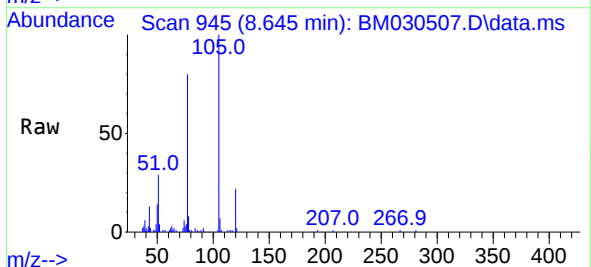

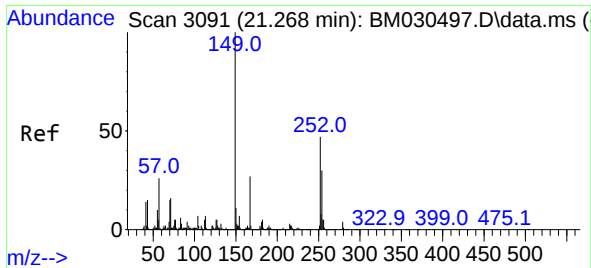

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.822 ng/ul
 RT: 21.268 min Scan# 3091
 Delta R.T. -0.000 min
 Lab File: BM030507.D
 Acq: 21 Jun 2021 16:42

Instrument :
 BNA_M
 ClientSampleId :
 JLX82

Tgt Ion:149 Resp: 114068
 Ion Ratio Lower Upper
 149 100
 167 25.0 20.9 31.3
 279 3.8 3.0 4.6

