

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062121\
 Data File : BM030498.D
 Acq On : 21 Jun 2021 10:34
 Operator : CG/JU
 Sample : PB137167BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030498.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	55	rVB	41889	107534	2.54%	0.228%
2	3.746	108	112	137	rBV	421246	1198750	28.35%	2.543%
3	6.992	657	664	678	rBV	854047	1493494	35.33%	3.168%
4	7.157	685	692	709	rVB	677572	1145799	27.10%	2.431%
5	7.363	718	727	738	rBV	913372	1576904	37.30%	3.345%
6	7.822	798	805	814	rVB	710231	1189298	28.13%	2.523%
7	8.528	916	925	937	rBV	1025868	1737816	41.11%	3.686%
8	8.975	994	1001	1014	rBV	809517	1376548	32.56%	2.920%
9	9.698	1114	1124	1138	rBV	667858	1168351	27.64%	2.478%
10	10.233	1207	1215	1228	rBV	1010278	1752838	41.46%	3.718%
11	10.610	1271	1279	1288	rBV	919970	1544142	36.52%	3.276%
12	10.745	1295	1302	1320	rBV	845023	1596190	37.76%	3.386%
13	11.869	1483	1493	1506	rVB5	11041	37509	0.89%	0.080%
14	12.198	1542	1549	1555	rBV	19193	32260	0.76%	0.068%
15	13.151	1704	1711	1714	rBV4	5183	9962	0.24%	0.021%
16	13.180	1714	1716	1723	rVB6	3565	4812	0.11%	0.010%
17	13.410	1752	1755	1760	rVB5	2646	4949	0.12%	0.010%
18	13.857	1824	1831	1843	rBV	1529241	2233802	52.84%	4.738%
19	14.139	1872	1879	1895	rBV	1893814	2834094	67.04%	6.012%
20	14.445	1924	1931	1942	rBV	1265680	1890385	44.71%	4.010%
21	14.645	1959	1965	1988	rBV	565000	1012066	23.94%	2.147%
22	15.439	2093	2100	2107	rBV	2359152	3371250	79.74%	7.151%
23	15.557	2114	2120	2131	rBV	534249	772594	18.27%	1.639%
24	15.680	2136	2141	2149	rVB	28838	43312	1.02%	0.092%
25	15.898	2175	2178	2180	rBV4	4414	5771	0.14%	0.012%
26	16.009	2193	2197	2200	rBV4	2792	5293	0.13%	0.011%
27	16.227	2227	2234	2239	rBV8	11690	22454	0.53%	0.048%
28	16.492	2275	2279	2281	rBV5	4507	6545	0.15%	0.014%
29	16.586	2289	2295	2307	rBV3	56145	136747	3.23%	0.290%
30	16.862	2340	2342	2346	rBV4	4595	4648	0.11%	0.010%
31	16.974	2357	2361	2369	rVB2	5960	10252	0.24%	0.022%
32	17.186	2390	2397	2404	rBV	1476810	2063074	48.80%	4.376%
33	17.286	2407	2414	2425	rVB	2466899	3506450	82.94%	7.438%
34	17.856	2507	2511	2513	rBV5	5503	7471	0.18%	0.016%
35	18.080	2546	2549	2554	rBV6	7366	10596	0.25%	0.022%
36	18.356	2591	2596	2600	rBV	63519	101050	2.39%	0.214%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062121\
Data File : BM030498.D
Acq On : 21 Jun 2021 10:34
Operator : CG/JU
Sample : PB137167BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Title : SVOA CALIBRATION

37	18.409	2600	2605	2619	rVB3	91424	206077	4.87%	0.437%
38	19.209	2737	2741	2746	rBV	28257	38249	0.90%	0.081%
39	19.462	2780	2784	2789	rBV2	23013	31424	0.74%	0.067%
40	19.574	2797	2803	2808	rBV	3036326	3966526	93.82%	8.414%
41	19.615	2808	2810	2816	rVB	43654	63609	1.50%	0.135%
42	21.356	3101	3106	3112	rBV	1657950	2194771	51.91%	4.656%
43	23.485	3461	3468	3477	rBV2	2232343	4227723	100.00%	8.968%
44	23.632	3486	3493	3500	rVB2	1233892	2398715	56.74%	5.088%




Sum of corrected areas: 47142104

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062121\
Data File : BM030498.D
Acq On : 21 Jun 2021 10:34
Operator : CG/JU
Sample : PB137167BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

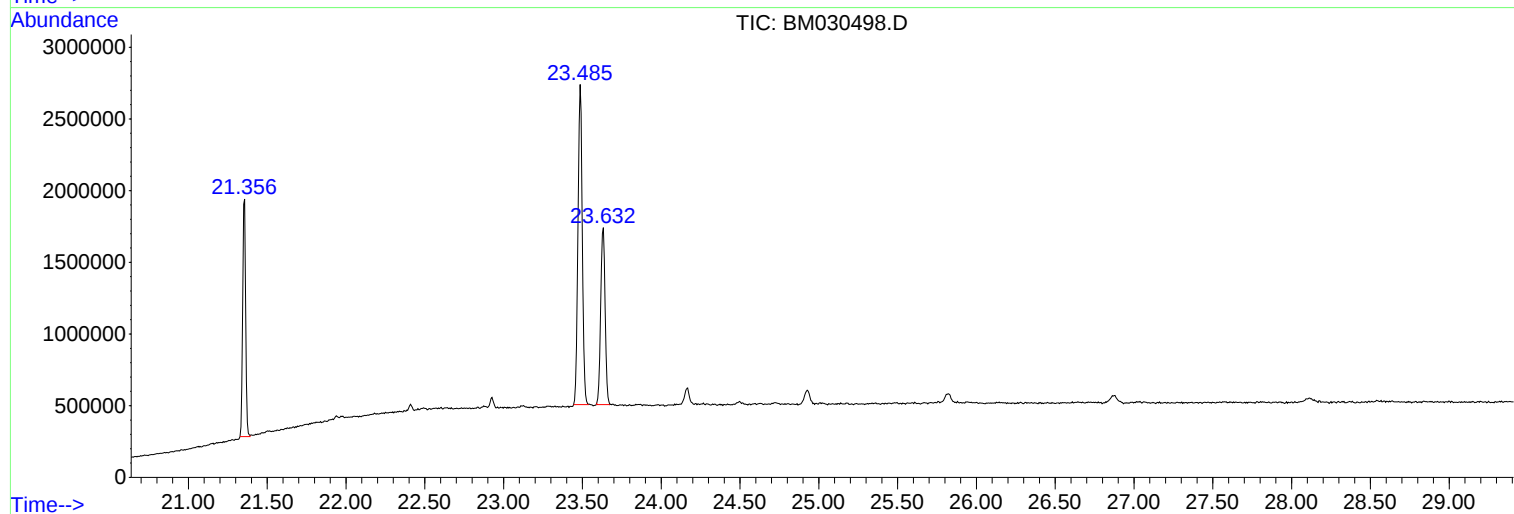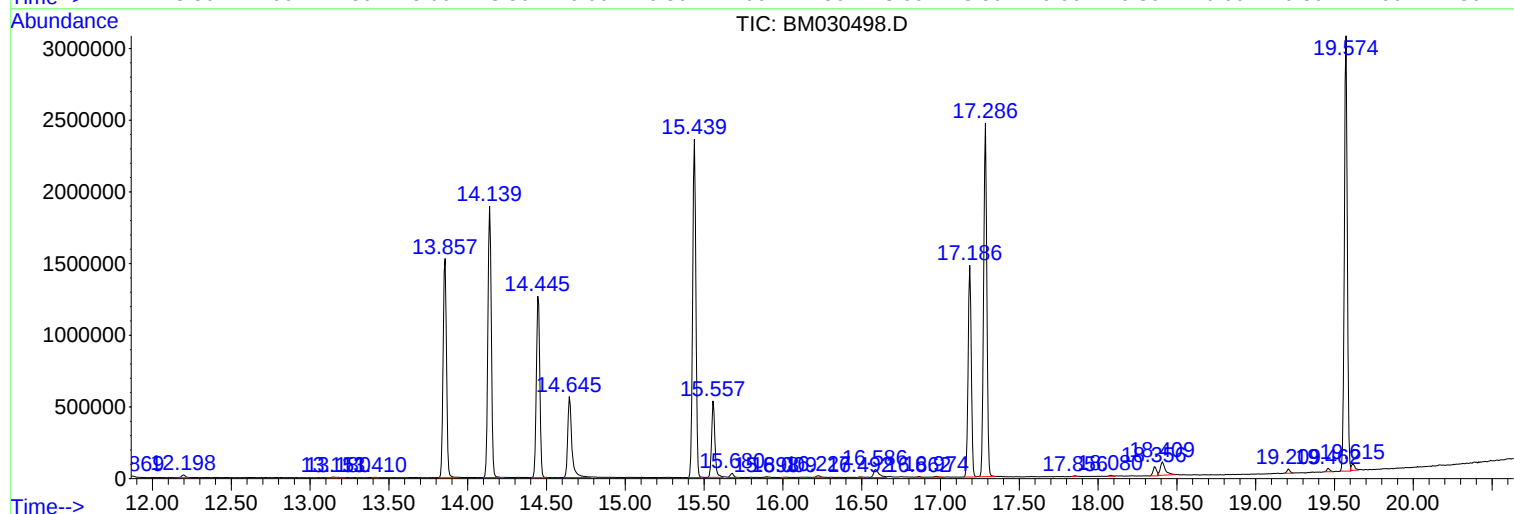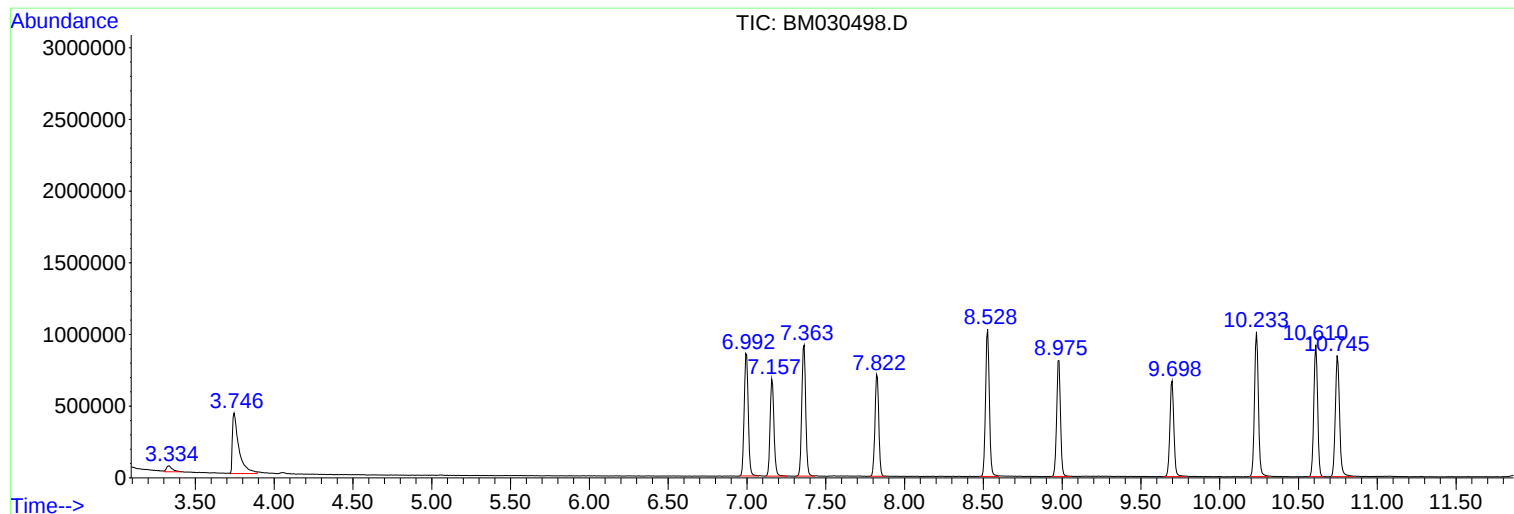

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062121\
Data File : BM030498.D
Acq On : 21 Jun 2021 10:34
Operator : CG/JU
Sample : PB137167BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062121\
Data File : BM030498.D
Acq On : 21 Jun 2021 10:34
Operator : CG/JU
Sample : PB137167BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK167

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
